


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF093020\
 Data File : BF121740.D
 Acq On : 30 Sep 2020 15:59
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 29 11:12:14 2020

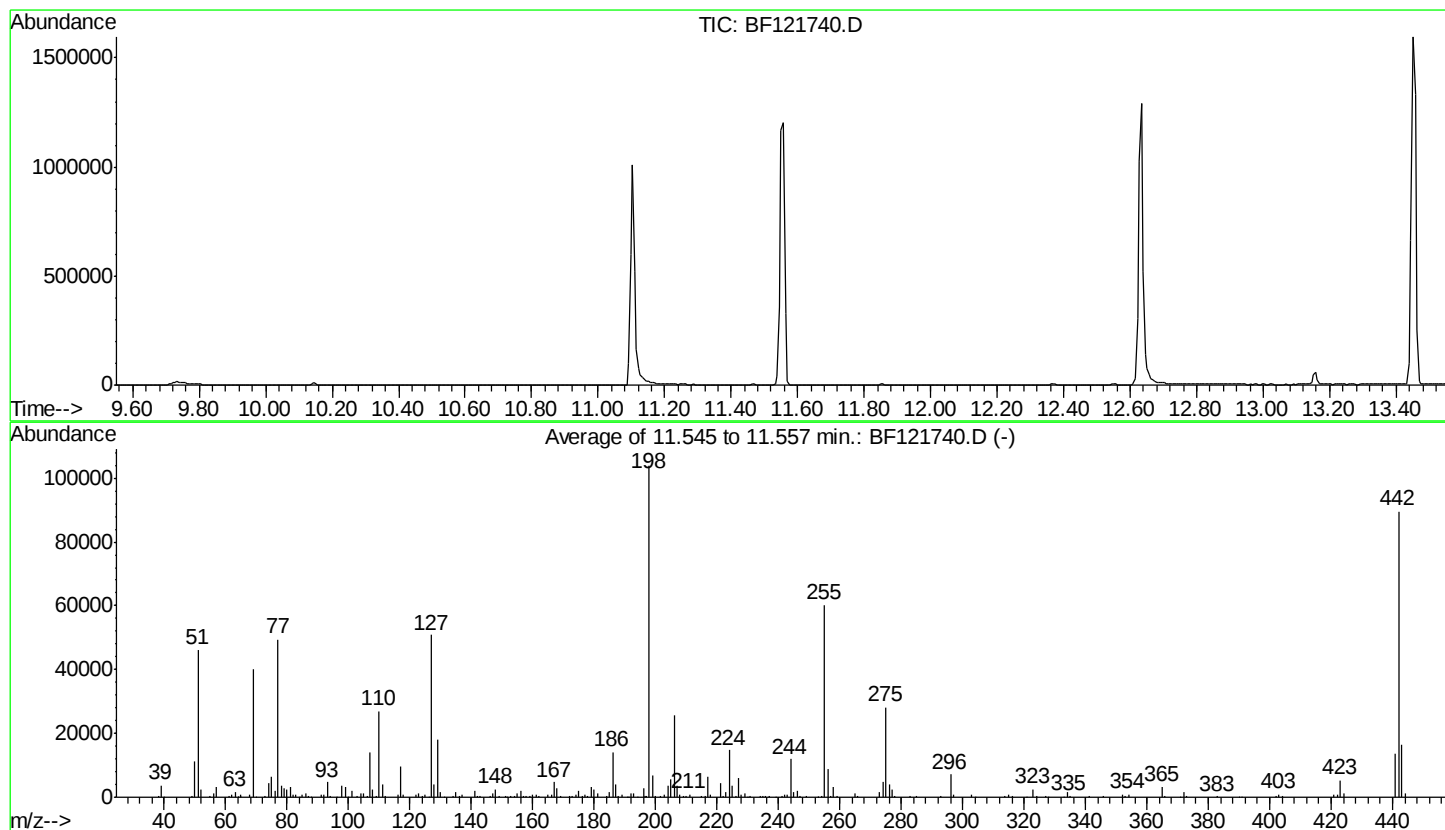

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.5	46240	PASS
68	69	0.00	2	2.0	806	PASS
69	198	0.00	100	38.7	40221	PASS
70	69	0.00	2	0.3	138	PASS
127	198	10	80	49.0	50912	PASS
197	198	0.00	2	0.3	305	PASS
198	198	100	100	100.0	103896	PASS
199	198	5	9	6.7	6968	PASS
275	198	10	60	27.1	28149	PASS
365	198	1	100	3.3	3418	PASS
441	198	0.01	100	13.2	13689	PASS
442	198	50	100	86.3	89642	PASS
443	442	15	24	18.5	16624	PASS