

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF093022\
 Data File : BF130484.D
 Acq On : 30 Sep 2022 15:07
 Operator : CG\JU
 Sample : N4896-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CRUSHED-MASONRY-PILE-9

Quant Time: Oct 01 01:35:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 28 02:59:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.639	152	108747	20.000	ng	0.00
21) Naphthalene-d8	7.922	136	423294	20.000	ng	# 0.00
39) Acenaphthene-d10	9.669	164	210759	20.000	ng	-0.01
64) Phenanthrene-d10	11.151	188	339152	20.000	ng	0.00
76) Chrysene-d12	13.780	240	197667	20.000	ng	-0.01
86) Perylene-d12	15.168	264	228681	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.251	112	10195	1.626	ng	0.00
7) Phenol-d6	6.275	99	170226	21.699	ng	-0.02
23) Nitrobenzene-d5	7.204	82	509430	61.484	ng	-0.01
42) 2,4,6-Tribromophenol	10.463	330	57	0.028	ng	0.00
45) 2-Fluorobiphenyl	8.998	172	987793	68.249	ng	-0.01
79) Terphenyl-d14	12.733	244	822248	68.906	ng	-0.01


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF093022\
Data File : BF130484.D
Acq On : 30 Sep 2022 15:07
Operator : CG\JU
Sample : N4896-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CRUSHED-MASONRY-PILE-9

Quant Time: Oct 01 01:35:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 02:59:31 2022
Response via : Initial Calibration




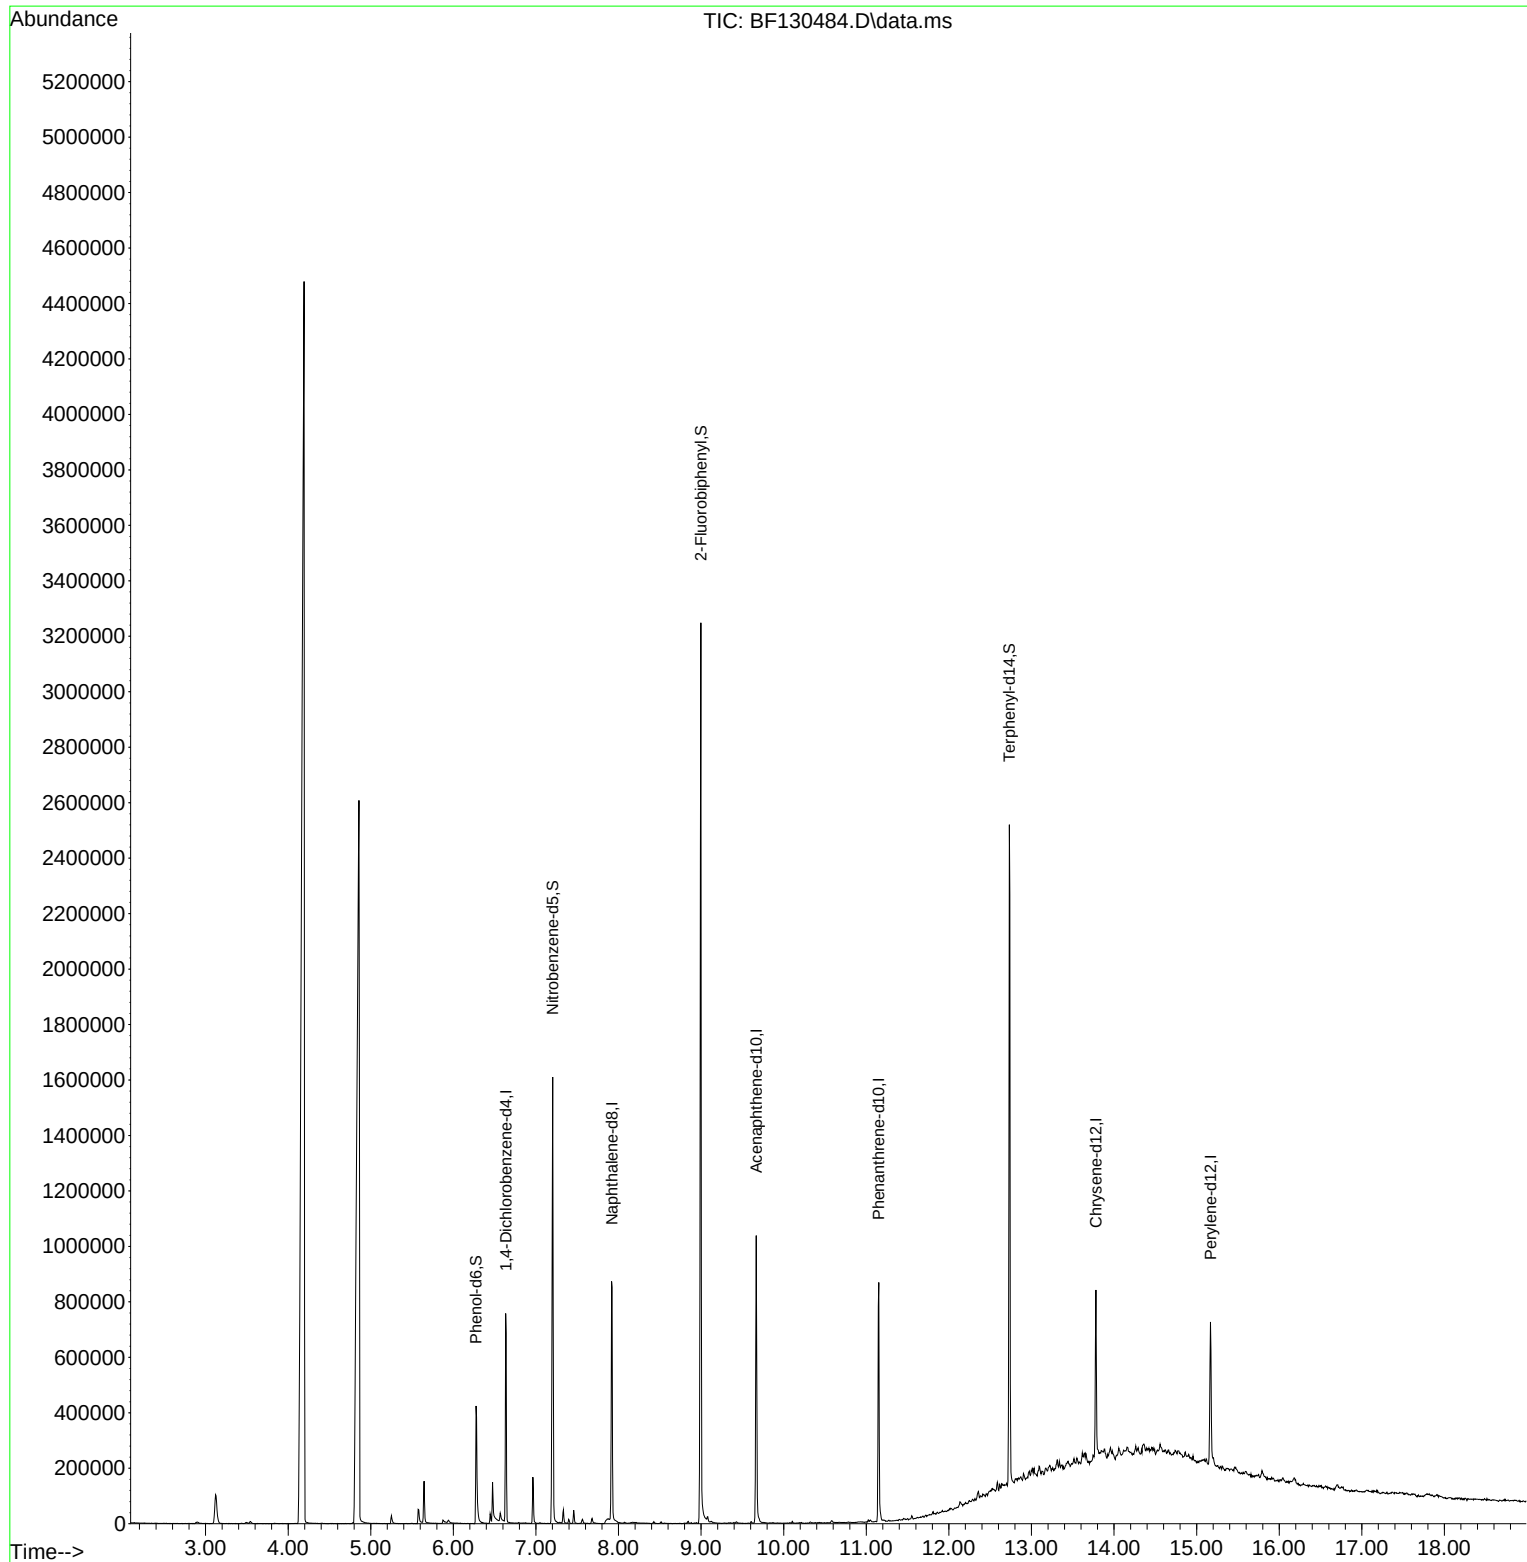




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.639 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF130484.D
Acq: 30 Sep 2022 15:07




Instrument :
BNA_F
ClientSampleId :
CRUSHED-MASONRY-PILE-9


Tgt Ion:152 Resp: 108747
Ion Ratio Lower Upper
152 100
150 152.0 122.8 184.2
115 61.1 53.8 80.8

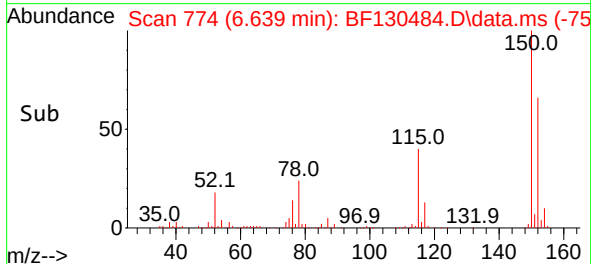

#5
2-Fluorophenol
Concen: 1.626 ng
RT: 5.251 min Scan# 538
Delta R.T. 0.006 min
Lab File: BF130484.D
Acq: 30 Sep 2022 15:07

Tgt Ion:112 Resp: 10195
Ion Ratio Lower Upper
112 100
64 58.2 51.4 77.0
63 30.8 28.8 43.2


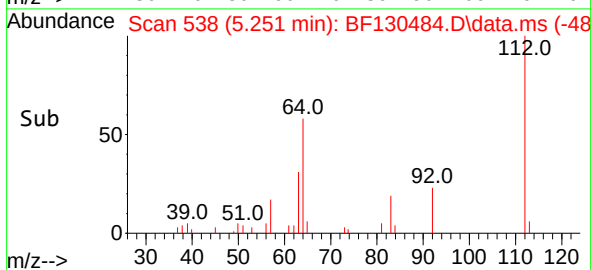

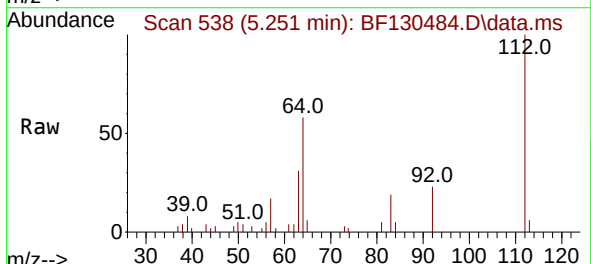




#7
Phenol-d6
Concen: 21.699 ng
RT: 6.275 min Scan# 71
Delta R.T. -0.018 min
Lab File: BF130484.D
Acq: 30 Sep 2022 15:07




Instrument :
BNA_F
ClientSampleId :
CRUSHED-MASONRY-PILE-9


Tgt Ion: 99 Resp: 170226
Ion Ratio Lower Upper
99 100
42 18.2 17.0 25.6
71 37.3 32.3 48.5

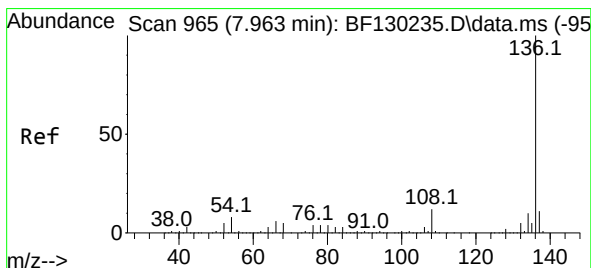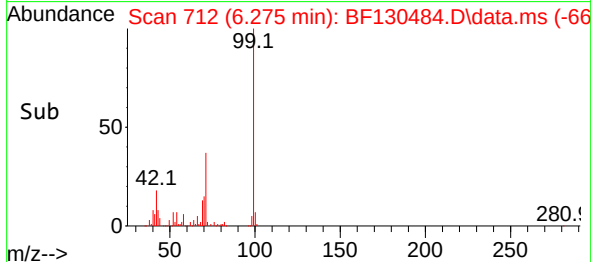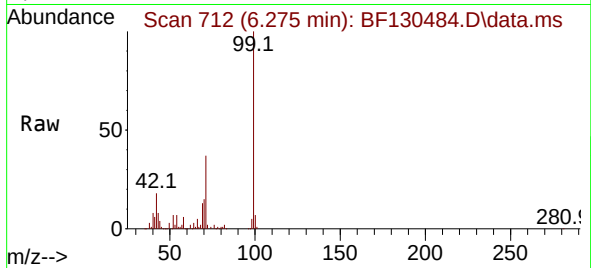

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 7.922 min Scan# 992
Delta R.T. -0.006 min
Lab File: BF130484.D
Acq: 30 Sep 2022 15:07

Tgt Ion: 136 Resp: 423294
Ion Ratio Lower Upper
136 100
137 10.7 9.1 13.7
54 6.3 7.1 10.7#
68 5.1 4.5 6.7


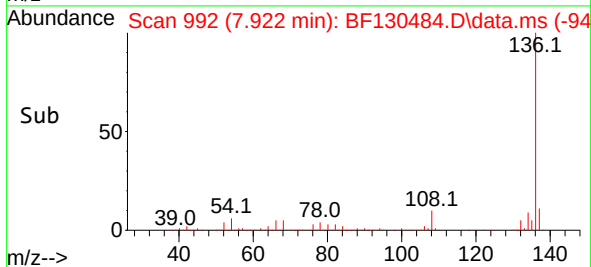

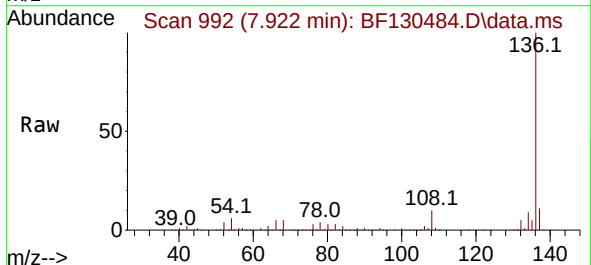




#23
Nitrobenzene-d5
Concen: 61.484 ng
RT: 7.204 min Scan# 81
Delta R.T. -0.012 min
Lab File: BF130484.D
Acq: 30 Sep 2022 15:07




Instrument :
BNA_F
ClientSampleId :
CRUSHED-MASONRY-PILE-9


Tgt Ion: 82 Resp: 509430
Ion Ratio Lower Upper
82 100
128 45.3 32.6 49.0
54 50.3 43.8 65.6

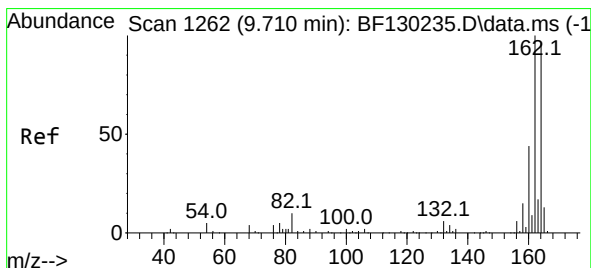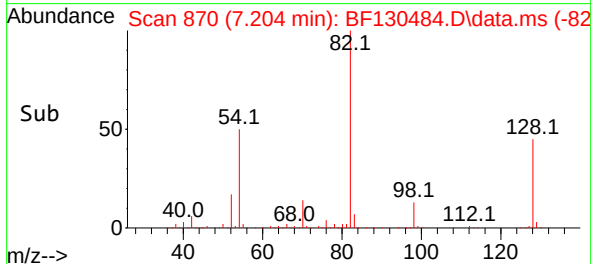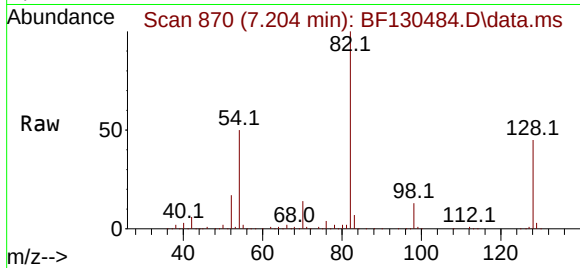

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.669 min Scan# 1289
Delta R.T. -0.012 min
Lab File: BF130484.D
Acq: 30 Sep 2022 15:07


Tgt Ion:164 Resp: 210759
Ion Ratio Lower Upper
164 100
162 100.2 81.4 122.0
160 45.1 36.2 54.4

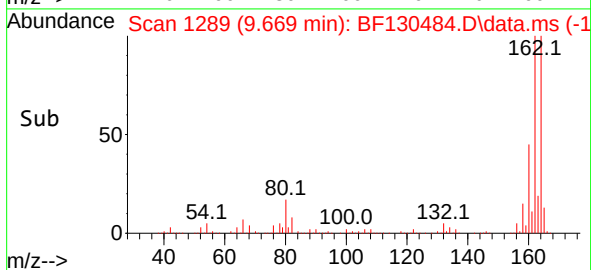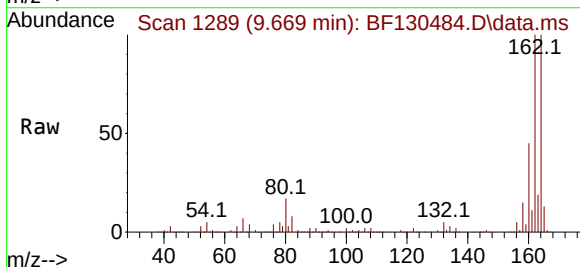






#42
2,4,6-Tribromophenol
Concen: 0.028 ng
RT: 10.463 min Scan# 1424
Delta R.T. -0.006 min
Lab File: BF130484.D
Acq: 30 Sep 2022 15:07

Instrument : BNA_F
ClientSampleId : CRUSHED-MASONRY-PILE-9







Tgt Ion: 330 Resp: 57
Ion Ratio Lower Upper
330 100
332 96.5 83.4 125.2
141 0.0 34.0 51.0#

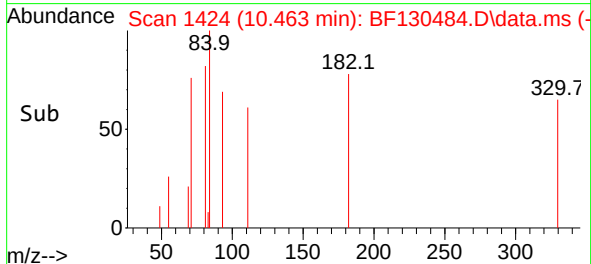

#45
2-Fluorobiphenyl
Concen: 68.249 ng
RT: 8.998 min Scan# 1175
Delta R.T. -0.012 min
Lab File: BF130484.D
Acq: 30 Sep 2022 15:07

Tgt Ion: 172 Resp: 987793
Ion Ratio Lower Upper
172 100
171 34.9 28.3 42.5
170 23.1 18.7 28.1


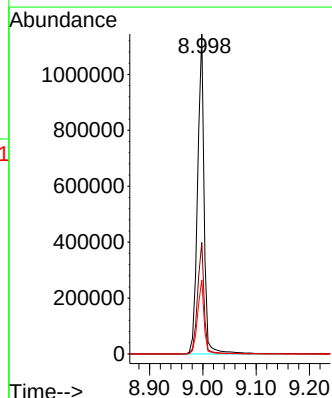
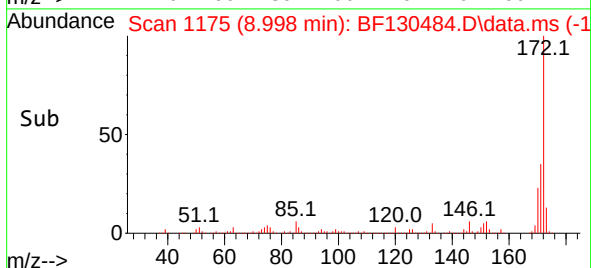
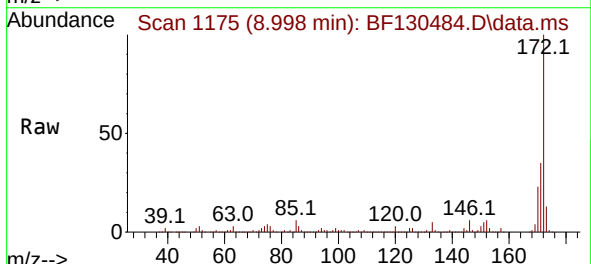




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.151 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF130484.D
Acq: 30 Sep 2022 15:07




Instrument :
BNA_F
ClientSampleId :
CRUSHED-MASONRY-PILE-9


Tgt Ion:188 Resp: 339152
Ion Ratio Lower Upper
188 100
94 8.1 7.4 11.2
80 8.6 7.9 11.9

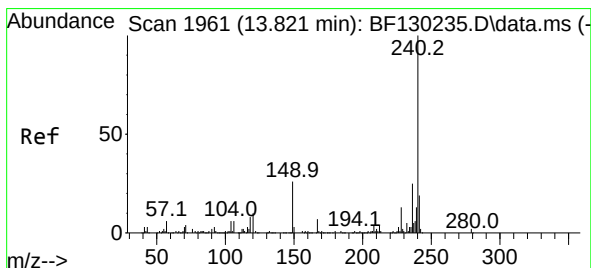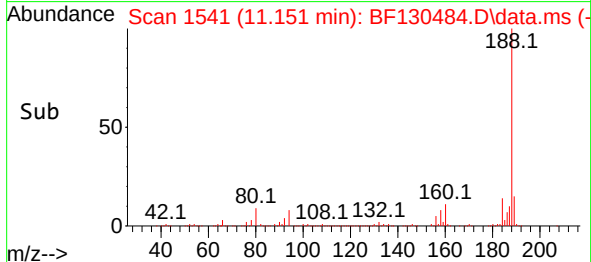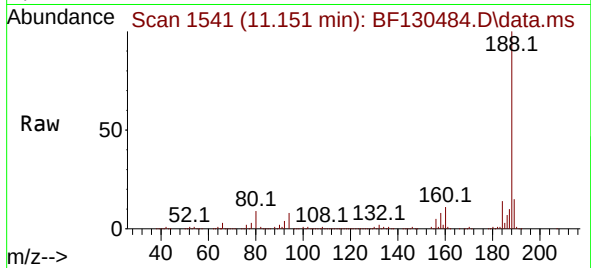

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.780 min Scan# 1988
Delta R.T. -0.012 min
Lab File: BF130484.D
Acq: 30 Sep 2022 15:07

Tgt Ion:240 Resp: 197667
Ion Ratio Lower Upper
240 100
120 10.0 8.7 13.1
236 25.2 20.9 31.3


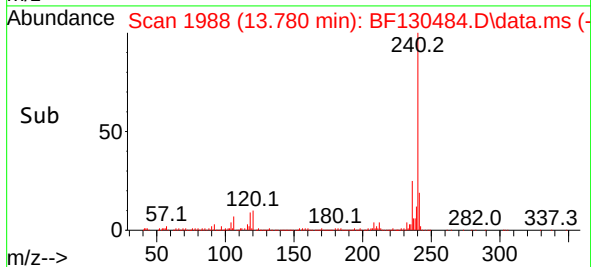

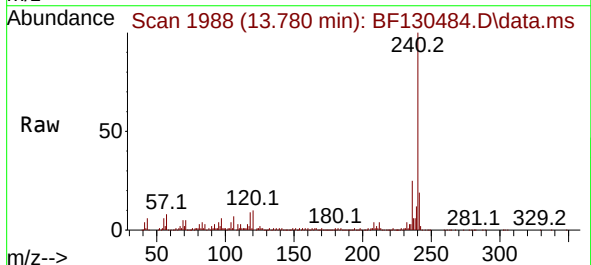




#79
 Terphenyl-d14
 Concen: 68.906 ng
 RT: 12.733 min Scan# 11
 Delta R.T. -0.012 min
 Lab File: BF130484.D
 Acq: 30 Sep 2022 15:07

Instrument :
 BNA_F
 ClientSampleId :
 CRUSHED-MASONRY-PILE-9

Tgt Ion:244 Resp: 822248
 Ion Ratio Lower Upper
 244 100
 212 7.5 5.9 8.9
 122 12.2 8.5 12.7

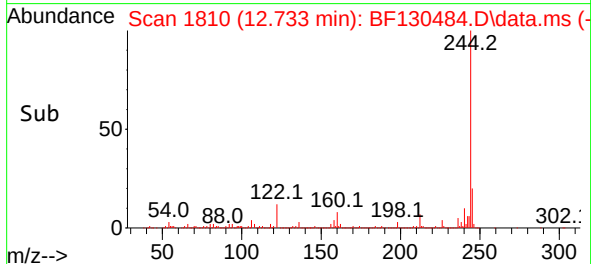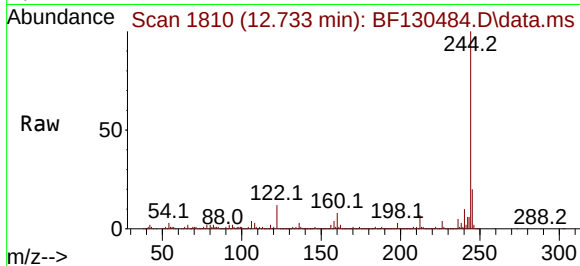

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.168 min Scan# 2224
 Delta R.T. -0.006 min
 Lab File: BF130484.D
 Acq: 30 Sep 2022 15:07

Tgt Ion:264 Resp: 228681
 Ion Ratio Lower Upper
 264 100
 260 23.8 19.3 28.9
 265 21.6 17.0 25.4

