


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF093022\
 Data File : BF130479.D
 Acq On : 30 Sep 2022 11:48
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 06 01:07:05 2022

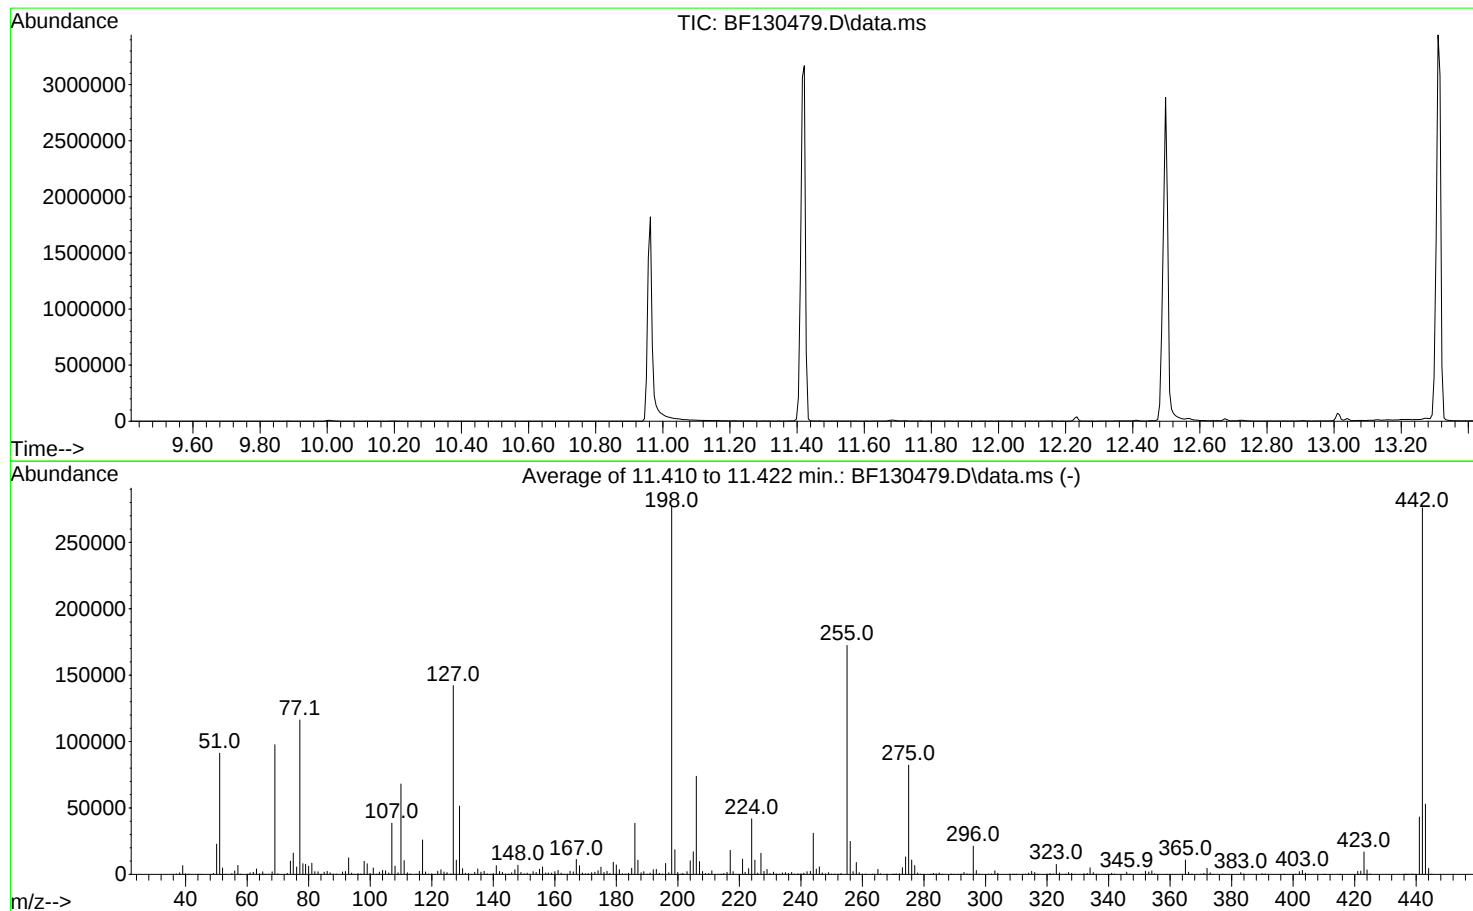




AutoFind: Scans 1585, 1586, 1587; Background Corrected with Scan 1579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	91251	PASS
68	69	0.00	2	2.0	1931	PASS
69	198	0.00	100	35.2	97629	PASS
70	69	0.00	2	0.6	548	PASS
127	198	10	80	51.3	142179	PASS
197	198	0.00	2	0.4	1244	PASS
198	198	100	100	100.0	277013	PASS
199	198	5	9	6.7	18532	PASS
275	198	10	60	29.7	82333	PASS
365	198	1	100	3.9	10811	PASS
441	198	0.01	100	15.6	43298	PASS
442	442	50	100	100.0	276053	PASS
443	442	15	24	19.1	52849	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF093022\
 Data File : BF130479.D
 Acq On : 30 Sep 2022 11:48
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 01 03:05:12 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 28 02:59:31 2022
 Response via : Initial Calibration

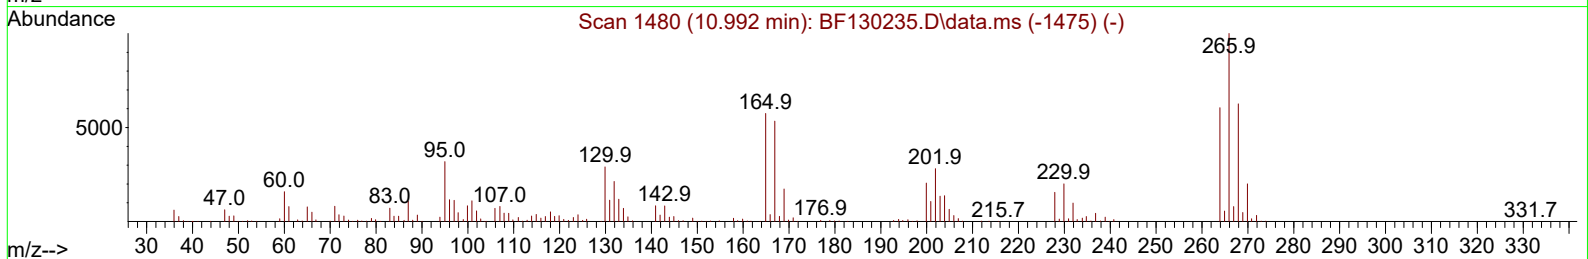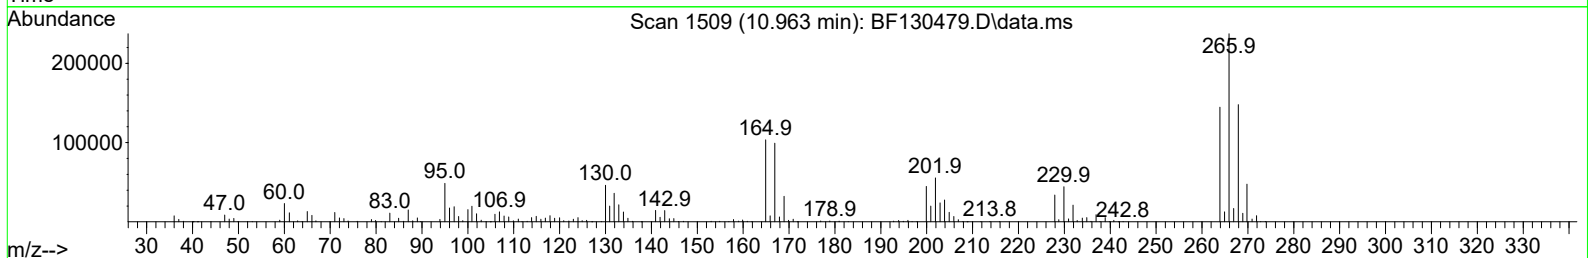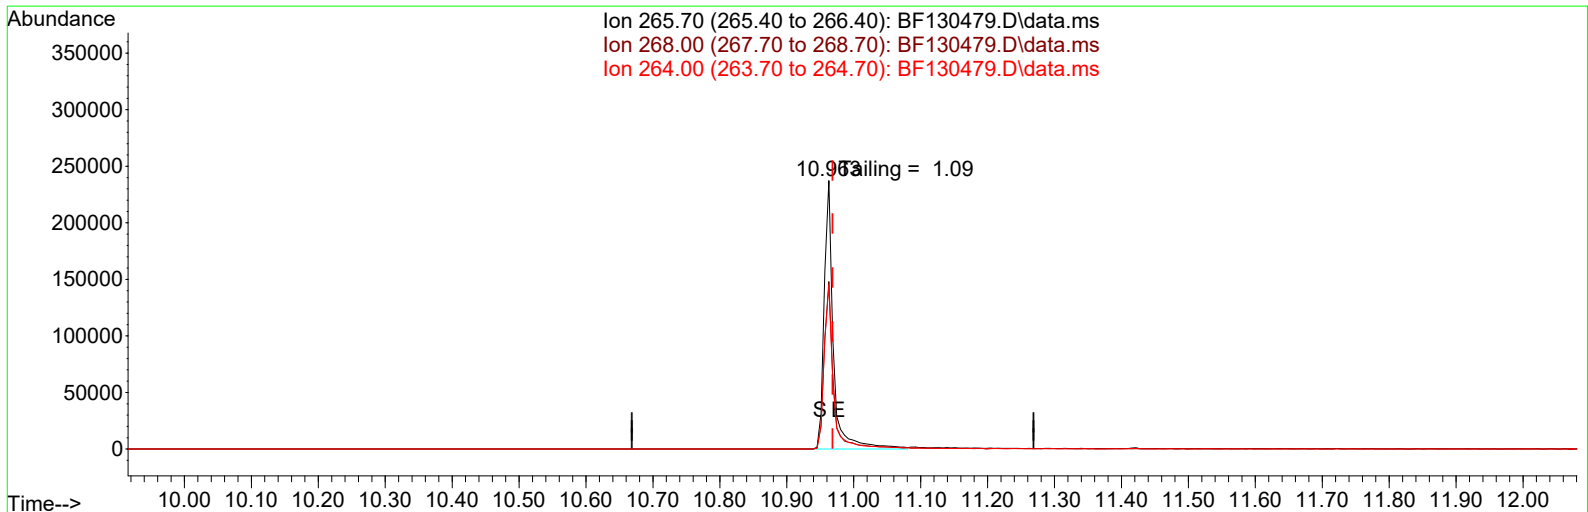

TIC: BF130479.D\data.ms

(70) Pentachlorophenol (C)

10.963min (-0.006) 264335.91 ng




response 228852

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.35
264.00	63.10	60.98
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF093022\  
Data File : BF130479.D  
Acq On    : 30 Sep 2022  11:48  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 01 03:05:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 02:59:31 2022
Response via : Initial Calibration

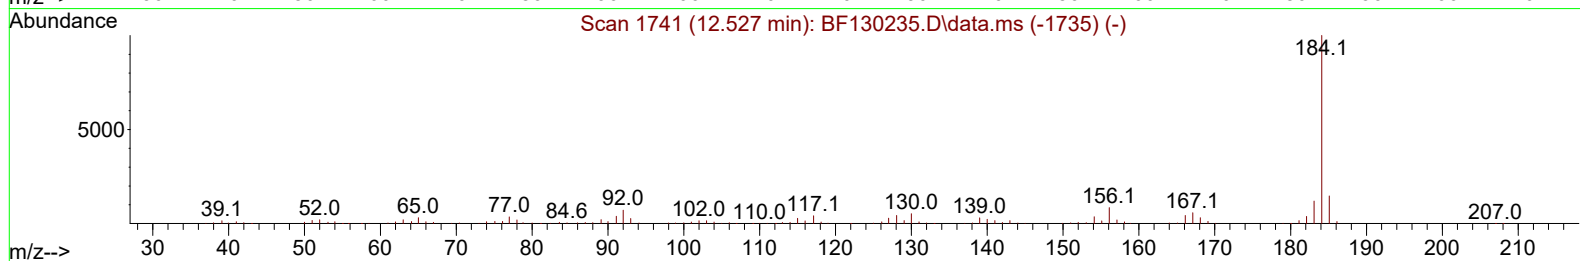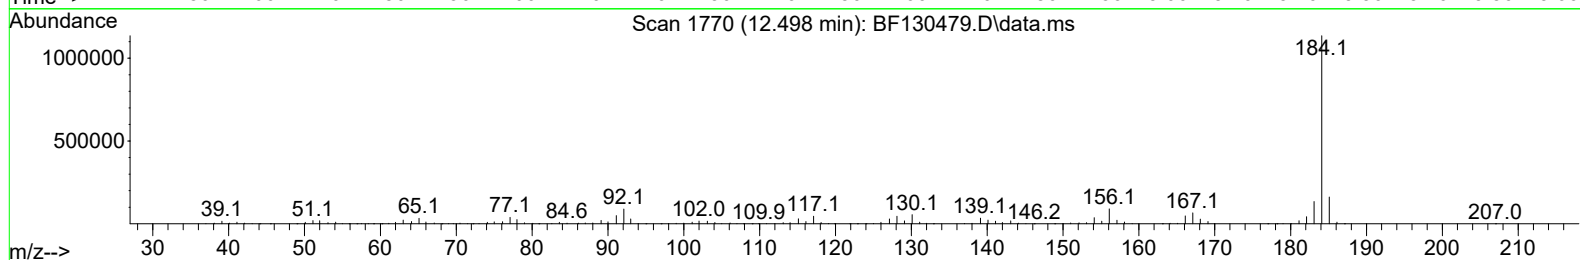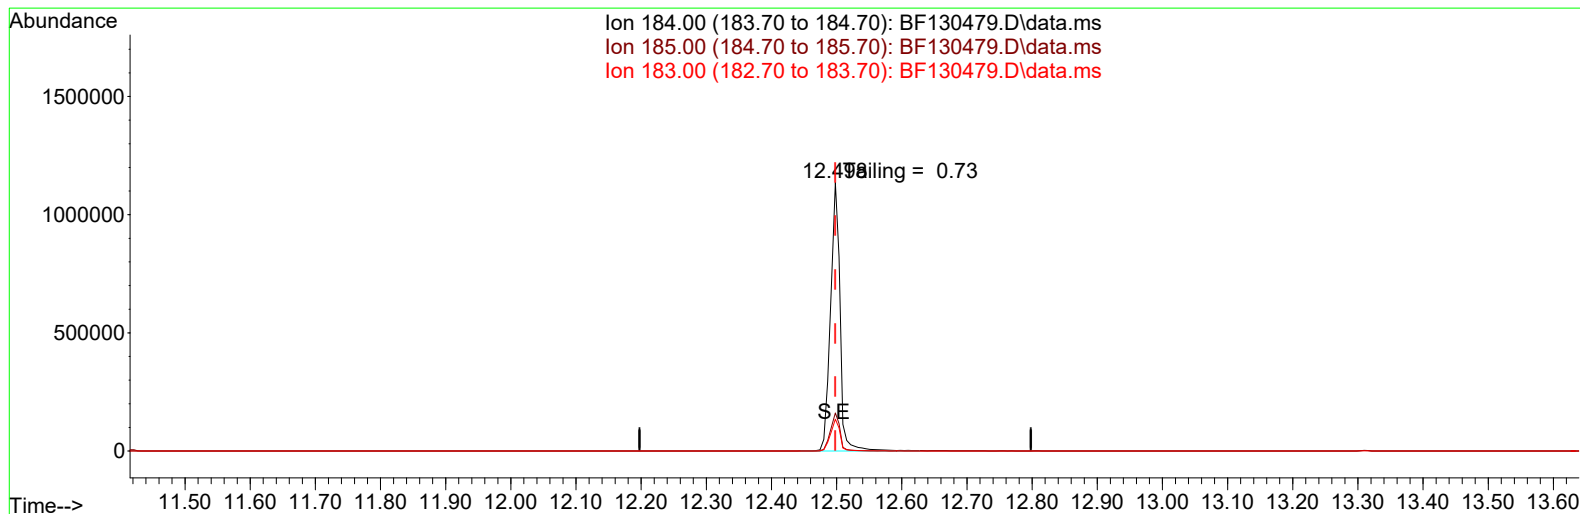

TIC: BF130479.D\data.ms

(77) Benzidine

12.498min (0.000) 71477.41 ng

response **1170258**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.20
183.00	11.40	11.88
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/30/2022	BNA_F	<u>BF130479.D</u>
Compound Name	Response	Retention Time
DDT	626594	13.31
DDD	15443	13.01
DDE	2433	12.674
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17876	644470	2.77

Instrument :
BNA_F
ClientSampleId :
DFTPP