
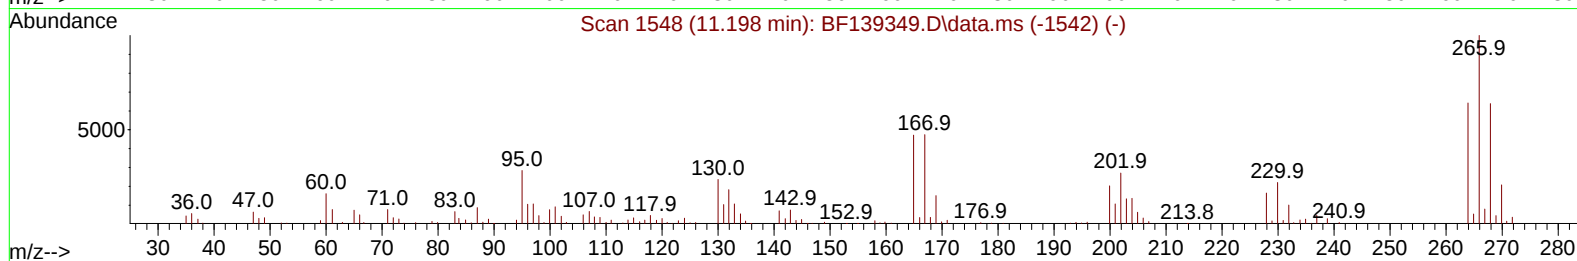
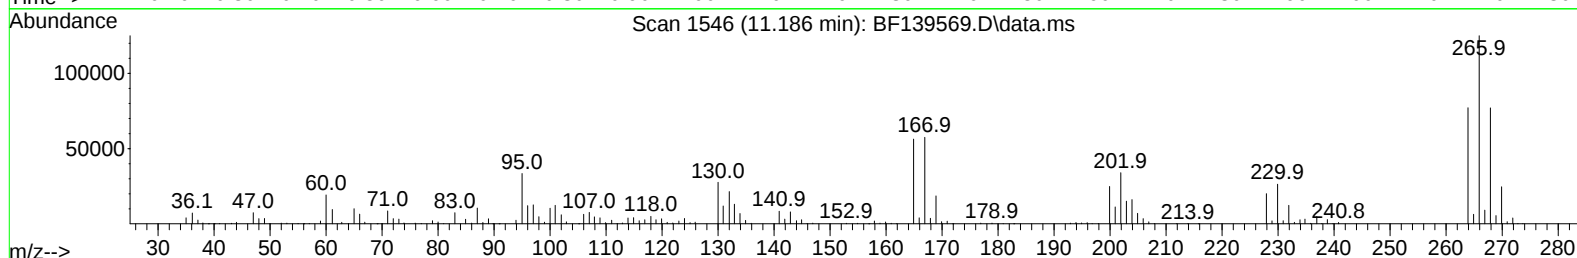


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF093024\
Data File : BF139569.D
Acq On : 30 Sep 2024 09:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 13:10:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

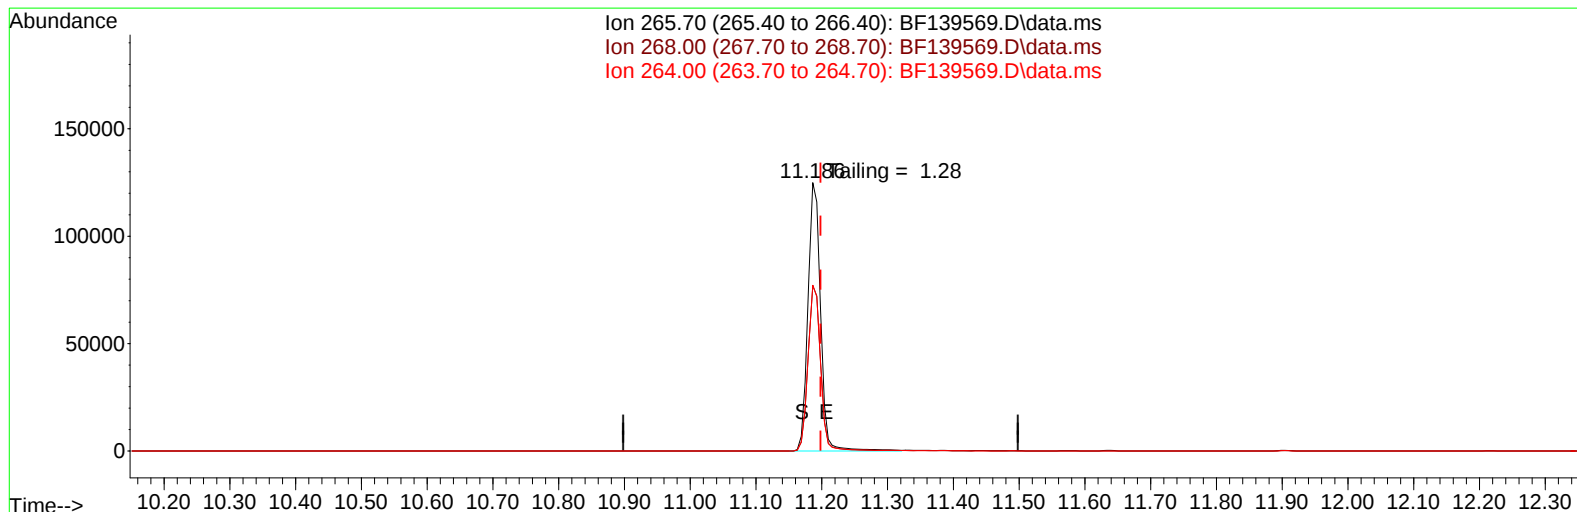

TIC: BF139569.D\data.ms

(70) Pentachlorophenol (C)

11.186min (-0.012) 435054.79 ng

response	166986
----------	--------

Ion	Exp%	Act%
-----	------	------

265.70	100.00	100.00
--------	--------	--------




268.00	63.90	61.67
--------	-------	-------

264.00	64.20	61.76
--------	-------	-------

0.00 0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF093024\
Data File : BF139569.D
Acq On : 30 Sep 2024 09:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 13:10:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

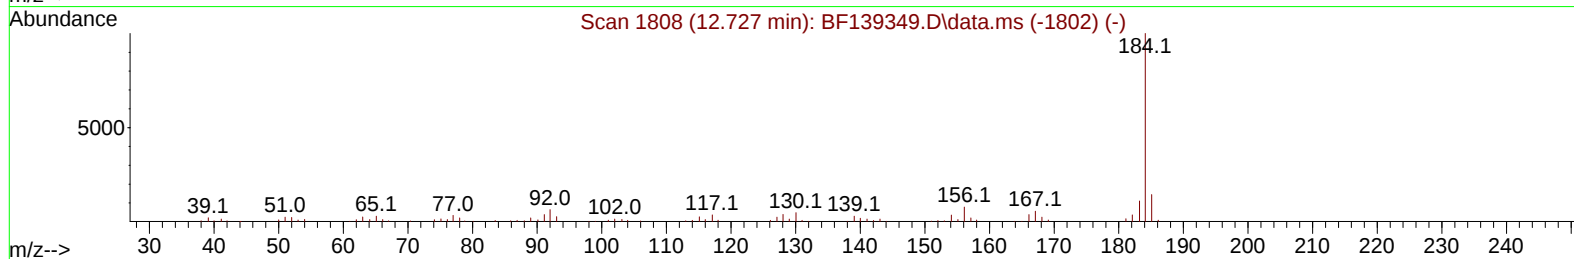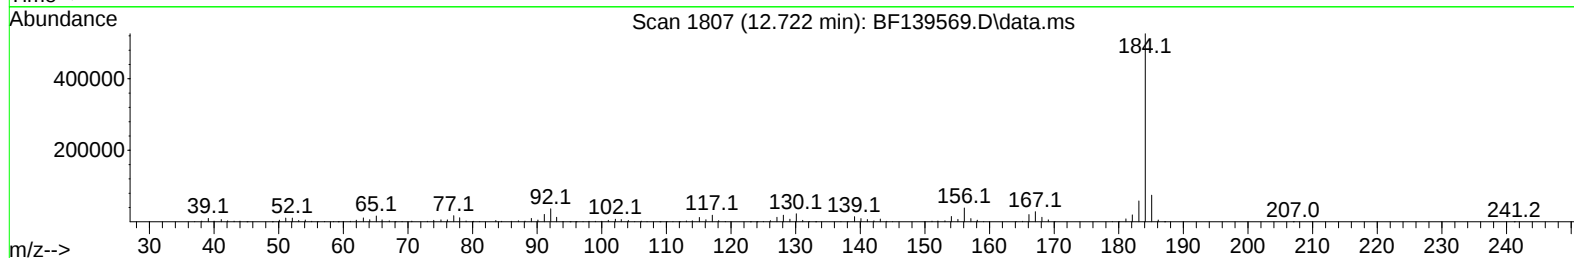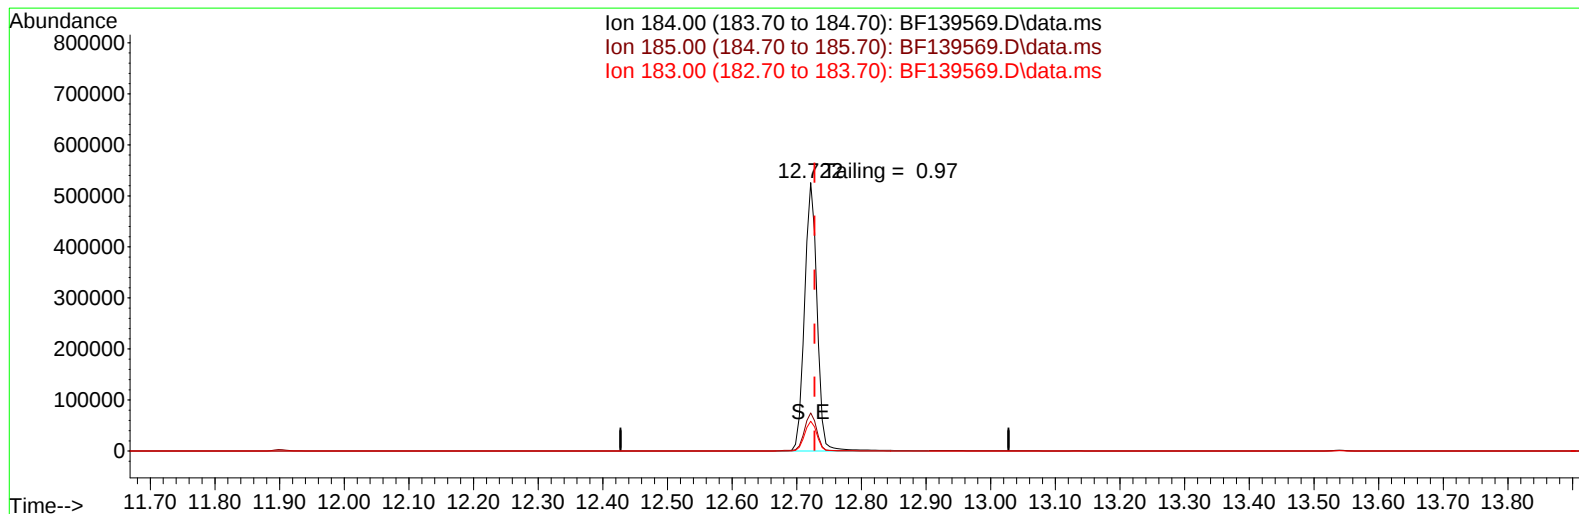

TIC: BF139569.D\data.ms

(77) Benzidine

12.722min (-0.006) 11020.57 ng

response 706569

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.18
183.00	11.10	11.10
0.00	0.00	0.00