


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF093024\
Data File : BF139569.D
Acq On : 30 Sep 2024 09:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Sep 14 02:58:23 2024

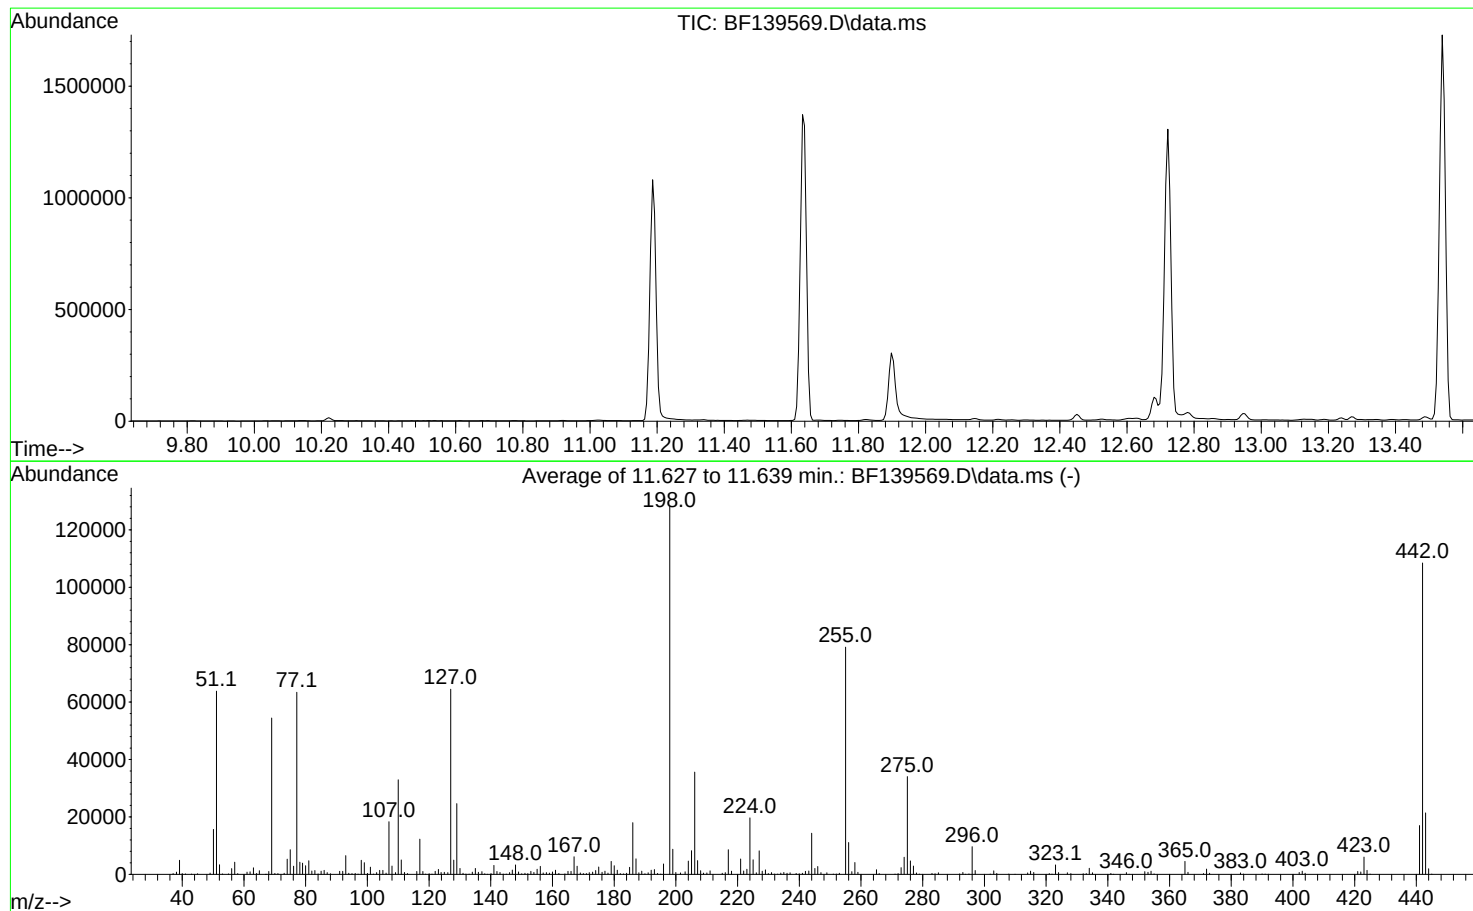




AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.8	63819	PASS
68	69	0.00	2	1.9	1014	PASS
69	198	0.00	100	42.5	54439	PASS
70	69	0.00	2	0.6	314	PASS
127	198	10	80	50.3	64507	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	128131	PASS
199	198	5	9	6.8	8744	PASS
275	198	10	60	26.6	34056	PASS
365	198	1	100	3.5	4503	PASS
441	198	0.01	100	13.3	17029	PASS
442	442	50	100	100.0	108445	PASS
443	442	15	24	19.7	21412	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF093024\
 Data File : BF139569.D
 Acq On : 30 Sep 2024 09:36
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 30 13:10:53 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 14 02:58:23 2024
 Response via : Initial Calibration

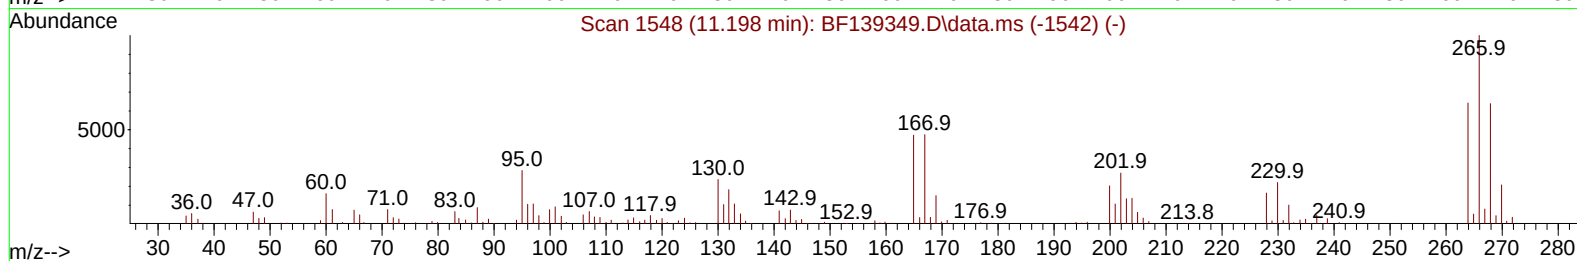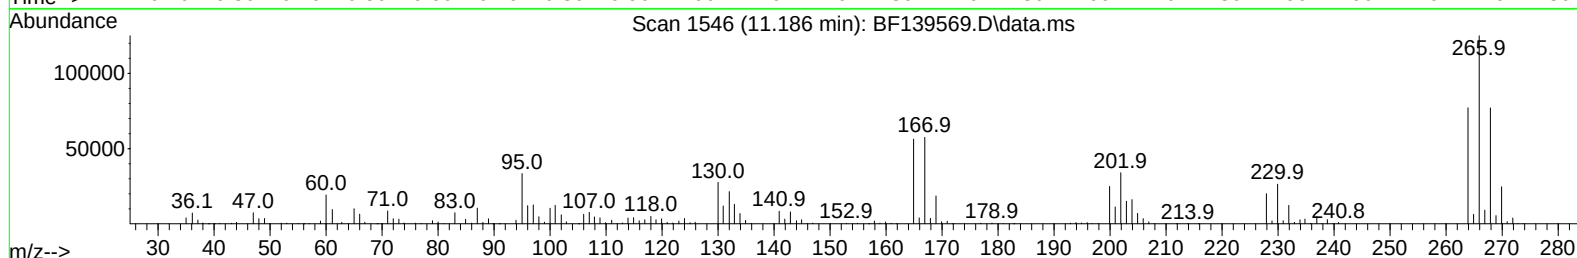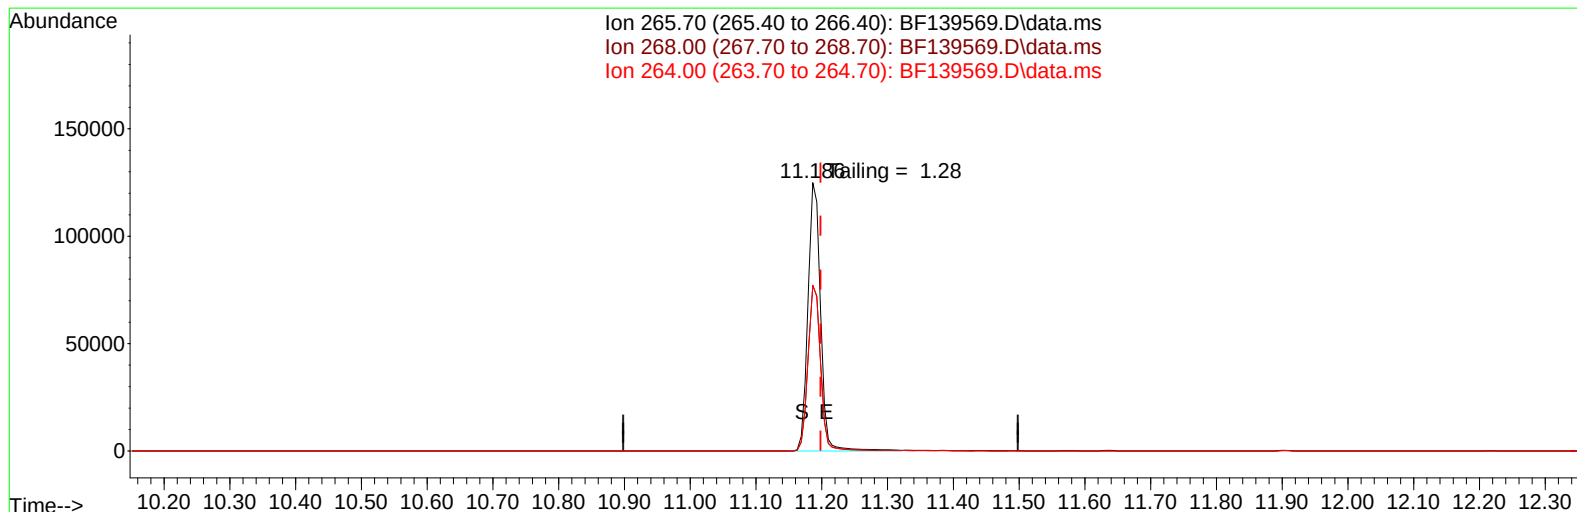

TIC: BF139569.D\data.ms

(70) Pentachlorophenol (C)

11.186min (-0.012) 435054.79 ng




response 166986

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	61.67
264.00	64.20	61.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF093024\
Data File : BF139569.D
Acq On : 30 Sep 2024 09:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 30 13:10:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

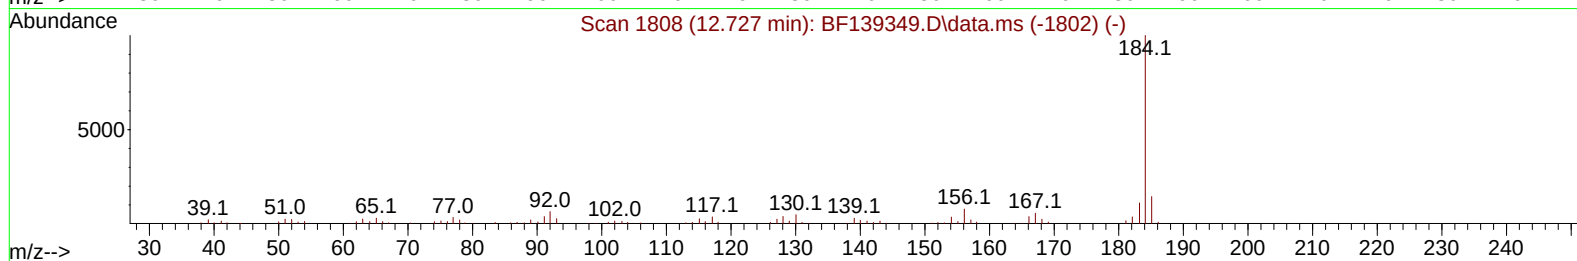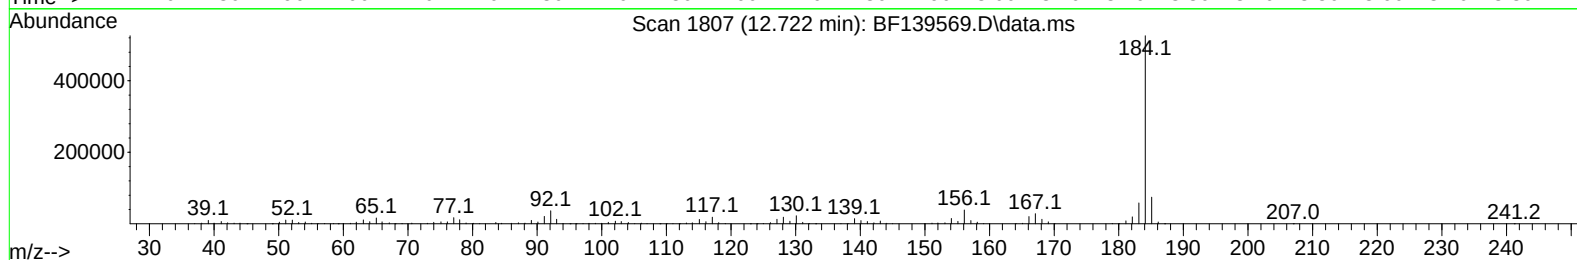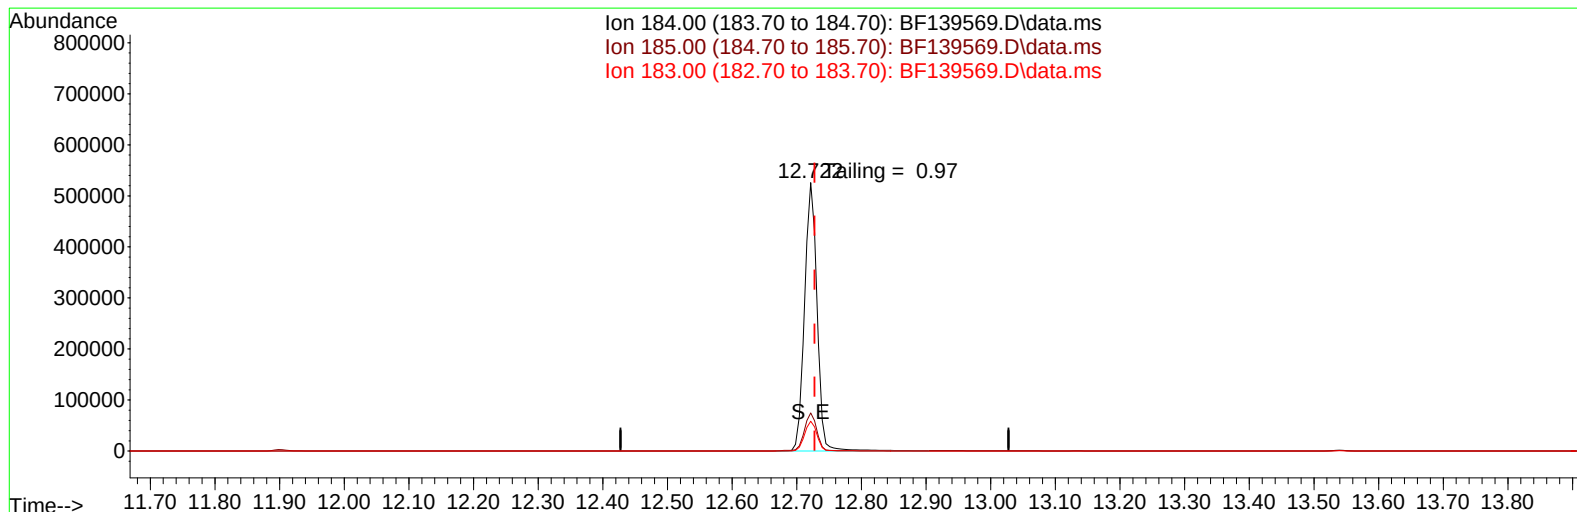

TIC: BF139569.D\data.ms

(77) Benzidine

12.722min (-0.006) 11020.57 ng

response 706569

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.18
183.00	11.10	11.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/30/2024	BNA_F	<u>BF139569.D</u>
Compound Name	Response	Retention Time
DDT	414195	13.539
DDD	7462	13.269
DDE	579	12.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8041	422236	1.90

Instrument :
BNA_F
ClientSampleId :
DFTPP