

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100115\
 Data File : BF081943.D
 Acq On : 1 Oct 2015 17:10
 Operator : UM/IZ
 Sample : PB85644BL
 Misc : LOD/LOQ
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB85644BL

Quant Time: Oct 02 02:32:36 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 28 18:10:42 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	120742	20.00	ng	-0.05
21) Naphthalene-d8	8.18	136	481949	20.00	ng	-0.03
38) Acenaphthene-d10	9.93	164	248140	20.00	ng	-0.05
63) Phenanthrene-d10	11.42	188	499726	20.00	ng	-0.05
75) Chrysene-d12	14.06	240	503468	20.00	ng	-0.06
86) Perylene-d12	15.51	264	371509	20.00	ng	-0.07
System Monitoring Compounds						
5) 2-Fluorophenol	5.50	112	716585	107.74	ng	-0.02
7) Phenol-d6	6.53	99	1001447	119.65	ng	-0.03
23) Nitrobenzene-d5	7.46	82	619861	85.73	ng	-0.03
41) 2,4,6-Tribromophenol	10.72	330	274574	109.26	ng	-0.05
44) 2-Fluorobiphenyl	9.26	172	1191625	79.32	ng	-0.05
78) Terphenyl-d14	13.01	244	1272187	80.40	ng	-0.05


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100115\
Data File : BF081943.D
Acq On : 1 Oct 2015 17:10
Operator : UM/IZ
Sample : PB85644BL
Misc : LOD/LOQ
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB85644BL

Quant Time: Oct 02 02:32:36 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 28 18:10:42 2015
Response via : Initial Calibration

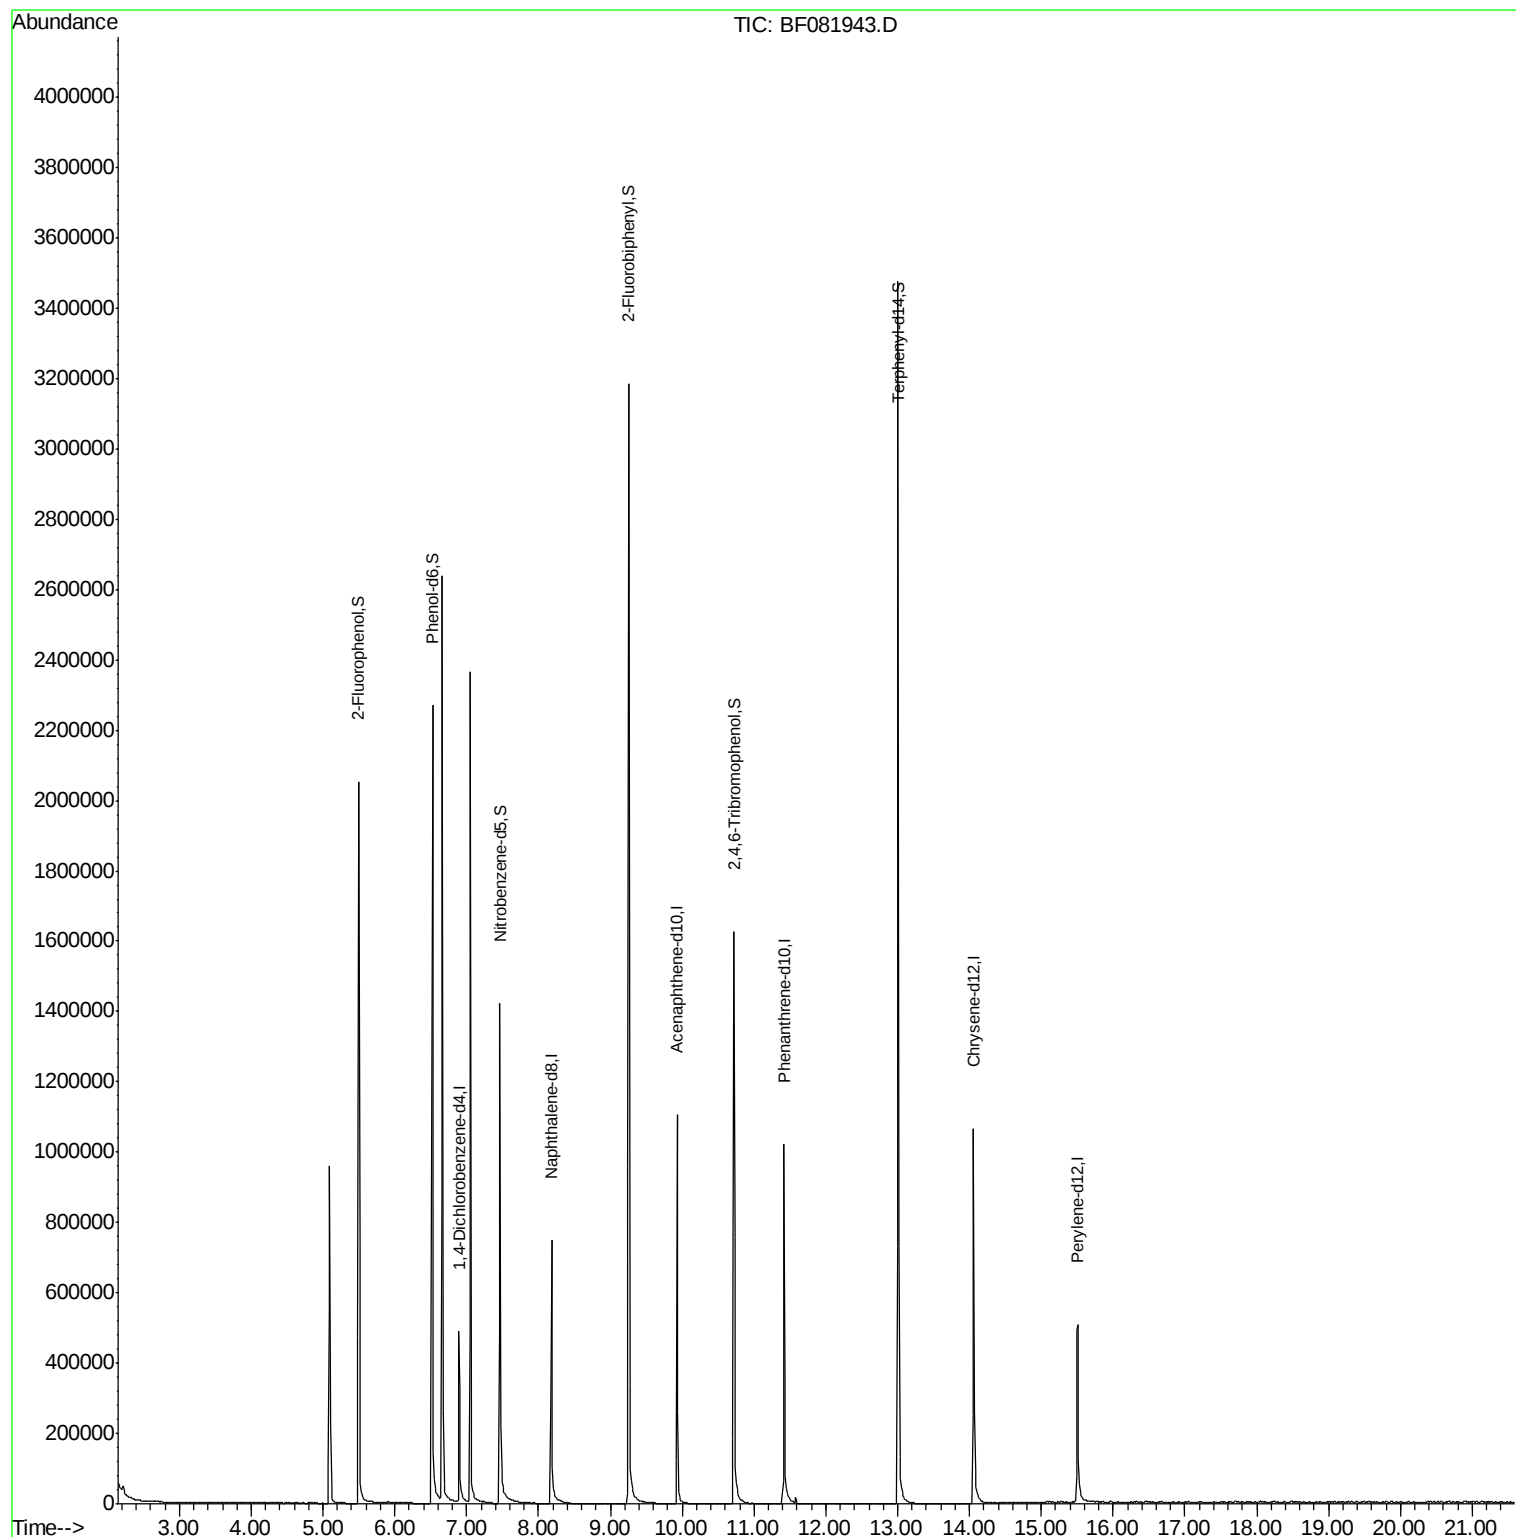







#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.89 min Scan# 416
 Delta R.T. -0.05 min
 Lab File: BF081943.D
 Acq: 1 Oct 2015 17:10

Instrument :
 BNA_F
 ClientSampleId :
 PB85644BL

Tgt Ion:152 Resp: 120742
 Ion Ratio Lower Upper
 152 100
 150 160.2 124.7 187.1
 115 63.9 39.0 58.4#

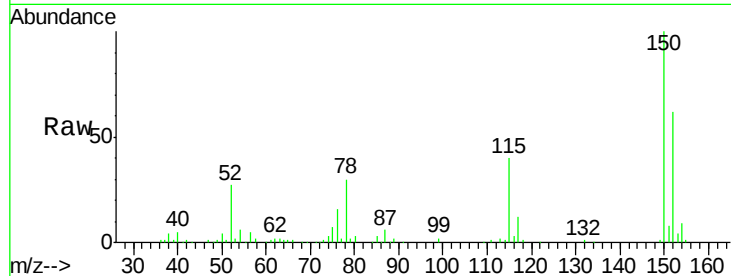


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

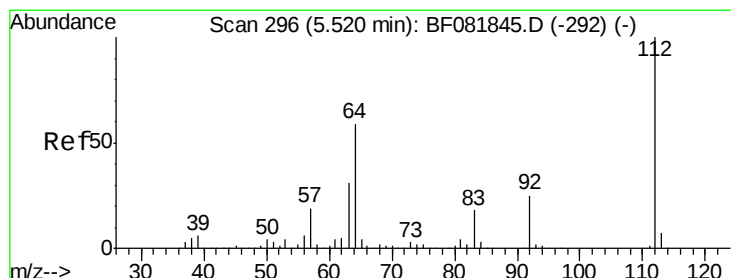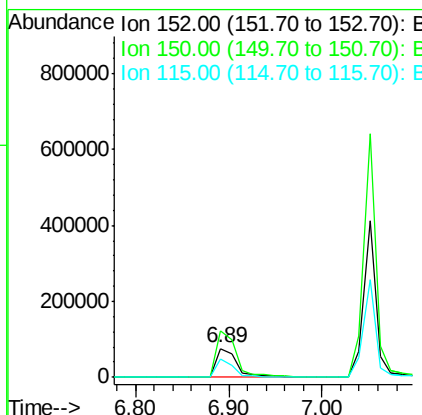
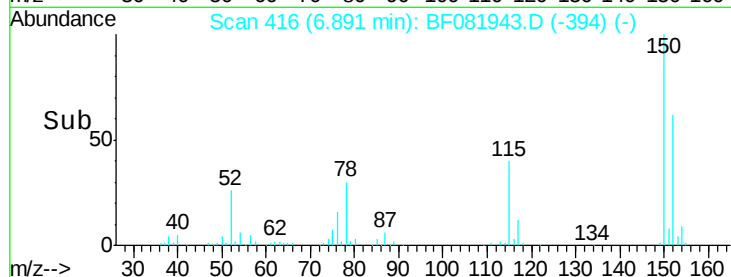



#5
 2-Fluorophenol
 Concen: 107.74 ng
 RT: 5.50 min Scan# 294
 Delta R.T. -0.02 min
 Lab File: BF081943.D
 Acq: 1 Oct 2015 17:10

Tgt Ion:112 Resp: 716585
 Ion Ratio Lower Upper
 112 100
 64 64.0 39.7 59.5#
 63 33.3 17.4 26.0#

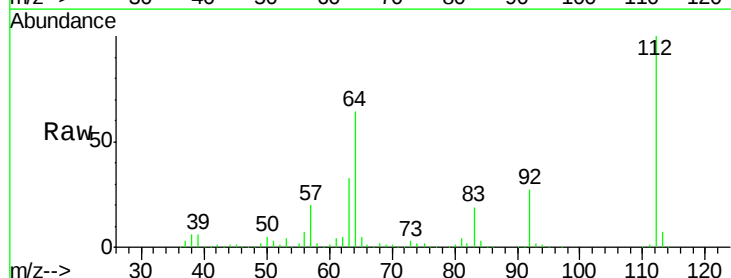

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

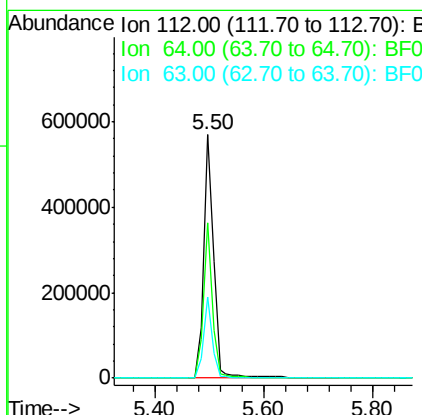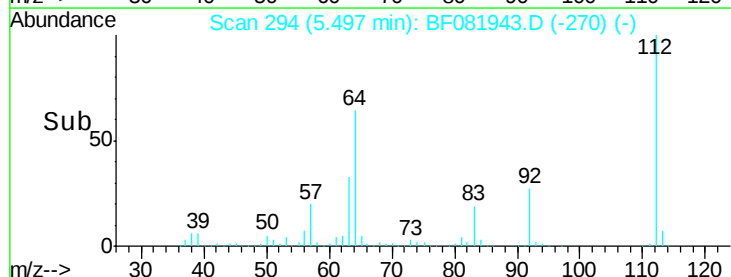

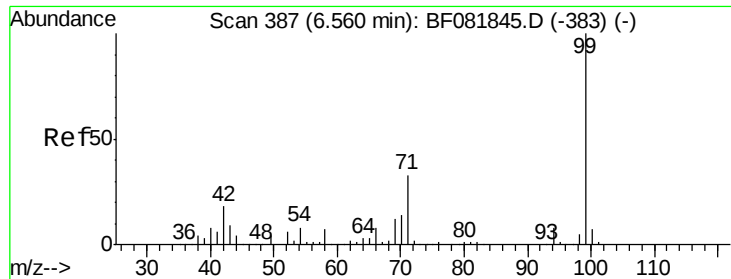

#7

Phenol-d6

Concen: 119.65 ng

RT: 6.53 min Scan# 384

Delta R.T. -0.03 min

Lab File: BF081943.D

Acq: 1 Oct 2015 17:10

Instrument :

BNA_F

ClientSampled :

PB85644BL


Tgt Ion: 99 Resp: 1001447

Ion Ratio Lower Upper

99 100

42 16.8 13.7 20.5




71 33.6 14.2 21.2#

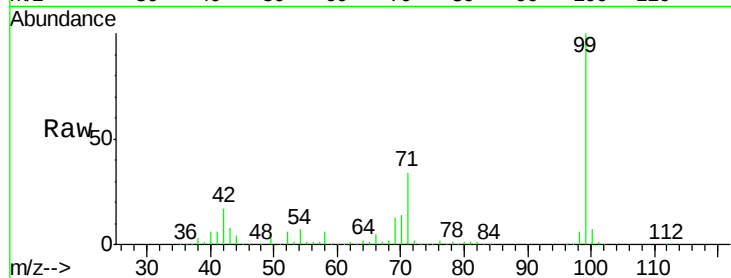

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

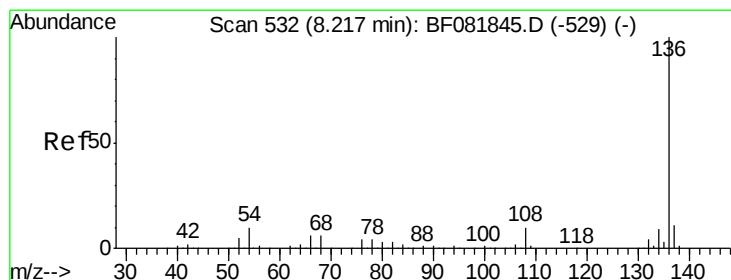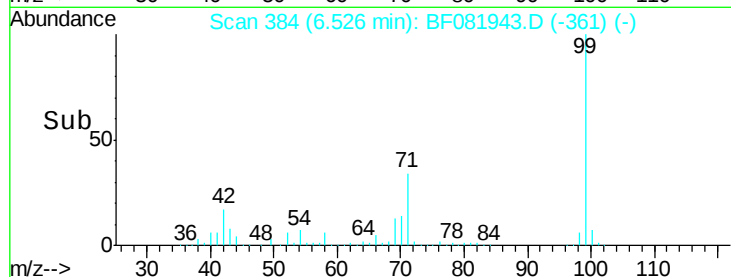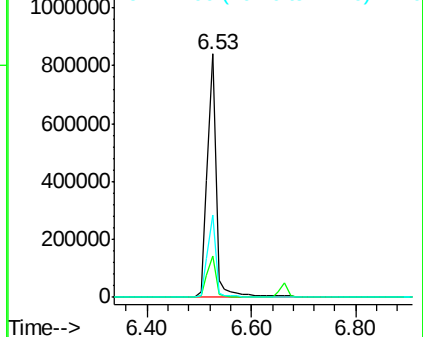

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.18 min Scan# 529

Delta R.T. -0.03 min

Lab File: BF081943.D

Acq: 1 Oct 2015 17:10

Tgt Ion: 136 Resp: 481949


Ion Ratio Lower Upper

136 100

137 10.9 9.0 13.6

54 6.8 8.2 12.2#

68 5.0 5.8 8.6#


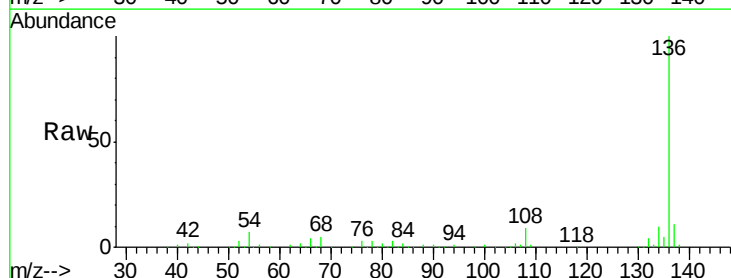



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

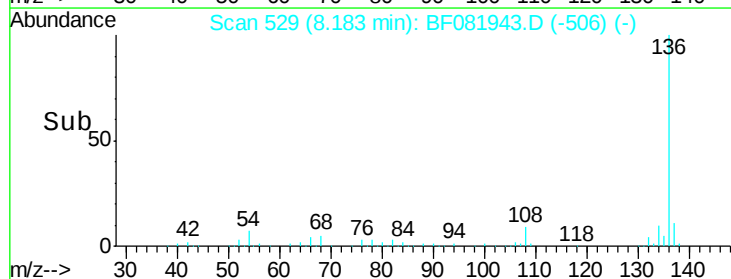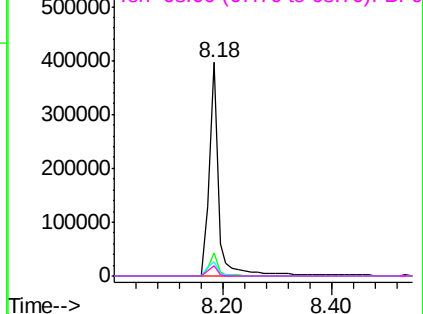


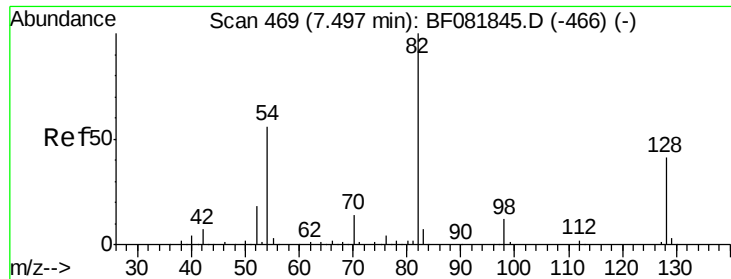




#23
 Nitrobenzene-d5
 Concen: 85.73 ng
 RT: 7.46 min Scan# 466
 Delta R.T. -0.03 min
 Lab File: BF081943.D
 Acq: 1 Oct 2015 17:10

Instrument :
 BNA_F
 ClientSampleId :
 PB85644BL

Tgt Ion: 82 Resp: 619861
 Ion Ratio Lower Upper
 82 100
 128 46.1 51.0 76.6#
 54 51.8 47.5 71.3

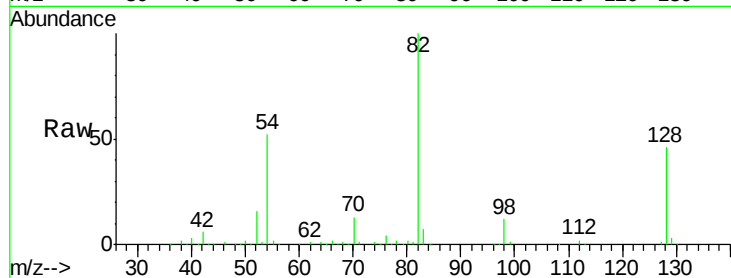


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): B
 Ion 54.00 (53.70 to 54.70): BF0

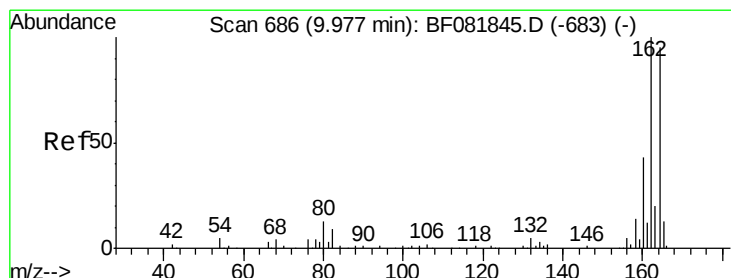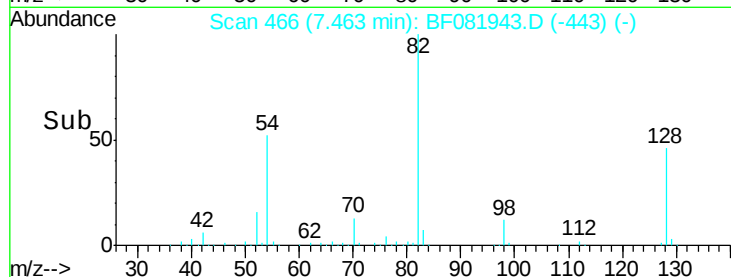
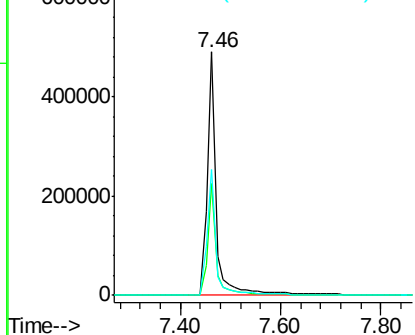



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.93 min Scan# 682
 Delta R.T. -0.05 min
 Lab File: BF081943.D
 Acq: 1 Oct 2015 17:10

Tgt Ion: 164 Resp: 248140
 Ion Ratio Lower Upper
 164 100
 162 101.5 75.2 112.8
 160 44.5 31.5 47.3

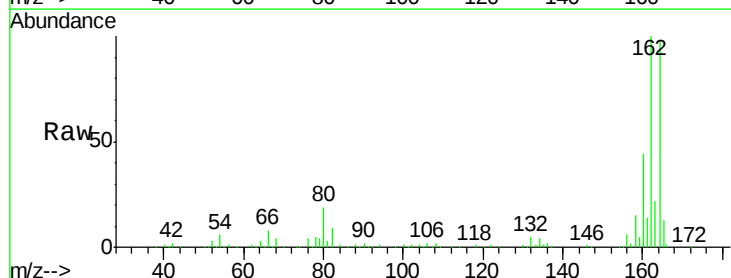

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

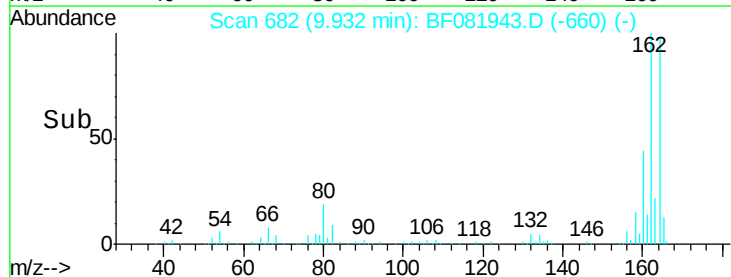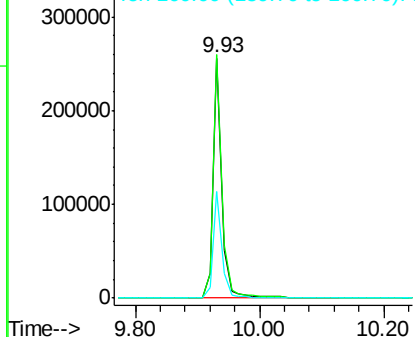


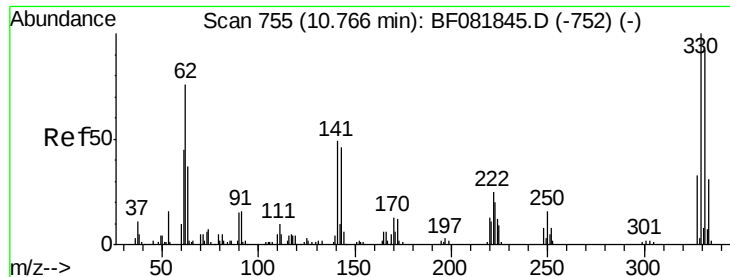




#41
 2,4,6-Tribromophenol
 Concen: 109.26 ng
 RT: 10.72 min Scan# 751
 Delta R.T. -0.05 min
 Lab File: BF081943.D
 Acq: 1 Oct 2015 17:10

Instrument :
 BNA_F
 ClientSampleId :
 PB85644BL

Tgt Ion:330 Resp: 274574
 Ion Ratio Lower Upper
 330 100
 332 96.2 76.6 114.8
 141 31.9 29.7 44.5

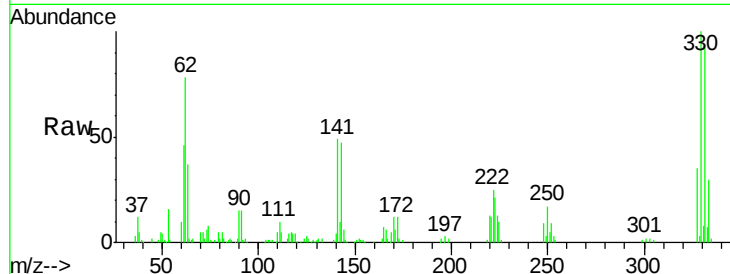


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

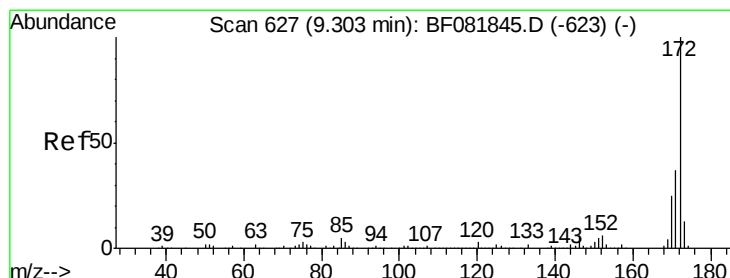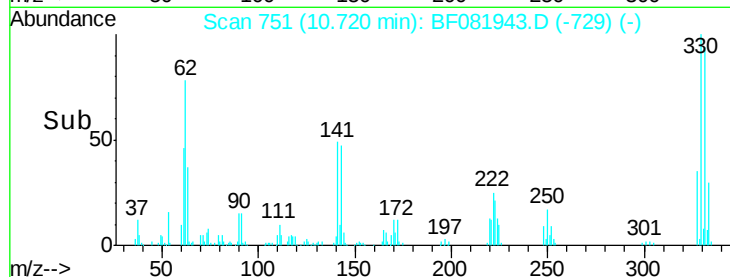
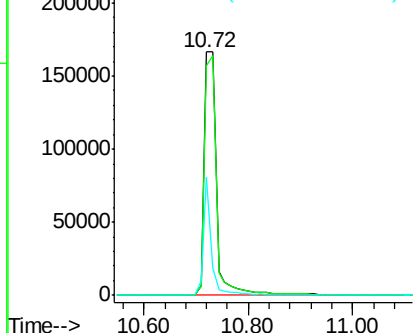



#44
 2-Fluorobiphenyl
 Concen: 79.32 ng
 RT: 9.26 min Scan# 623
 Delta R.T. -0.05 min
 Lab File: BF081943.D
 Acq: 1 Oct 2015 17:10

Tgt Ion:172 Resp: 1191625
 Ion Ratio Lower Upper
 172 100
 171 36.8 26.1 39.1
 170 25.1 17.4 26.2

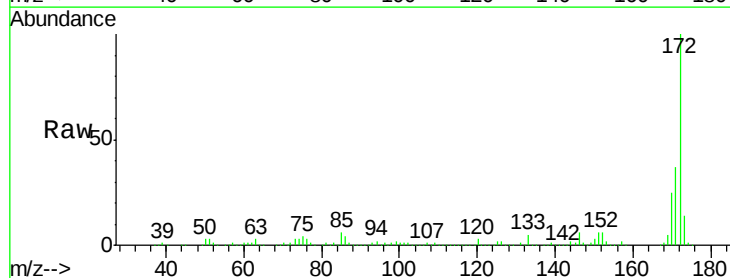

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

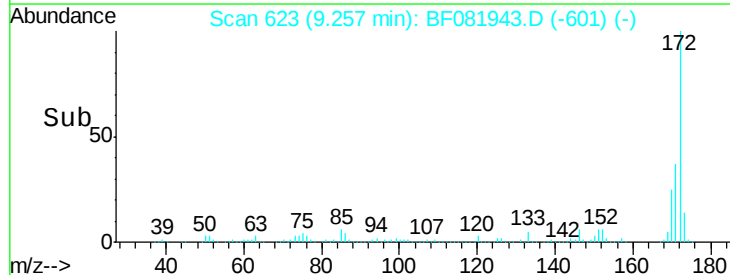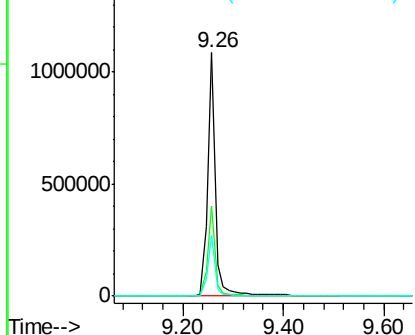

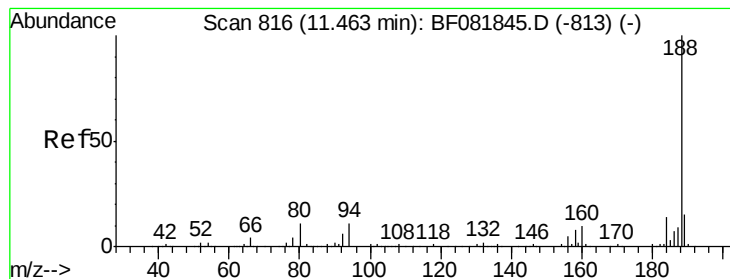

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.42 min Scan# 812

Delta R.T. -0.05 min

Lab File: BF081943.D

Acq: 1 Oct 2015 17:10

Instrument :

BNA_F

ClientSampleId :

PB85644BL


Tgt Ion:188 Resp: 499726

Ion Ratio Lower Upper

188 100

94 9.9 11.1 16.7#




80 10.5 11.0 16.4#

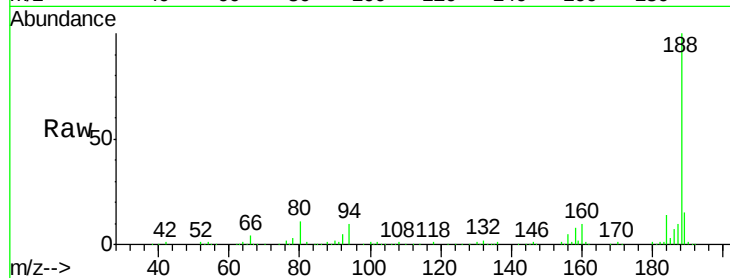

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

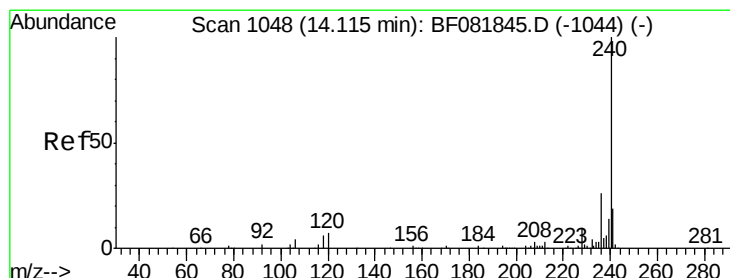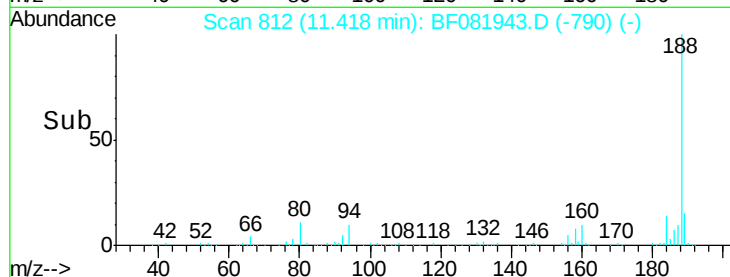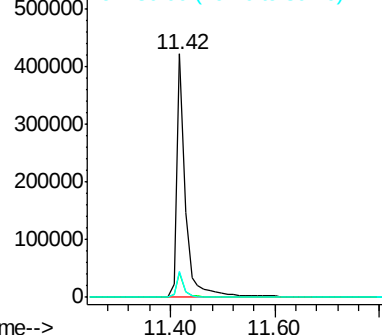

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.06 min Scan# 1043

Delta R.T. -0.06 min

Lab File: BF081943.D

Acq: 1 Oct 2015 17:10


Tgt Ion:240 Resp: 503468

Ion Ratio Lower Upper

240 100

120 9.4 16.2 24.2#



236 26.1 18.4 27.6

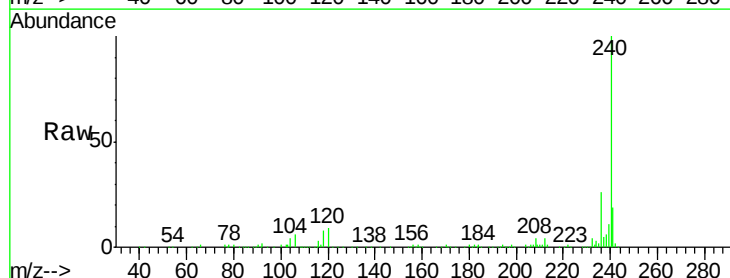


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

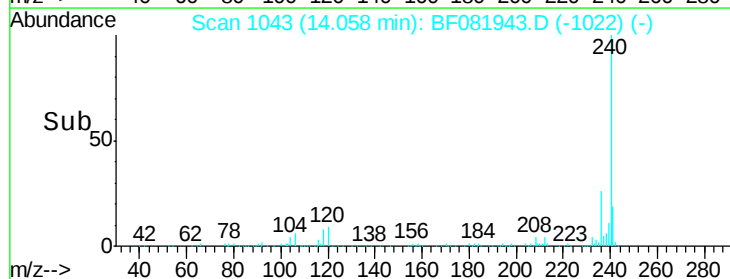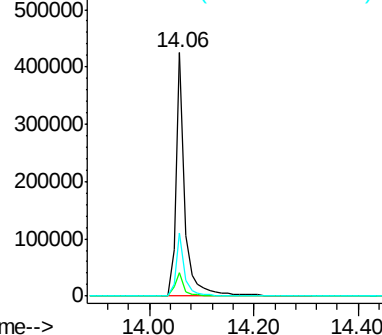

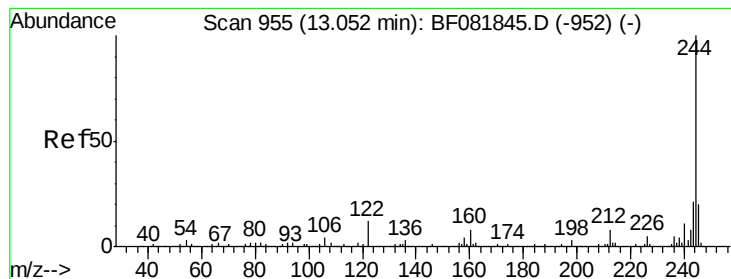

#78

Terphenyl-d14

Concen: 80.40 ng

RT: 13.01 min Scan# 951

Delta R.T. -0.05 min

Lab File: BF081943.D

Acq: 1 Oct 2015 17:10

Instrument :

BNA_F

ClientSampleId :

PB85644BL


Tgt Ion:244 Resp: 1272187

Ion Ratio Lower Upper

244 100

212 7.7 4.3 6.5#




122 11.2 17.4 26.2#

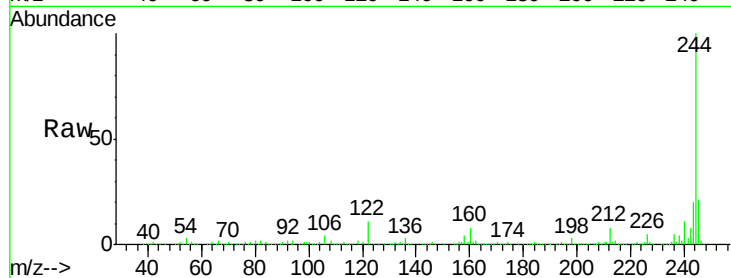

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

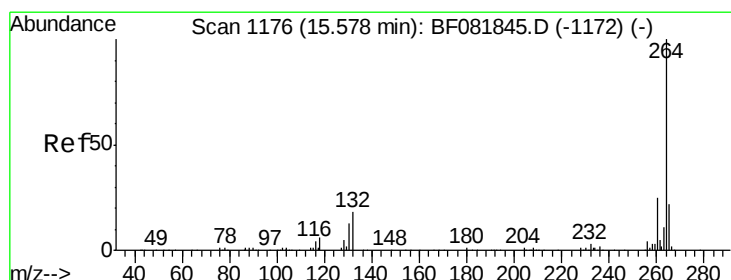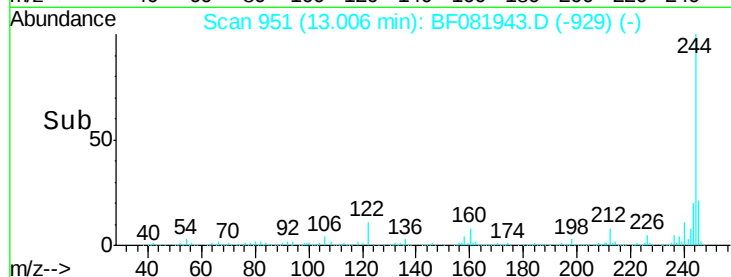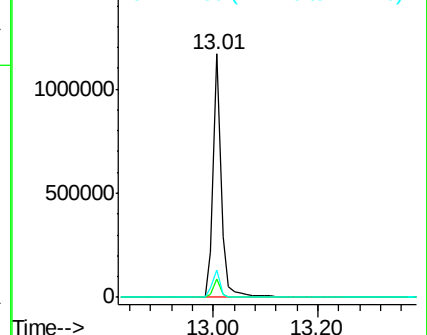

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.51 min Scan# 1170

Delta R.T. -0.07 min

Lab File: BF081943.D

Acq: 1 Oct 2015 17:10


Tgt Ion:264 Resp: 371509

Ion Ratio Lower Upper

264 100

260 23.8 16.7 25.1

265 20.8 17.2 25.8

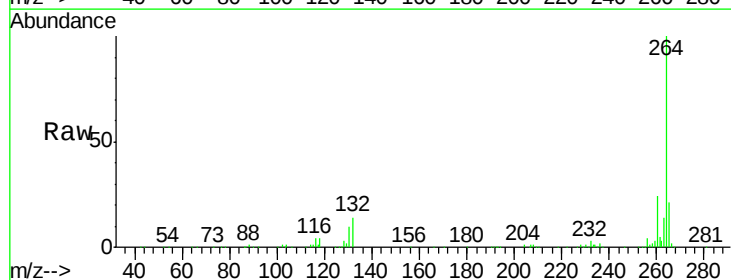

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

