


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF100115\  
 Data File : BF081930.D  
 Acq On : 1 Oct 2015 10:34  
 Operator : UM/IZ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF092815.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Sep 28 18:10:42 2015

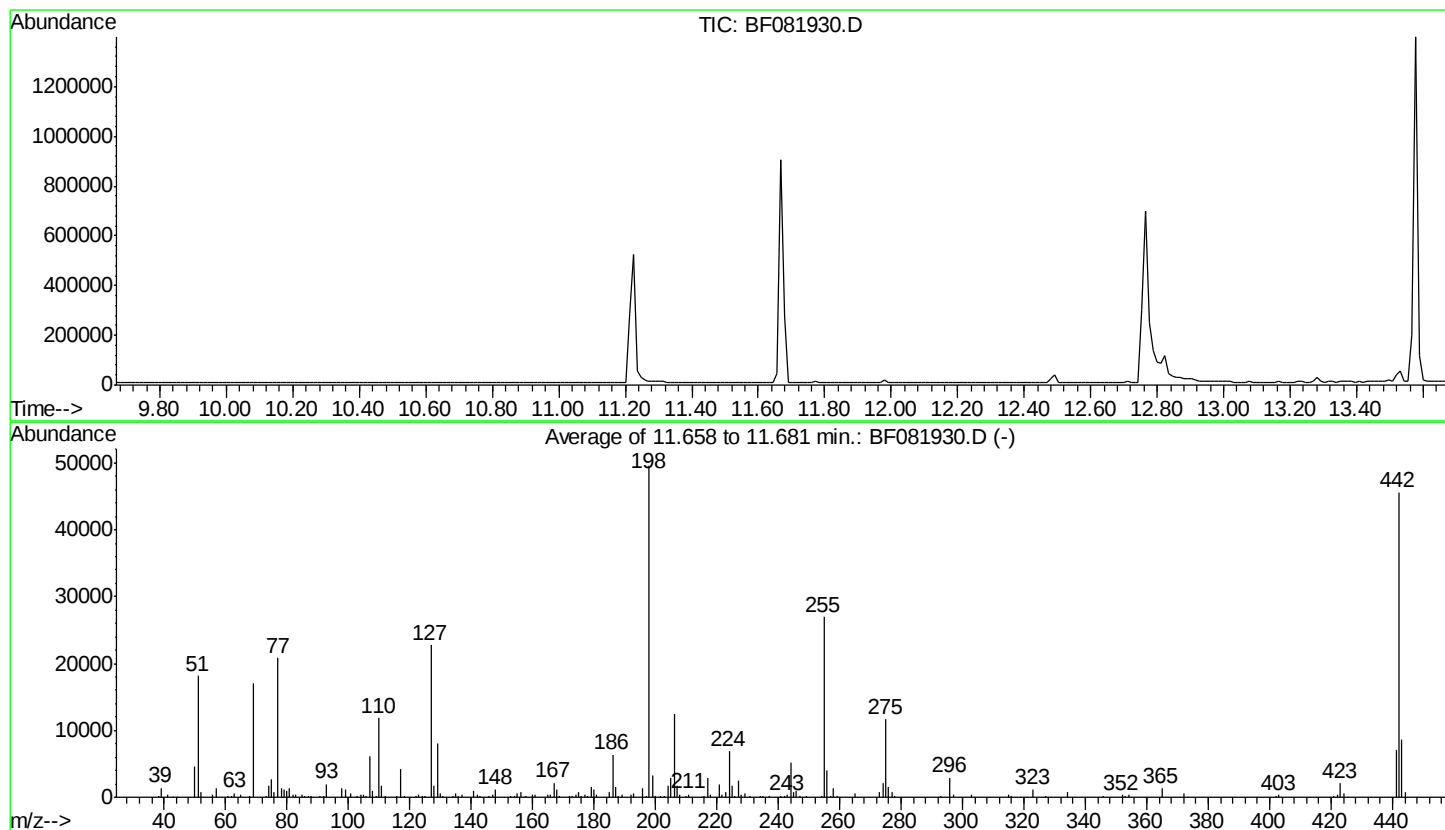

AutoFind: Scans 833, 834, 835; Background Corrected with Scan 830

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 36.6      | 18158   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.4       | 247     | PASS             |
| 69          | 198          | 0.00         | 100          | 34.4      | 17043   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 45.9      | 22769   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.4       | 209     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 49590   | PASS             |
| 199         | 198          | 5            | 9            | 6.5       | 3201    | PASS             |
| 275         | 198          | 10           | 60           | 23.4      | 11613   | PASS             |
| 365         | 198          | 1            | 100          | 2.7       | 1333    | PASS             |
| 441         | 442          | 0.01         | 24           | 15.5      | 7073    | PASS             |
| 442         | 198          | 50           | 100          | 91.8      | 45520   | PASS             |
| 443         | 442          | 15           | 24           | 18.9      | 8616    | PASS             |