


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100115\
 Data File : BF081969.D
 Acq On : 2 Oct 2015 6:16
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 28 18:10:42 2015

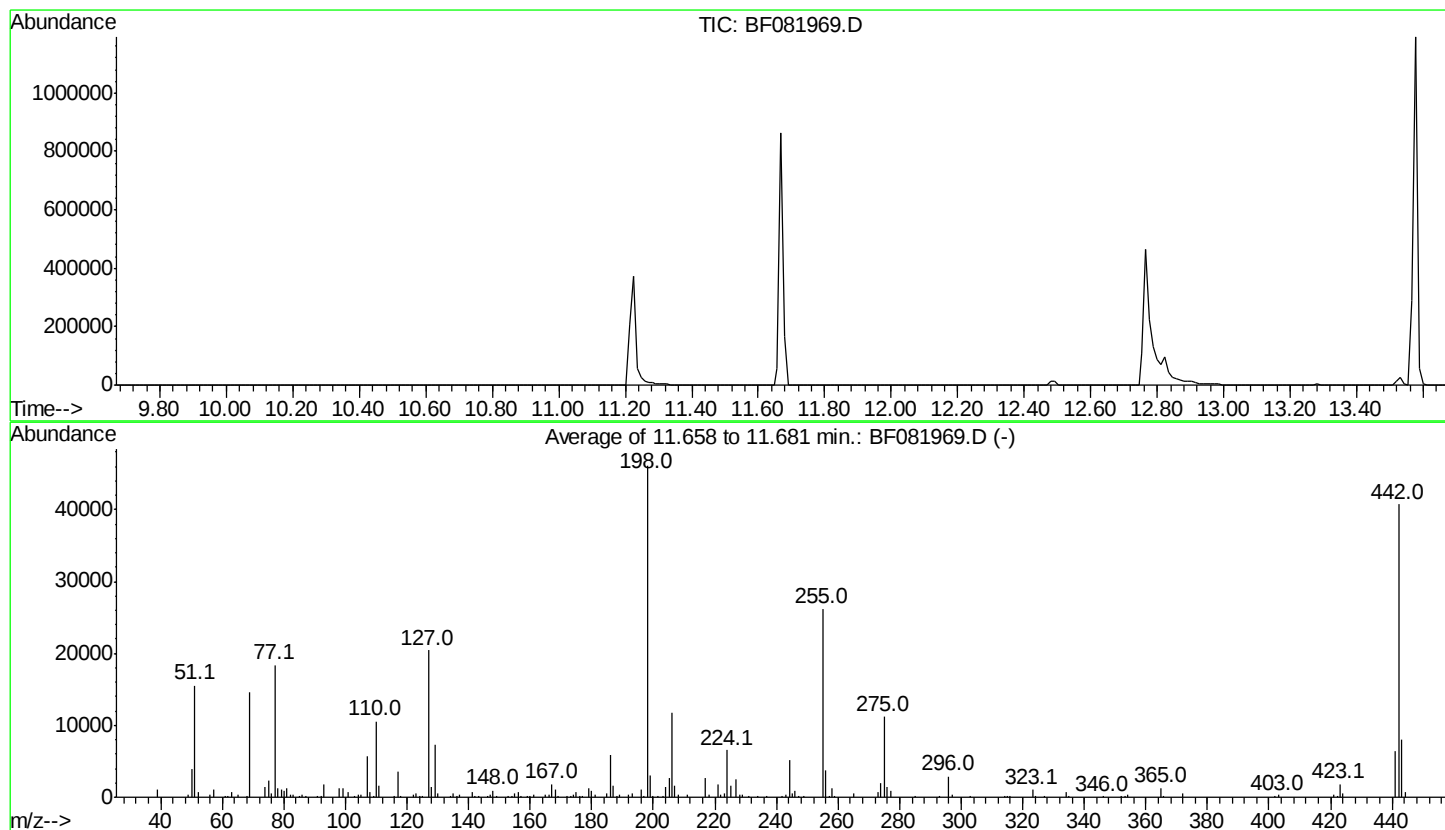

AutoFind: Scans 833, 834, 835; Background Corrected with Scan 830

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	15518	PASS
68	69	0.00	2	1.2	169	PASS
69	198	0.00	100	31.7	14602	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.3	20418	PASS
197	198	0.00	2	0.5	212	PASS
198	198	100	100	100.0	46114	PASS
199	198	5	9	6.6	3046	PASS
275	198	10	60	24.3	11184	PASS
365	198	1	100	2.8	1283	PASS
441	442	0.01	24	15.6	6331	PASS
442	198	50	100	88.2	40685	PASS
443	442	15	24	19.5	7932	PASS