
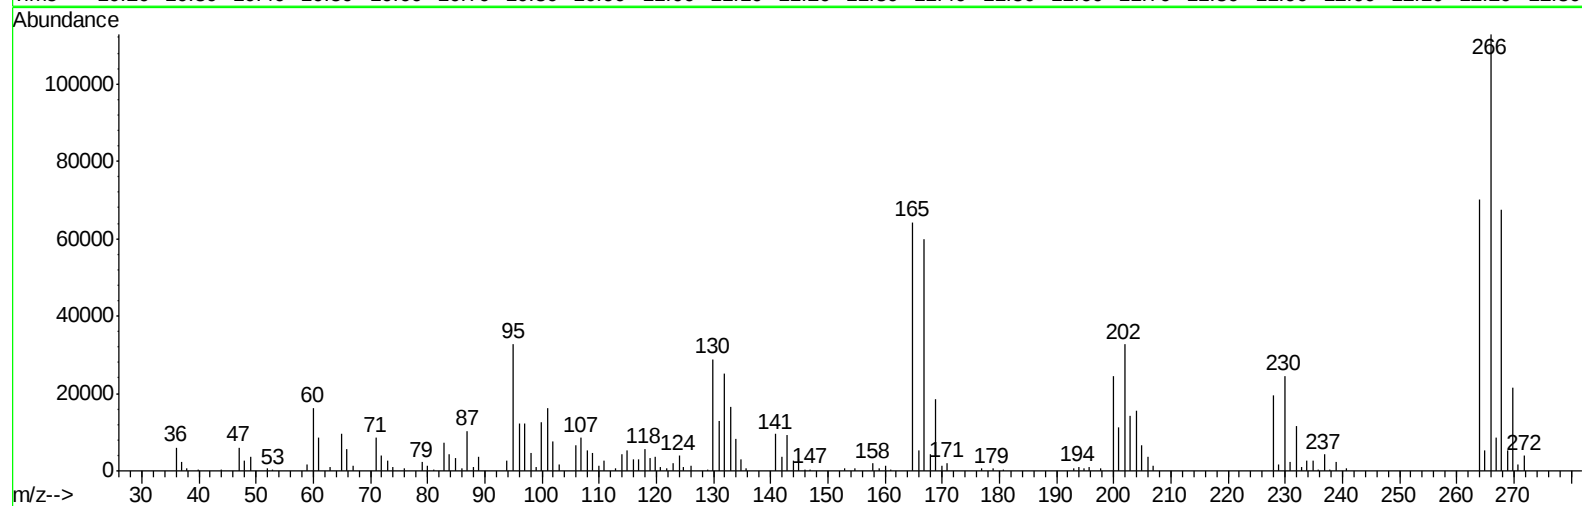


Data Path : Z:\HPCHEM1\BNA F\DATA\BF100117\
Data File : BF098983.D
Acq On : 1 Oct 2017 10:18
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 02 08:00:25 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

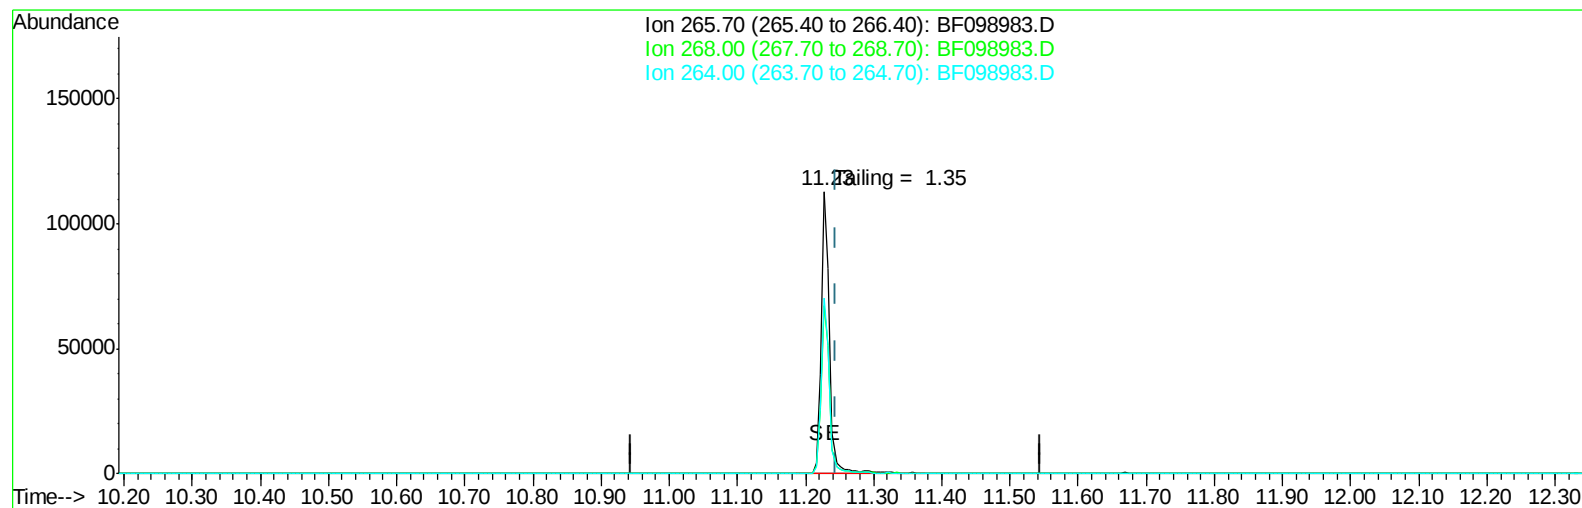

TIC: BF098983.D

(69) Pentachlorophenol (C)



11.228min (-0.018) 35384.62ng

response 95774

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.78
264.00	61.90	62.14
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100117\
Data File : BF098983.D
Acq On : 1 Oct 2017 10:18
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 02 08:00:25 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

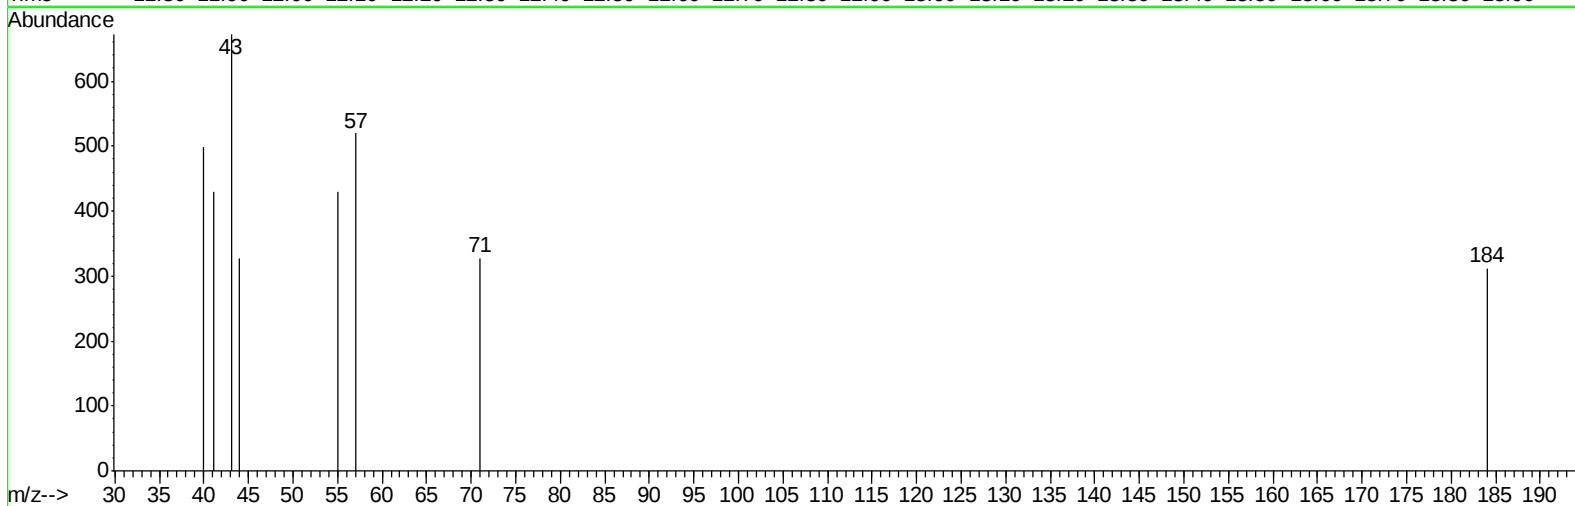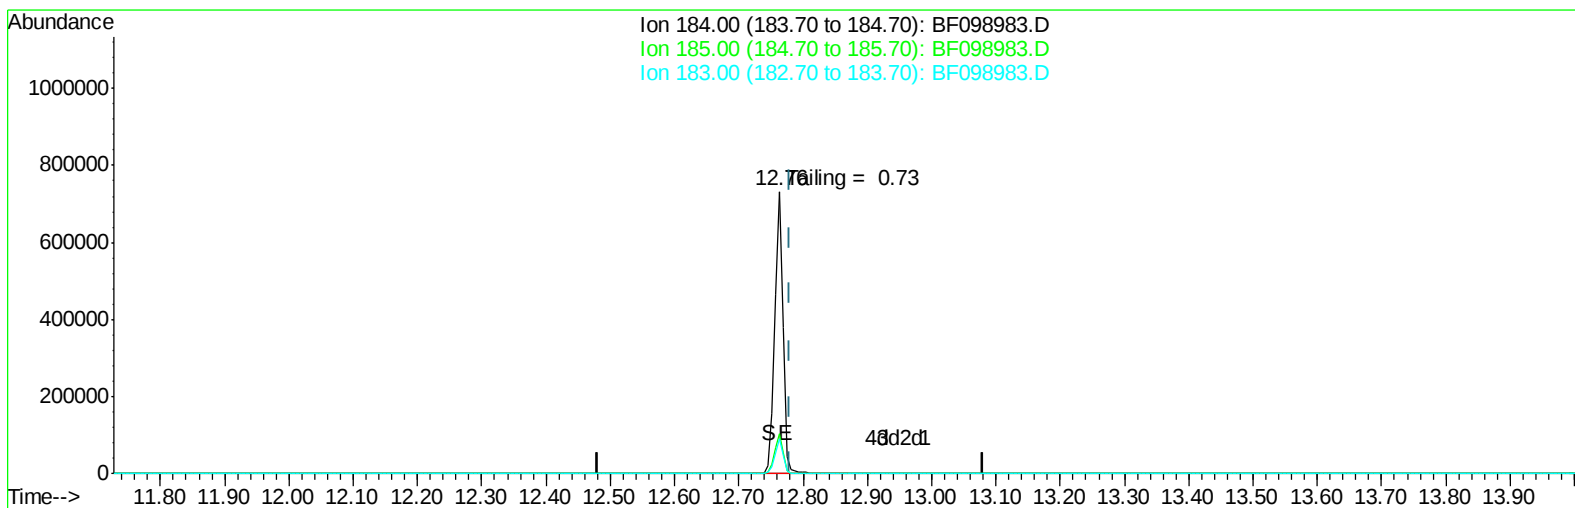

TIC: BF098983.D

(76) Benzidine

12.992min (+0.212) 11.39ng

response 110

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	0.00#
183.00	11.60	0.00#
0.00	0.00	0.00