


Data Path : Z:\HPCHEM1\BNA F\Data\BF100117\
 Data File : BF098983.D
 Acq On : 1 Oct 2017 10:18
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 23 13:50:58 2017

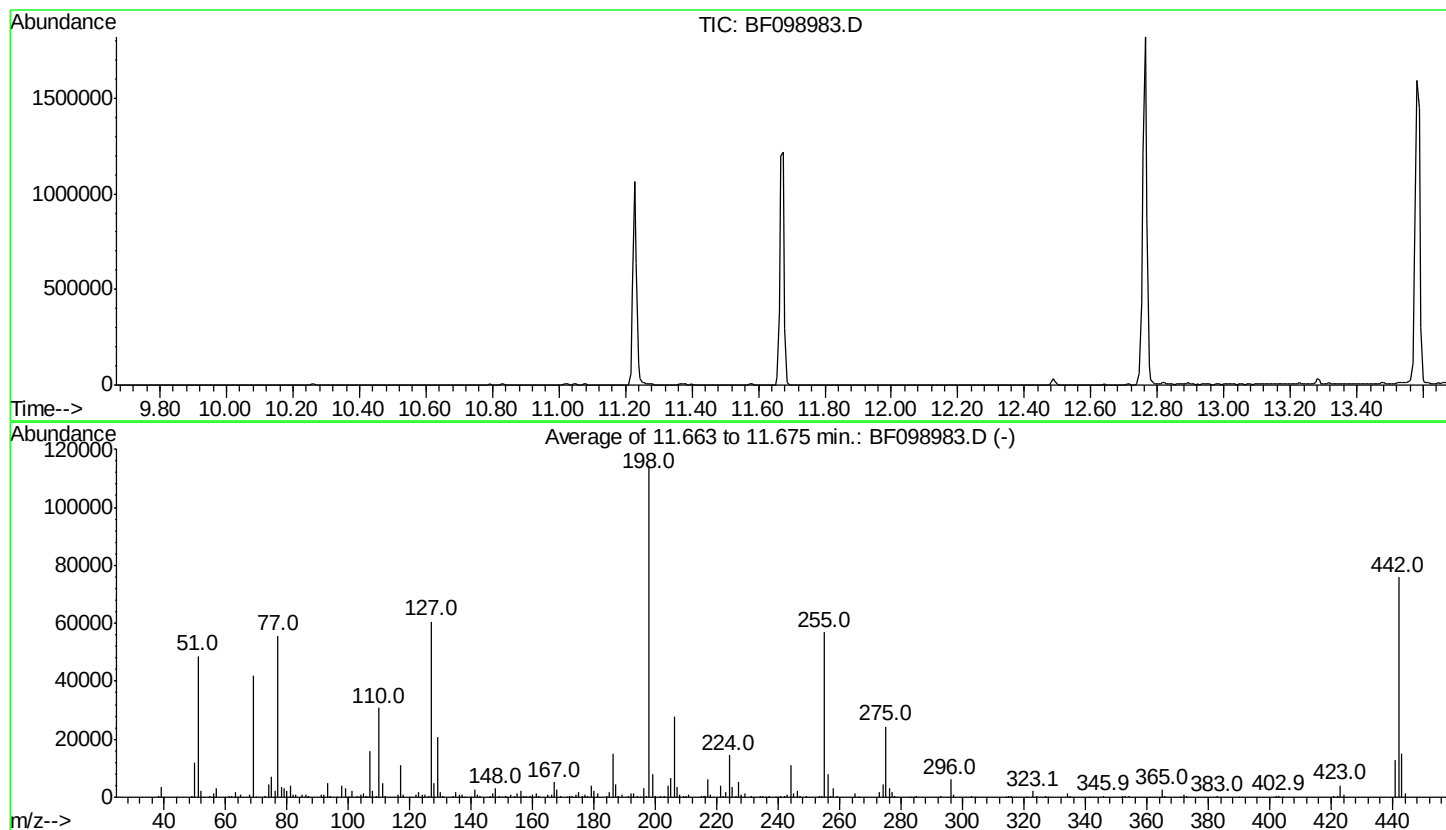

AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1623

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	48786	PASS
68	69	0.00	2	1.7	697	PASS
69	198	0.00	100	36.8	42149	PASS
70	69	0.00	2	0.6	232	PASS
127	198	10	80	53.0	60600	PASS
197	198	0.00	2	0.6	653	PASS
198	198	100	100	100.0	114381	PASS
199	198	5	9	6.8	7798	PASS
275	198	10	60	21.4	24437	PASS
365	198	1	100	2.2	2512	PASS
441	442	0.01	24	16.7	12641	PASS
442	198	50	100	66.4	75894	PASS
443	442	15	24	19.8	15016	PASS