
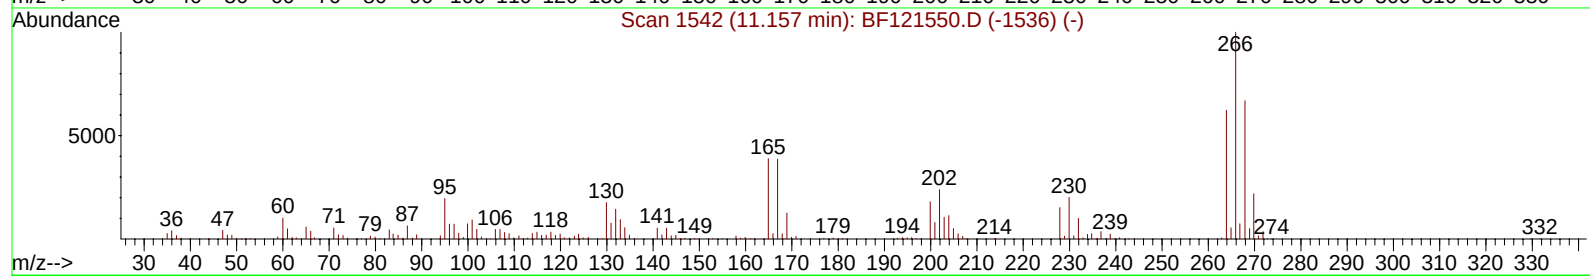
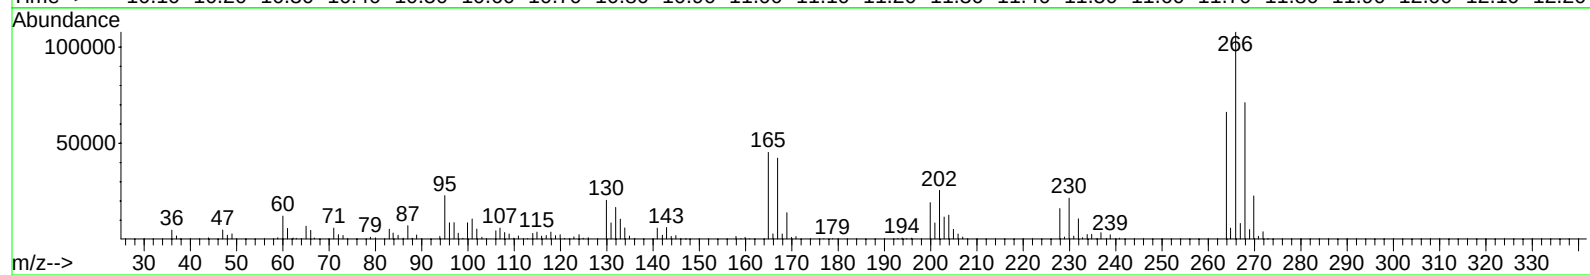


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF100120\
Data File : BF121763.D
Acq On : 1 Oct 2020 13:02
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 01 18:51:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 01 14:29:14 2020
Response via : Initial Calibration

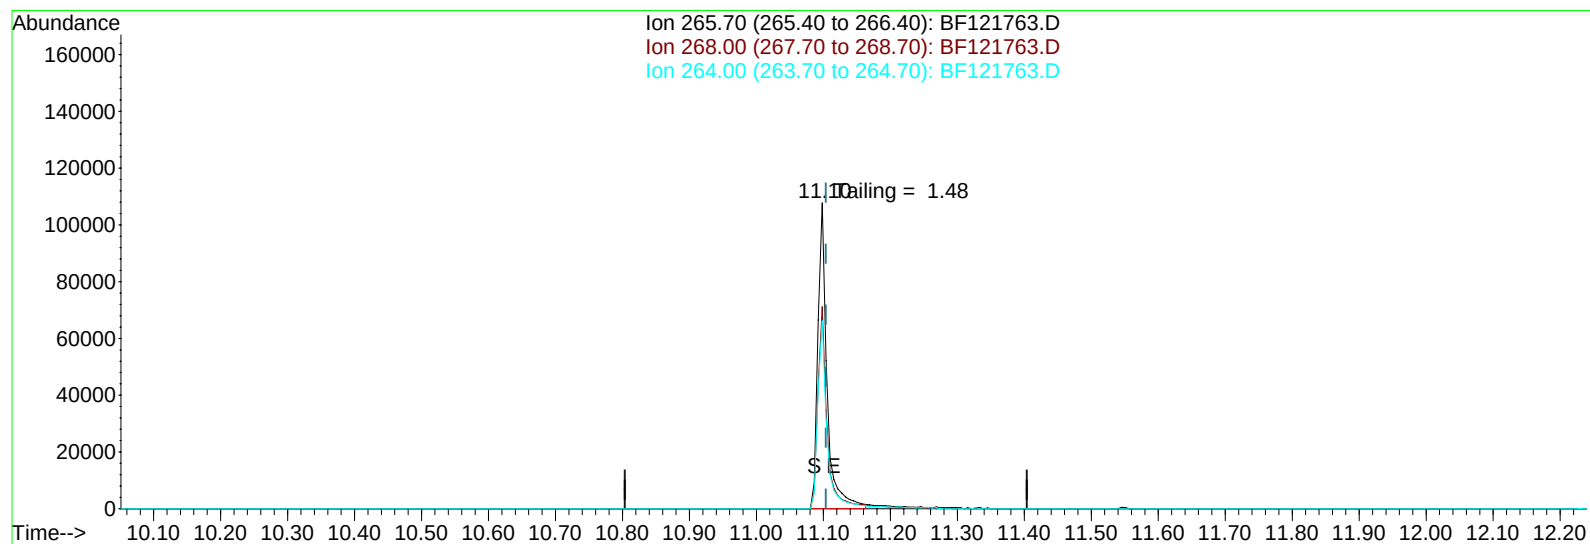

TIC: BF121763.D

(70) Pentachlorophenol (C)




11.098min (-0.006) 40227.99ng

response 107017

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	66.02
264.00	62.40	61.44
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF100120\
Data File : BF121763.D
Acq On : 1 Oct 2020 13:02
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 01 18:51:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 01 14:29:14 2020
Response via : Initial Calibration

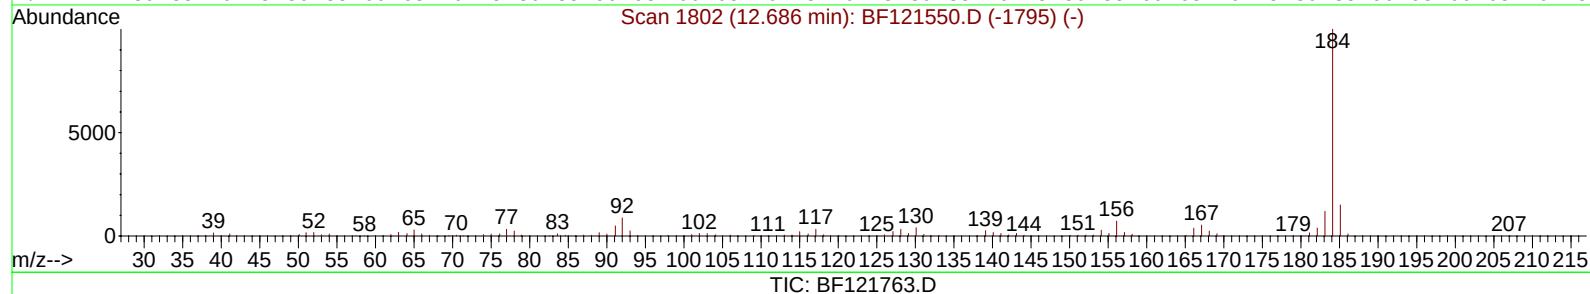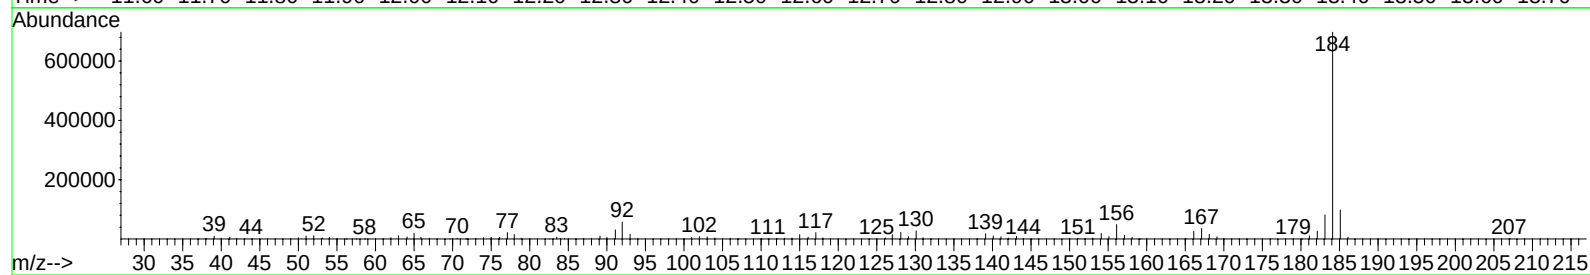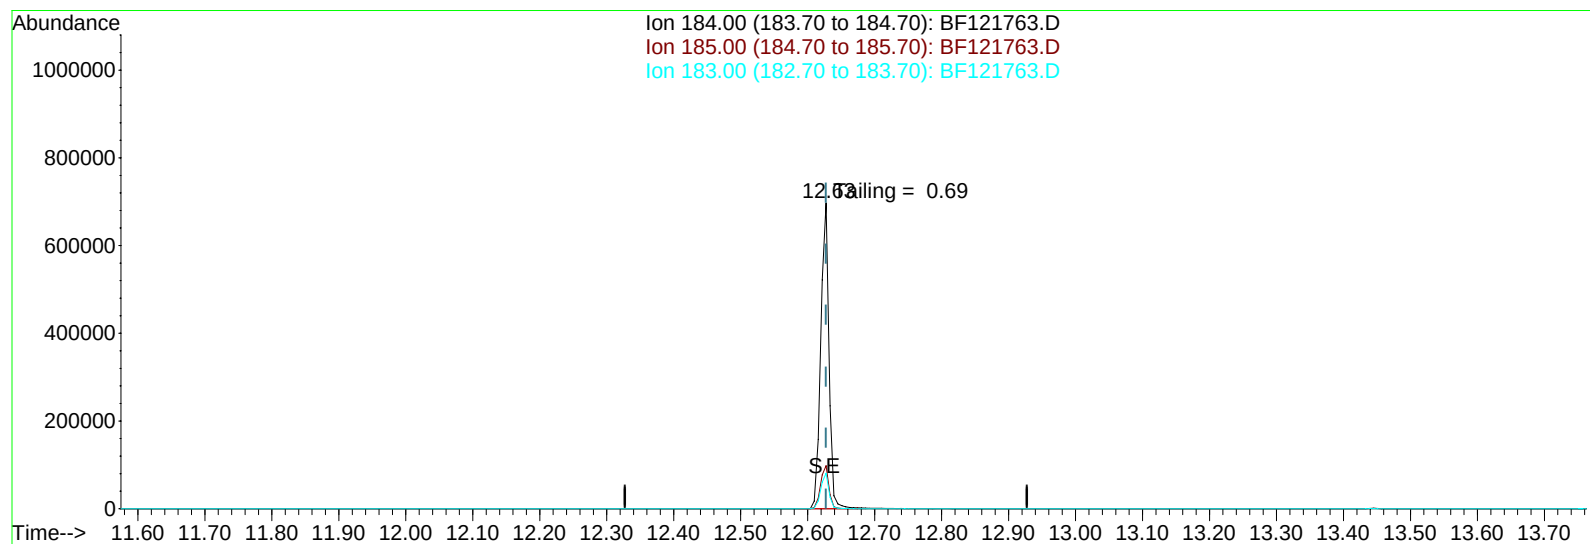

(77) Benzidine

12.627min (+0.000) 0.00ng

response 600759

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	14.07
183.00	11.70	11.62
0.00	0.00	0.00