


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100120\
 Data File : BF121763.D
 Acq On : 1 Oct 2020 13:02
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 01 14:29:14 2020

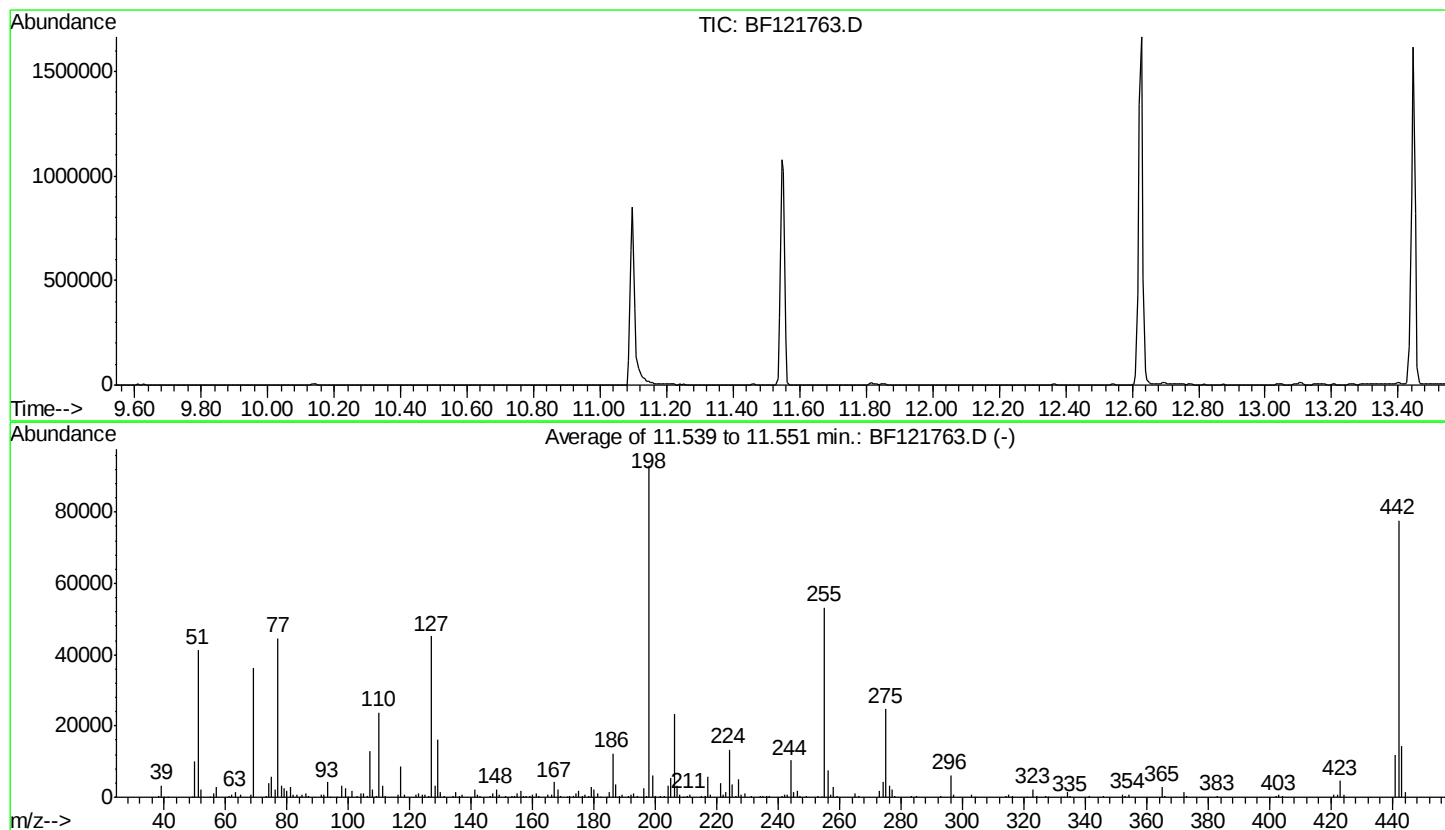

AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.5	41376	PASS
68	69	0.00	2	1.7	611	PASS
69	198	0.00	100	39.1	36336	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.6	45234	PASS
197	198	0.00	2	0.3	310	PASS
198	198	100	100	100.0	93042	PASS
199	198	5	9	6.6	6181	PASS
275	198	10	60	26.8	24911	PASS
365	198	1	100	3.3	3028	PASS
441	198	0.01	100	12.9	12027	PASS
442	198	50	100	83.6	77740	PASS
443	442	15	24	18.7	14508	PASS