


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100124\
Data File : BF139583.D
Acq On : 01 Oct 2024 13:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 02 04:58:47 2024

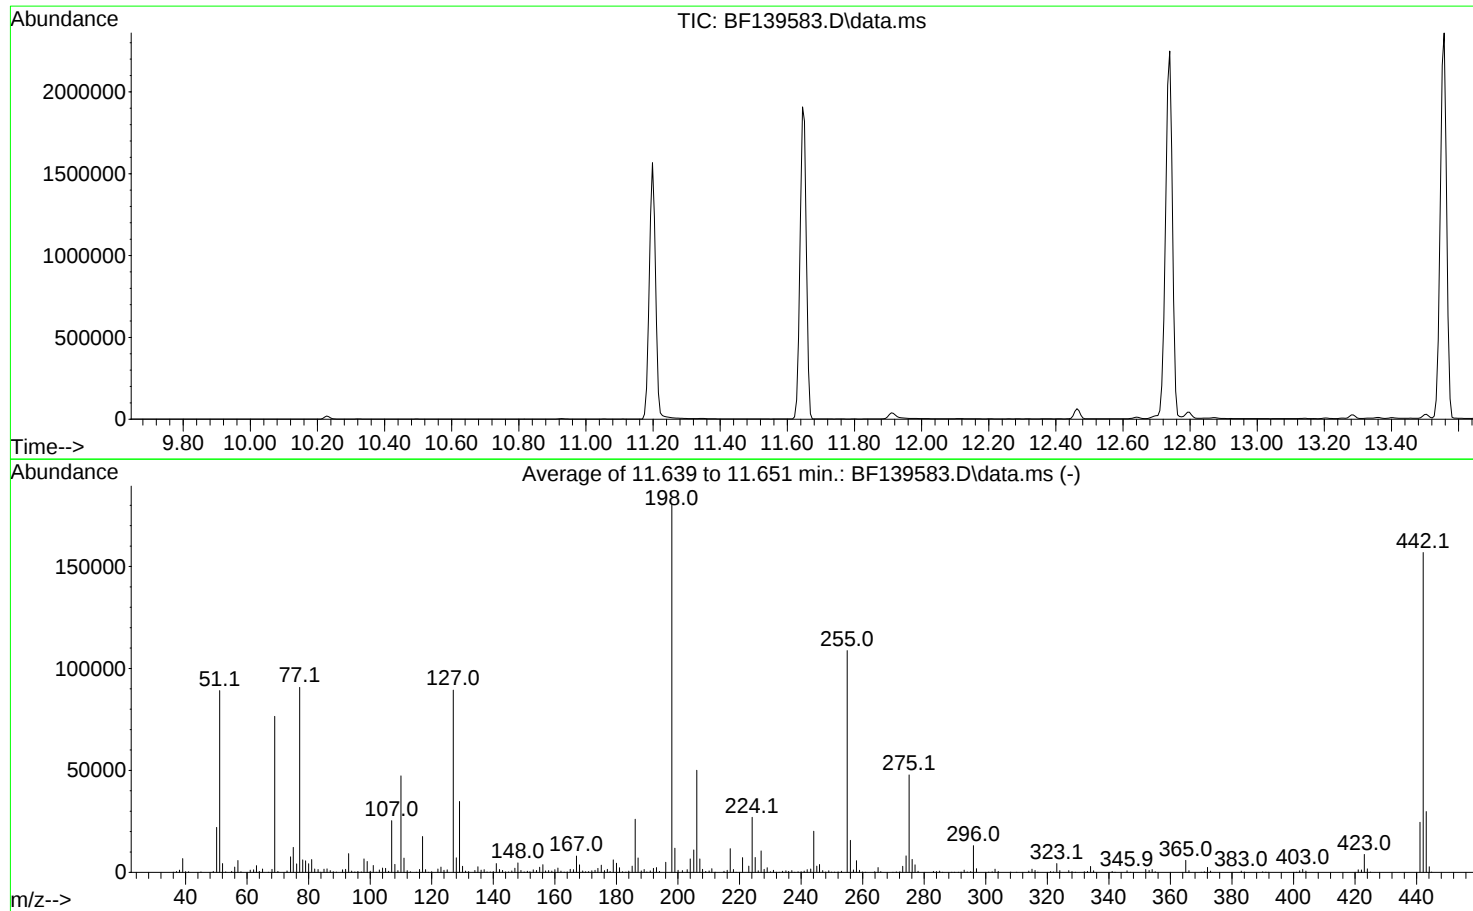




AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.4	89173	PASS
68	69	0.00	2	1.9	1474	PASS
69	198	0.00	100	42.4	76475	PASS
70	69	0.00	2	0.6	475	PASS
127	198	10	80	49.6	89397	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	180395	PASS
199	198	5	9	6.6	11825	PASS
275	198	10	60	26.5	47827	PASS
365	198	1	100	3.2	5859	PASS
441	198	0.01	100	13.6	24545	PASS
442	442	50	100	100.0	156851	PASS
443	442	15	24	19.0	29797	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100124\
Data File : BF139583.D
Acq On : 01 Oct 2024 13:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 02 05:09:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

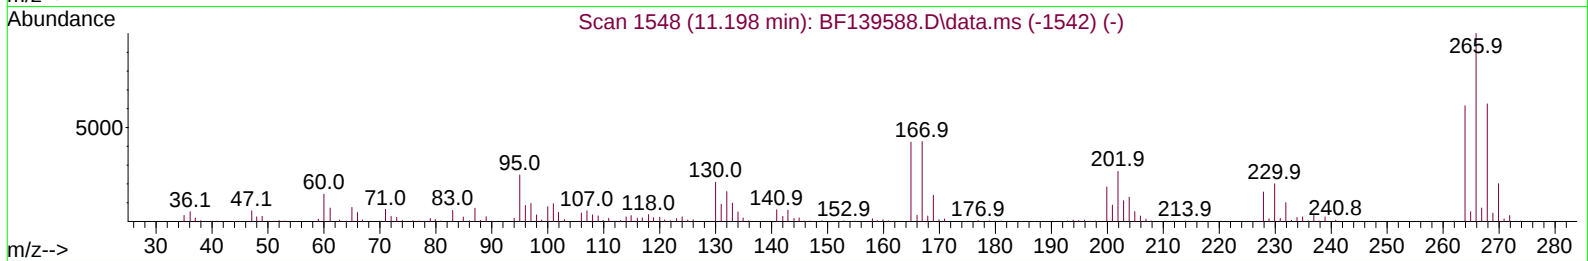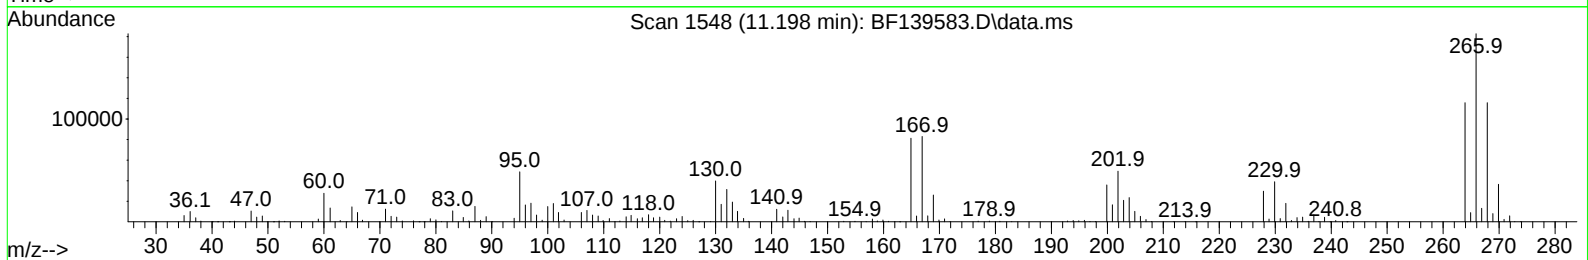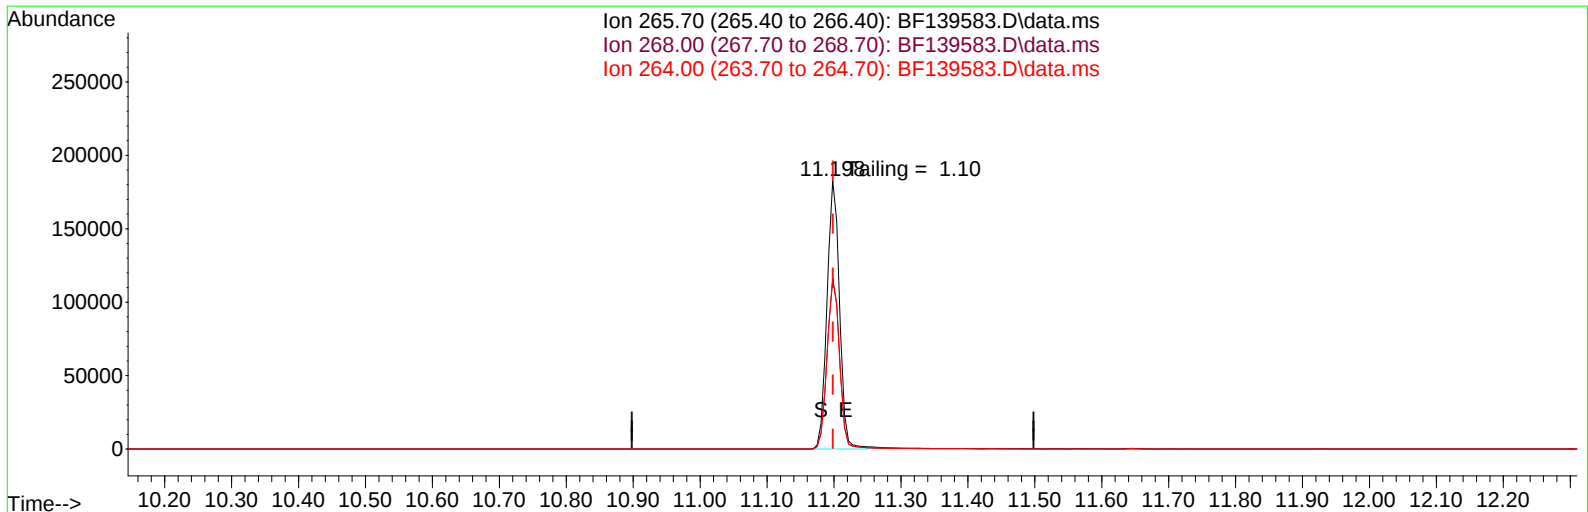

TIC: BF139583.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.000) 38009.92 ng

response 241021

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	63.37
264.00	61.60	63.38
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/1/2024	BNA_F	<u>BF139583.D</u>
Compound Name	Response	Retention Time
DDT	591188	13.557
DDD	7487	13.286
DDE	55	12.922
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7542	598730	1.26

Instrument :
BNA_F
ClientSampleId :
DFTPP