
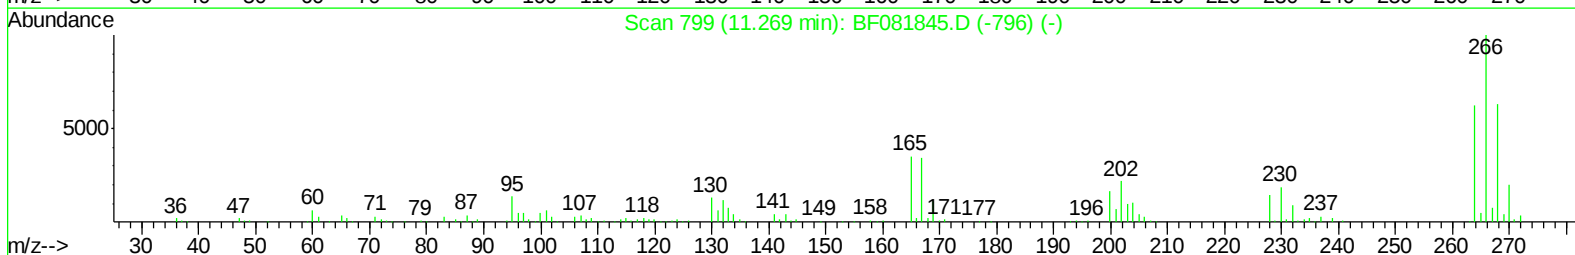
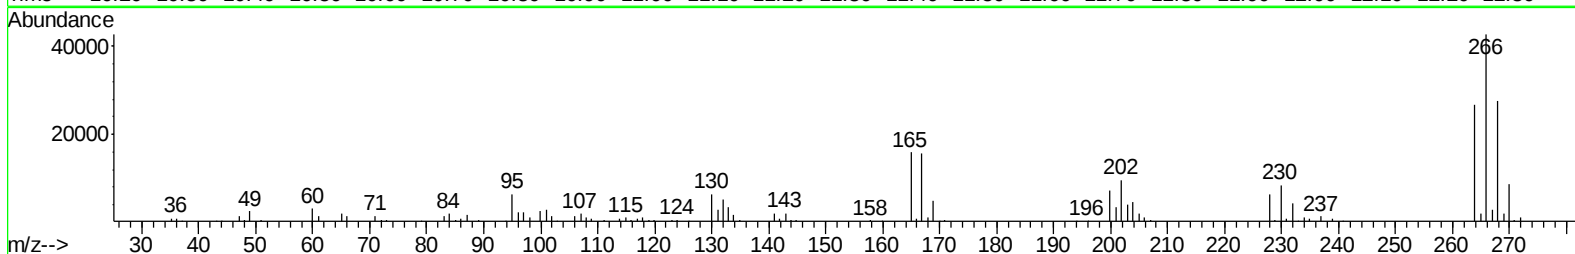


Data Path : Z:\HPCHEM1\BNA_F\Data\BF100215\
Data File : BF081979.D
Acq On : 2 Oct 2015 13:35
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 05:47:08 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 28 18:10:42 2015
Response via : Initial Calibration

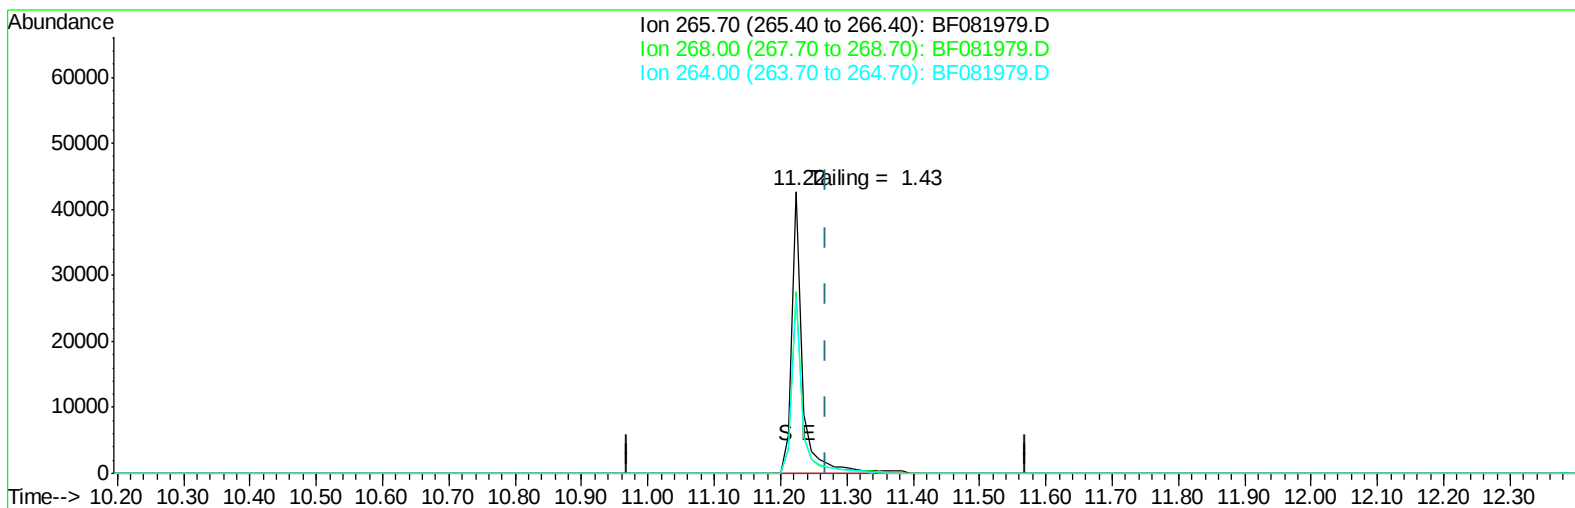

TIC: BF081979.D

(69) Pentachlorophenol (C)




11.223min (-0.046) 0.00ng

response 48033

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	64.37
264.00	62.70	62.94
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF100215\
Data File : BF081979.D
Acq On : 2 Oct 2015 13:35
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 05:47:08 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 28 18:10:42 2015
Response via : Initial Calibration

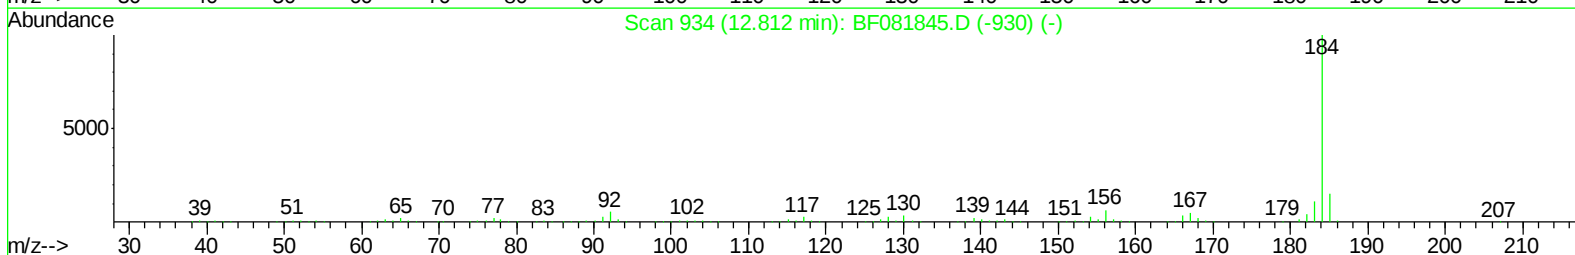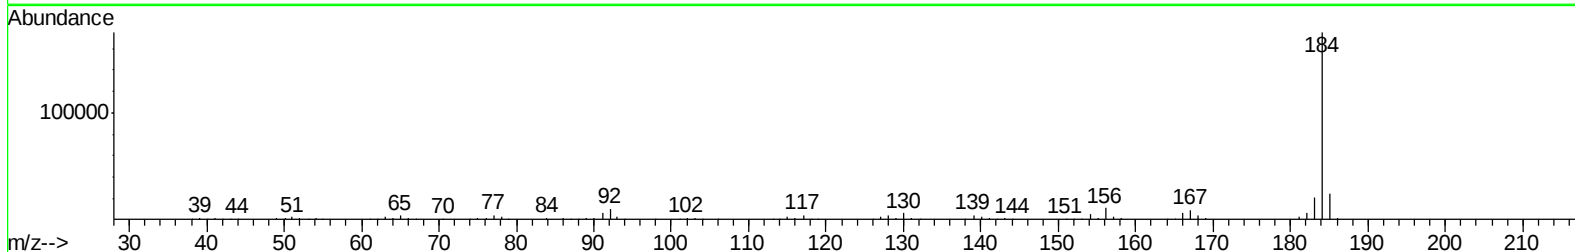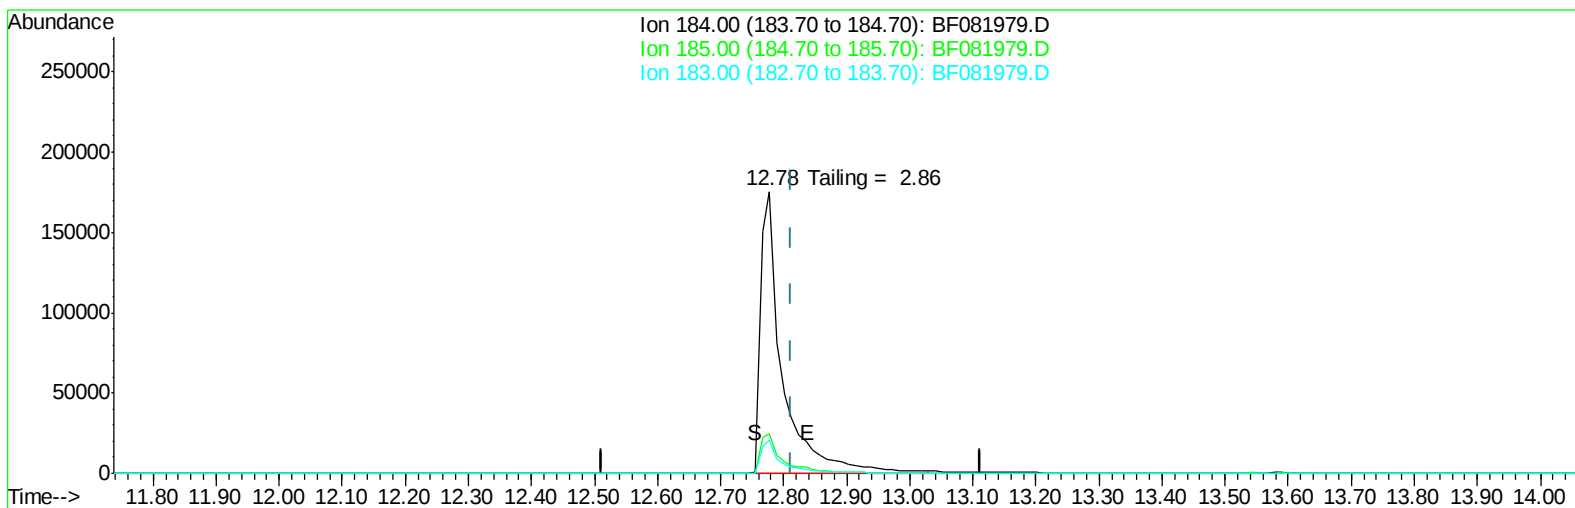

TIC: BF081979.D

(76) Benzidine

12.778min (-0.034) 0.00ng

response 428555

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.12
183.00	9.50	11.73#
0.00	0.00	0.00