
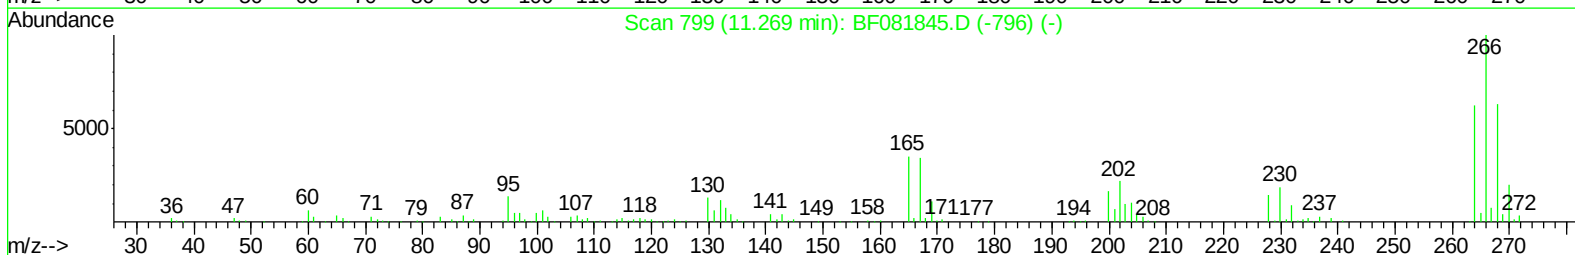
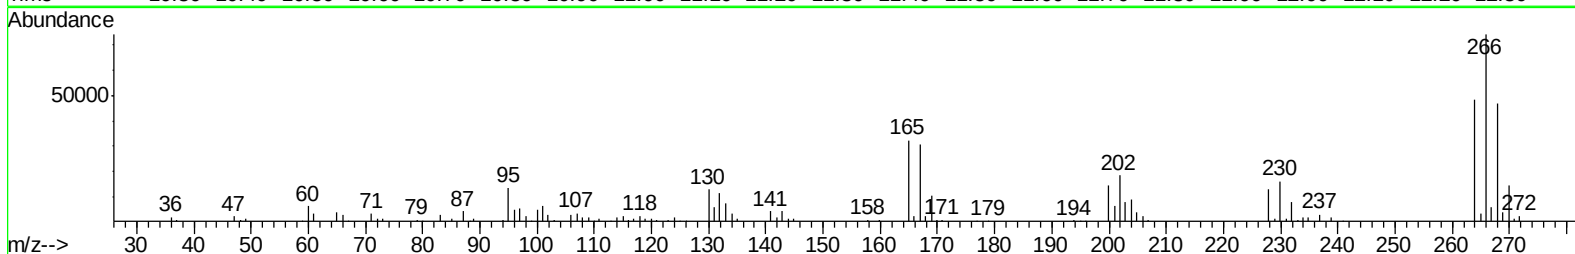


Data Path : Z:\HPCHEM1\BNA\_F\Data\BF100215\  
Data File : BF081998.D  
Acq On : 3 Oct 2015 2:05  
Operator : UM/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 05:45:50 2015  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF092815.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Sep 28 18:10:42 2015  
Response via : Initial Calibration

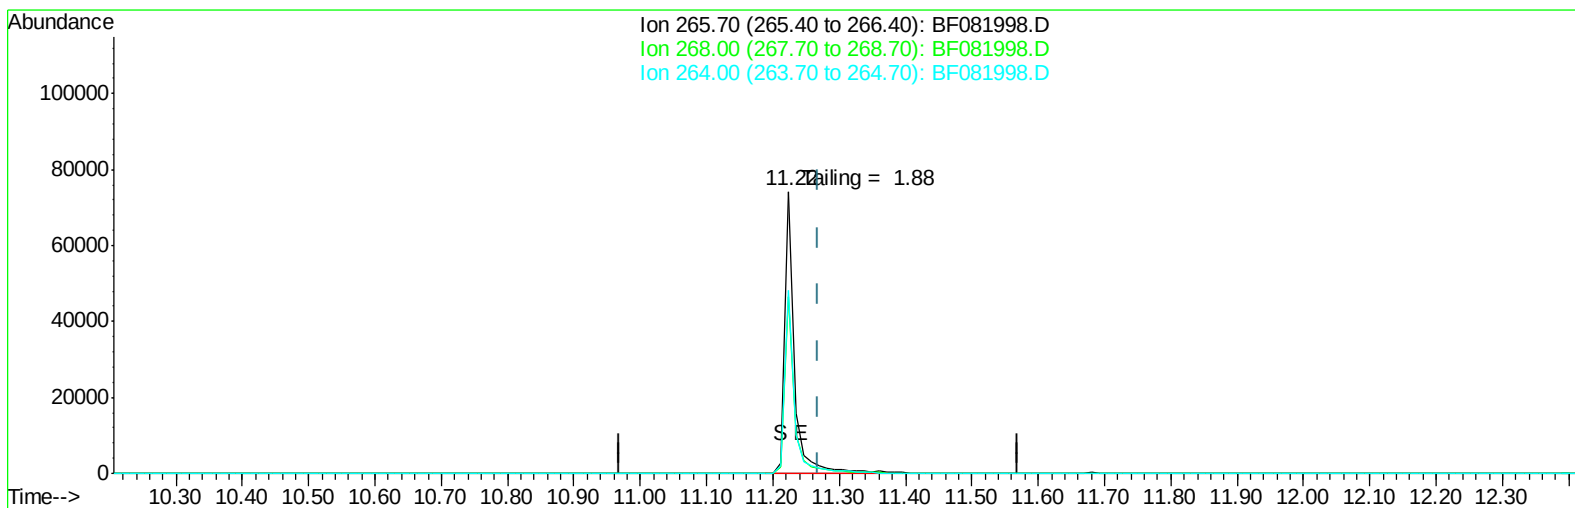

TIC: BF081998.D

(69) Pentachlorophenol (C)




11.223min (-0.046) 47791.42ng

response 75917

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 62.20 | 62.86 |
| 264.00 | 62.70 | 65.22 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_F\Data\BF100215\  
 Data File : BF081998.D  
 Acq On : 3 Oct 2015 2:05  
 Operator : UM/IZ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 05:45:50 2015  
 Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF092815.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Sep 28 18:10:42 2015  
 Response via : Initial Calibration

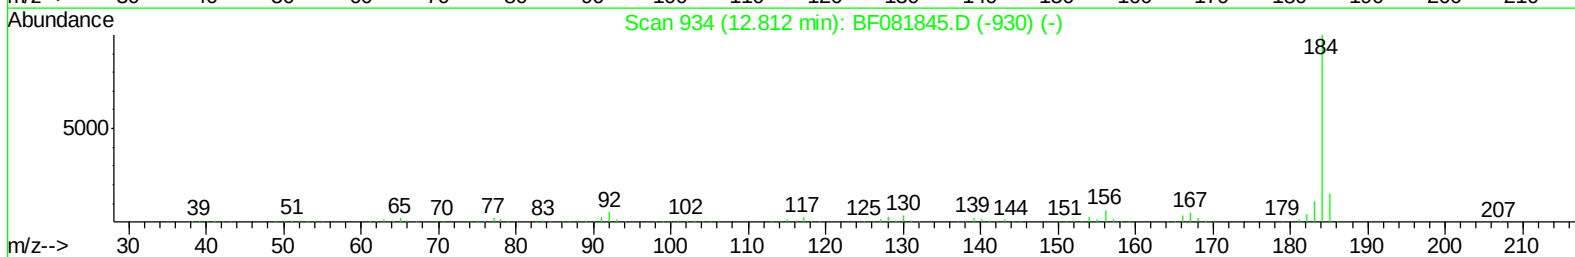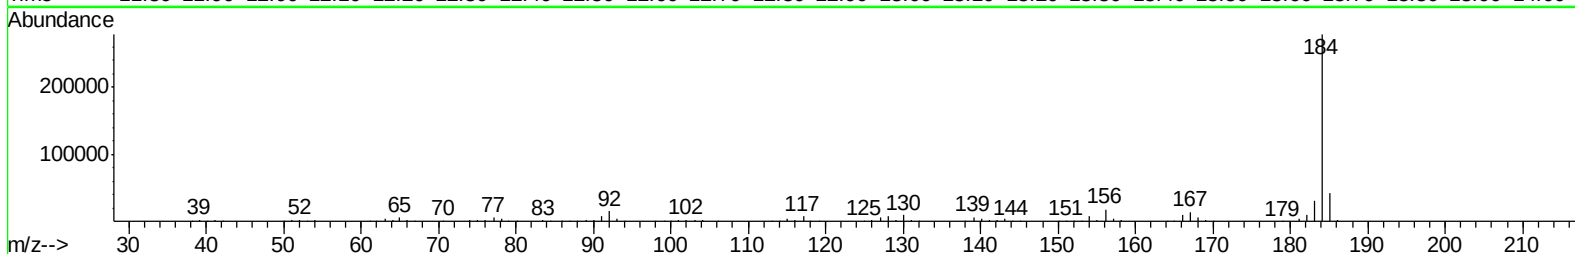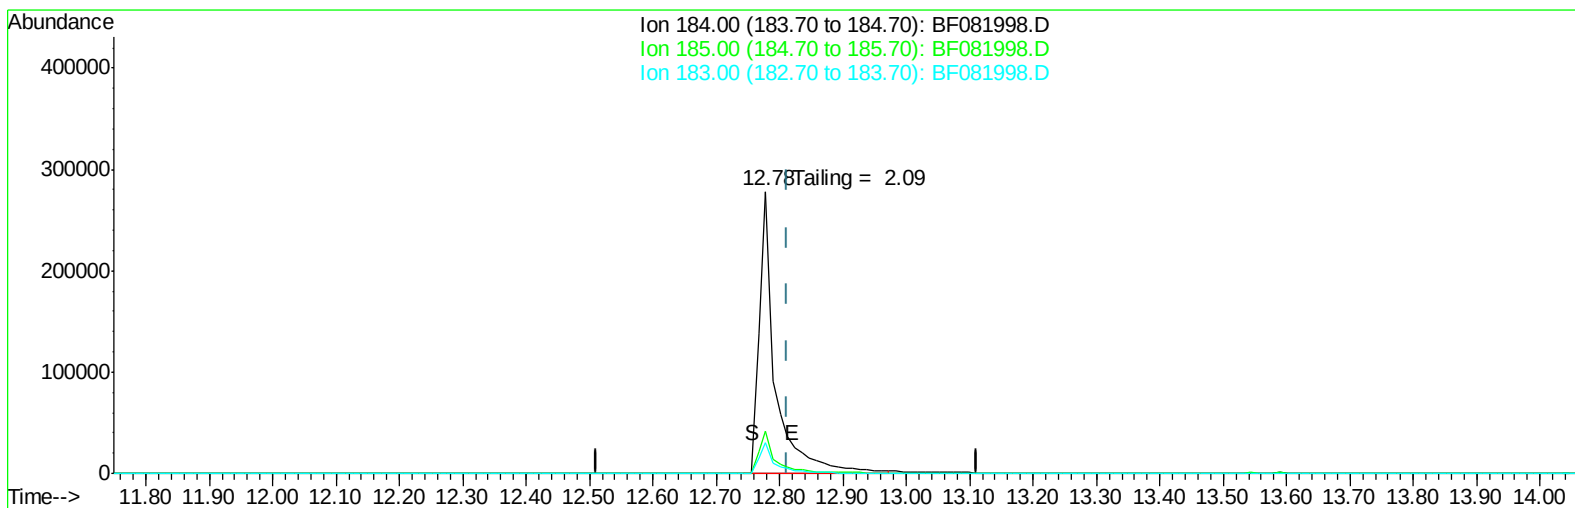

TIC: BF081998.D

(76) Benzidine

12.778min (-0.034) 0.00ng

response 503767

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 14.70 | 15.21 |
| 183.00 | 9.50  | 11.02 |
| 0.00   | 0.00  | 0.00  |