
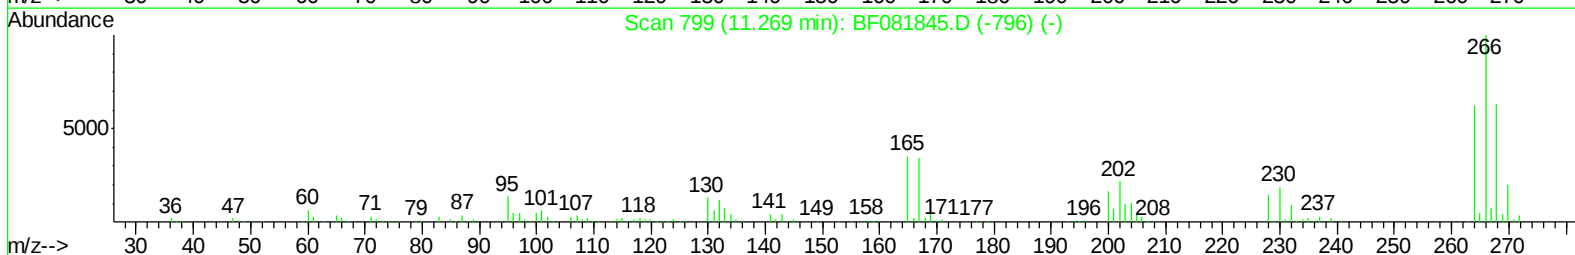
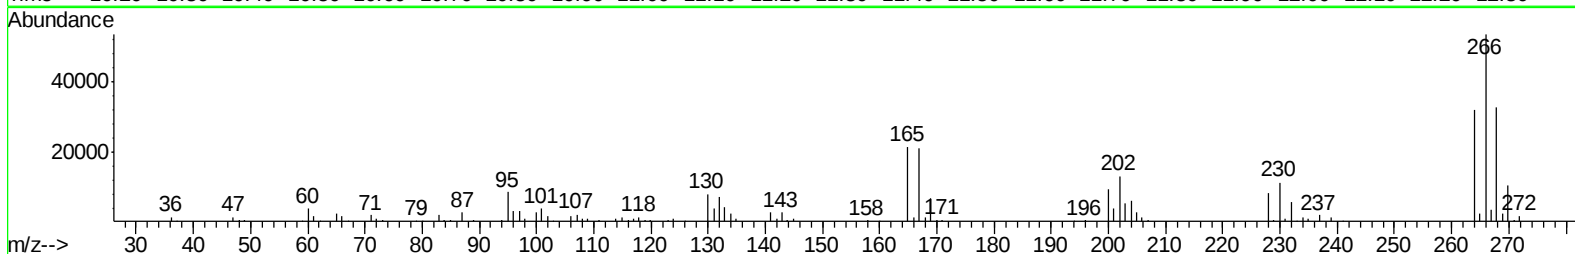


Data Path : Z:\HPCHEM1\BNA_F\Data\BF100215\
Data File : BF082019.D
Acq On : 3 Oct 2015 13:59
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 05:43:54 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 28 18:10:42 2015
Response via : Initial Calibration

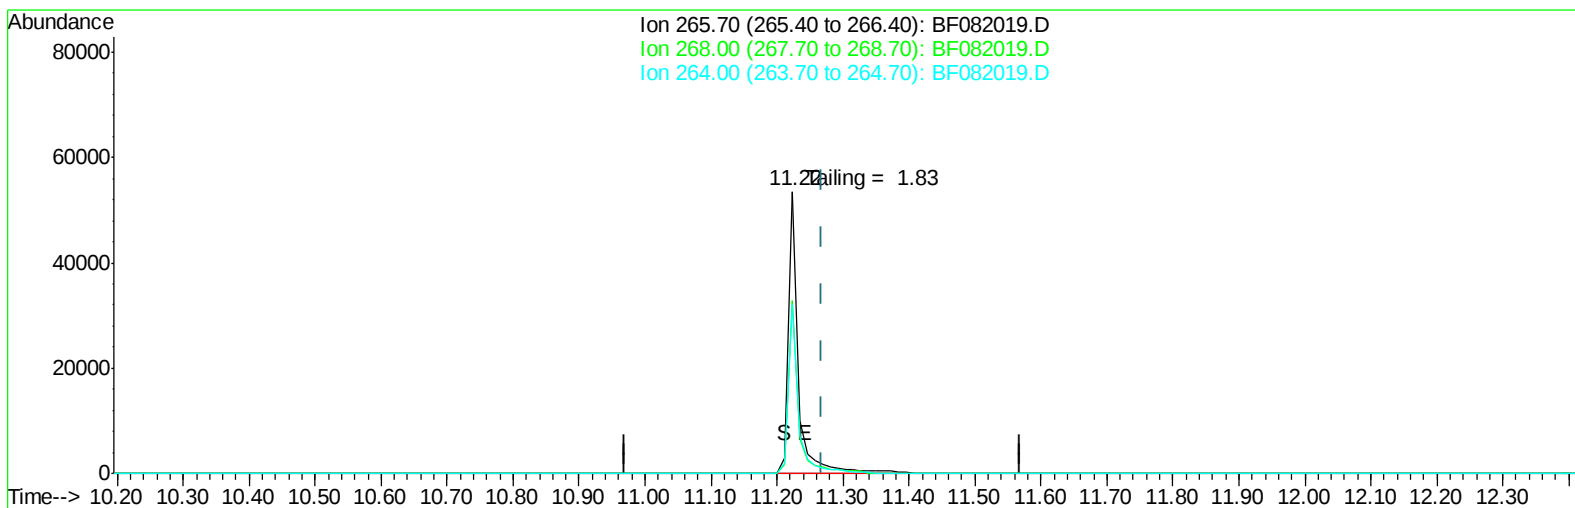

TIC: BF082019.D

(69) Pentachlorophenol (C)




11.224min (-0.045) 0.00ng

response 55693

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	61.52
264.00	62.70	59.85
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF100215\
Data File : BF082019.D
Acq On : 3 Oct 2015 13:59
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 05:43:54 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 28 18:10:42 2015
Response via : Initial Calibration

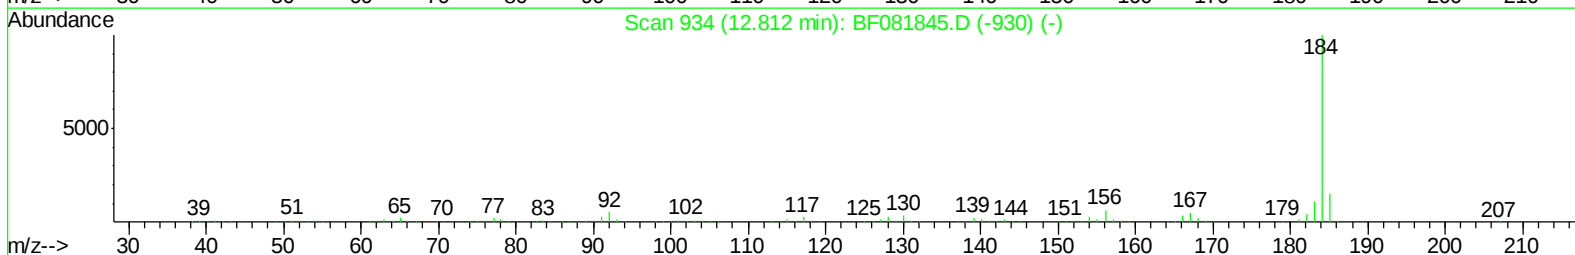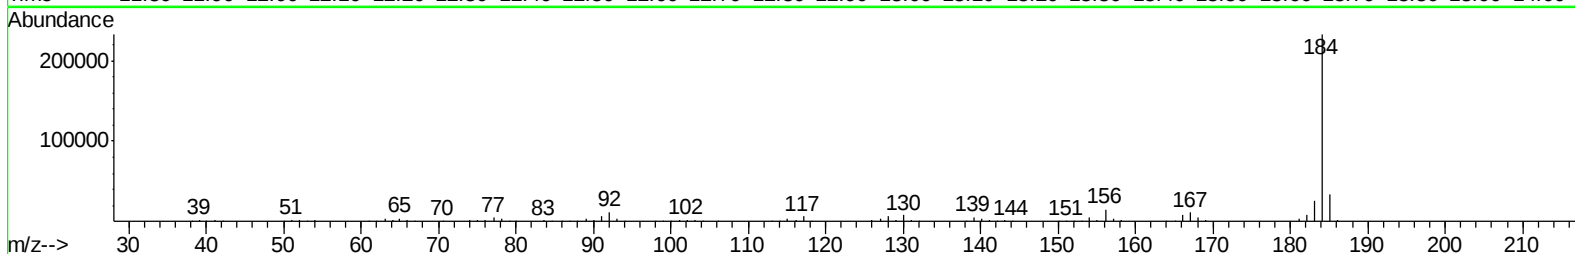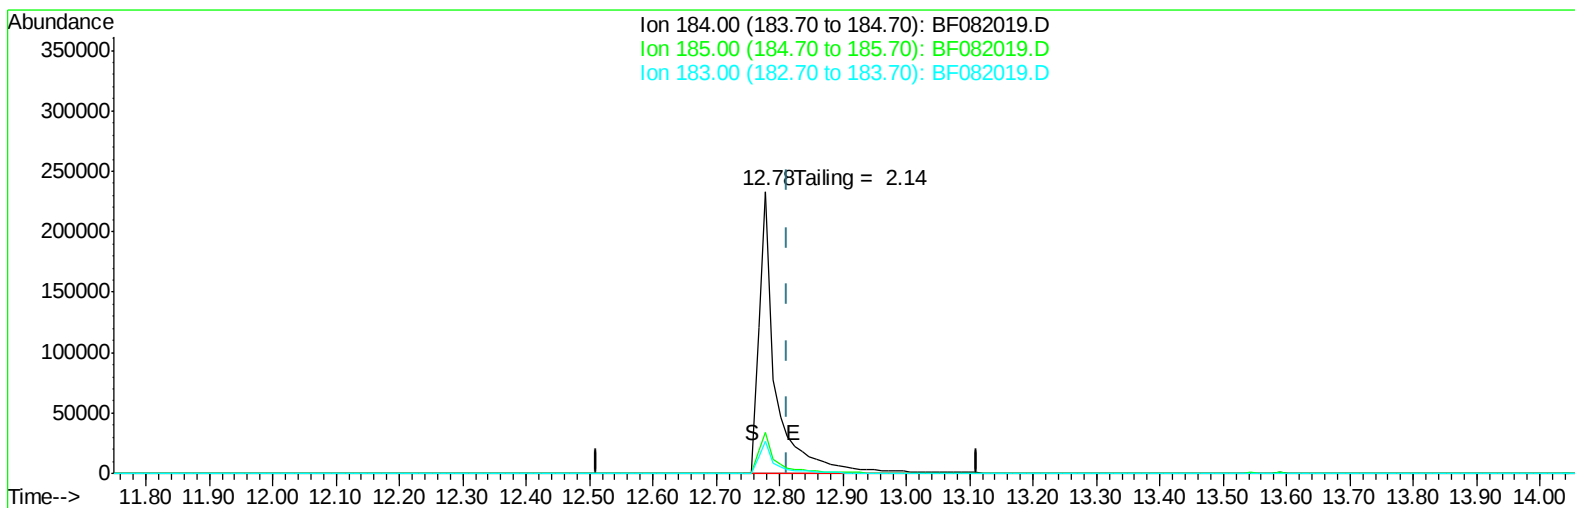

TIC: BF082019.D

(76) Benzidine

12.778min (-0.034) 0.00ng

response 431343

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.67
183.00	9.50	11.21
0.00	0.00	0.00