

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100215\
 Data File : BF081985.D
 Acq On : 2 Oct 2015 18:04
 Operator : UM/IZ
 Sample : PB85878BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB85878BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.074	254	257	266	rBV	752295	992034	33.28%	4.789%
2	5.486	290	293	295	rBV	1768948	1968270	66.03%	9.502%
3	6.514	380	383	385	rBV	1749857	1958574	65.71%	9.456%
4	6.652	392	395	397	rBV	2125103	2037113	68.34%	9.835%
5	6.892	414	416	427	rVB	296772	443800	14.89%	2.143%
6	7.040	427	429	442	rBV	1847917	1694707	56.85%	8.182%
7	7.452	463	465	479	rBV	1122424	1253933	42.07%	6.054%
8	8.172	526	528	537	rBV	565028	604910	20.29%	2.920%
9	9.258	620	623	625	rBV	1577807	2411375	80.90%	11.642%
10	9.932	679	682	698	rBV	733479	731398	24.54%	3.531%
11	10.720	749	751	754	rBV	1230354	1414835	47.46%	6.831%
12	11.429	810	813	831	rBV	436295	757030	25.40%	3.655%
13	13.018	949	952	971	rBV	2880254	2980823	100.00%	14.391%
14	14.069	1041	1044	1060	rBV	663317	838856	28.14%	4.050%
15	15.532	1169	1172	1186	rBV	335435	625779	20.99%	3.021%


Sum of corrected areas: 20713437

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100215\
Data File : BF081985.D
Acq On : 2 Oct 2015 18:04
Operator : UM/IZ
Sample : PB85878BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB85878BL

Quant Method : H:\HPCHEM1\BNA_F\Method\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

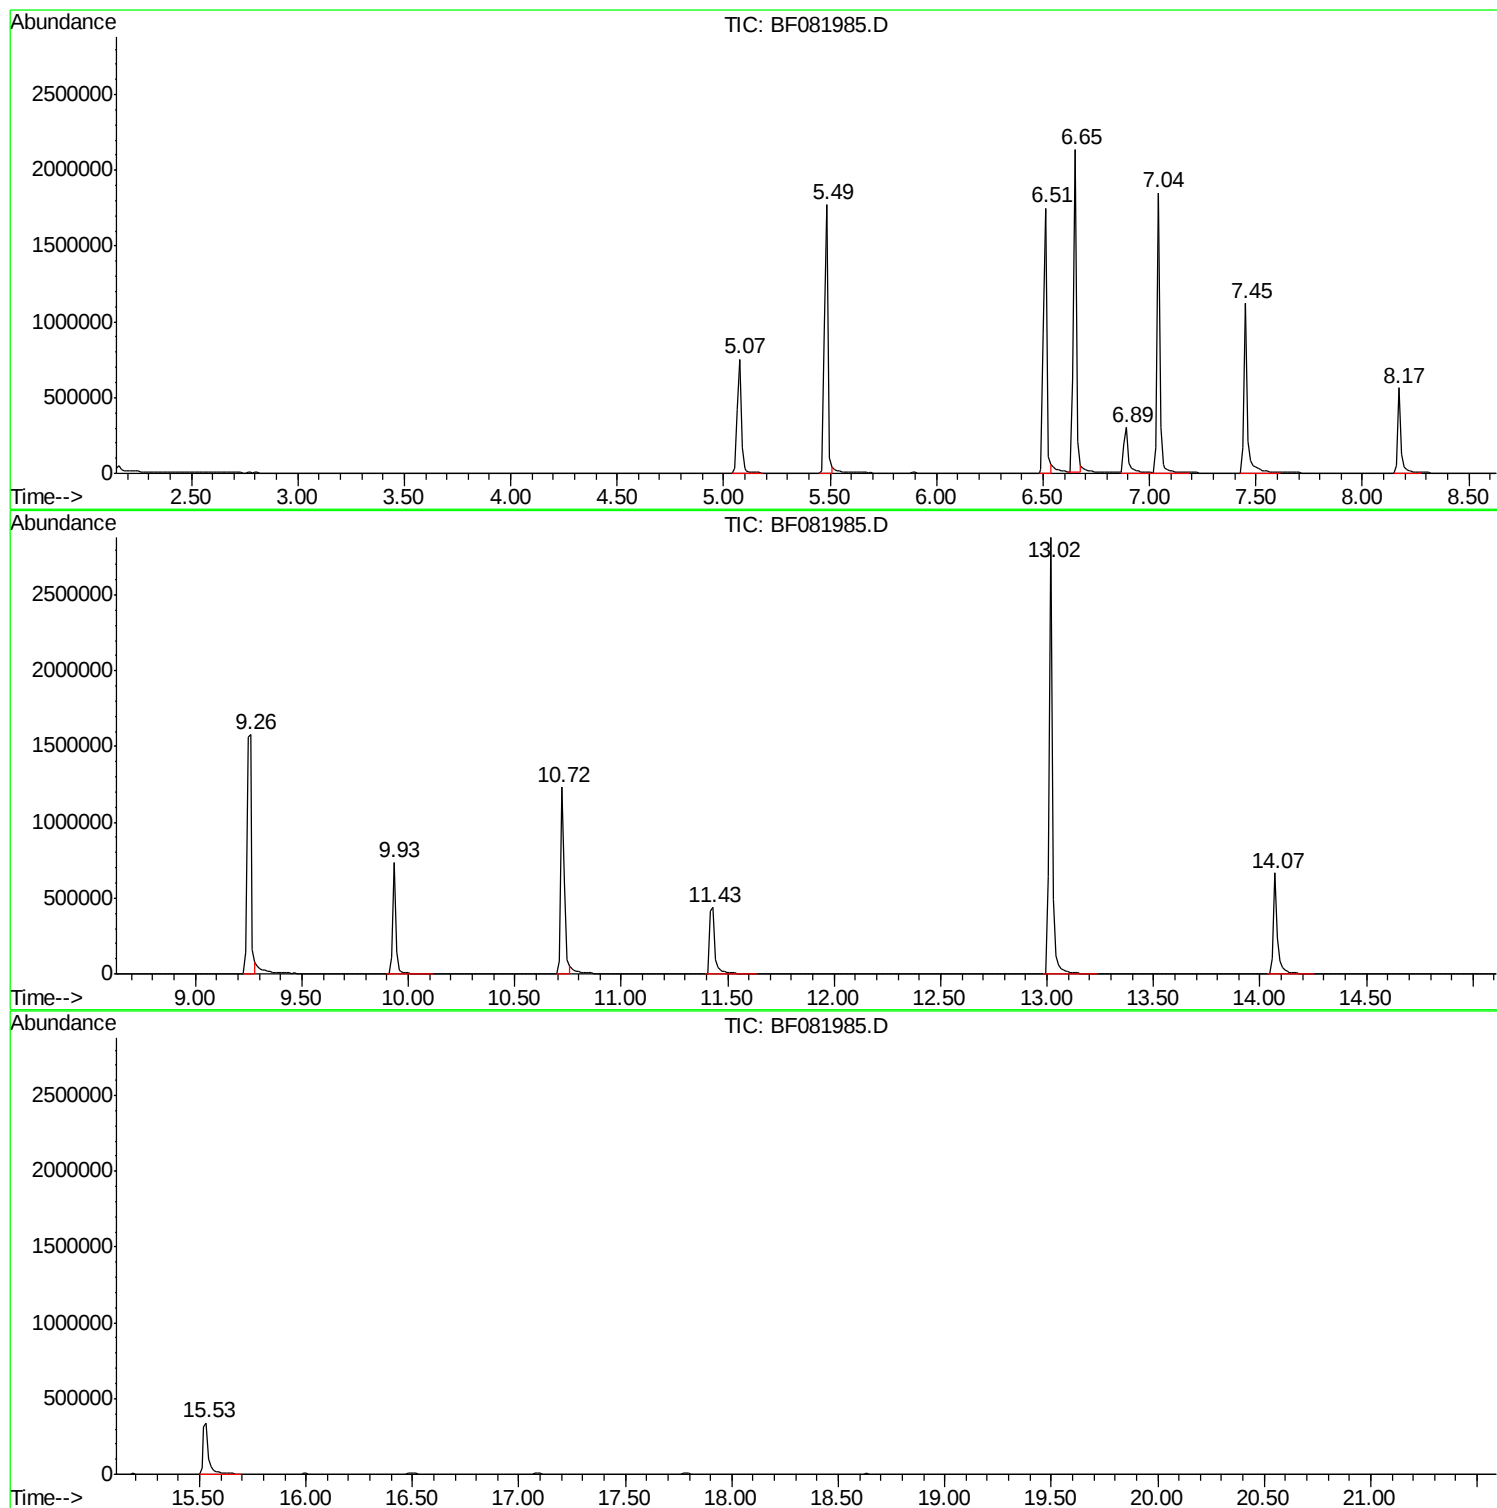

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100215\
Data File : BF081985.D
Acq On : 2 Oct 2015 18:04
Operator : UM/IZ
Sample : PB85878BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB85878BL










Quant Method : H:\HPCHEM1\BNA_F\Method\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.07	44.71 ng	992034	1,4-Dichlorobenzene-d4	6.89

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2		Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	39
3		Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	36
4		3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	28
5		Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23

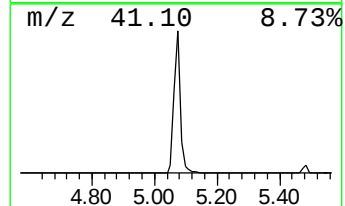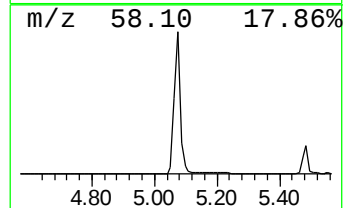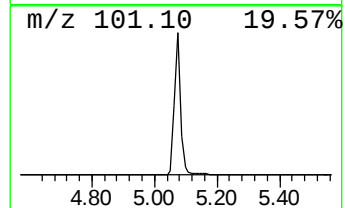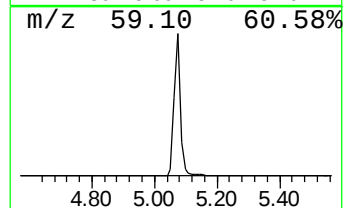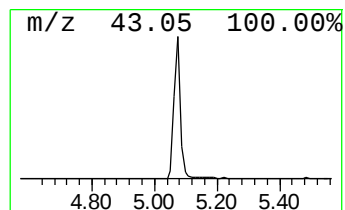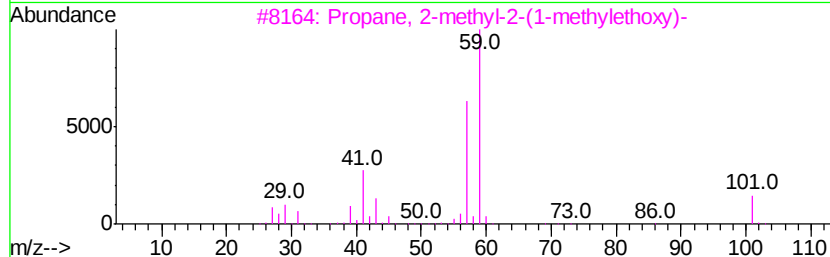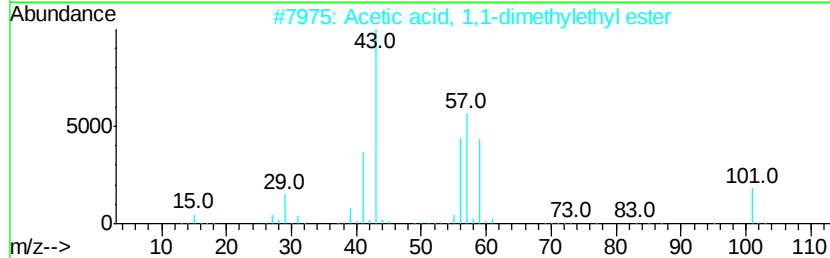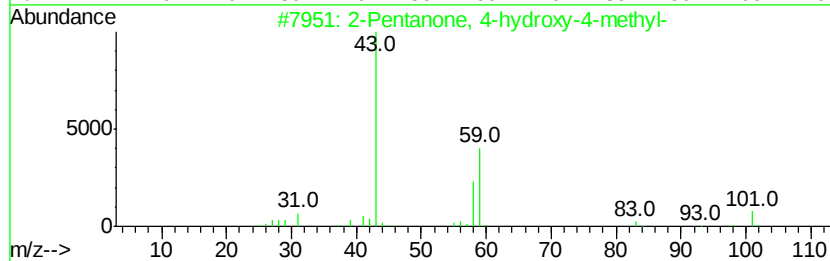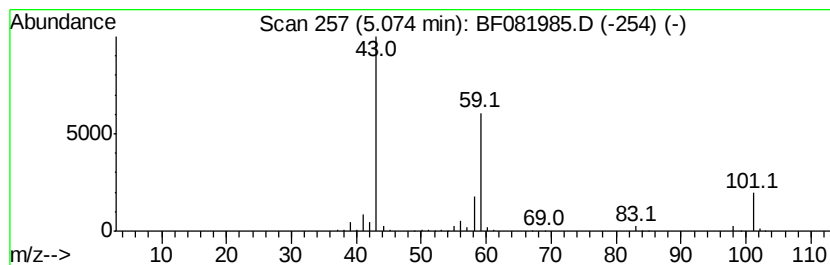

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100215\
Data File : BF081985.D
Acq On : 2 Oct 2015 18:04
Operator : UM/IZ
Sample : PB85878BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB85878BL










Quant Method : H:\HPCHEM1\BNA_F\Method\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.65 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.65	91.80 ng	2037110	1,4-Dichlorobenzene-d4	6.89

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9

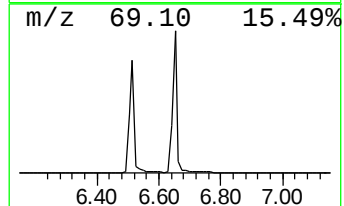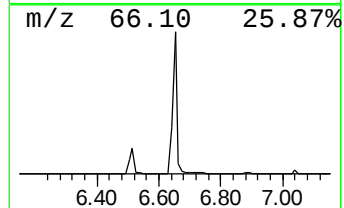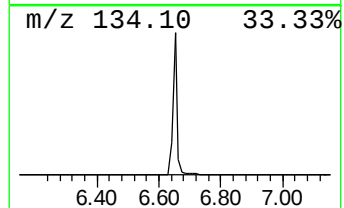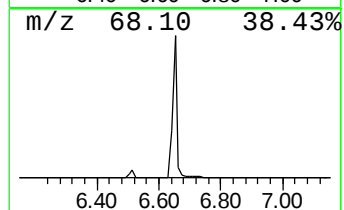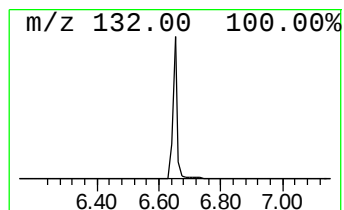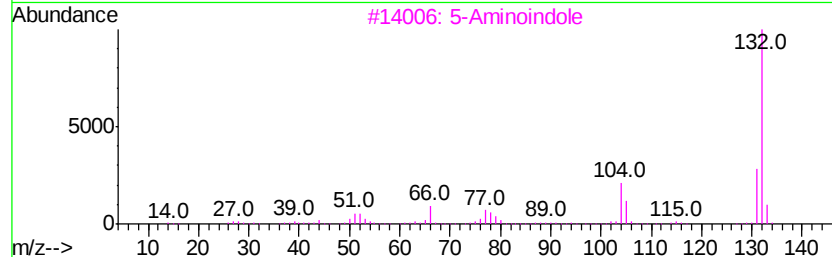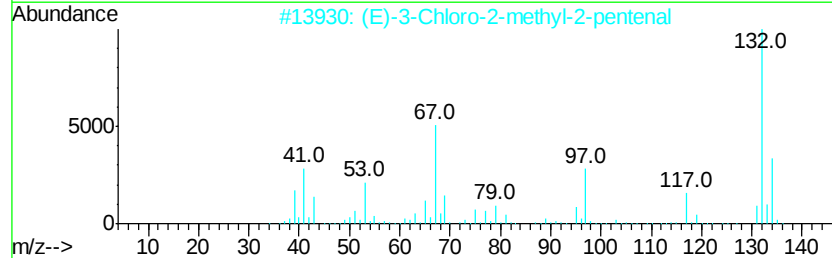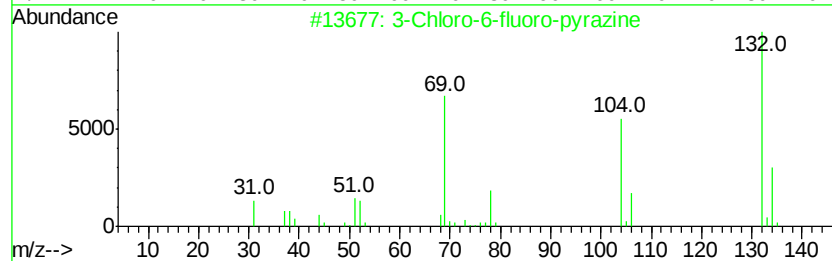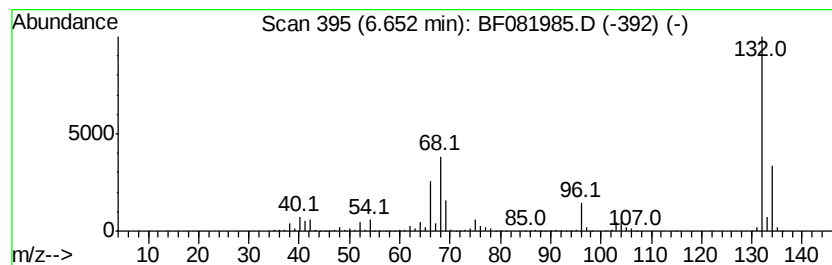

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100215\
Data File : BF081985.D
Acq On : 2 Oct 2015 18:04
Operator : UM/IZ
Sample : PB85878BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB85878BL

Quant Method : H:\HPCHEM1\BNA_F\Method\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.07	44.7	ng	992034	1	6.89	443800	20.0
unknown6.65	6.65	91.8	ng	2037110	1	6.89	443800	20.0