


Data Path : Z:\HPCHEM1\BNA F\Data\BF100215\
 Data File : BF081979.D
 Acq On : 2 Oct 2015 13:35
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 05 17:58:12 2015

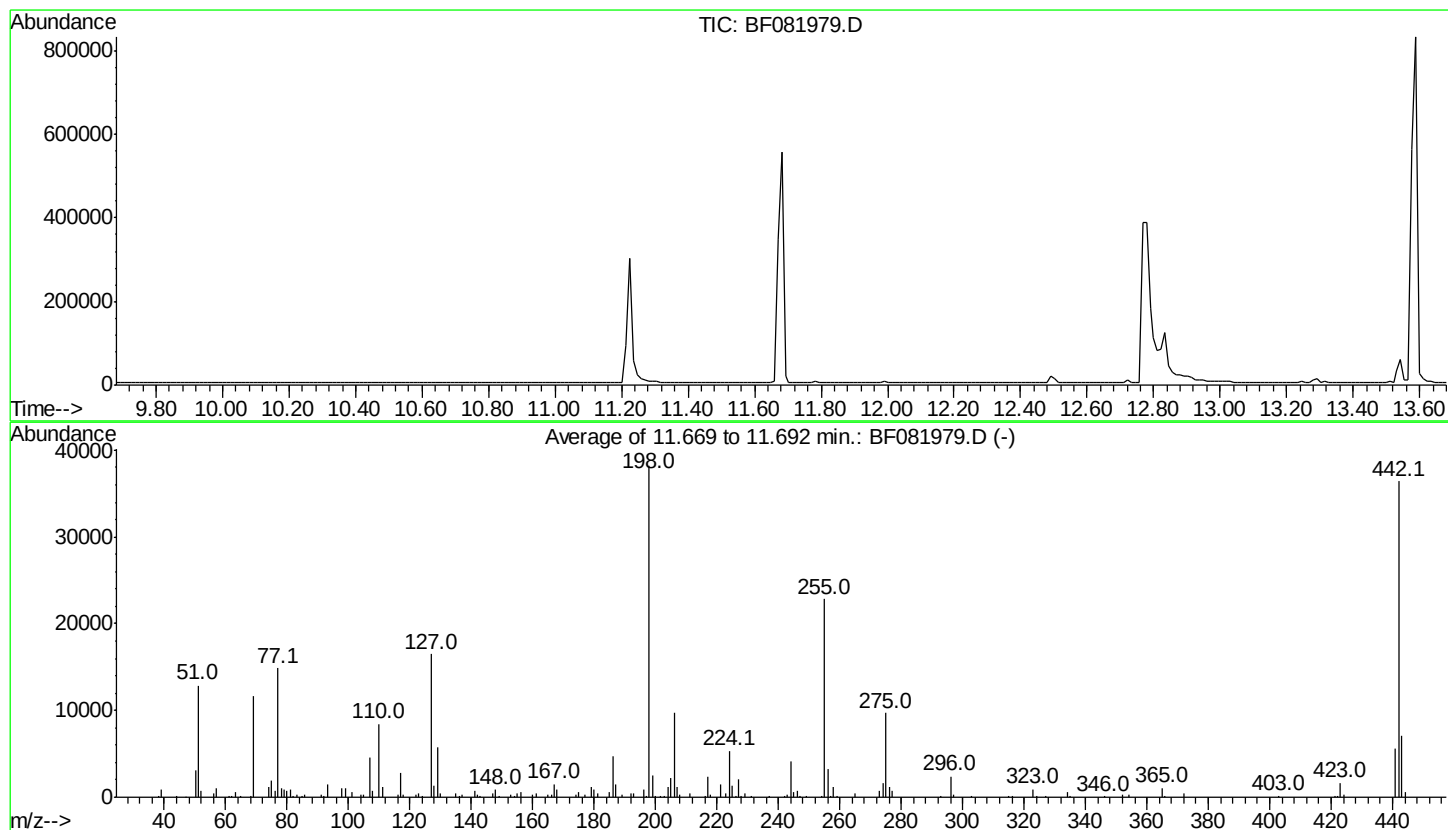

AutoFind: Scans 834, 835, 836; Background Corrected with Scan 831

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	12837	PASS
68	69	0.00	2	1.2	135	PASS
69	198	0.00	100	30.6	11701	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.2	16520	PASS
197	198	0.00	2	0.4	148	PASS
198	198	100	100	100.0	38215	PASS
199	198	5	9	6.6	2515	PASS
275	198	10	60	25.4	9712	PASS
365	198	1	100	2.9	1101	PASS
441	442	0.01	24	15.6	5667	PASS
442	198	50	100	95.3	36427	PASS
443	442	15	24	19.4	7076	PASS