


Data Path : Z:\HPCHEM1\BNA F\DATA\BF100215\
 Data File : BF081998.D
 Acq On : 3 Oct 2015 2:05
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 05 17:58:12 2015

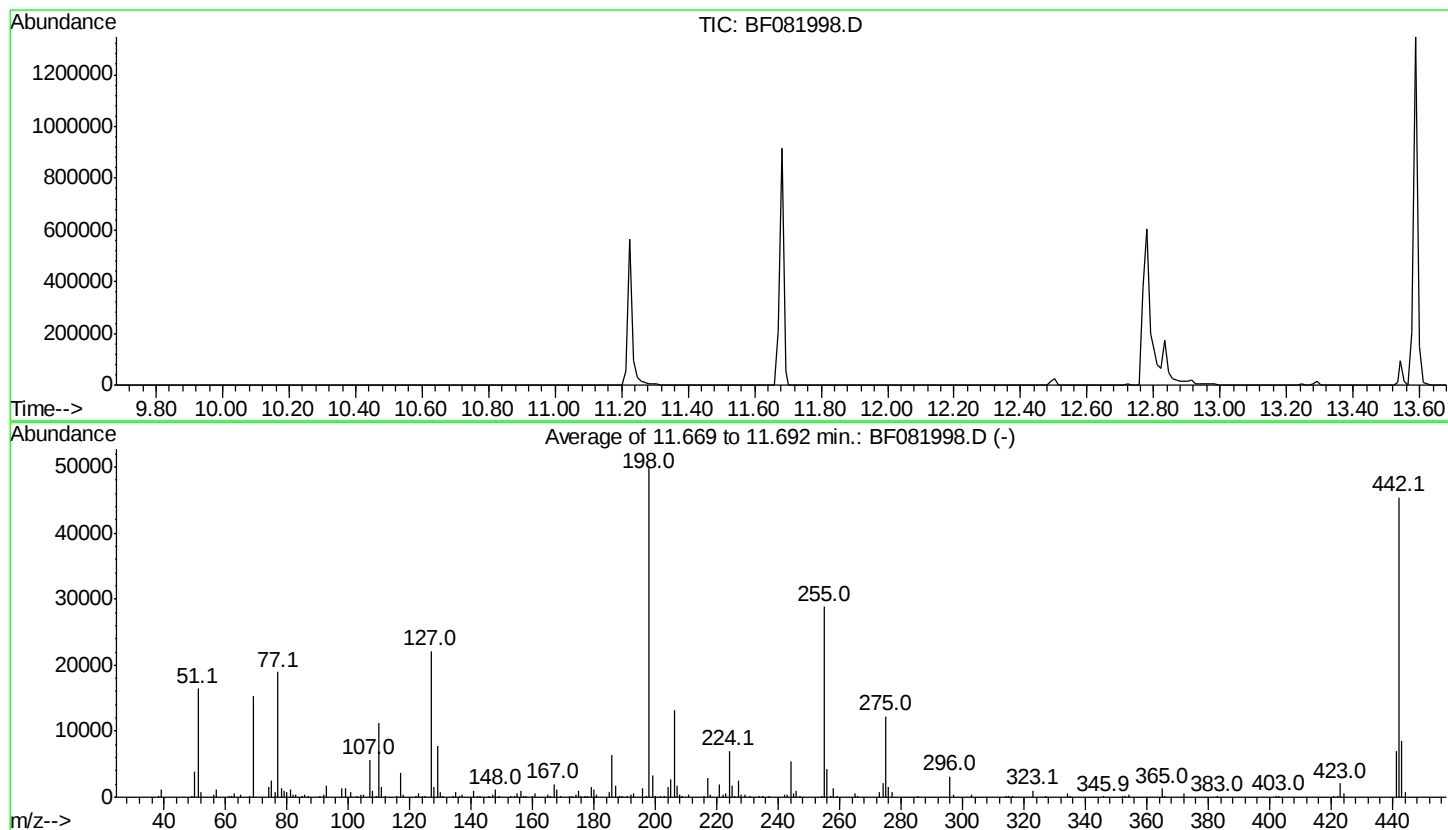

AutoFind: Scans 834, 835, 836; Background Corrected with Scan 831

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	16471	PASS
68	69	0.00	2	1.8	271	PASS
69	198	0.00	100	30.3	15237	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.2	22172	PASS
197	198	0.00	2	0.3	175	PASS
198	198	100	100	100.0	50219	PASS
199	198	5	9	6.6	3321	PASS
275	198	10	60	24.5	12300	PASS
365	198	1	100	2.6	1306	PASS
441	442	0.01	24	15.3	6968	PASS
442	198	50	100	90.4	45413	PASS
443	442	15	24	18.7	8513	PASS