
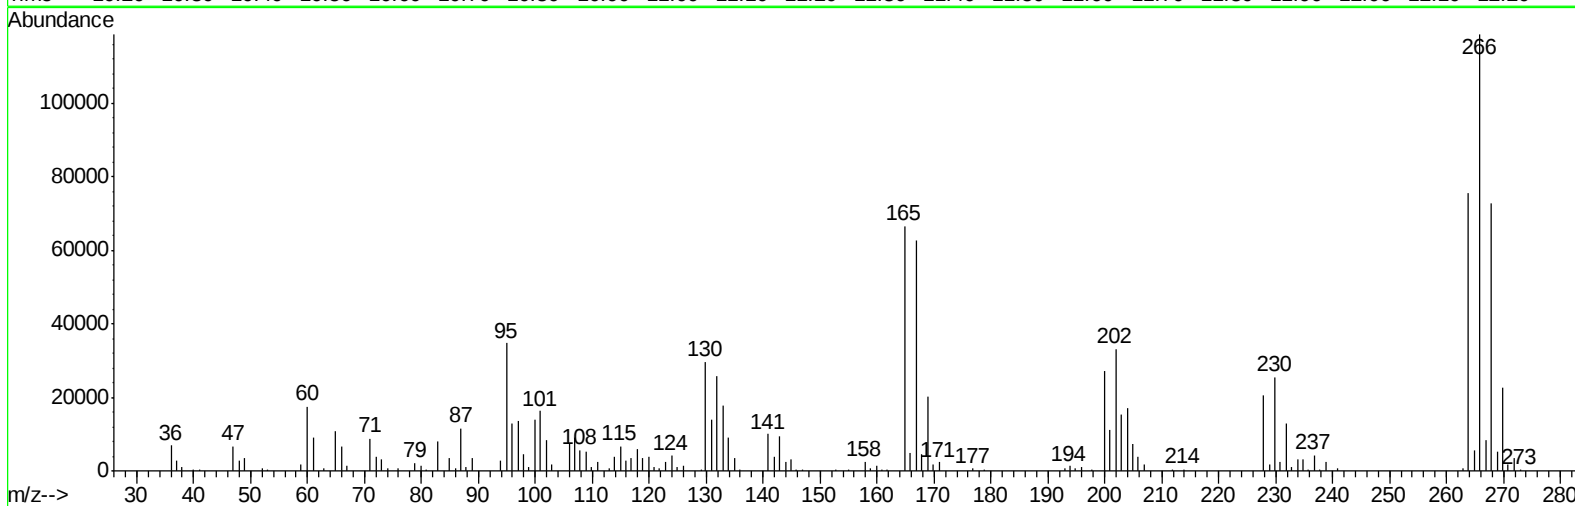


Data Path : Z:\HPCHEM1\BNA F\DATA\BF100217\
 Data File : BF098997.D
 Acq On : 2 Oct 2017 14:02
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Oct 03 06:40:30 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 23 13:50:58 2017
 Response via : Initial Calibration

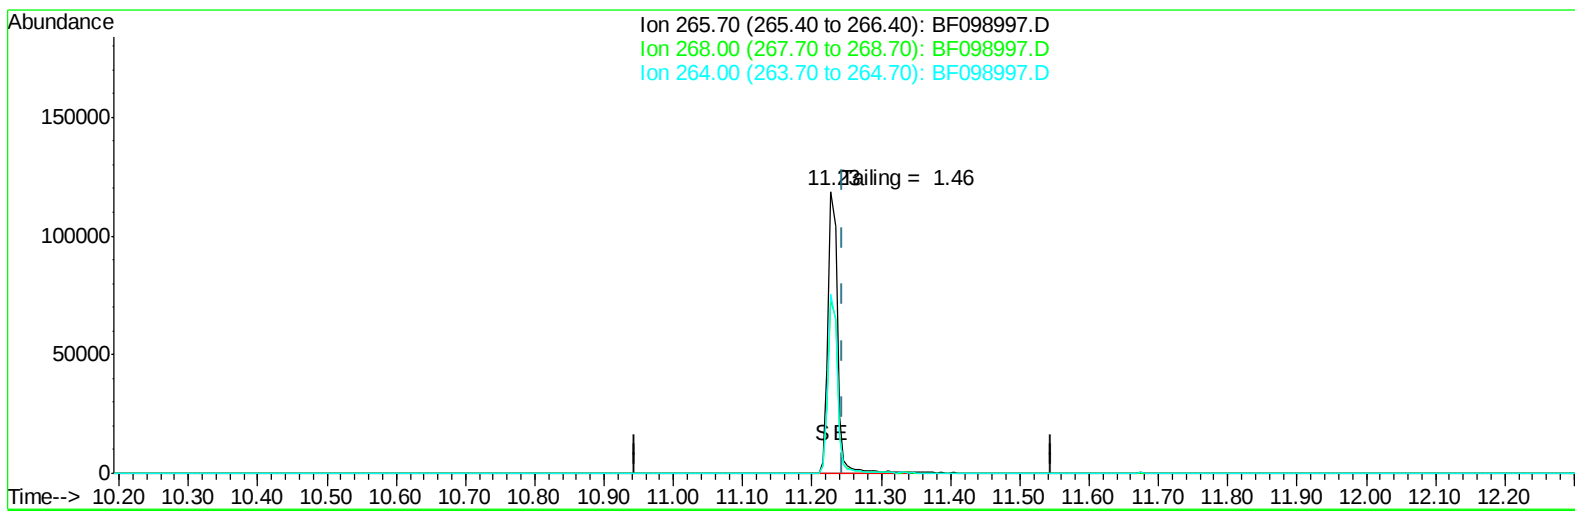

TIC: BF098997.D

(69) Pentachlorophenol (C)

11.228min (-0.018) 39618.85ng



response 111359

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.16
264.00	61.90	63.60
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100217\
Data File : BF098997.D
Acq On : 2 Oct 2017 14:02
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Oct 03 06:40:30 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

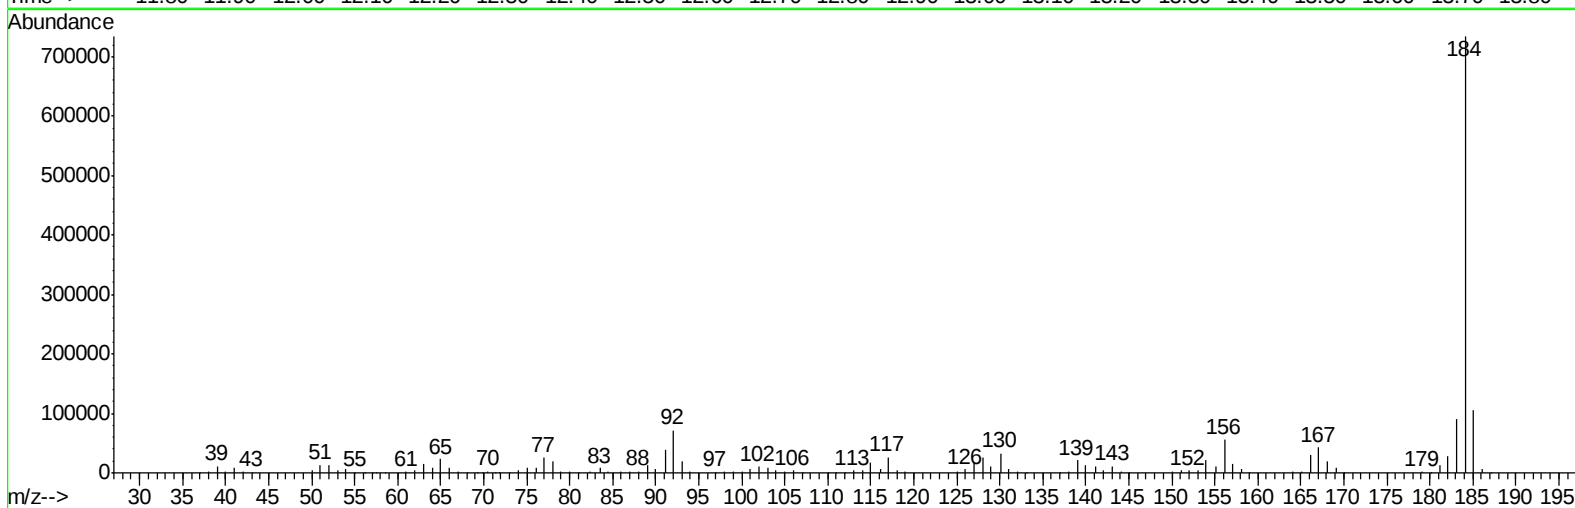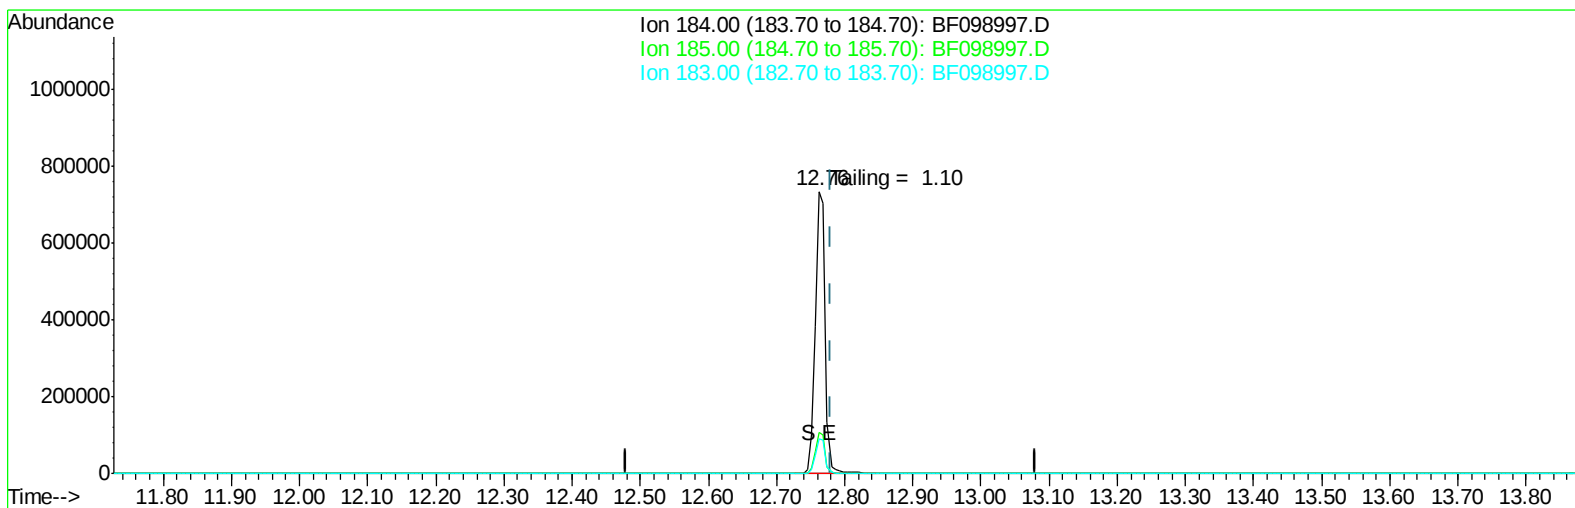

TIC: BF098997.D

(76) Benzidine

12.763min (-0.018) 0.00ng

response 747732

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.35
183.00	11.60	12.31
0.00	0.00	0.00