

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100217\
 Data File : BF099020.D
 Acq On : 3 Oct 2017 00:42
 Operator : SJ/JU
 Sample : I5531-01 5X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-62-0-2.5

Quant Time: Oct 03 04:54:43 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 23 13:50:58 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	120266	20.00	ng	-0.02
21) Naphthalene-d8	8.19	136	458735	20.00	ng	-0.02
38) Acenaphthene-d10	9.95	164	174273	20.00	ng	-0.02
63) Phenanthrene-d10	11.43	188	268566	20.00	ng	-0.01
75) Chrysene-d12	14.07	240	251088	20.00	ng	-0.01
86) Perylene-d12	15.57	264	209262	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.52	112	73749	9.76	ng	-0.02
7) Phenol-d6	6.52	99	174692	18.74	ng	-0.02
23) Nitrobenzene-d5	7.46	82	110455	15.44	ng	-0.02
41) 2,4,6-Tribromophenol	10.73	330	1494	1.05	ng	-0.02
44) 2-Fluorobiphenyl	9.26	172	209401	20.06	ng	-0.02
78) Terphenyl-d14	13.01	244	149207	13.51	ng	-0.02
Target Compounds						
49) Dimethylphthalate	9.65	163	31071	2.362	ng	Qvalue # 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100217\
Data File : BF099020.D
Acq On : 3 Oct 2017 00:42
Operator : SJ/JU
Sample : I5531-01 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-62-0-2.5

Quant Time: Oct 03 04:54:43 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

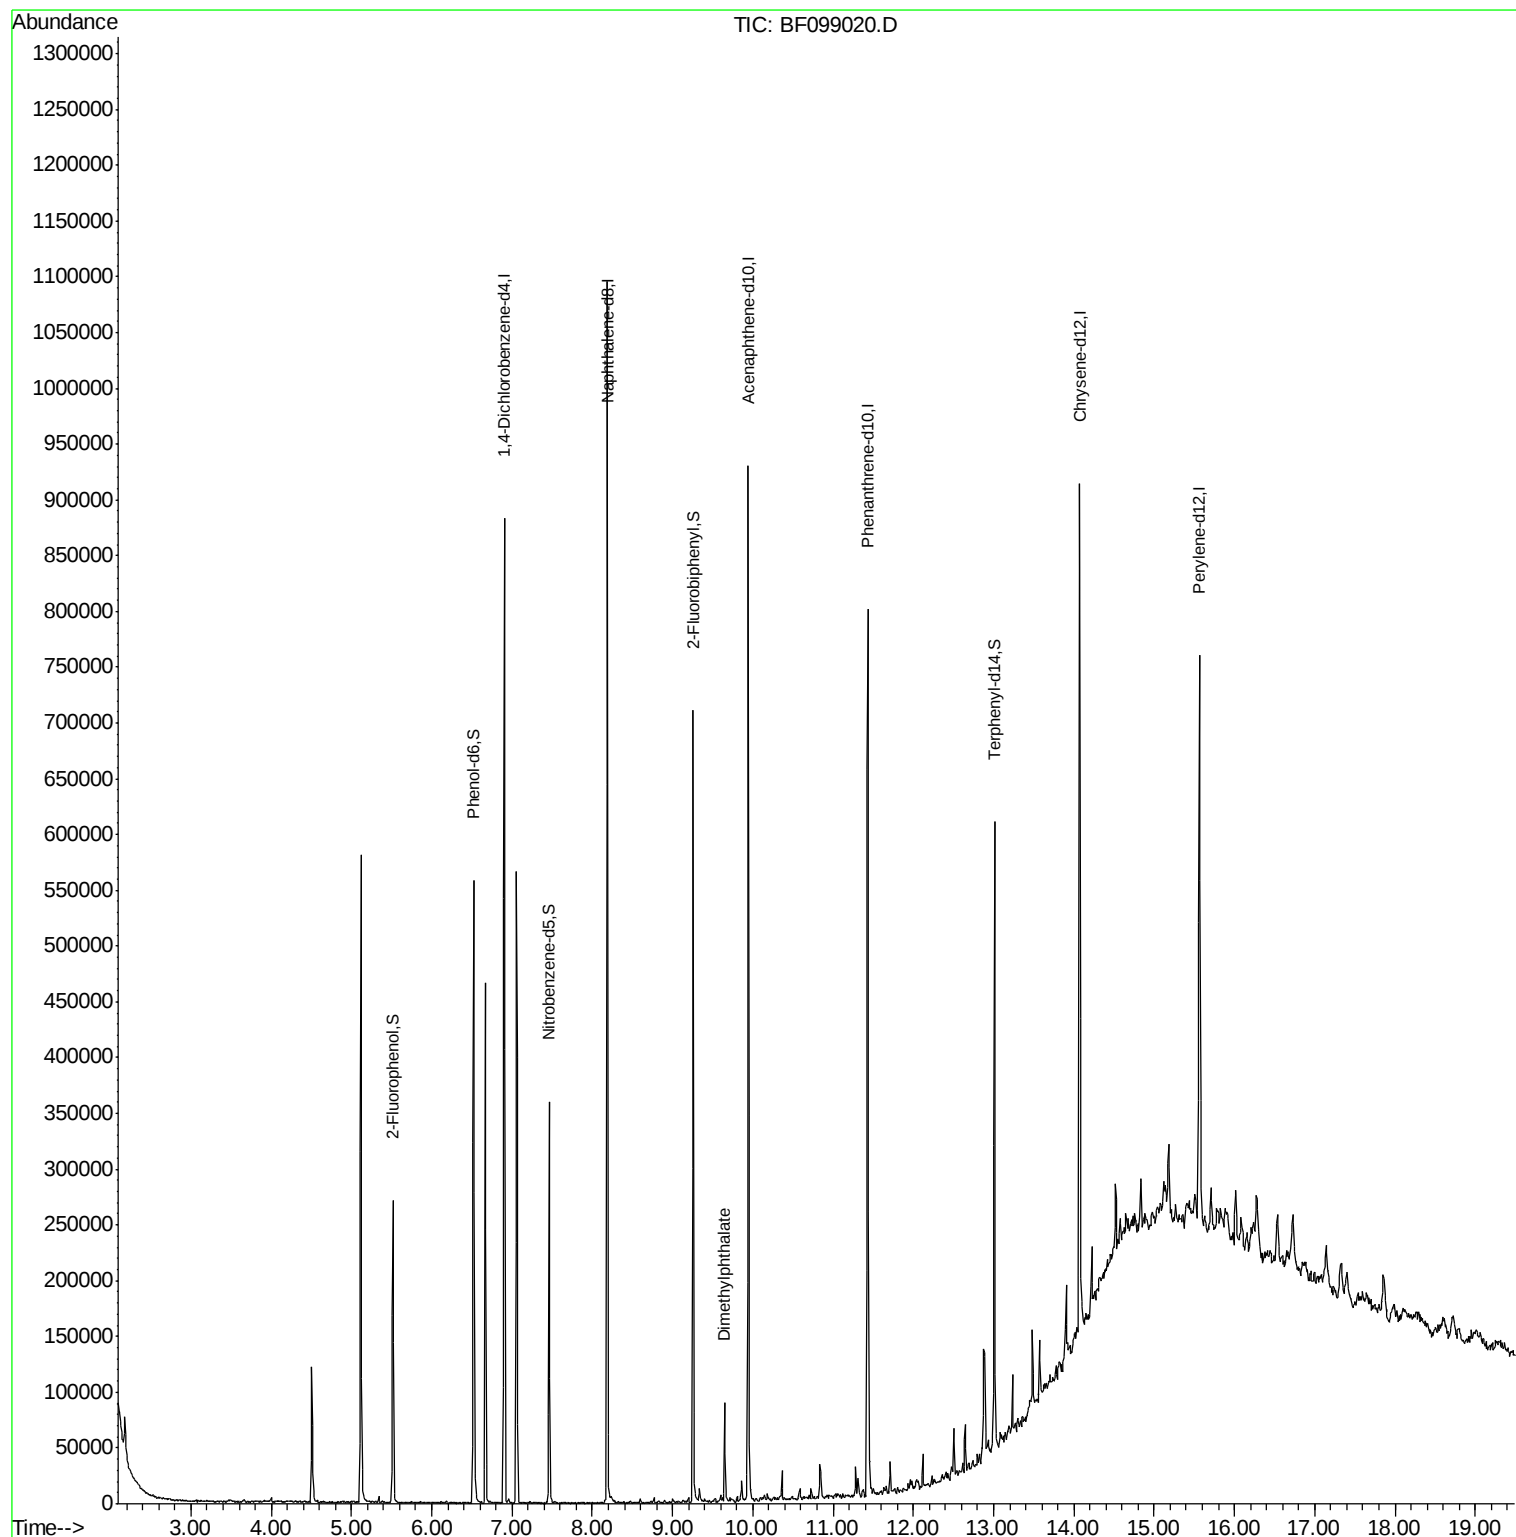

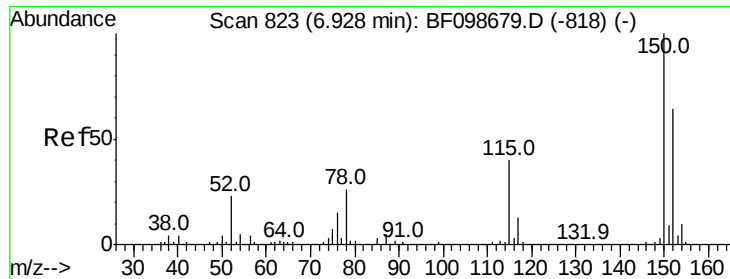


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.90 min Scan# 819
Delta R.T. -0.02 min
Lab File: BF099020.D
Acq: 3 Oct 2017 00:42

Instrument :
BNA_F
ClientSampleId :
G-62-0-2.5

Tot Ion:152 Resp: 120266
Ion Ratio Lower Upper
152 100
150 155.6 124.6 186.8
115 60.2 50.1 75.1

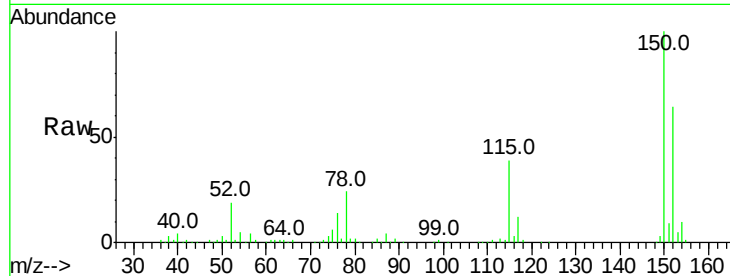


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

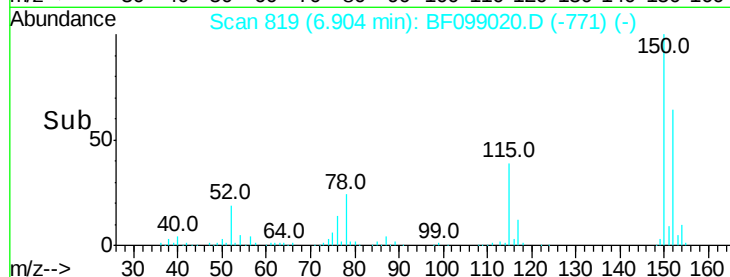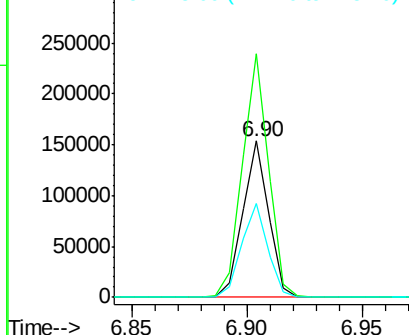



#5

2-Fluorophenol
Concen: 9.762 ng
RT: 5.52 min Scan# 583
Delta R.T. -0.02 min
Lab File: BF099020.D
Acq: 3 Oct 2017 00:42

Tgt Ion:112 Resp: 73749
Ion Ratio Lower Upper
112 100
64 56.0 47.9 71.9
63 26.7 23.7 35.5

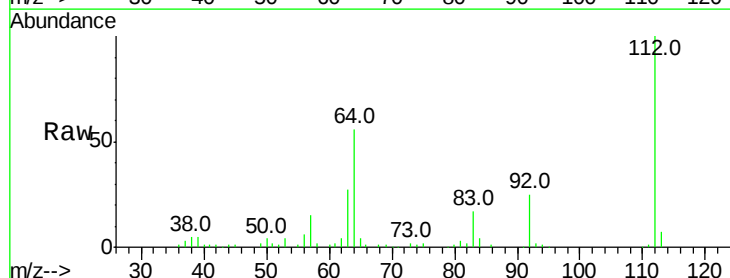

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

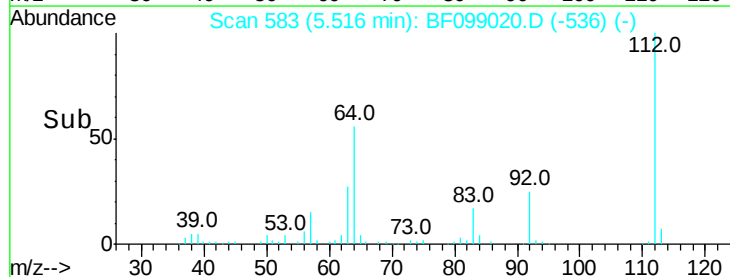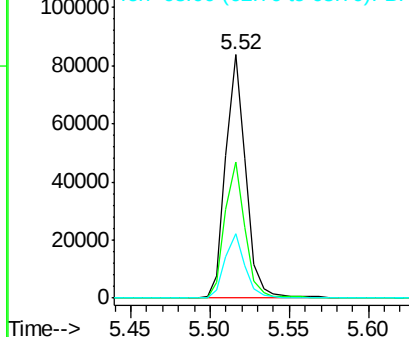



#7

Phenol-d6

Concen: 18.744 ng

RT: 6.52 min Scan# 754

Delta R.T. -0.02 min

Lab File: BF099020.D

Acq: 3 Oct 2017 00:42

Instrument :

BNA_F

ClientSampleId :

G-62-0-2.5


Tot Ion: 99 Resp: 174692

Ion Ratio Lower Upper

99 100

42 15.8 14.5 21.7




71 30.0 25.4 38.0

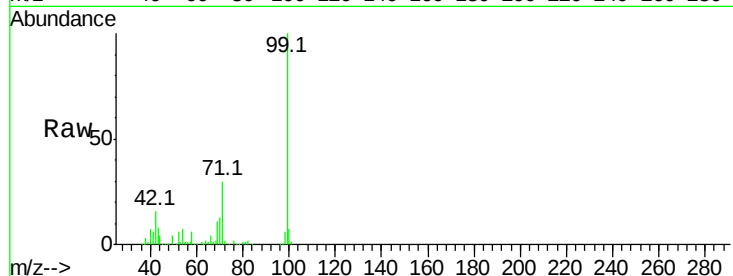

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

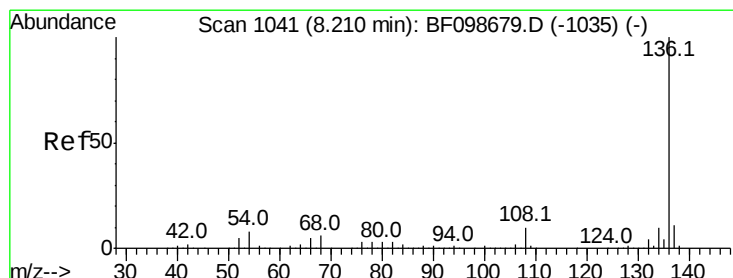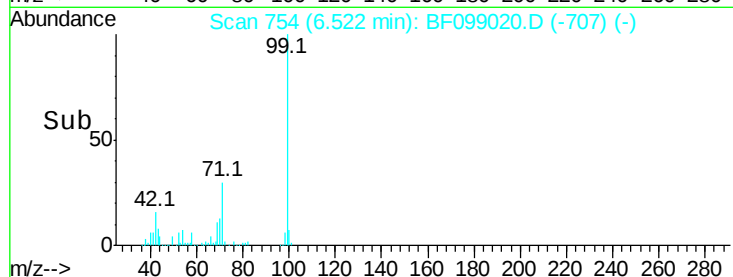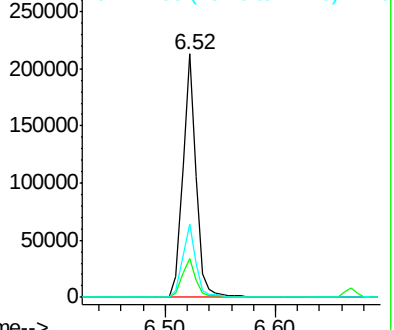

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.19 min Scan# 1037

Delta R.T. -0.02 min

Lab File: BF099020.D

Acq: 3 Oct 2017 00:42

Tgt Ion: 136 Resp: 458735


Ion Ratio Lower Upper

136 100

137 11.2 8.9 13.3

54 7.8 6.6 9.8

68 6.2 5.0 7.4


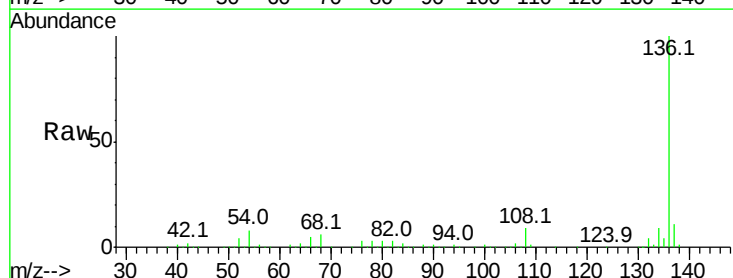


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



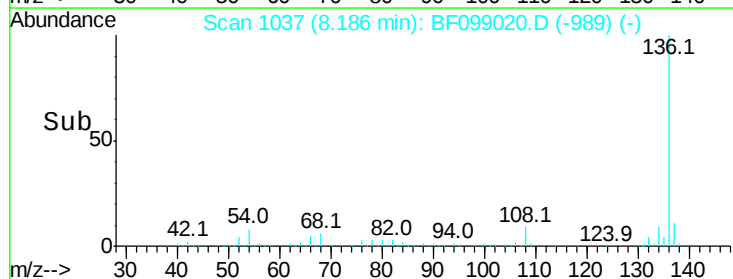
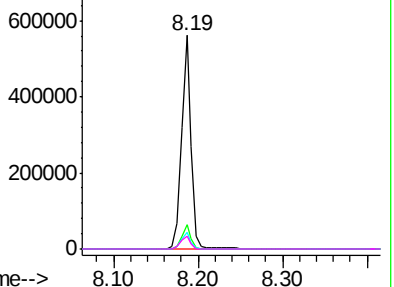




#23
 Nitrobenzene-d5
 Concen: 15.441 ng
 RT: 7.46 min Scan# 914
 Delta R.T. -0.02 min
 Lab File: BF099020.D
 Acq: 3 Oct 2017 00:42




Instrument :
 BNA_F
 ClientSampleId :
 G-62-0-2.5

Tot Ion: 82 Resp: 110455
 Ion Ratio Lower Upper
 82 100
 128 46.4 36.1 54.1
 54 47.8 41.4 62.2

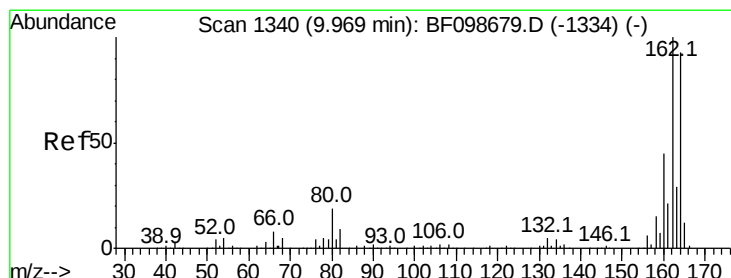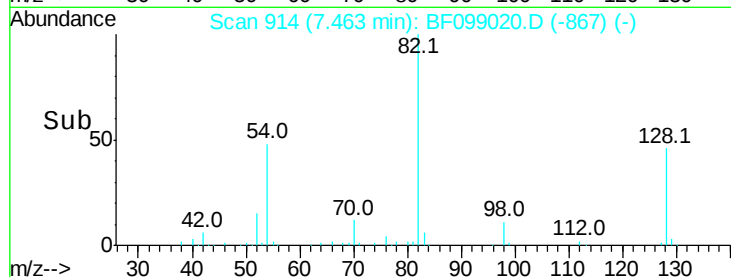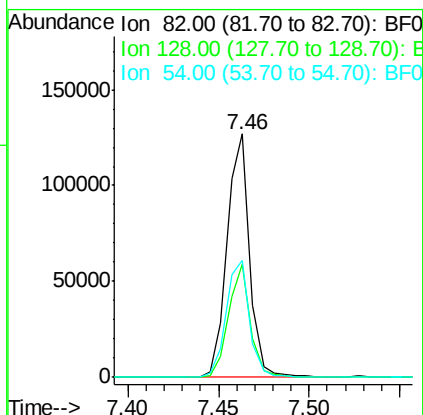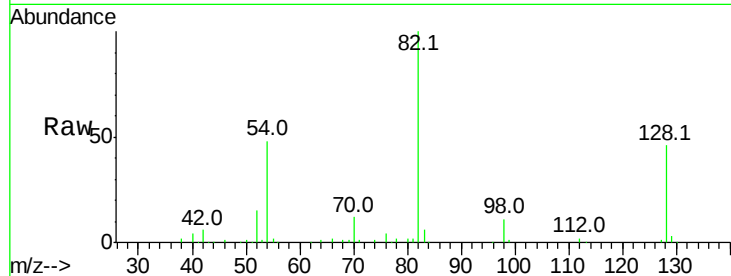

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.95 min Scan# 1336
 Delta R.T. -0.02 min
 Lab File: BF099020.D
 Acq: 3 Oct 2017 00:42

Tgt Ion:164 Resp: 174273
 Ion Ratio Lower Upper
 164 100
 162 106.0 86.1 129.1
 160 45.8 38.3 57.5

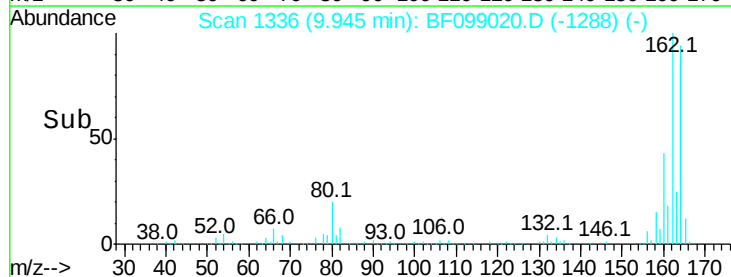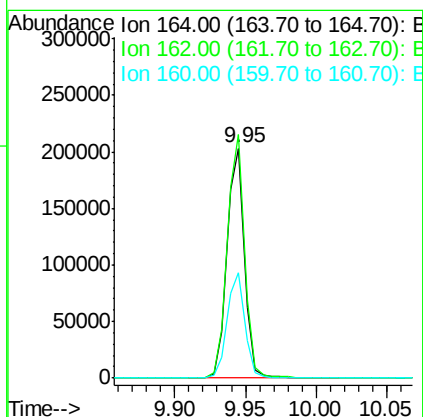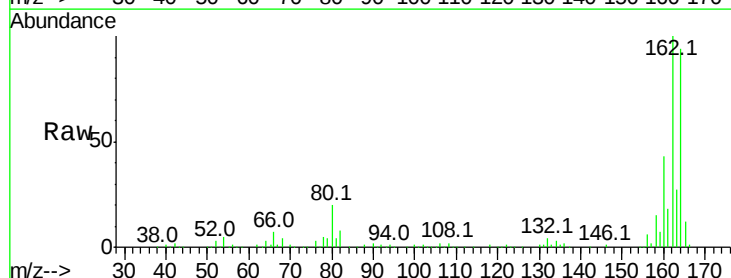







#41
 2,4,6-Tribromophenol
 Concen: 1.048 ng
 RT: 10.73 min Scan# 1470
 Delta R.T. -0.02 min
 Lab File: BF099020.D
 Acq: 3 Oct 2017 00:42

Instrument :
 BNA_F
 ClientSampleId :
 G-62-0-2.5

Tot Ion:330 Resp: 1494
 Ion Ratio Lower Upper
 330 100
 332 81.7 77.0 115.6
 141 53.3 29.9 44.9#

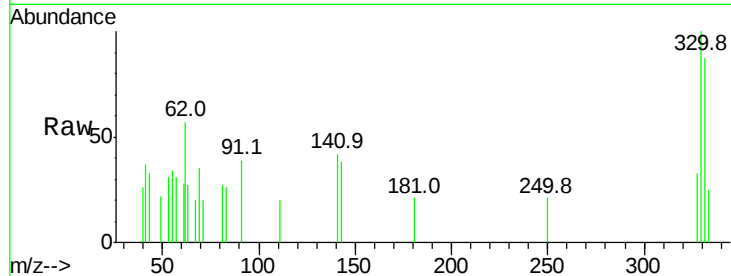


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

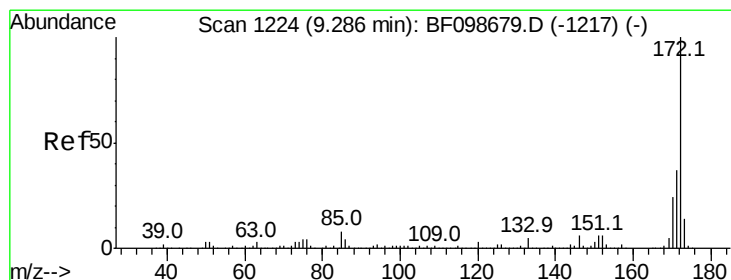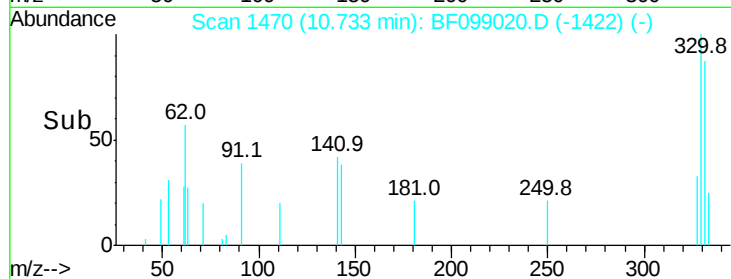
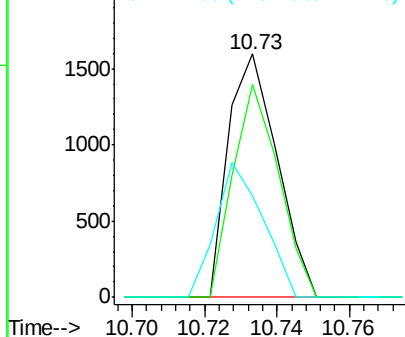



#44
 2-Fluorobiphenyl
 Concen: 20.059 ng
 RT: 9.26 min Scan# 1219
 Delta R.T. -0.02 min
 Lab File: BF099020.D
 Acq: 3 Oct 2017 00:42

Tgt Ion:172 Resp: 209401
 Ion Ratio Lower Upper
 172 100
 171 35.5 29.7 44.5
 170 23.4 19.6 29.4

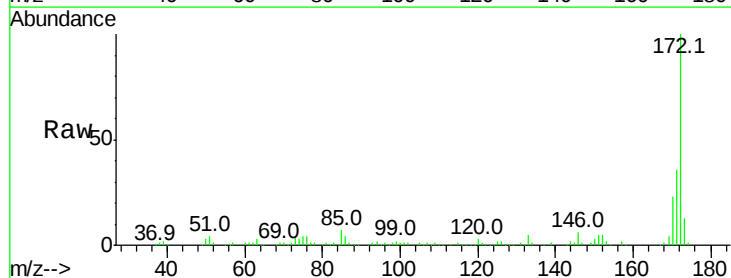

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

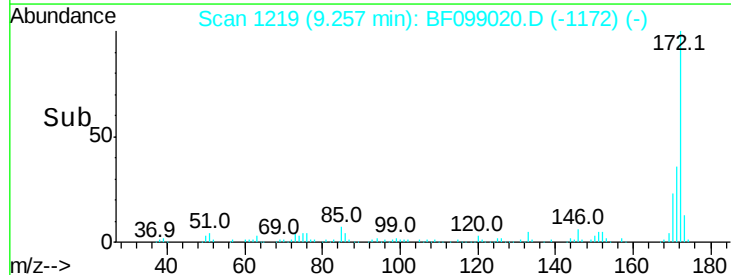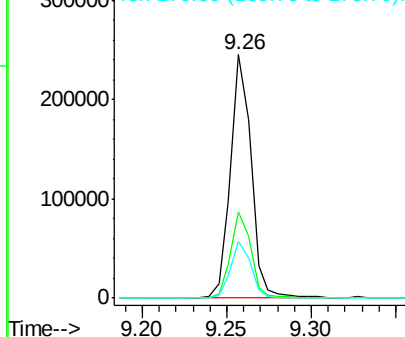

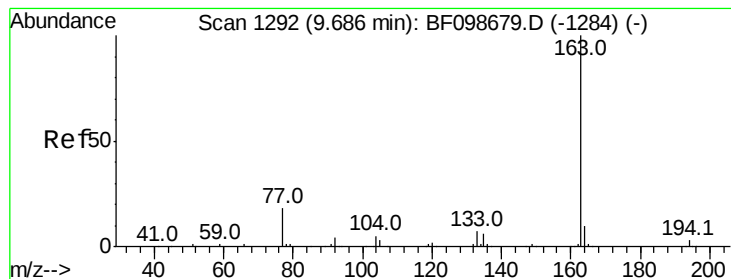

#49

Dimethylphthalate

Concen: 2.362 ng

RT: 9.65 min Scan# 1286

Delta R.T. -0.03 min

Lab File: BF099020.D

Acq: 3 Oct 2017 00:42

Instrument :

BNA_F

ClientSampleId :

G-62-0-2.5





Tot Ion:163 Resp: 31071

Ion Ratio Lower Upper

163 100

194 4.4 2.7 4.1#

164 10.1 8.2 12.2

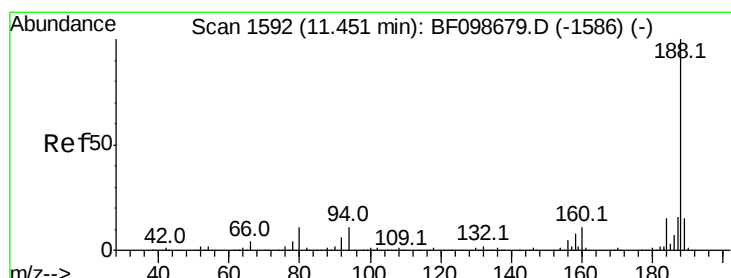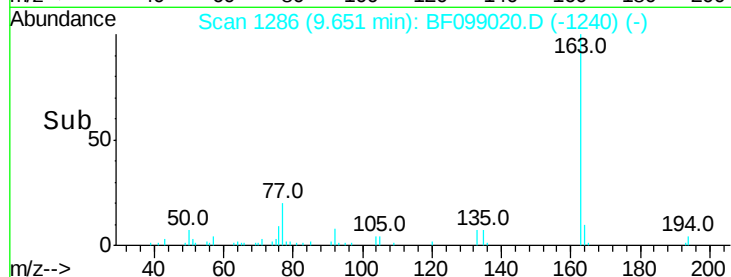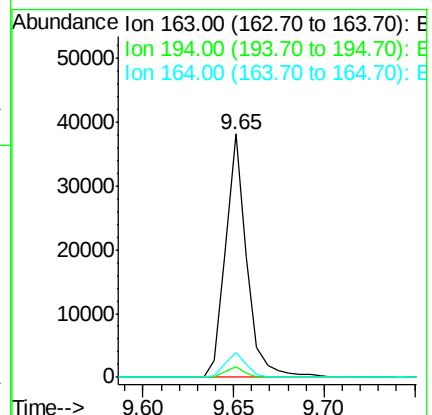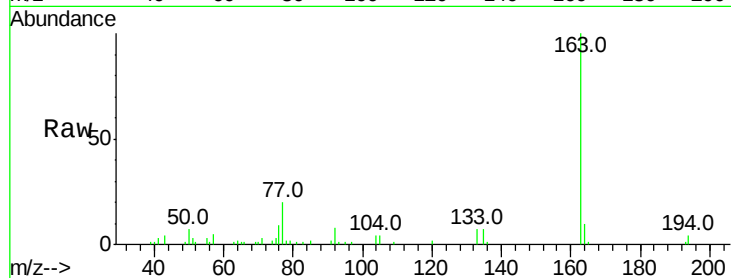

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.43 min Scan# 1589

Delta R.T. -0.01 min

Lab File: BF099020.D

Acq: 3 Oct 2017 00:42




Tgt Ion:188 Resp: 268566


Ion Ratio Lower Upper

188 100

94 10.5 8.5 12.7

80 10.4 9.2 13.8

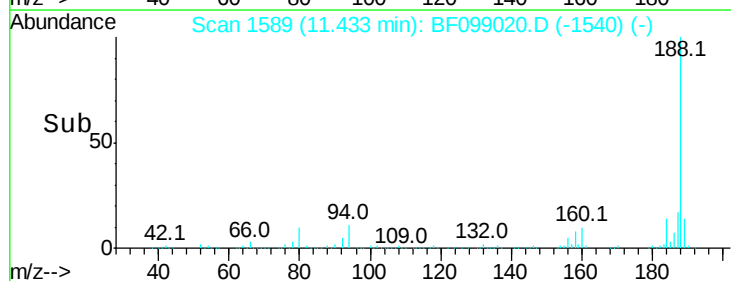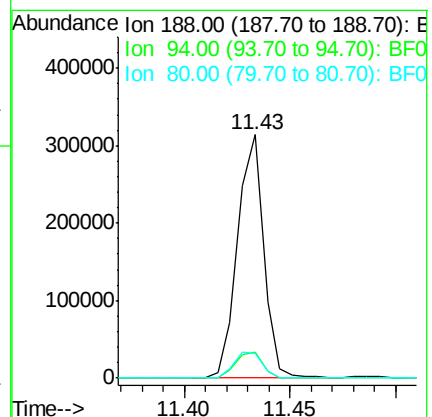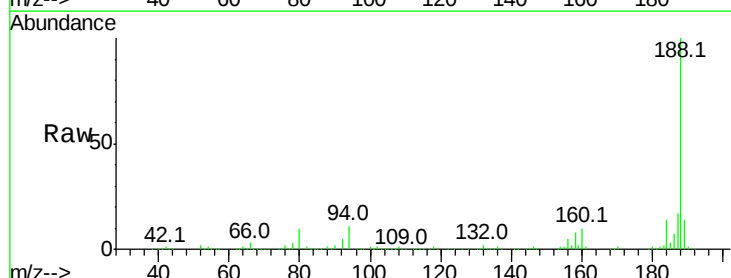

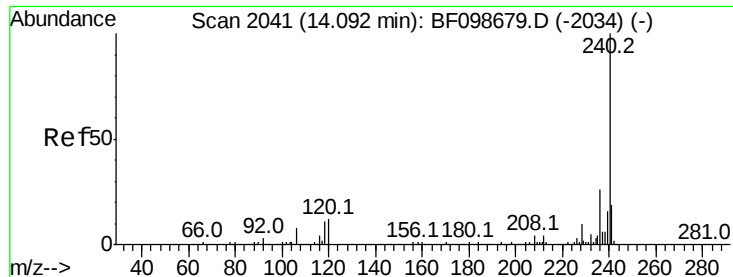

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.07 min Scan# 2038

Delta R.T. -0.01 min

Lab File: BF099020.D

Acq: 3 Oct 2017 00:42

Instrument :

BNA_F

ClientSampleId :

G-62-0-2.5


Tot Ion:240 Resp: 251088

Ion Ratio Lower Upper

240 100

120 13.0 9.5 14.3




236 26.1 20.7 31.1

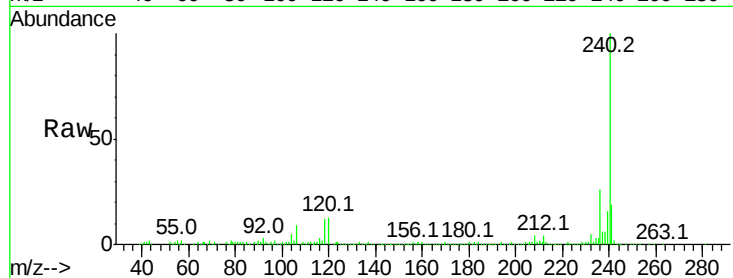

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

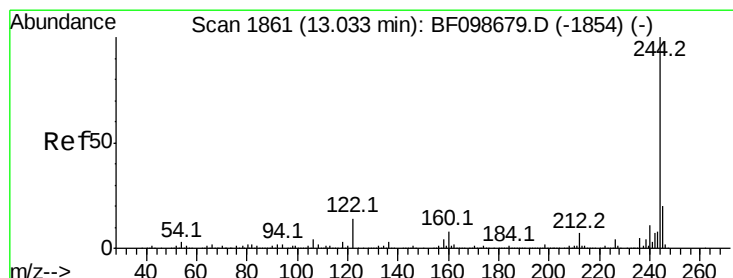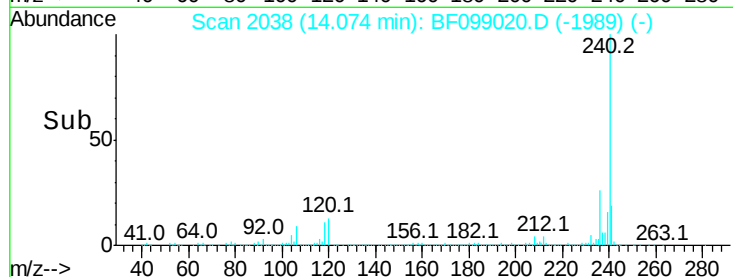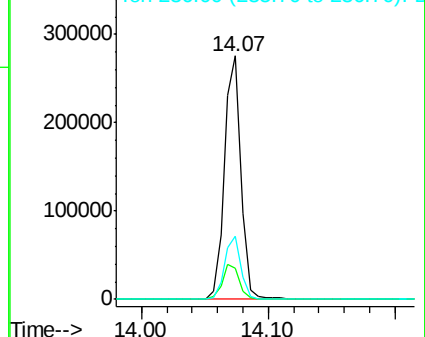

#78

Terphenyl-d14

Concen: 13.514 ng

RT: 13.01 min Scan# 1857

Delta R.T. -0.02 min

Lab File: BF099020.D

Acq: 3 Oct 2017 00:42


Tgt Ion:244 Resp: 149207

Ion Ratio Lower Upper

244 100

212 7.7 5.4 8.0



122 15.1 11.0 16.4

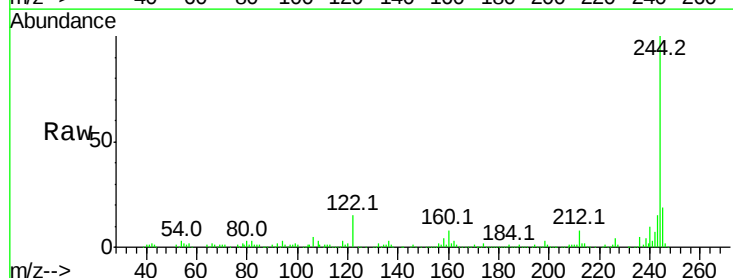


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

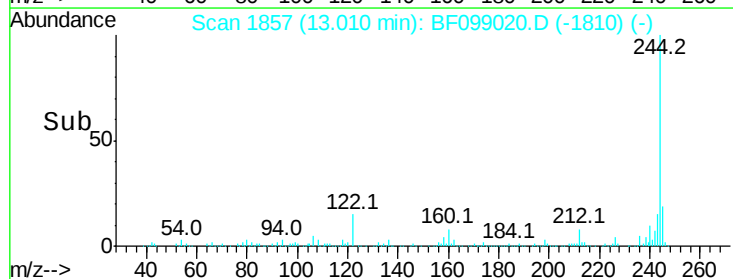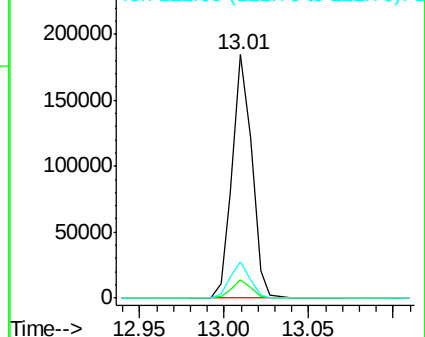


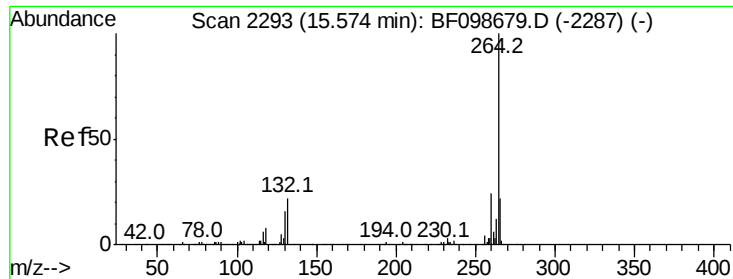

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.57 min Scan# 2292
Delta R.T. -0.01 min
Lab File: BF099020.D
Acq: 3 Oct 2017 00:42

Instrument :
BNA_F
ClientSampleId :
G-62-0-2.5

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.3	19.2	28.8
265	21.4	17.5	26.3

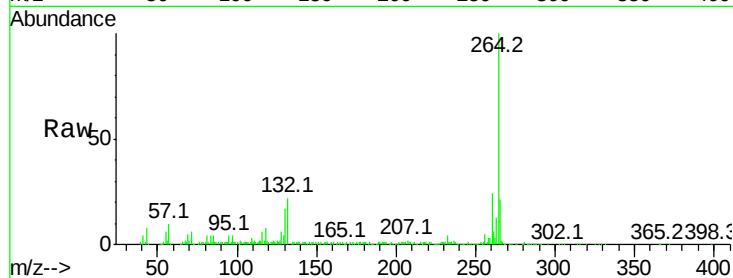

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

