


Data Path : Z:\HPCHEM1\BNA F\Data\BF100217\
 Data File : BF098997.D
 Acq On : 2 Oct 2017 14:02
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 23 13:50:58 2017

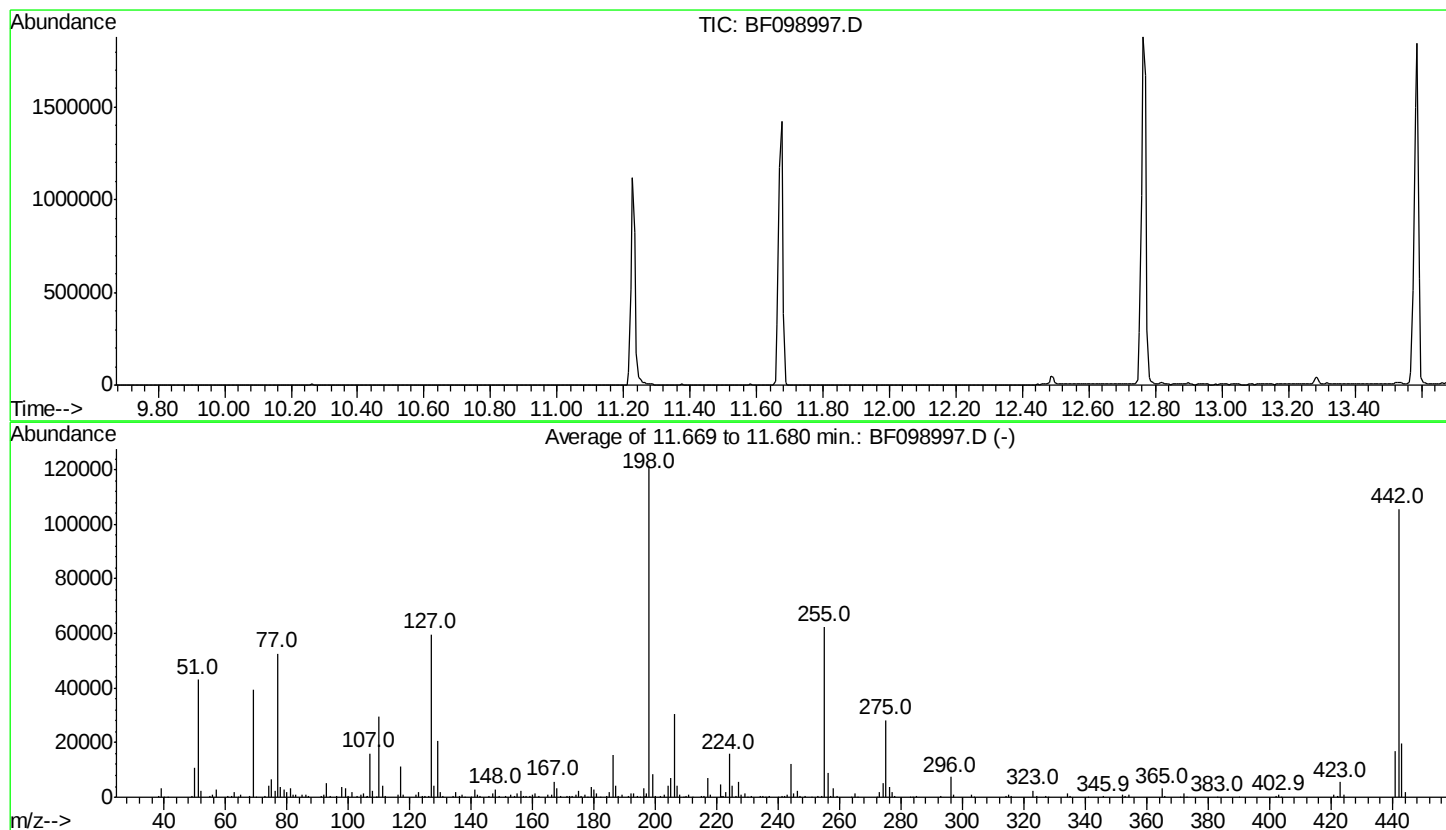

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	43059	PASS
68	69	0.00	2	1.7	684	PASS
69	198	0.00	100	32.6	39556	PASS
70	69	0.00	2	0.6	242	PASS
127	198	10	80	49.2	59733	PASS
197	198	0.00	2	1.1	1289	PASS
198	198	100	100	100.0	121464	PASS
199	198	5	9	7.0	8500	PASS
275	198	10	60	23.2	28219	PASS
365	198	1	100	2.7	3278	PASS
441	442	0.01	24	15.9	16811	PASS
442	198	50	100	87.0	105637	PASS
443	442	15	24	18.5	19549	PASS