

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF100218\  
 Data File : BF109507.D  
 Acq On : 2 Oct 2018 17:48  
 Operator : JU/SJ  
 Sample : J5186-05  
 Misc :  
 ALS Vial : 16 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 092718-SIDI-F-U-M

Quant Time: Oct 03 03:08:00 2018  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF092218.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Sat Sep 22 13:32:18 2018  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|---------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 6.70  | 152  | 101387   | 20.00 | ng    | 0.00     |
| 21) Naphthalene-d8        | 7.99  | 136  | 384029   | 20.00 | ng    | 0.00     |
| 38) Acenaphthene-d10      | 9.73  | 164  | 179455   | 20.00 | ng    | 0.00     |
| 63) Phenanthrene-d10      | 11.21 | 188  | 315039   | 20.00 | ng    | 0.00     |
| 75) Chrysene-d12          | 13.84 | 240  | 252817   | 20.00 | ng    | 0.00     |
| 86) Perylene-d12          | 15.24 | 264  | 254600   | 20.00 | ng    | 0.00     |

| System Monitoring Compounds | R.T.  | QIon | Response | Conc   | Units | Dev(Min) |
|-----------------------------|-------|------|----------|--------|-------|----------|
| 5) 2-Fluorophenol           | 5.32  | 112  | 248793   | 40.42  | ng    | 0.00     |
| 7) Phenol-d6                | 6.35  | 99   | 191930   | 24.43  | ng    | -0.01    |
| 23) Nitrobenzene-d5         | 7.27  | 82   | 664321   | 102.12 | ng    | -0.01    |
| 41) 2,4,6-Tribromophenol    | 10.52 | 330  | 165861   | 93.76  | ng    | -0.01    |
| 44) 2-Fluorobiphenyl        | 9.06  | 172  | 1159426  | 97.44  | ng    | -0.01    |
| 78) Terphenyl-d14           | 12.79 | 244  | 1026431  | 99.64  | ng    | -0.01    |


| Target Compounds               | R.T.  | QIon | Response | Conc   | Units | Qvalue |
|--------------------------------|-------|------|----------|--------|-------|--------|
| 9) Benzaldehyde                | 6.47  | 77   | 10872    | 2.155  | ng    | # 76   |
| 19) n-Nitroso-di-n-propylamine | 7.27  | 70   | 89190    | 17.329 | ng    | # 77   |
| 25) Isophorone                 | 7.27  | 82   | 636805   | 54.360 | ng    | # 64   |
| 49) Dimethylphthalate          | 9.45  | 163  | 77595    | 5.945  | ng    | # 98   |
| 50) 2,6-Dinitrotoluene         | 9.73  | 165  | 22410    | 8.669  | ng    | # 25   |
| 56) 2,4-Dinitrotoluene         | 9.73  | 165  | 22410    | 6.851  | ng    | # 23   |
| 64) 4,6-Dinitro-2-methylphenol | 10.52 | 198  | 272      | 6.706  | ng    | # 1    |
| 66) 4-Bromophenyl-phenylether  | 10.52 | 248  | 10017    | 2.863  | ng    | # 1    |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF100218\  
Data File : BF109507.D  
Acq On : 2 Oct 2018 17:48  
Operator : JU/SJ  
Sample : J5186-05  
Misc :  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
092718-SIDI-F-U-M

Quant Time: Oct 03 03:08:00 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF092218.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Sep 22 13:32:18 2018  
Response via : Initial Calibration

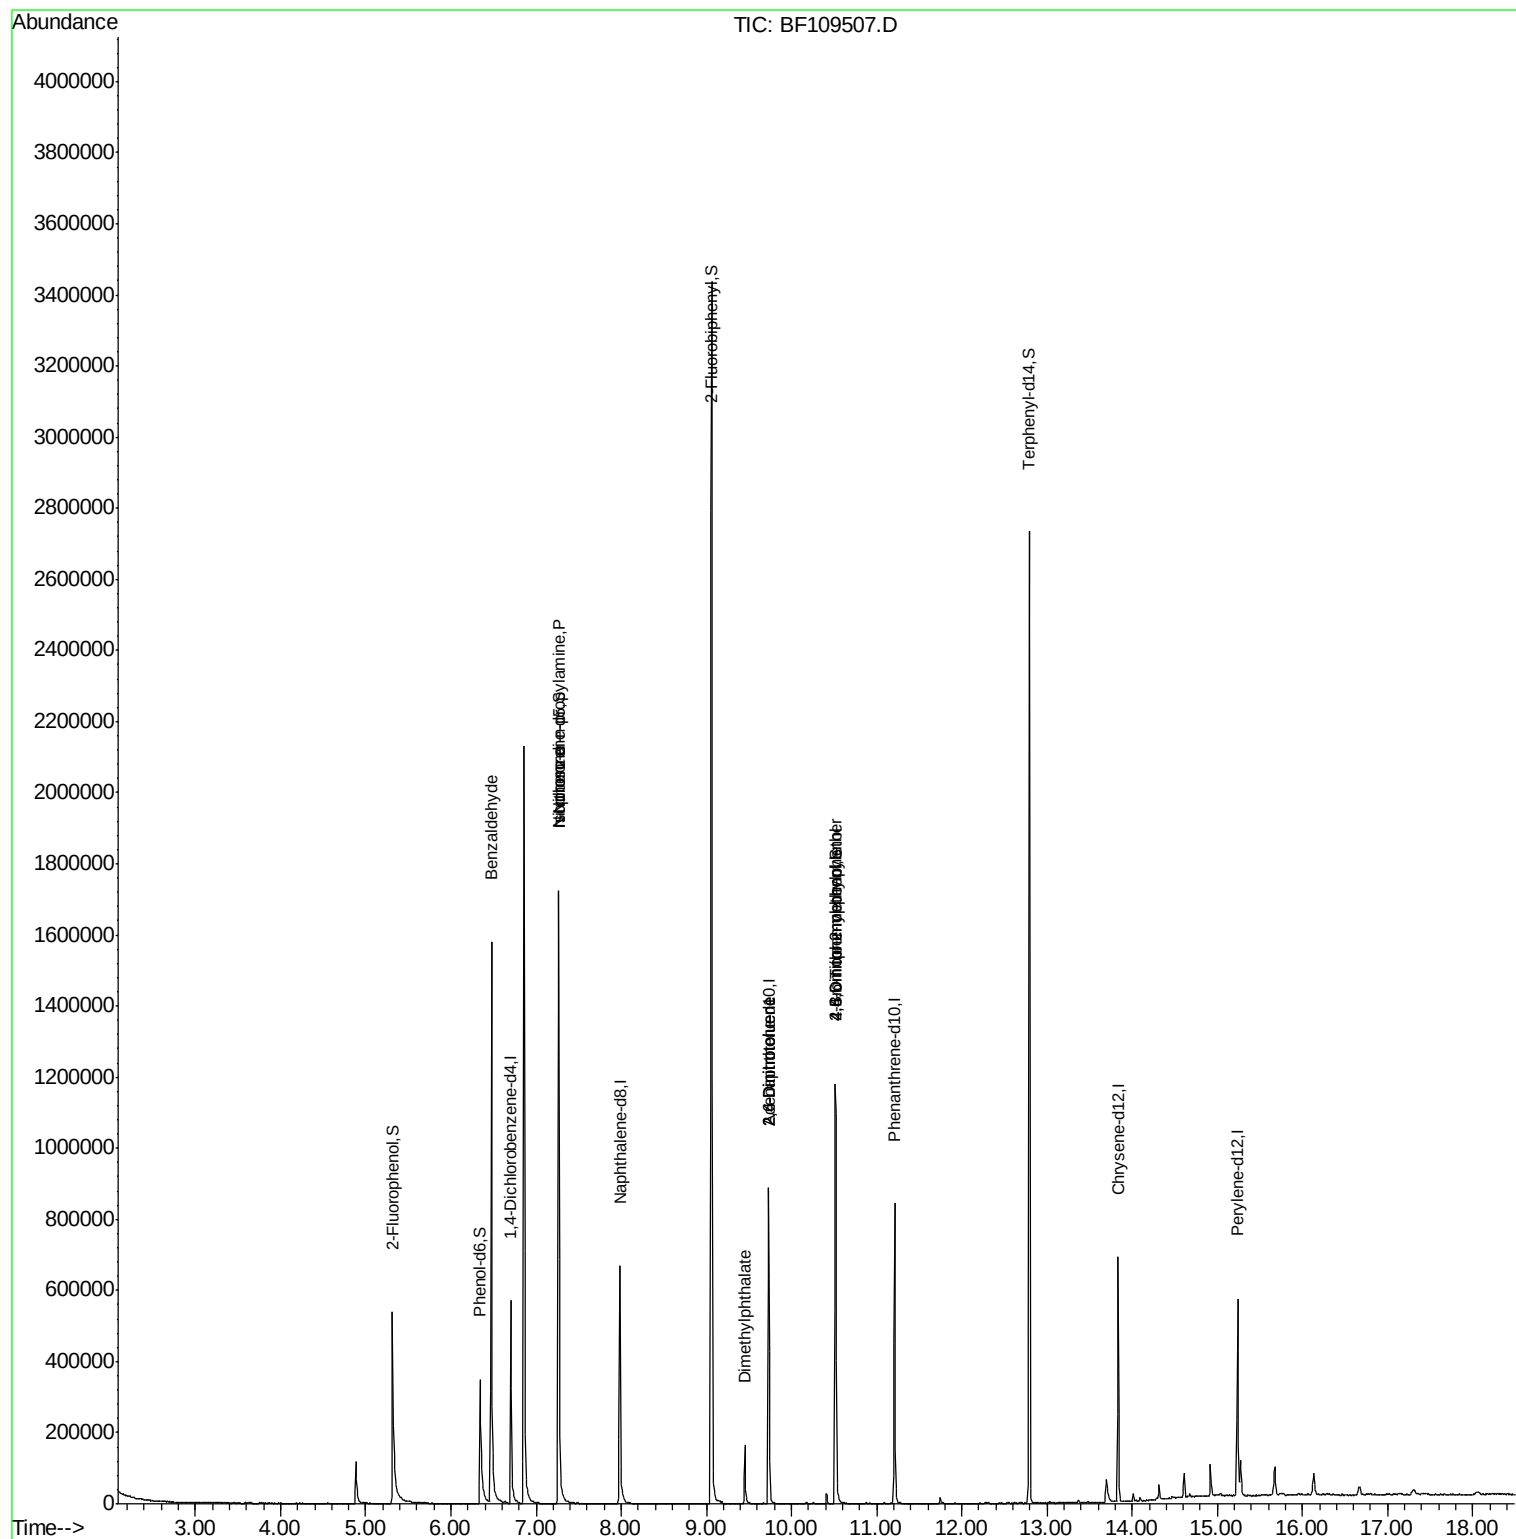


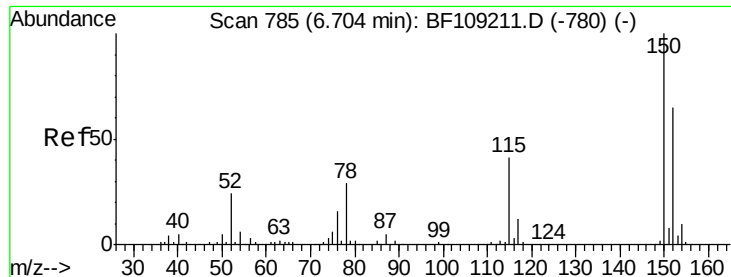




#1  
 1,4-Dichlorobenzene-d4  
 Concen: 20.000 ng  
 RT: 6.70 min Scan# 785  
 Delta R.T. -0.01 min  
 Lab File: BF109507.D  
 Acq: 2 Oct 2018 17:48

Instrument :  
 BNA\_F  
 ClientSampleId :  
 092718-SIDI-F-U-M

Tgt Ion:152 Resp: 101387  
 Ion Ratio Lower Upper  
 152 100  
 150 158.4 124.6 186.8  
 115 60.4 50.1 75.1

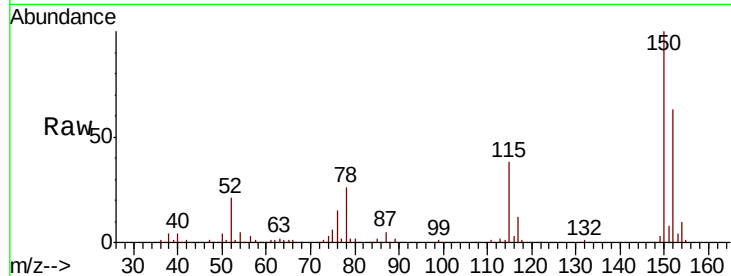


Abundance Ion 152.00 (151.70 to 152.70): E  
 Ion 150.00 (149.70 to 150.70): E  
 Ion 115.00 (114.70 to 115.70): E

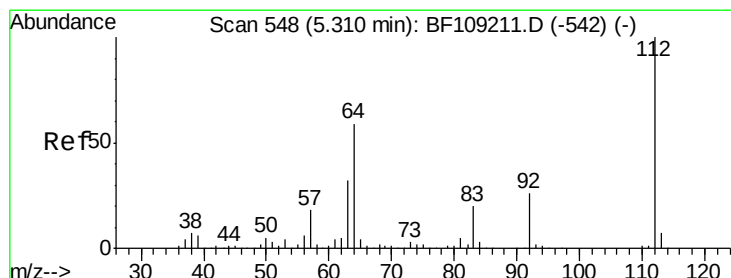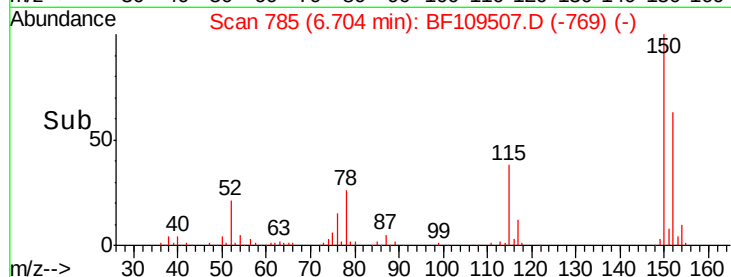
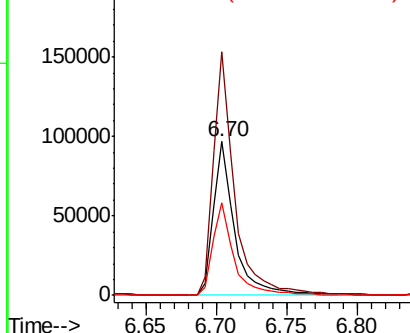



#5  
 2-Fluorophenol  
 Concen: 40.418 ng  
 RT: 5.32 min Scan# 549  
 Delta R.T. -0.00 min  
 Lab File: BF109507.D  
 Acq: 2 Oct 2018 17:48

Tgt Ion:112 Resp: 248793  
 Ion Ratio Lower Upper  
 112 100  
 64 56.9 47.9 71.9  
 63 29.2 23.7 35.5

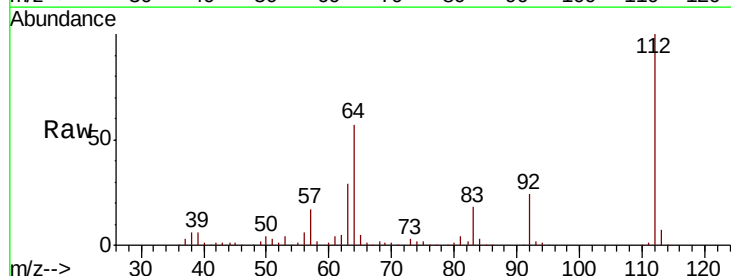

Abundance Ion 112.00 (111.70 to 112.70): E  
 Ion 64.00 (63.70 to 64.70): BF1  
 Ion 63.00 (62.70 to 63.70): BF1

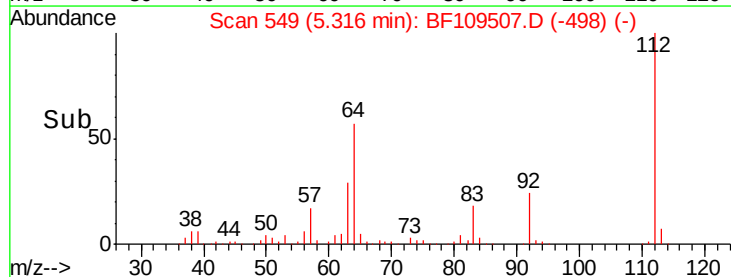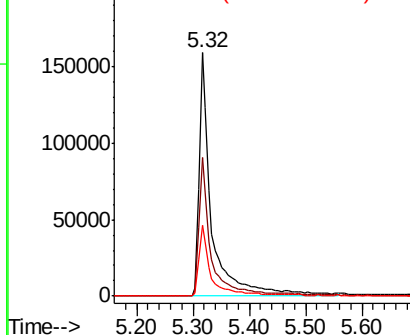

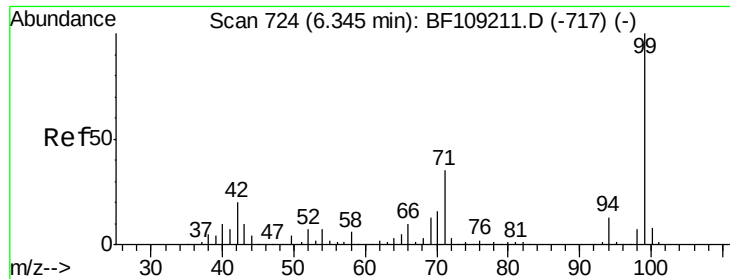

#7

Phenol-d6

Concen: 24.435 ng

RT: 6.35 min Scan# 724

Delta R.T. -0.01 min

Lab File: BF109507.D

Acq: 2 Oct 2018 17:48

Instrument :

BNA\_F

ClientSampleId :

092718-SIDI-F-U-M


Tgt Ion: 99 Resp: 191930

Ion Ratio Lower Upper




99 100

42 17.2 14.5 21.7

71 33.2 25.4 38.0

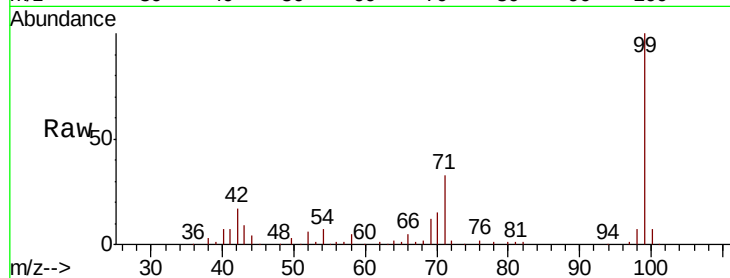

Abundance Ion 99.00 (98.70 to 99.70): BF1  
Ion 42.00 (41.70 to 42.70): BF1  
Ion 71.00 (70.70 to 71.70): BF1

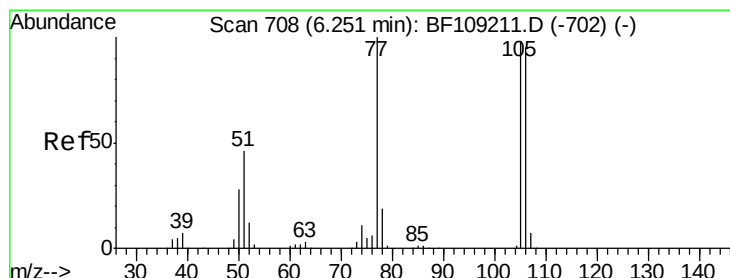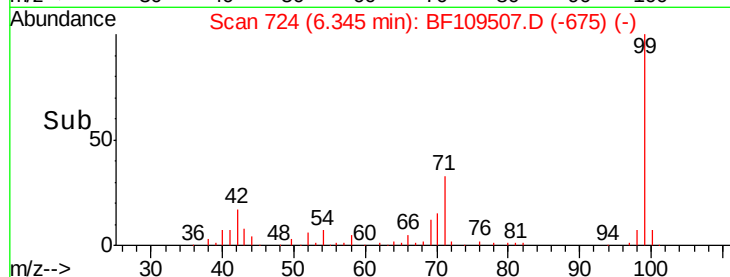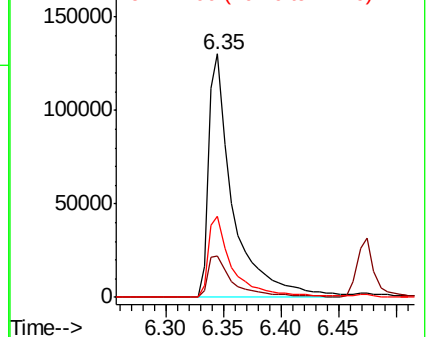

#9

Benzaldehyde

Concen: 2.155 ng

RT: 6.47 min Scan# 746

Delta R.T. 0.22 min

Lab File: BF109507.D

Acq: 2 Oct 2018 17:48


Tgt Ion: 77 Resp: 10872

Ion Ratio Lower Upper



77 100


105 81.4 81.1 121.1

106 66.7 74.5 114.5#

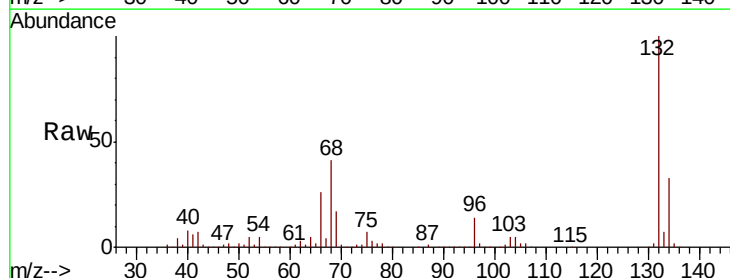

Abundance Ion 77.00 (76.70 to 77.70): BF1  
Ion 105.00 (104.70 to 105.70): E  
Ion 106.00 (105.70 to 106.70): E



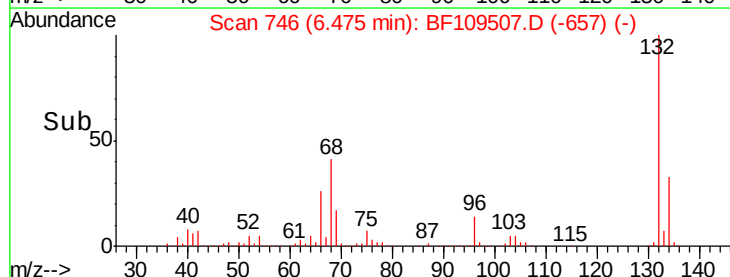
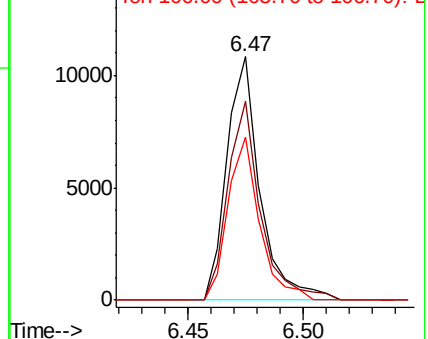


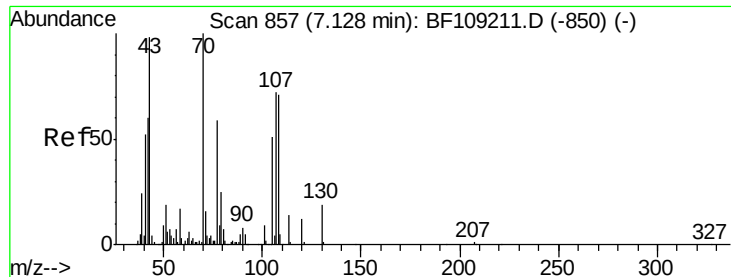

#19  
n-Nitroso-di-n-propylamine  
Concen: 17.329 ng  
RT: 7.27 min Scan# 881  
Delta R.T. 0.12 min  
Lab File: BF109507.D  
Acq: 2 Oct 2018 17:48




Instrument :  
BNA\_F  
ClientSampleId :  
092718-SIDI-F-U-M


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 70    | Resp: | 89190 |
| Ion      | Ratio | Lower | Upper |
| 70       | 100   |       |       |
| 42       | 47.1  | 47.5  | 71.3# |
| 101      | 0.0   | 7.4   | 11.2# |
| 130      | 2.0   | 16.6  | 25.0# |

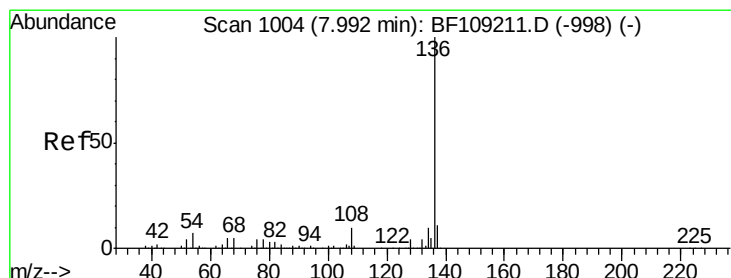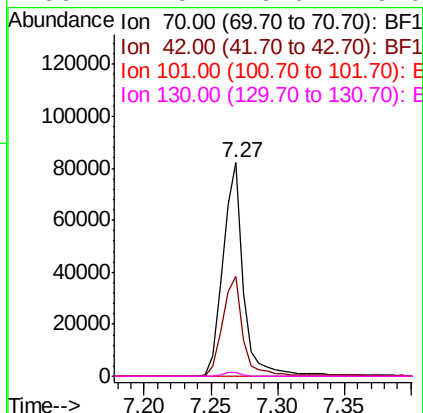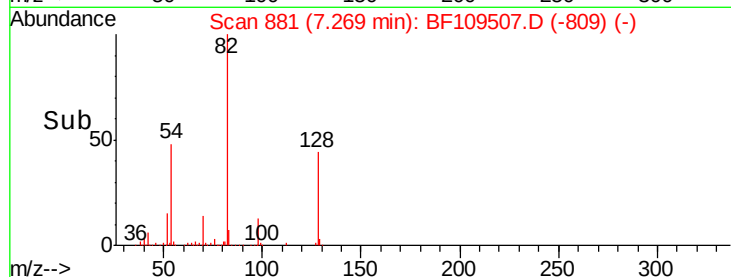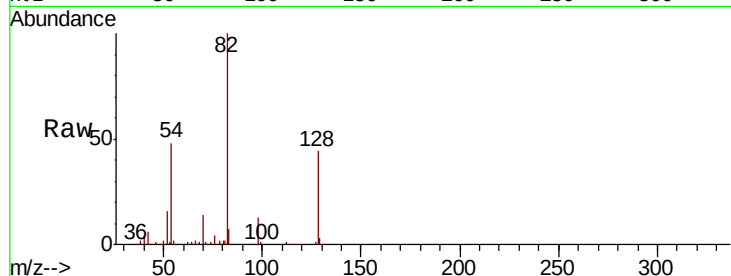

#21  
Naphthalene-d8  
Concen: 20.000 ng  
RT: 7.99 min Scan# 1003  
Delta R.T. -0.01 min  
Lab File: BF109507.D  
Acq: 2 Oct 2018 17:48

|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 136   | Resp: | 384029 |
| Ion      | Ratio | Lower | Upper  |
| 136      | 100   |       |        |
| 137      | 10.4  | 8.9   | 13.3   |
| 54       | 6.2   | 6.6   | 9.8#   |
| 68       | 5.3   | 5.0   | 7.4    |

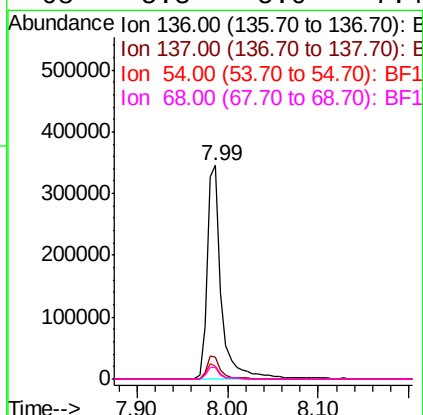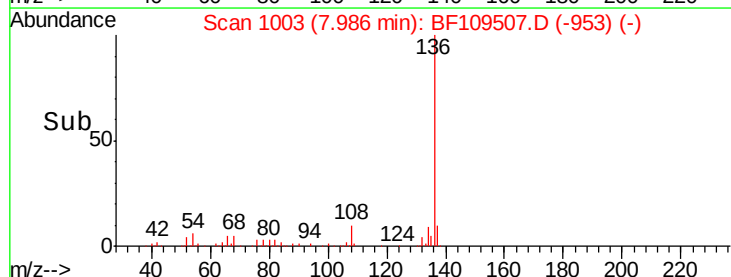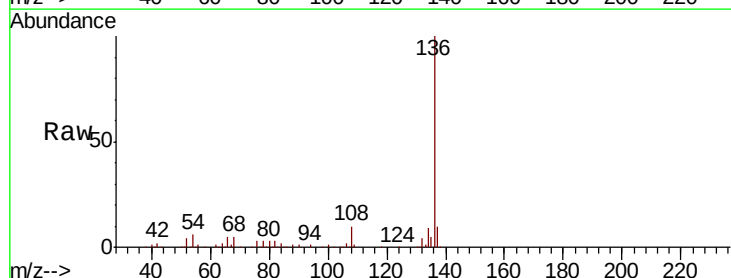


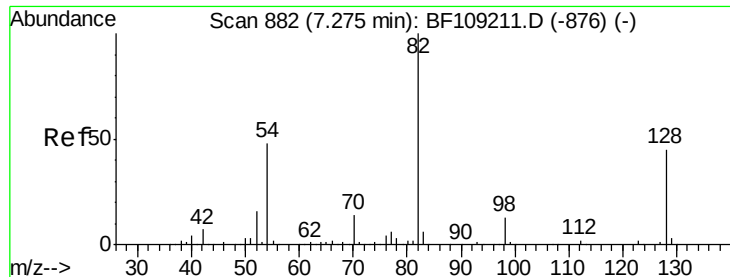




#23  
Nitrobenzene-d5  
Concen: 102.117 ng  
RT: 7.27 min Scan# 881  
Delta R.T. -0.01 min  
Lab File: BF109507.D  
Acq: 2 Oct 2018 17:48

Instrument :  
BNA\_F  
ClientSampleId :  
092718-SIDI-F-U-M

Tgt Ion: 82 Resp: 664321  
Ion Ratio Lower Upper  
82 100  
128 44.4 36.1 54.1  
54 48.0 41.4 62.2

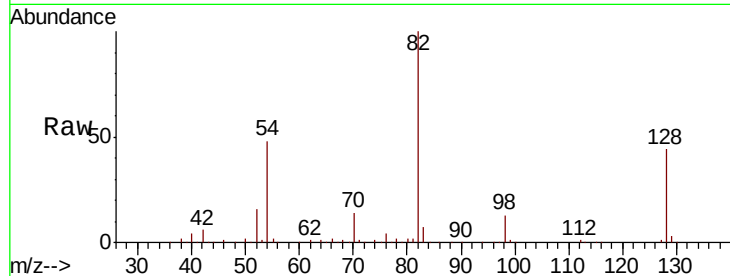


Abundance Ion 82.00 (81.70 to 82.70): BF1  
800000 Ion 128.00 (127.70 to 128.70): BF1  
Ion 54.00 (53.70 to 54.70): BF1

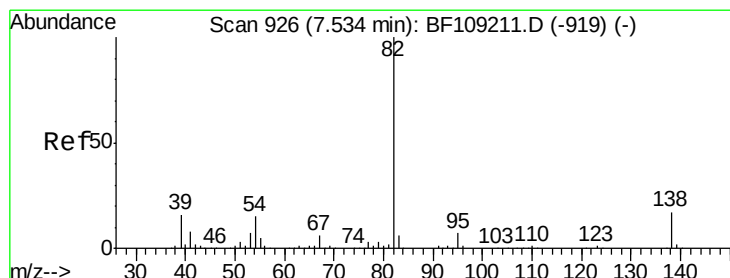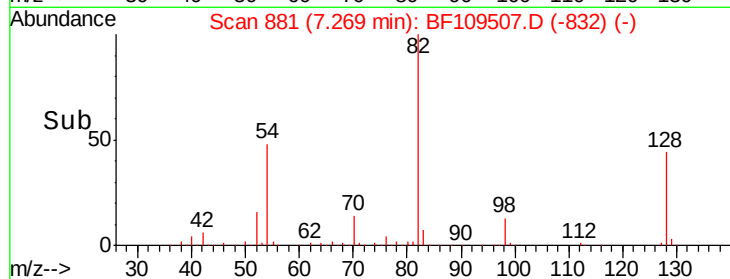
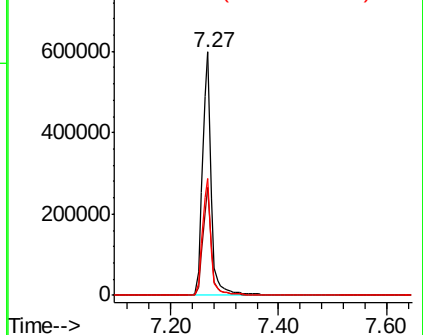



#25  
Isophorone  
Concen: 54.360 ng  
RT: 7.27 min Scan# 881  
Delta R.T. -0.28 min  
Lab File: BF109507.D  
Acq: 2 Oct 2018 17:48

Tgt Ion: 82 Resp: 636805  
Ion Ratio Lower Upper  
82 100  
95 0.0 5.2 7.8#  
138 0.0 14.9 22.3#

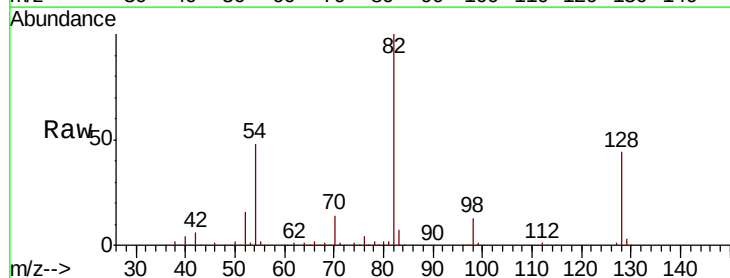

Abundance Ion 82.00 (81.70 to 82.70): BF1  
800000 Ion 95.00 (94.70 to 95.70): BF1  
Ion 138.00 (137.70 to 138.70): BF1



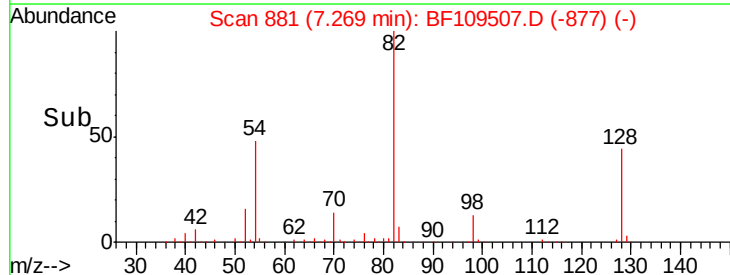
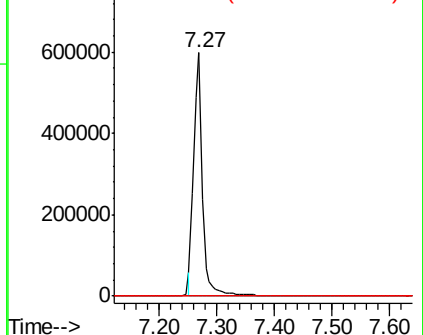


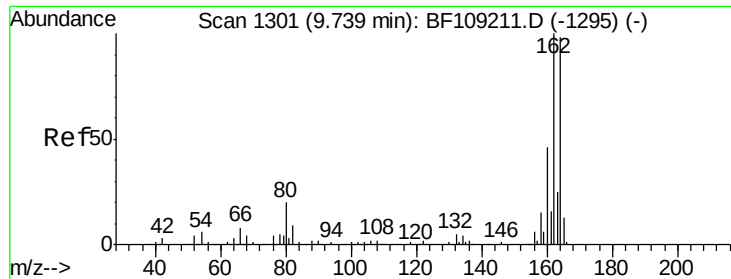

#38  
 Acenaphthene-d10  
 Concen: 20.000 ng  
 RT: 9.73 min Scan# 1300  
 Delta R.T. -0.01 min  
 Lab File: BF109507.D  
 Acq: 2 Oct 2018 17:48




Instrument :  
 BNA\_F  
 ClientSampleId :  
 092718-SIDI-F-U-M


| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 164     | 100   |       |       |
| 162     | 102.3 | 86.1  | 129.1 |
| 160     | 48.1  | 38.3  | 57.5  |

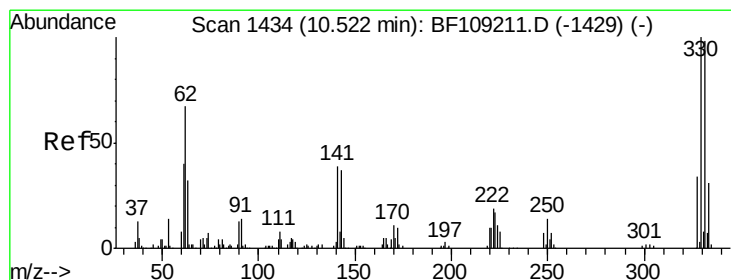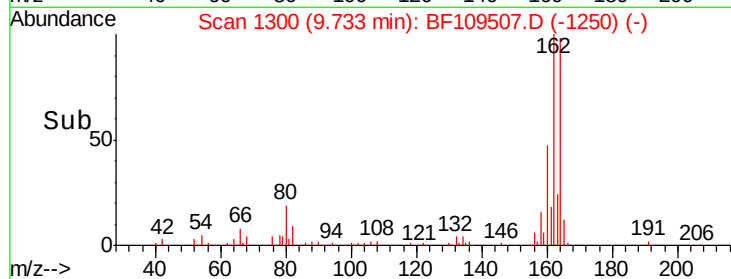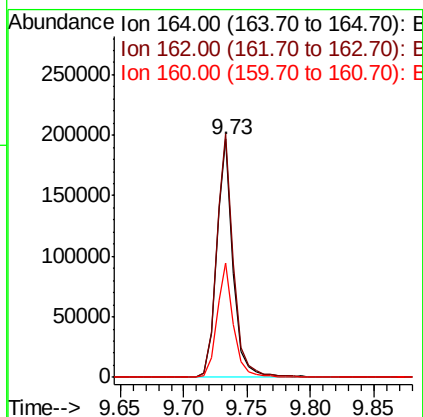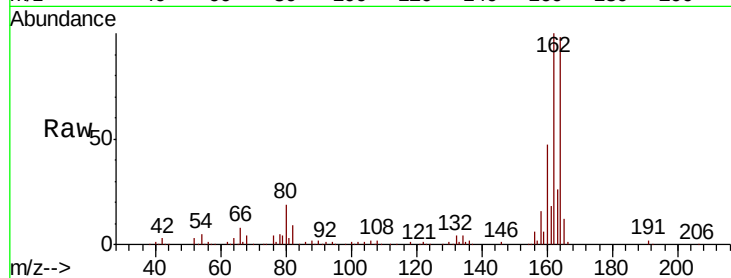

#41  
 2,4,6-Tribromophenol  
 Concen: 93.757 ng  
 RT: 10.52 min Scan# 1434  
 Delta R.T. -0.01 min  
 Lab File: BF109507.D  
 Acq: 2 Oct 2018 17:48

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 330     | 100   |       |       |
| 332     | 95.7  | 77.0  | 115.6 |
| 141     | 33.3  | 29.9  | 44.9  |


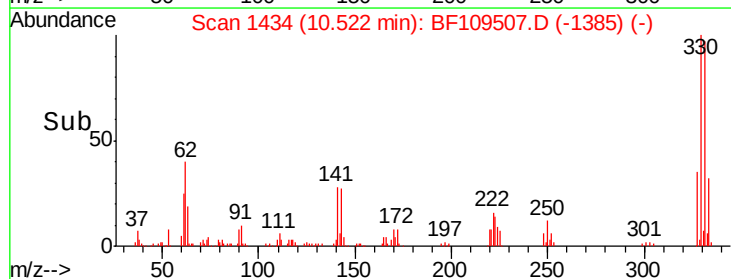
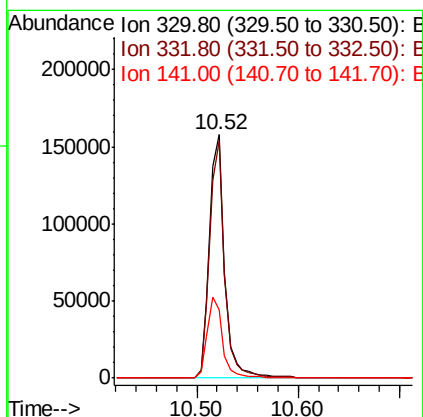
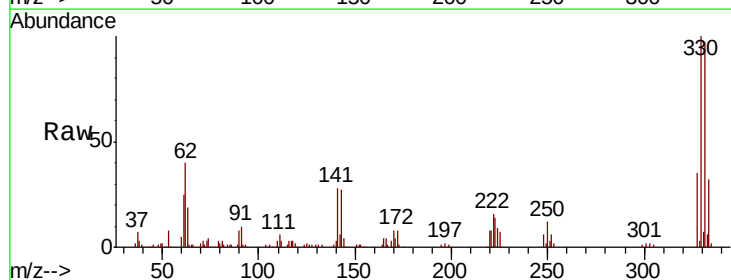


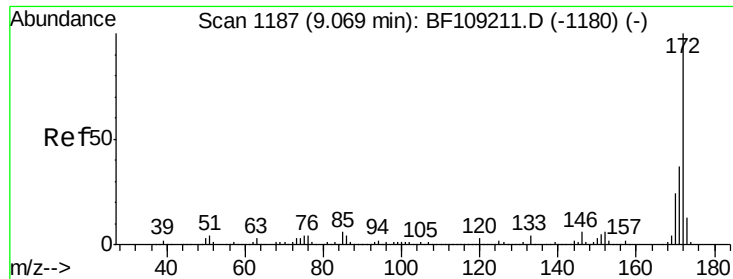

#44  
2-Fluorobiphenyl  
Concen: 97.442 ng  
RT: 9.06 min Scan# 1186  
Delta R.T. -0.01 min  
Lab File: BF109507.D  
Acq: 2 Oct 2018 17:48




Instrument :  
BNA\_F  
ClientSampleId :  
092718-SIDI-F-U-M

Tgt Ion:172 Resp: 1159426  
Ion Ratio Lower Upper  
172 100  
171 36.2 29.7 44.5  
170 24.2 19.6 29.4

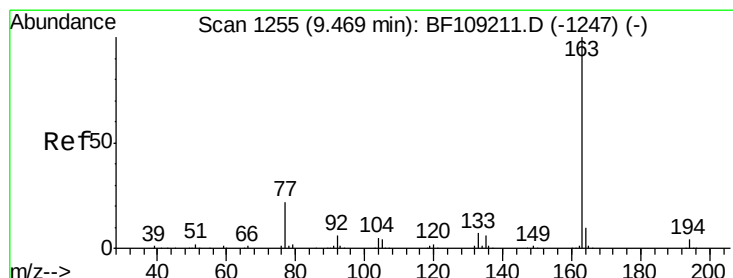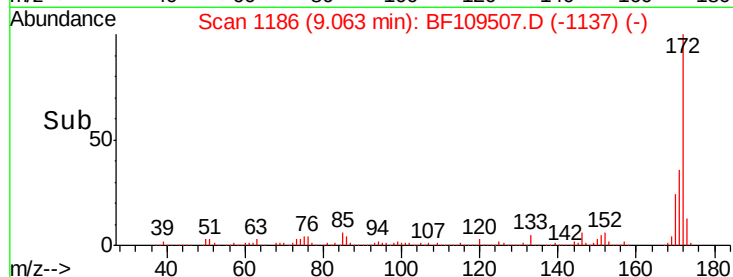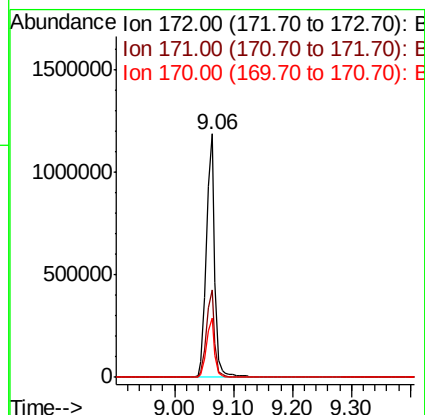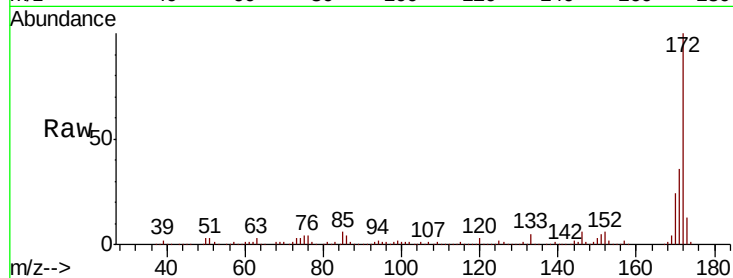


#49  
Dimethylphthalate  
Concen: 5.945 ng  
RT: 9.45 min Scan# 1252  
Delta R.T. -0.03 min  
Lab File: BF109507.D  
Acq: 2 Oct 2018 17:48

Tgt Ion:163 Resp: 77595  
Ion Ratio Lower Upper  
163 100  
194 3.7 2.7 4.1  
164 10.9 8.2 12.2

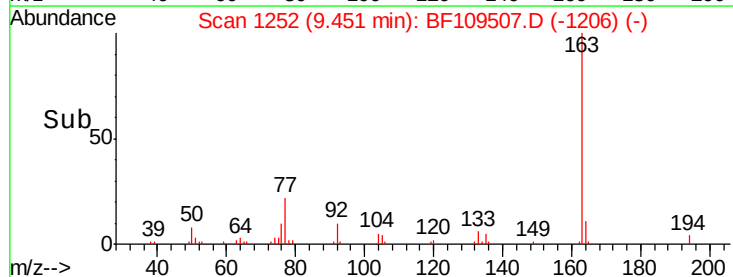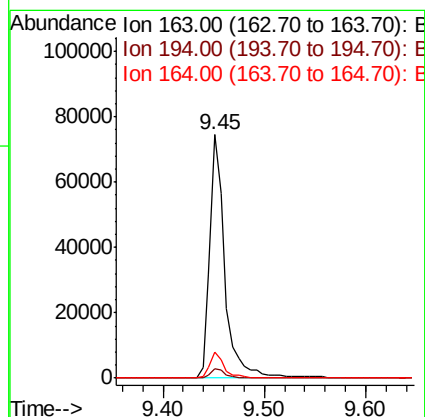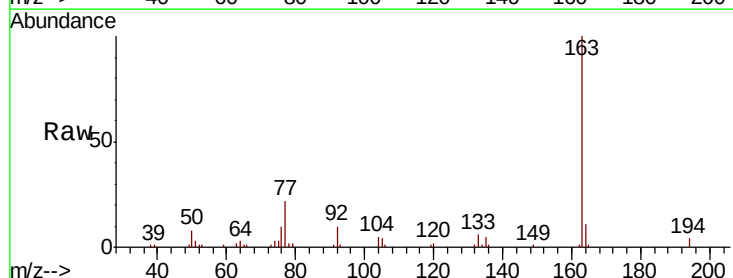







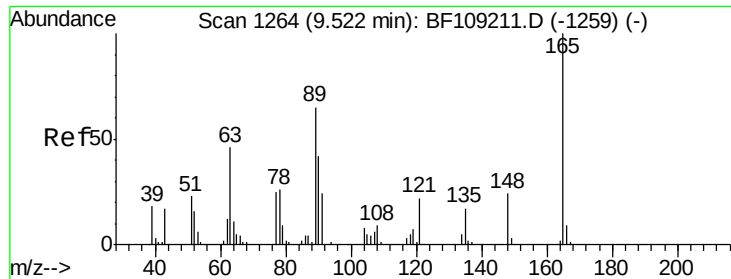

#50  
 2,6-Dinitrotoluene  
 Concen: 8.669 ng  
 RT: 9.73 min Scan# 1300  
 Delta R.T. 0.20 min  
 Lab File: BF109507.D  
 Acq: 2 Oct 2018 17:48




Instrument :  
 BNA\_F  
 ClientSampleId :  
 092718-SIDI-F-U-M


Tgt Ion:165 Resp: 22410  
 Ion Ratio Lower Upper  
 165 100  
 63 1.3 44.7 67.1#  
 89 1.4 44.0 66.0#

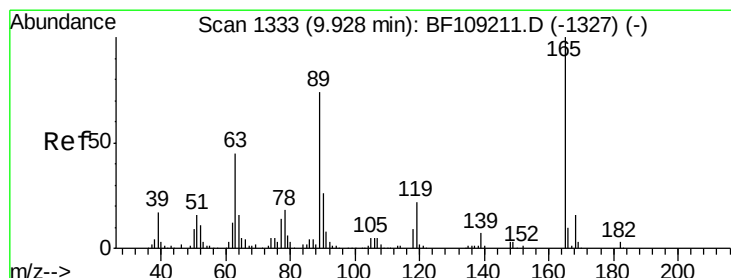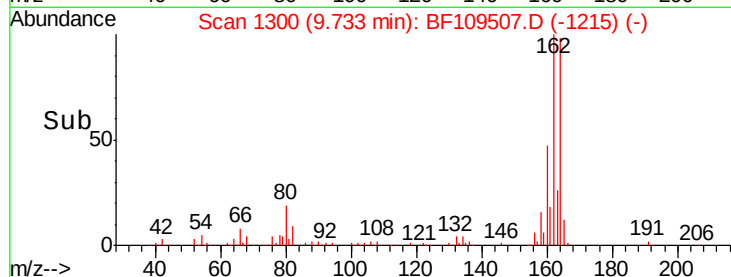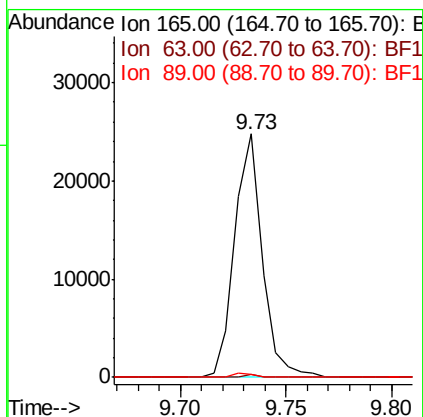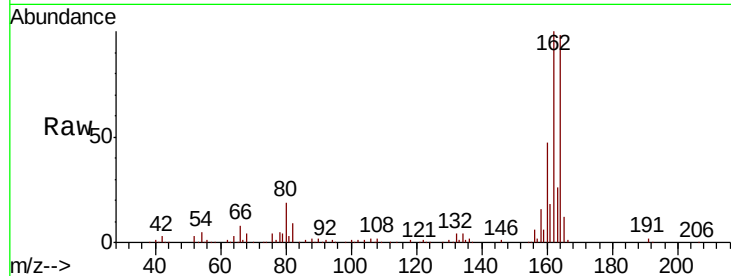

#56  
 2,4-Dinitrotoluene  
 Concen: 6.851 ng  
 RT: 9.73 min Scan# 1300  
 Delta R.T. -0.21 min  
 Lab File: BF109507.D  
 Acq: 2 Oct 2018 17:48

Tgt Ion:165 Resp: 22410  
 Ion Ratio Lower Upper  
 165 100  
 63 1.3 36.4 54.6#  
 89 1.4 57.8 86.6#  
 182 0.0 1.6 2.4#

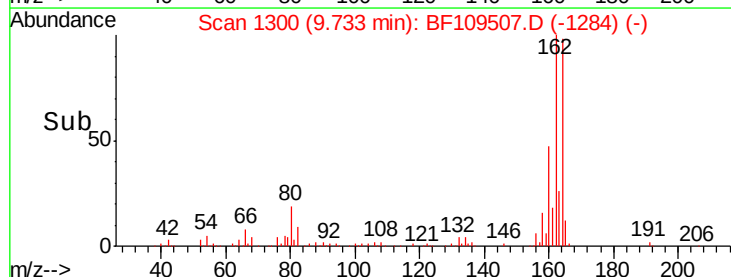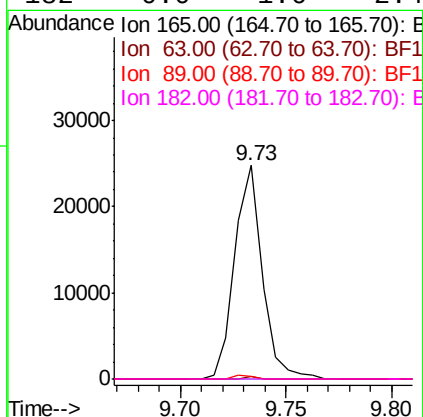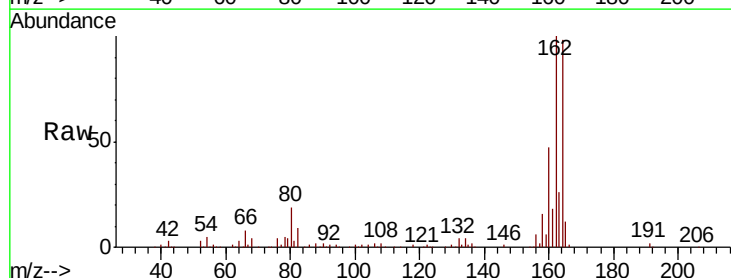


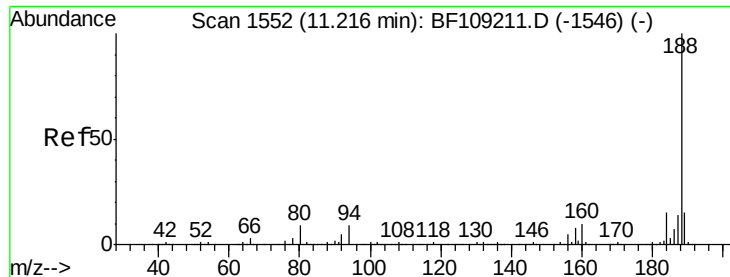




#63  
Phenanthrene-d10  
Concen: 20.000 ng  
RT: 11.21 min Scan# 1551  
Delta R.T. -0.01 min  
Lab File: BF109507.D  
Acq: 2 Oct 2018 17:48

Instrument :  
BNA\_F  
ClientSampleId :  
092718-SIDI-F-U-M

Tgt Ion:188 Resp: 315039  
Ion Ratio Lower Upper  
188 100  
94 9.1 8.5 12.7  
80 9.5 9.2 13.8

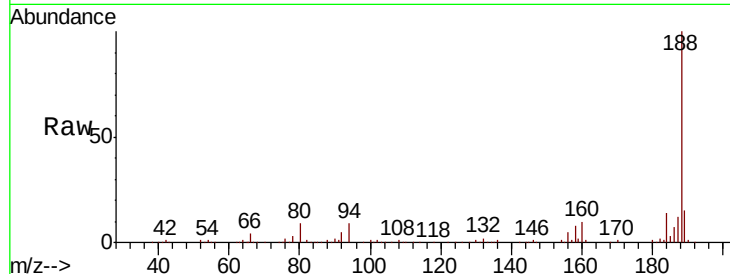


Abundance Ion 188.00 (187.70 to 188.70): E  
Ion 94.00 (93.70 to 94.70): BF1  
Ion 80.00 (79.70 to 80.70): BF1

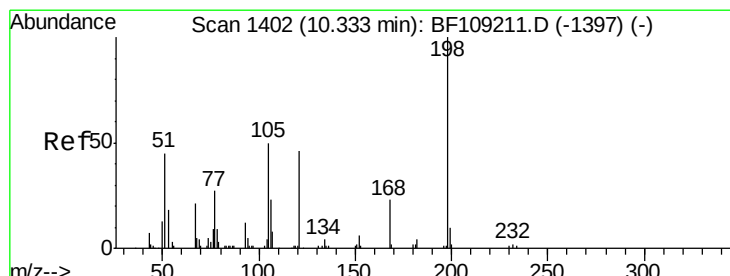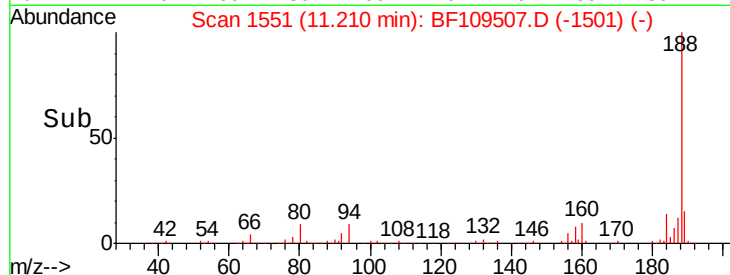
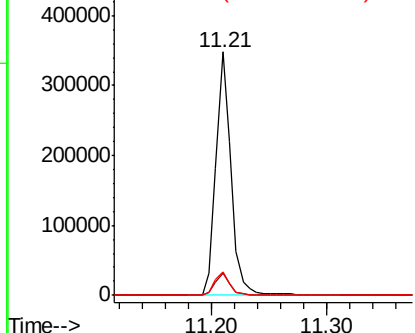



#64  
4,6-Dinitro-2-methylphenol  
Concen: 6.706 ng  
RT: 10.52 min Scan# 1434  
Delta R.T. 0.18 min  
Lab File: BF109507.D  
Acq: 2 Oct 2018 17:48

Tgt Ion:198 Resp: 272  
Ion Ratio Lower Upper  
198 100  
51 138.3 37.7 77.7#  
105 169.2 36.3 76.3#

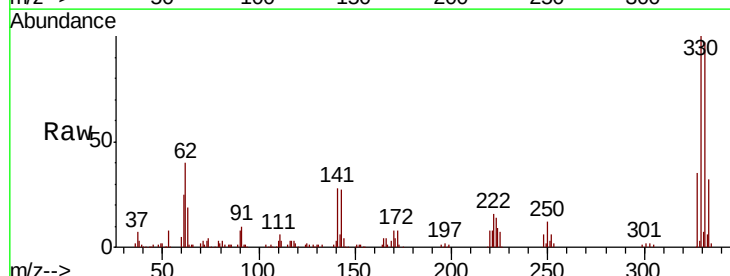

Abundance Ion 198.00 (197.70 to 198.70): E  
Ion 51.00 (50.70 to 51.70): BF1  
Ion 105.00 (104.70 to 105.70): E

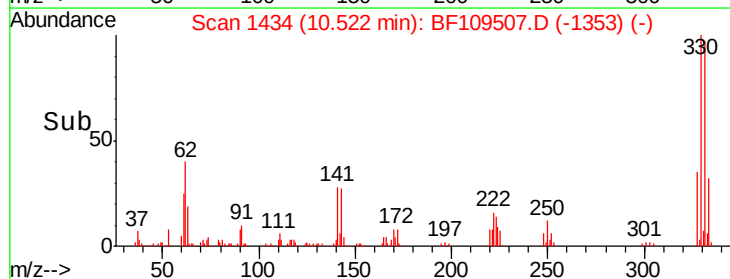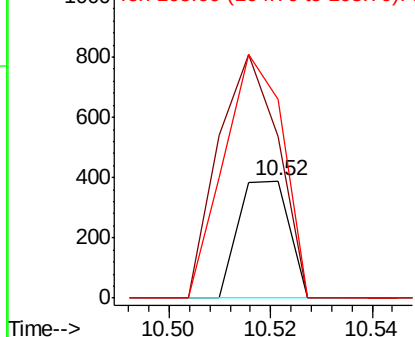


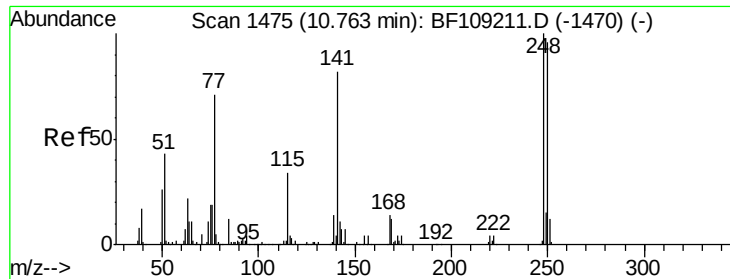




#66  
4-Bromophenyl-phenylether  
Concen: 2.863 ng  
RT: 10.52 min Scan# 1434  
Delta R.T. -0.25 min  
Lab File: BF109507.D  
Acq: 2 Oct 2018 17:48

Instrument :  
BNA\_F  
ClientSampleId :  
092718-SIDI-F-U-M

Tgt Ion:248 Resp: 10017  
Ion Ratio Lower Upper  
248 100  
250 196.0 76.9 115.3#  
141 458.3 74.4 111.6#

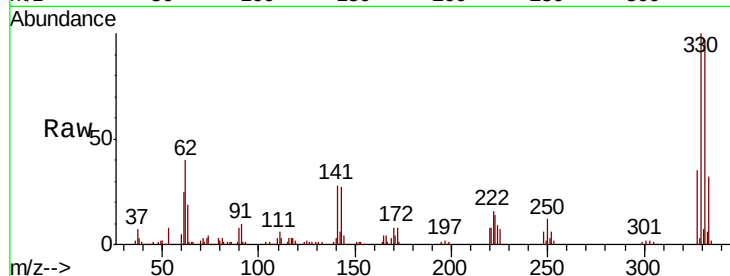


Abundance Ion 248.00 (247.70 to 248.70): E  
Ion 250.00 (249.70 to 250.70): E  
Ion 141.00 (140.70 to 141.70): E

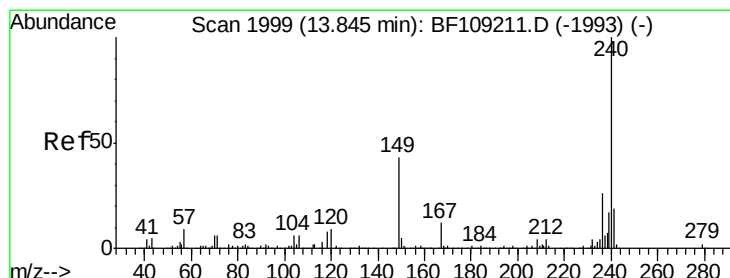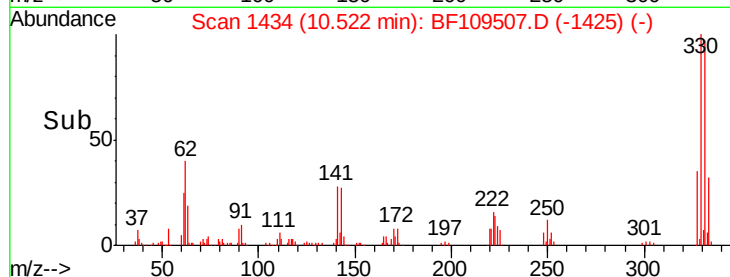
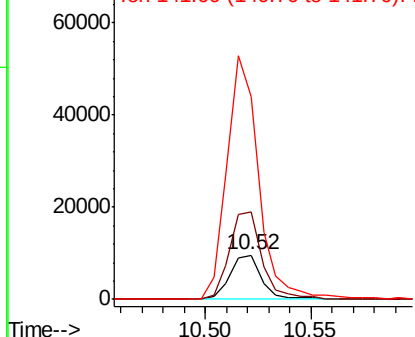



#75  
Chrysene-d12  
Concen: 20.000 ng  
RT: 13.84 min Scan# 1998  
Delta R.T. -0.01 min  
Lab File: BF109507.D  
Acq: 2 Oct 2018 17:48

Tgt Ion:240 Resp: 252817  
Ion Ratio Lower Upper  
240 100  
120 10.0 9.5 14.3  
236 24.7 20.7 31.1

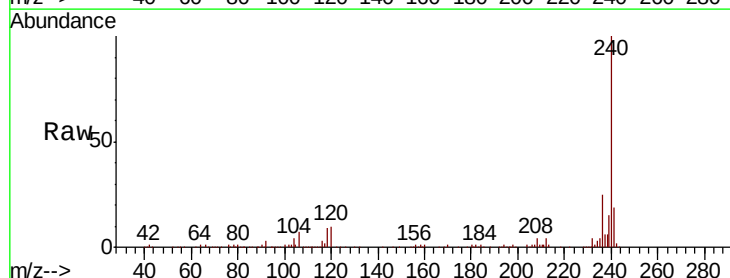

Abundance Ion 240.00 (239.70 to 240.70): E  
Ion 120.00 (119.70 to 120.70): E  
Ion 236.00 (235.70 to 236.70): E



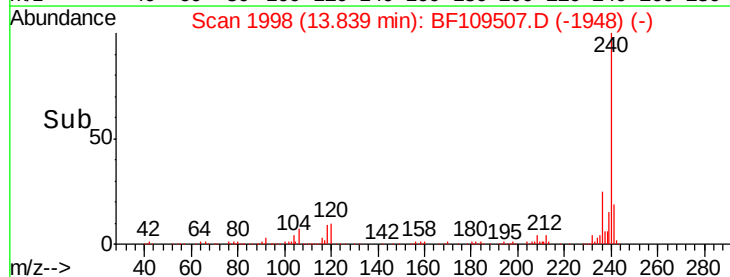
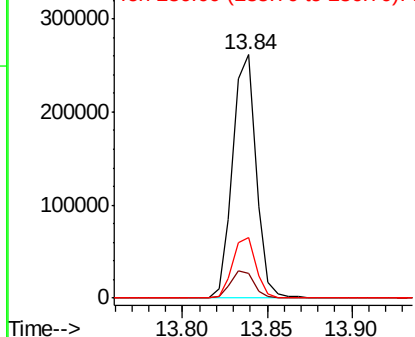


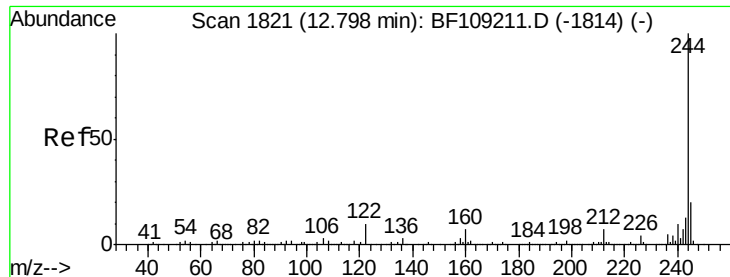

#78  
 Terphenyl-d14  
 Concen: 99.638 ng  
 RT: 12.79 min Scan# 1820  
 Delta R.T. -0.01 min  
 Lab File: BF109507.D  
 Acq: 2 Oct 2018 17:48

Instrument :  
 BNA\_F  
 ClientSampleId :  
 092718-SIDI-F-U-M

Tgt Ion:244 Resp: 1026431  
 Ion Ratio Lower Upper  
 244 100  
 212 7.4 5.4 8.0  
 122 12.5 11.0 16.4

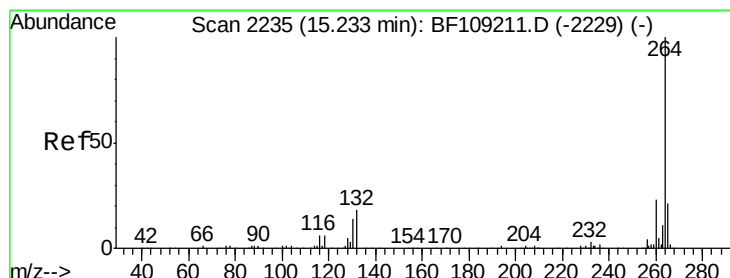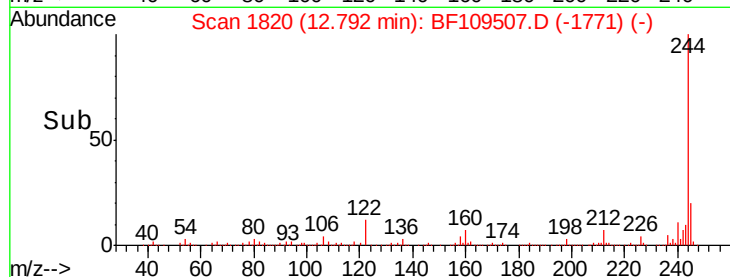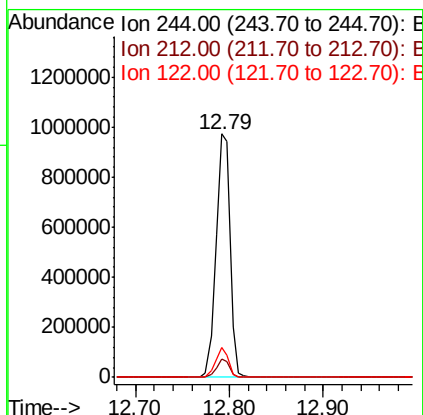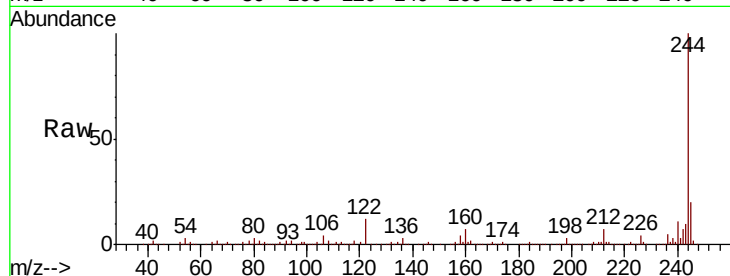

#86  
 Perylene-d12  
 Concen: 20.000 ng  
 RT: 15.24 min Scan# 2236  
 Delta R.T. -0.00 min  
 Lab File: BF109507.D  
 Acq: 2 Oct 2018 17:48

Tgt Ion:264 Resp: 254600  
 Ion Ratio Lower Upper  
 264 100  
 260 23.5 19.2 28.8  
 265 21.0 17.5 26.3

