
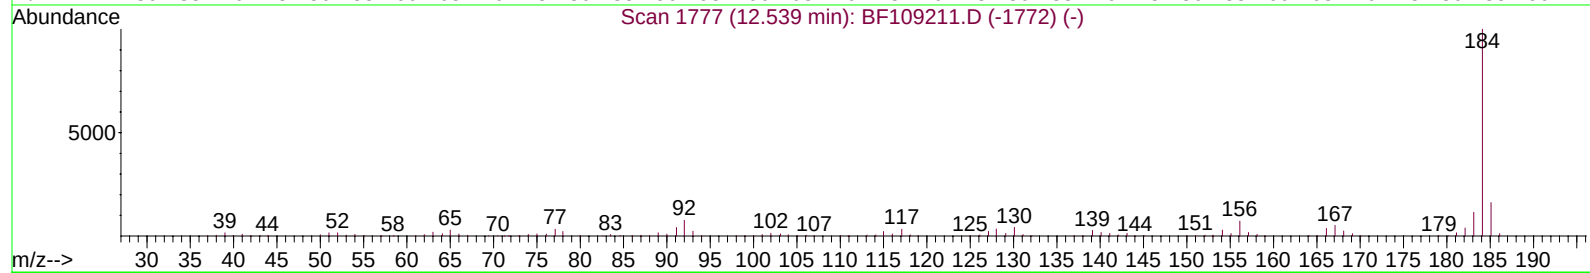
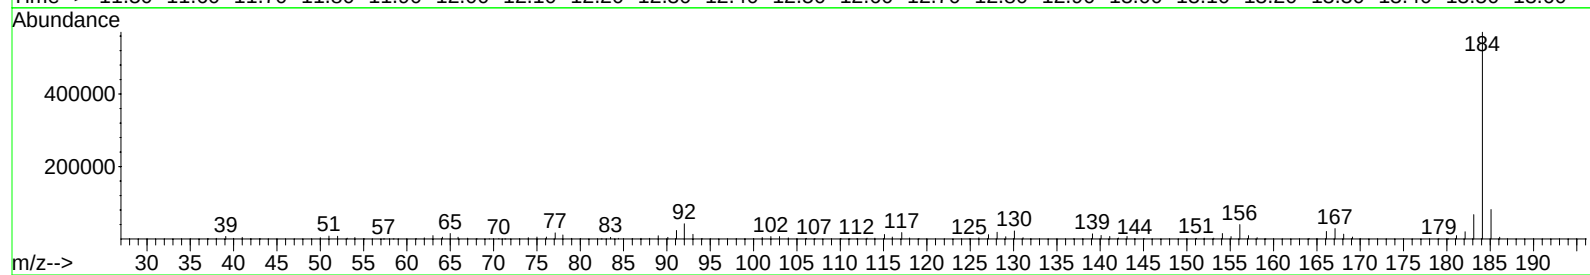


```
Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF100218\  
Data File : BF109492.D  
Acq On    : 2 Oct 2018 11:14  
Operator  : JU/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: Oct 02 11:52:58 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

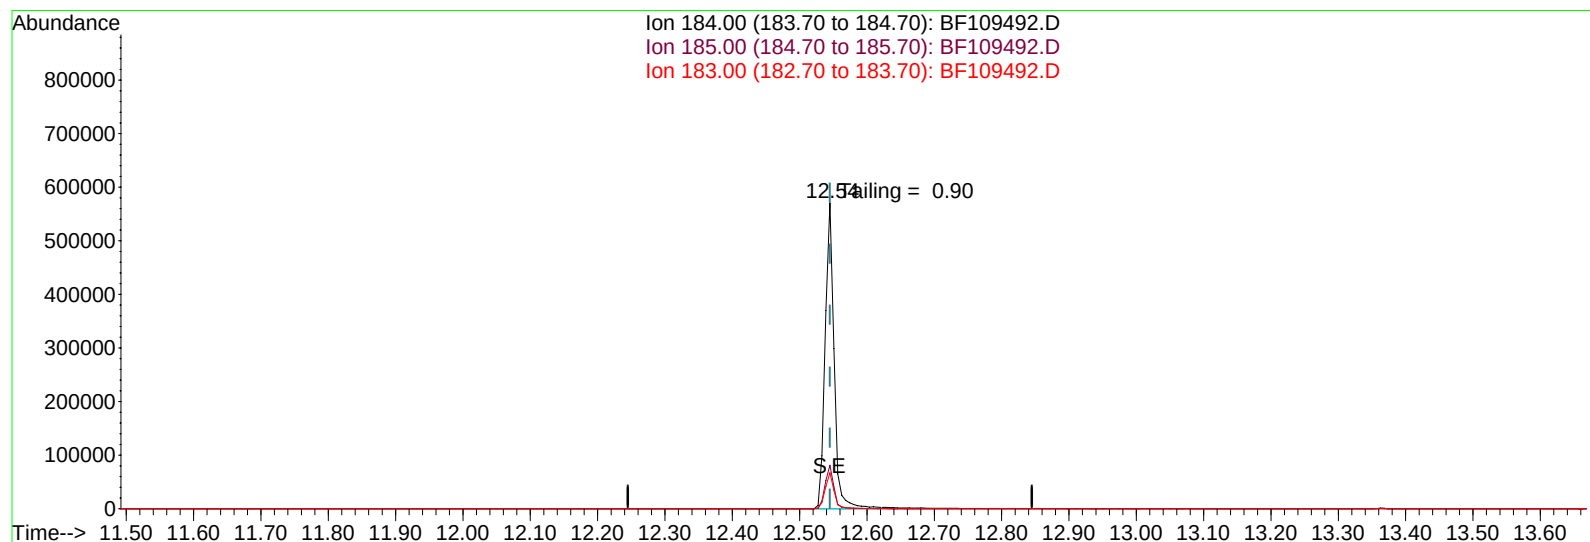

TIC: BF109492.D

(76) Benzidine




12.545min (-0.000) 0.00ng

response 533145

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.26
183.00	11.60	11.78
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF100218\  
Data File : BF109492.D  
Acq On    : 2 Oct 2018 11:14  
Operator  : JU/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: Oct 02 11:52:58 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

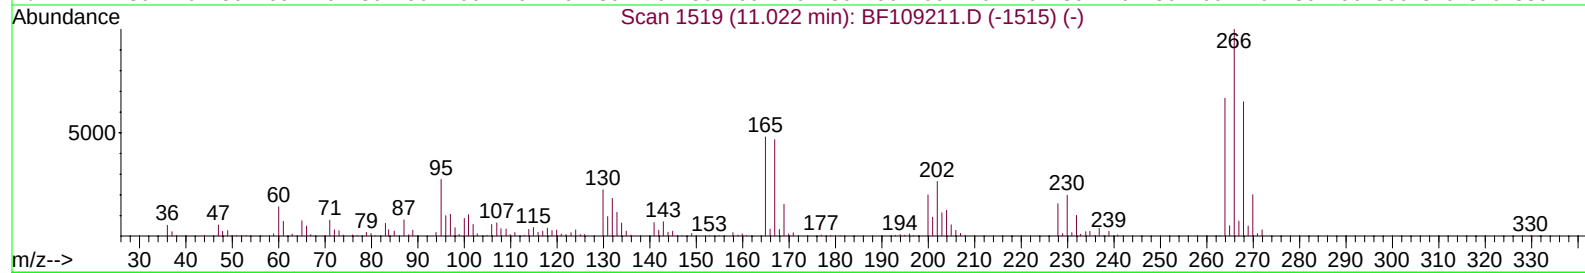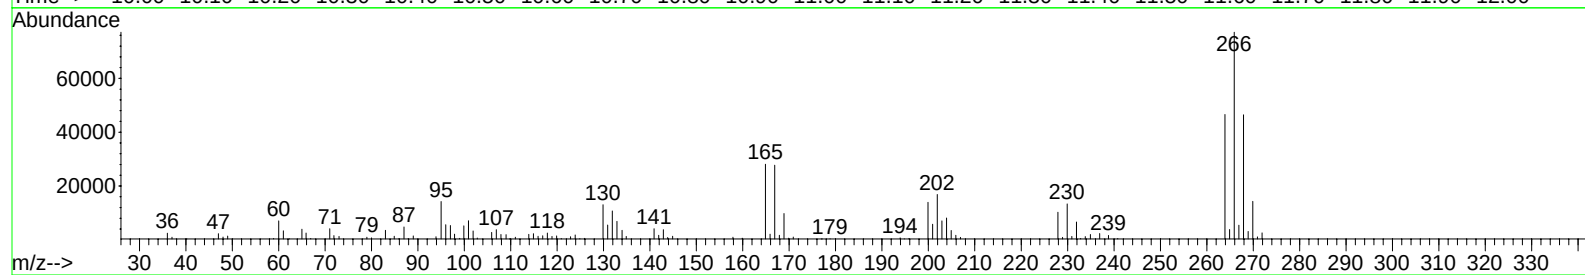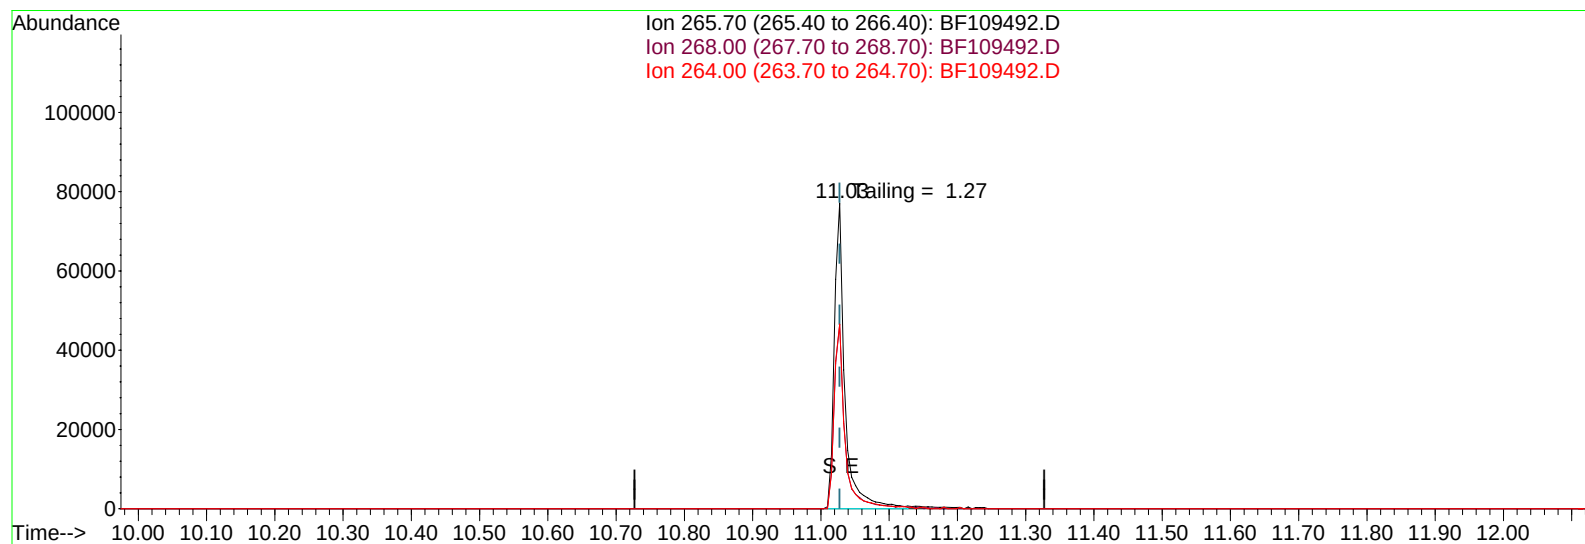

(69) Pentachlorophenol (C)

11.027min (-0.000) 39681.25ng

response 82629

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.23
264.00	61.90	60.38
0.00	0.00	0.00