
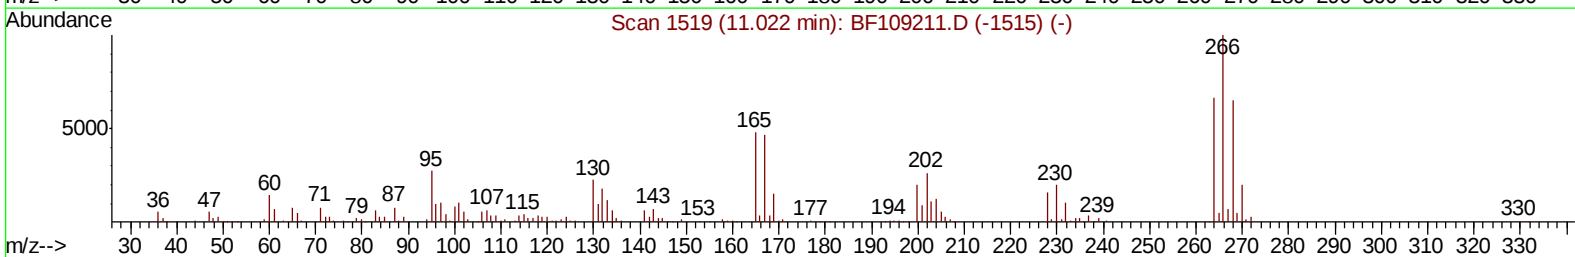
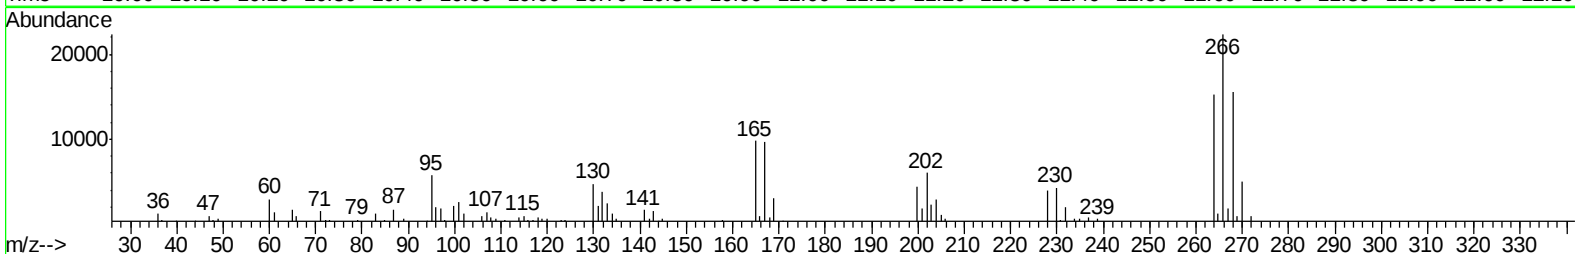


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF100218\
Data File : BF109519.D
Acq On : 2 Oct 2018 23:56
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 03 05:27:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

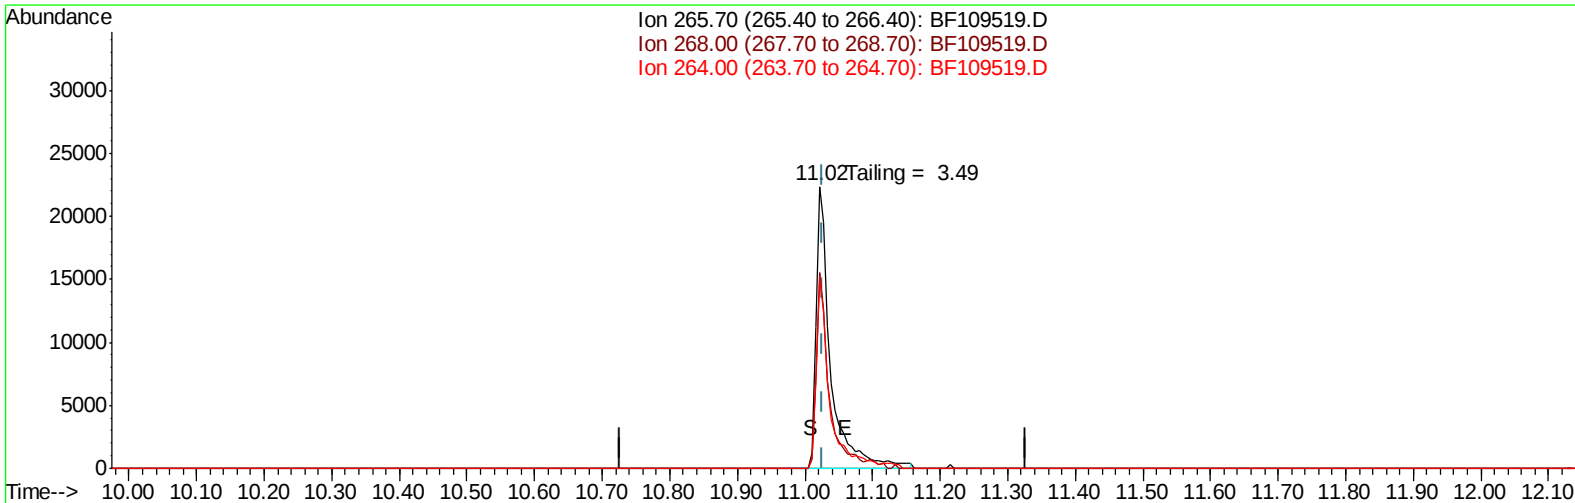

TIC: BF109519.D

(69) Pentachlorophenol (C)




11.022min (-0.006) 43031.64ng

response 33716

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	69.46
264.00	61.90	68.30
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF100218\
Data File : BF109519.D
Acq On : 2 Oct 2018 23:56
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 03 05:27:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

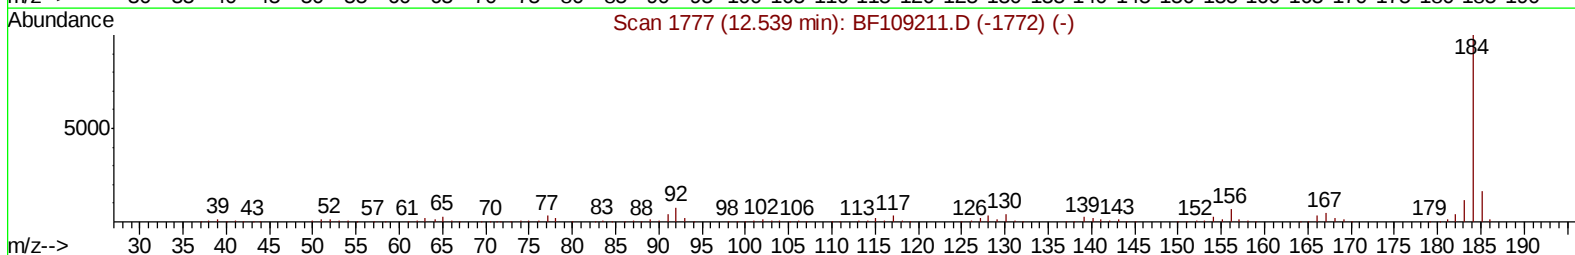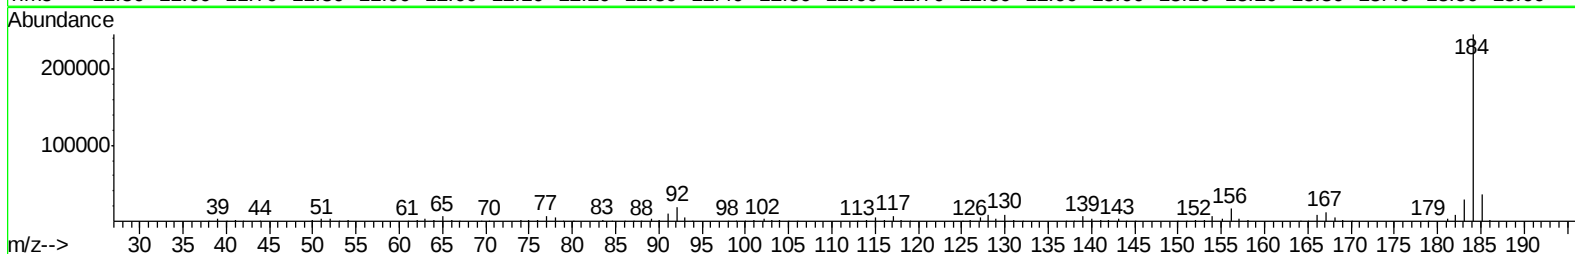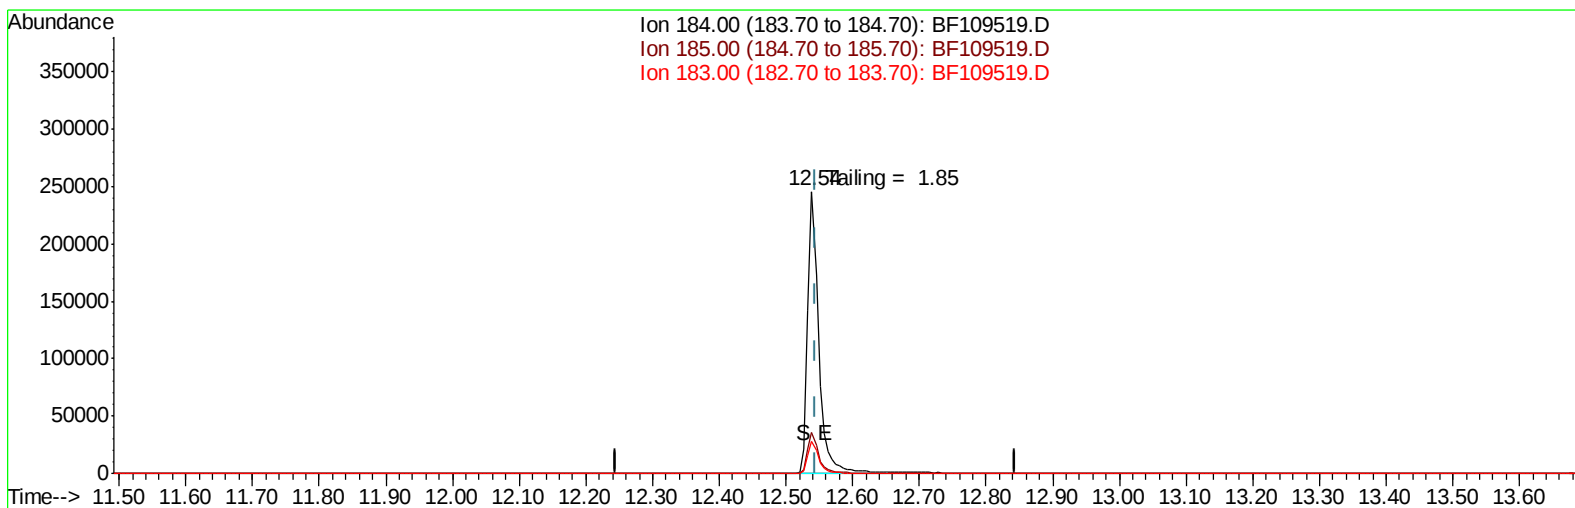

TIC: BF109519.D

(76) Benzidine

12.539min (-0.006) 0.00ng

response 273367

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.66
183.00	11.60	11.48
0.00	0.00	0.00