

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF100218\
 Data File : BF109513.D
 Acq On : 2 Oct 2018 20:26
 Operator : JU/SJ
 Sample : J5186-11
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 092718-TIPC-F-D-B

Quant Time: Oct 03 04:43:58 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 22 13:32:18 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.70	152	101946	20.00	ng	0.00
21) Naphthalene-d8	7.98	136	390575	20.00	ng	-0.01
38) Acenaphthene-d10	9.73	164	176538	20.00	ng	0.00
63) Phenanthrene-d10	11.21	188	313550	20.00	ng	0.00
75) Chrysene-d12	13.83	240	261705	20.00	ng	-0.01
86) Perylene-d12	15.24	264	260423	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	248276	40.11	ng	0.00
7) Phenol-d6	6.34	99	220976	27.98	ng	-0.02
23) Nitrobenzene-d5	7.27	82	663233	100.24	ng	-0.01
41) 2,4,6-Tribromophenol	10.52	330	159251	91.51	ng	-0.02
44) 2-Fluorobiphenyl	9.06	172	1121862	95.84	ng	-0.01
78) Terphenyl-d14	12.79	244	1018769	95.54	ng	-0.01
Target Compounds						Qvalue
49) Dimethylphthalate	9.45	163	100418	7.821	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF100218\
Data File : BF109513.D
Acq On : 2 Oct 2018 20:26
Operator : JU/SJ
Sample : J5186-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
092718-TIPC-F-D-B

Quant Time: Oct 03 04:43:58 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

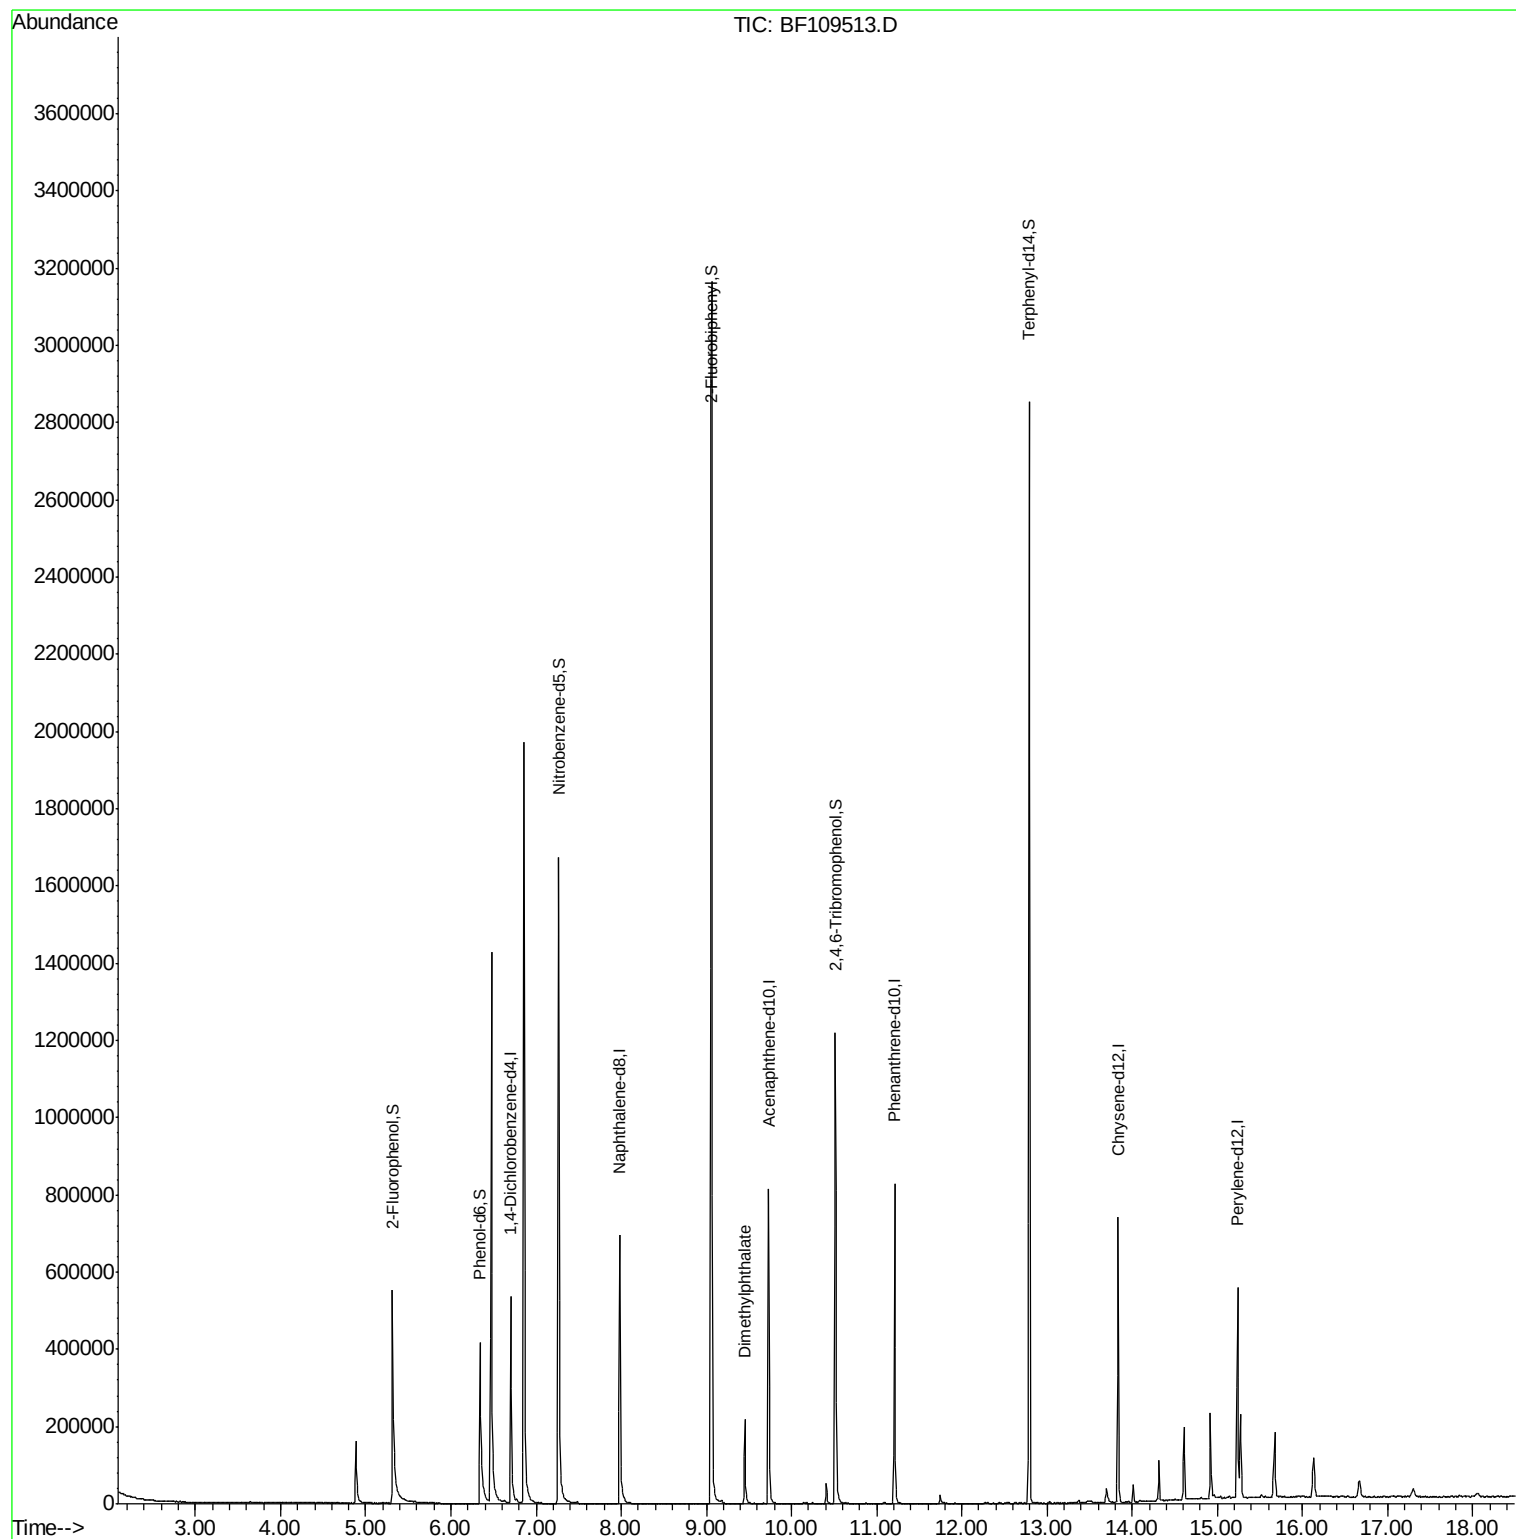

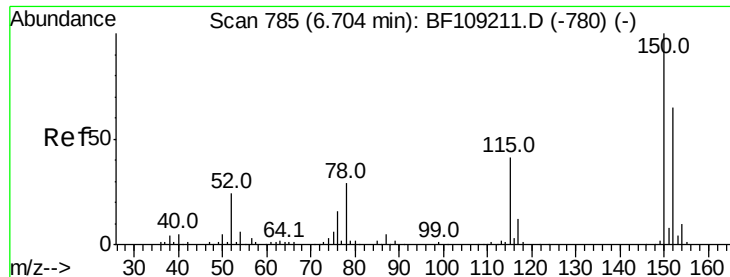


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.70 min Scan# 785
Delta R.T. -0.01 min
Lab File: BF109513.D
Acq: 2 Oct 2018 20:26

Instrument :
BNA_F
ClientSampleId :
092718-TIPC-F-D-B

Tot Ion:152 Resp: 101946
Ion Ratio Lower Upper
152 100
150 153.3 124.6 186.8
115 60.3 50.1 75.1

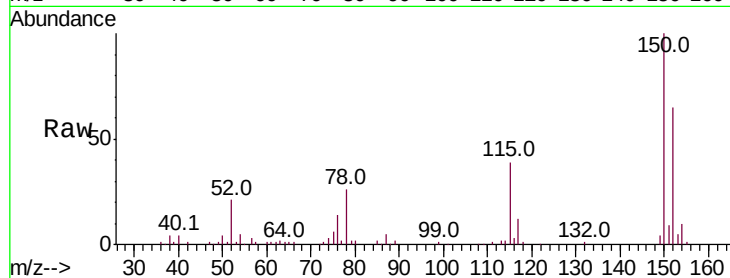


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

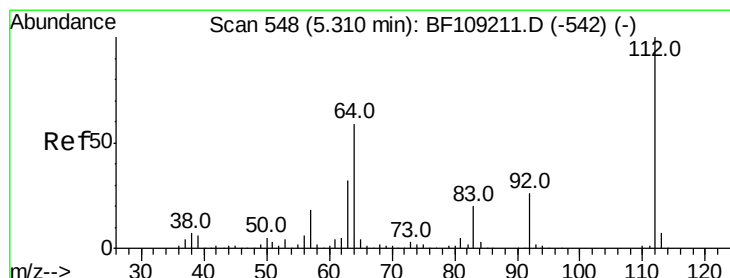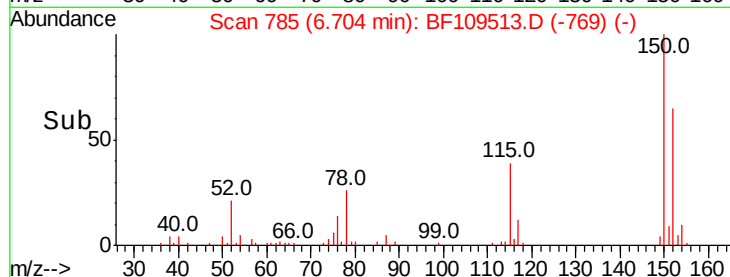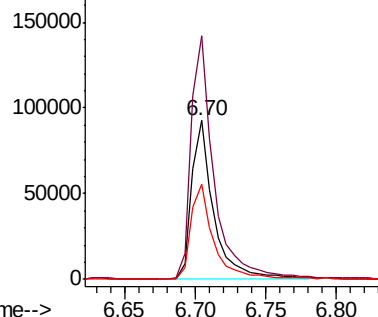



#5


2-Fluorophenol
Concen: 40.112 ng
RT: 5.32 min Scan# 549
Delta R.T. 0.00 min
Lab File: BF109513.D
Acq: 2 Oct 2018 20:26

Tgt Ion:112 Resp: 248276
Ion Ratio Lower Upper
112 100
64 58.0 47.9 71.9
63 30.2 23.7 35.5

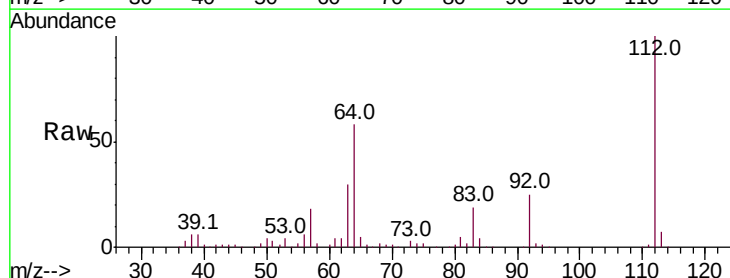

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

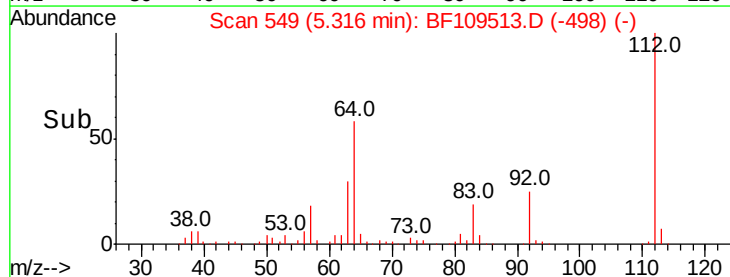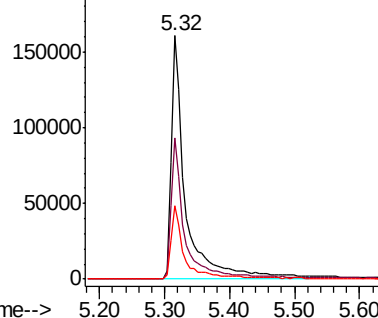

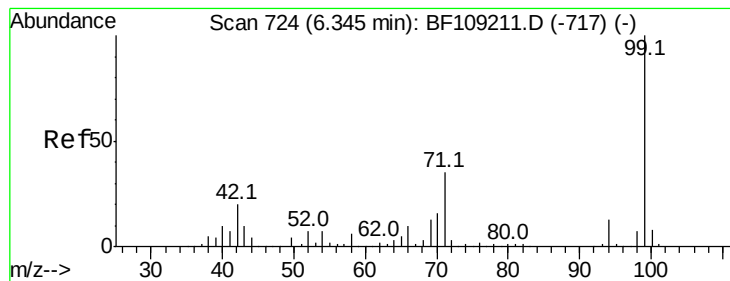

#7

Phenol-d6

Concen: 27.979 ng

RT: 6.34 min Scan# 723

Delta R.T. -0.02 min

Lab File: BF109513.D

Acq: 2 Oct 2018 20:26

Instrument :

BNA_F

ClientSampleId :

092718-TIPC-F-D-B


Tot Ion: 99 Resp: 220976

Ion Ratio Lower Upper




99 100

42 18.4 14.5 21.7

71 34.9 25.4 38.0

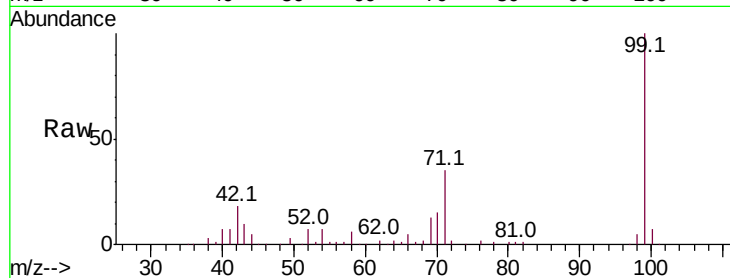

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

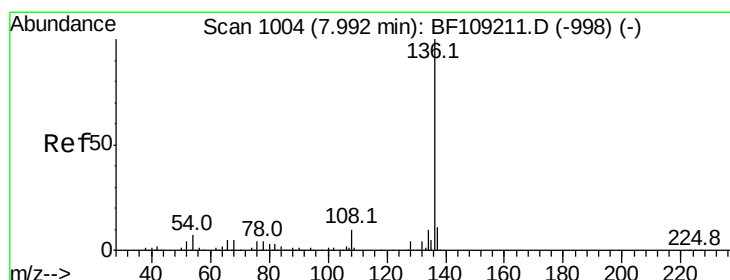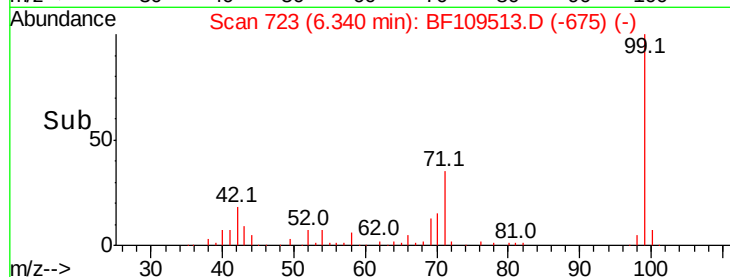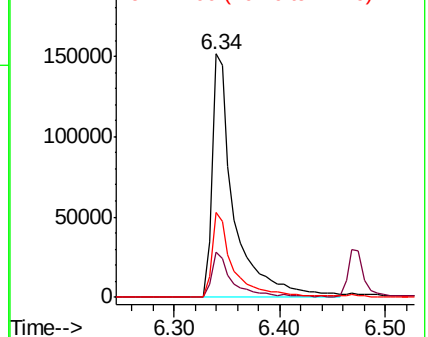

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.98 min Scan# 1002

Delta R.T. -0.01 min

Lab File: BF109513.D

Acq: 2 Oct 2018 20:26

Tgt Ion: 136 Resp: 390575


Ion Ratio Lower Upper

136 100



137 11.1 8.9 13.3


54 7.4 6.6 9.8

68 5.8 5.0 7.4

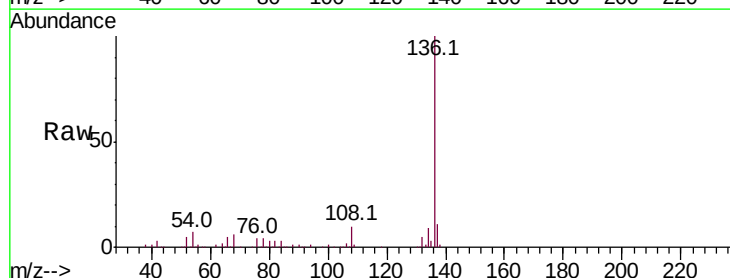

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

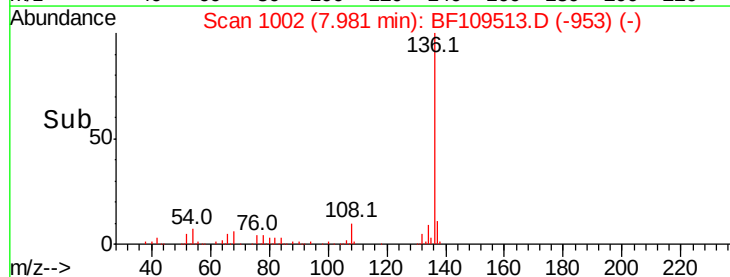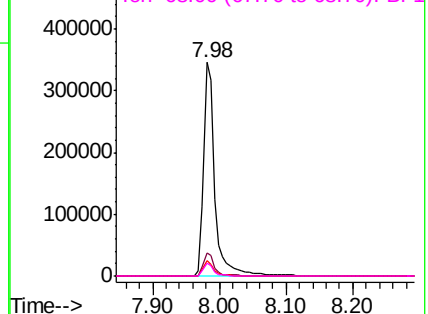


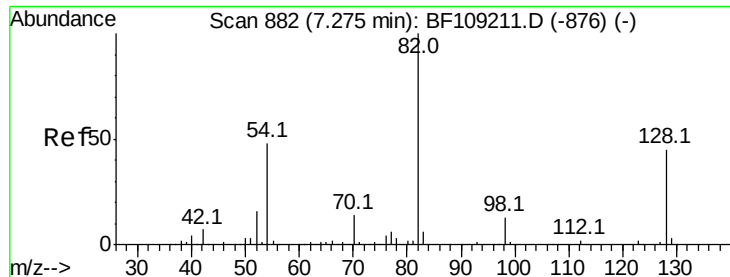




#23
 Nitrobenzene-d5
 Concen: 100.241 ng
 RT: 7.27 min Scan# 881
 Delta R.T. -0.01 min
 Lab File: BF109513.D
 Acq: 2 Oct 2018 20:26

Instrument :
 BNA_F
 ClientSampleId :
 092718-TIPC-F-D-B

Tot Ion	82	Resp	663233
Ion Ratio	Lower	Upper	
82	100		
128	43.8	36.1	54.1
54	47.0	41.4	62.2

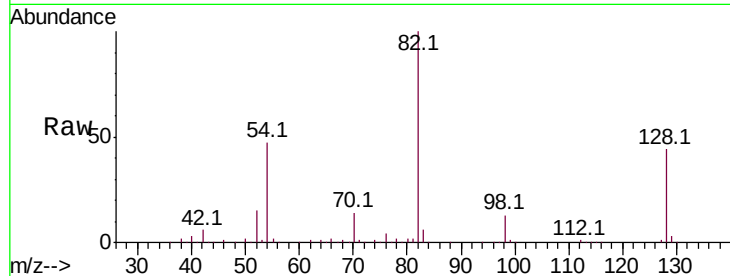


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF1

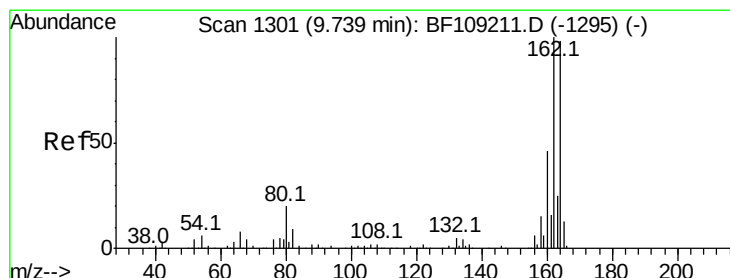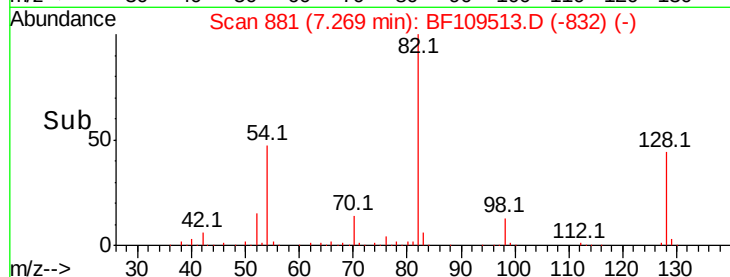
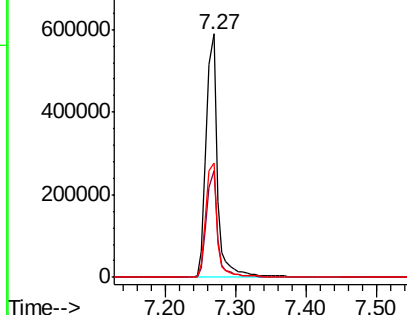



#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.73 min Scan# 1300
 Delta R.T. -0.01 min
 Lab File: BF109513.D
 Acq: 2 Oct 2018 20:26

Tgt Ion	164	Resp	176538
Ion Ratio	Lower	Upper	
164	100		
162	105.1	86.1	129.1
160	48.0	38.3	57.5

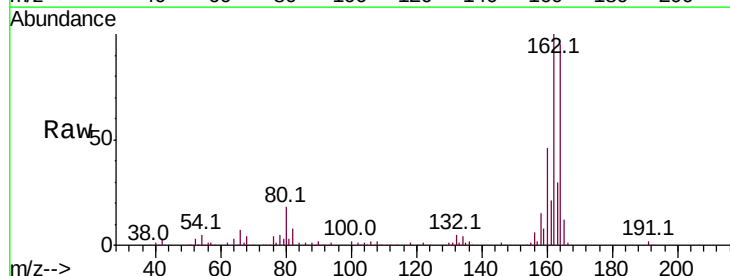

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

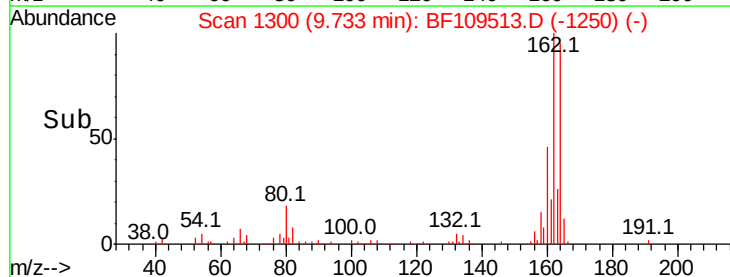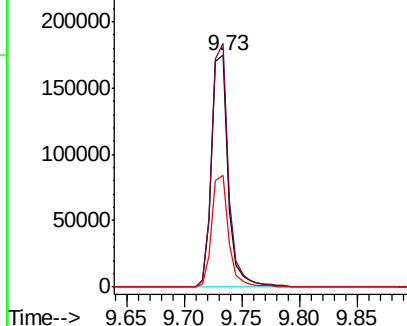


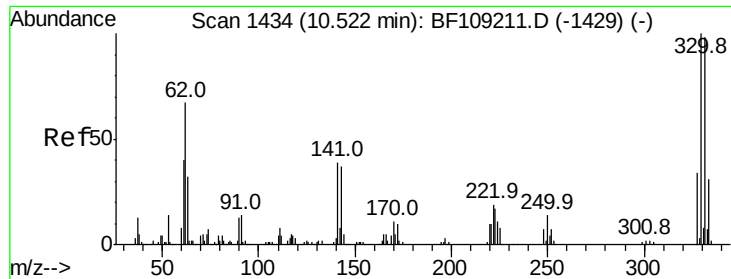

#41
 2,4,6-Tribromophenol
 Concen: 91.508 ng
 RT: 10.52 min Scan# 1433
 Delta R.T. -0.02 min
 Lab File: BF109513.D
 Acq: 2 Oct 2018 20:26

Instrument :
 BNA_F
 ClientSampleId :
 092718-TIPC-F-D-B

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.2	77.0	115.6
141	34.2	29.9	44.9



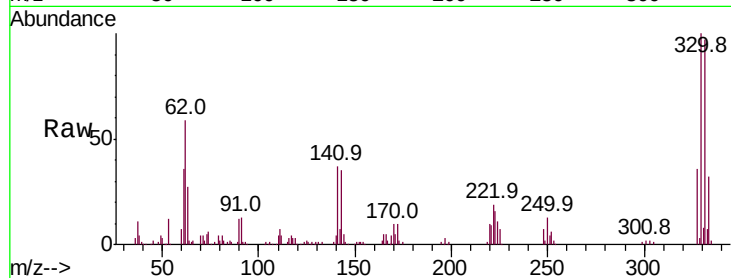


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

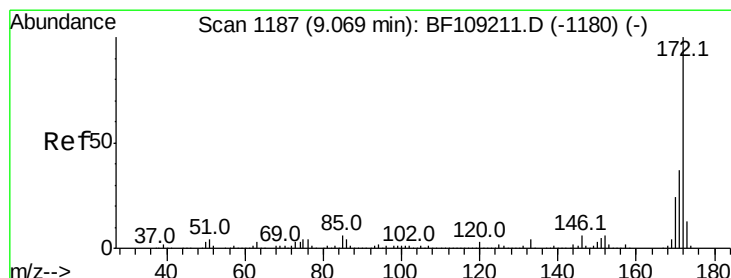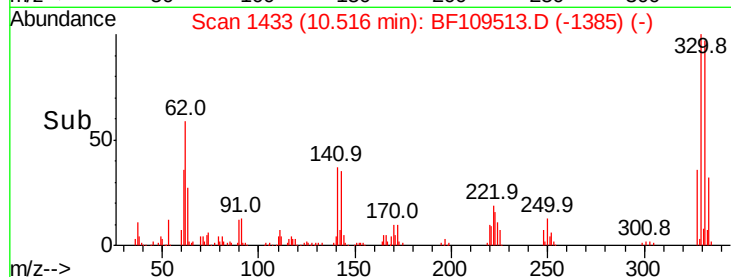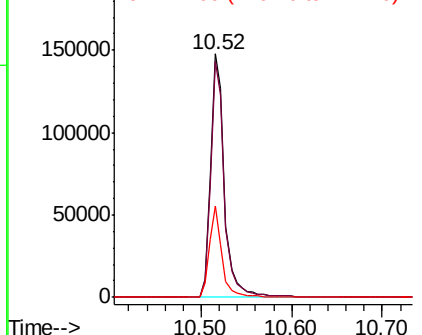

#44
 2-Fluorobiphenyl
 Concen: 95.842 ng
 RT: 9.06 min Scan# 1186
 Delta R.T. -0.01 min
 Lab File: BF109513.D
 Acq: 2 Oct 2018 20:26

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.1	29.7	44.5
170	24.0	19.6	29.4


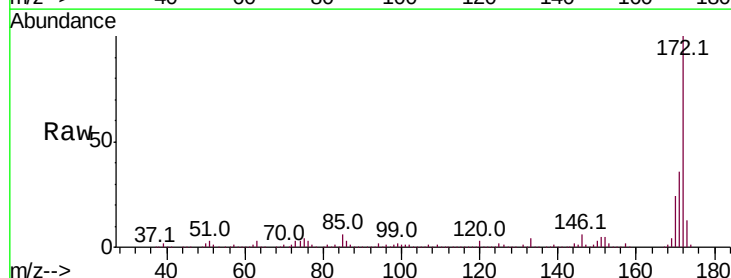



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

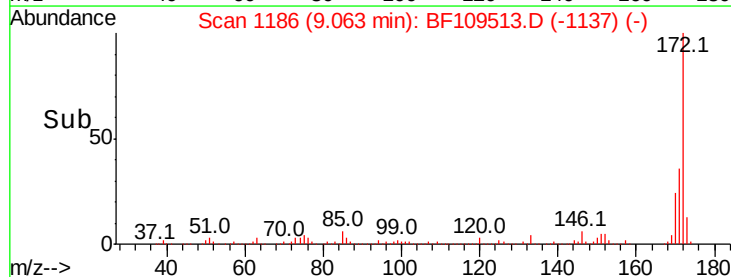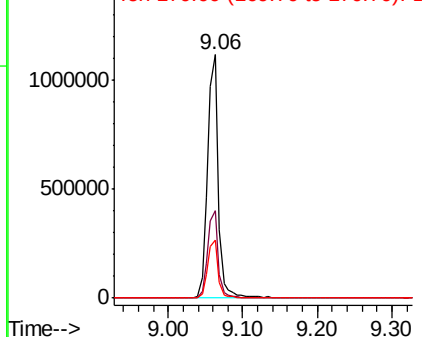


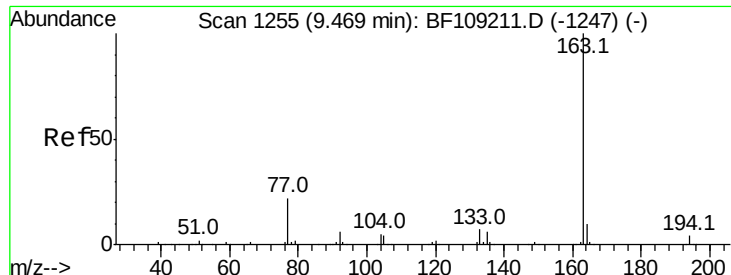




#49
Dimethylphthalate
Concen: 7.821 ng
RT: 9.45 min Scan# 1252
Delta R.T. -0.03 min
Lab File: BF109513.D
Acq: 2 Oct 2018 20:26

Instrument :
BNA_F
ClientSampleId :
092718-TIPC-F-D-B

Tot Ion:163 Resp: 100418
Ion Ratio Lower Upper
163 100
194 3.5 2.7 4.1
164 10.0 8.2 12.2

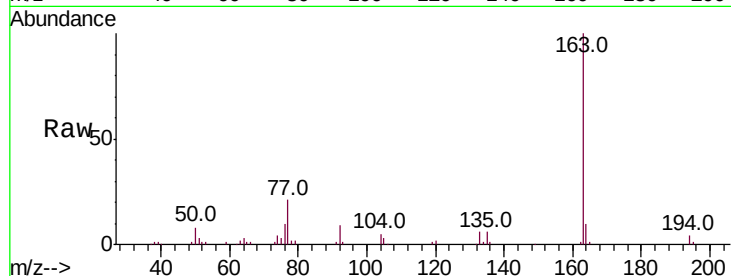


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

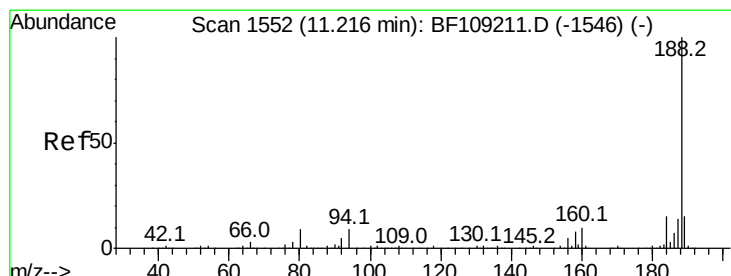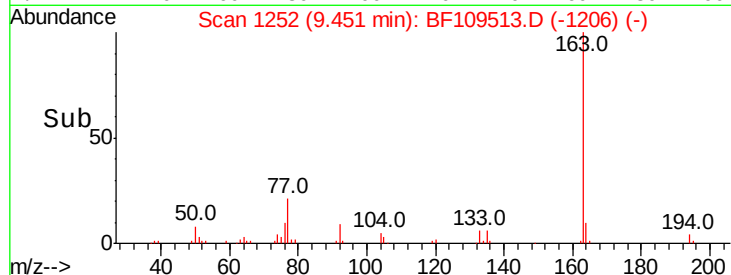
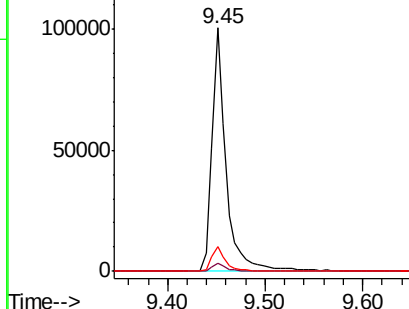



#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.21 min Scan# 1551
Delta R.T. -0.01 min
Lab File: BF109513.D
Acq: 2 Oct 2018 20:26

Tgt Ion:188 Resp: 313550
Ion Ratio Lower Upper
188 100
94 9.0 8.5 12.7
80 9.2 9.2 13.8

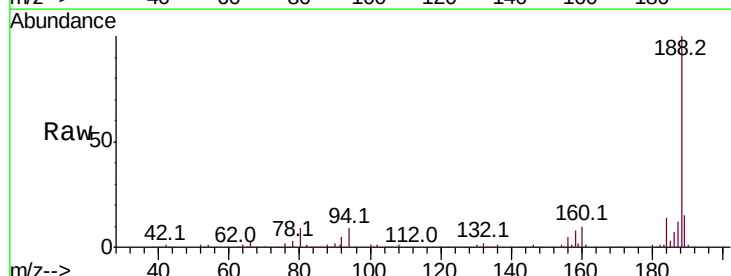

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

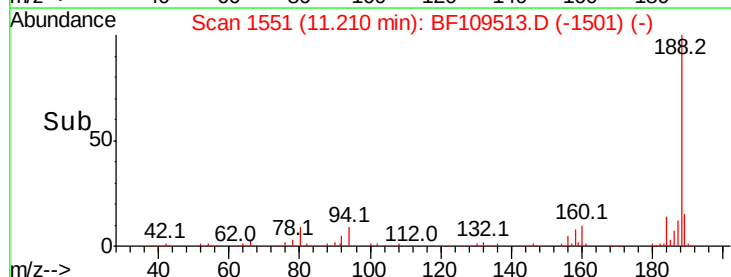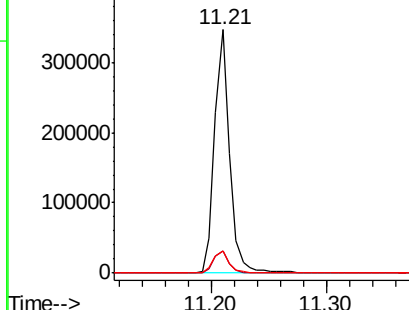

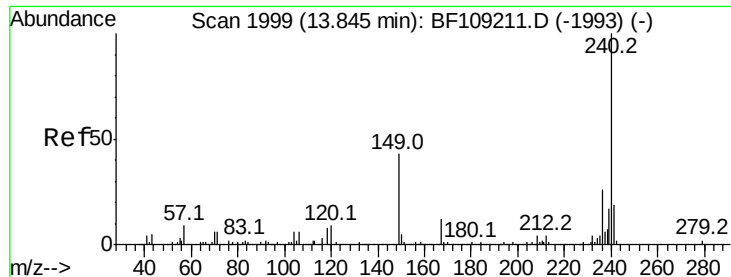

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.83 min Scan# 1997

Delta R.T. -0.01 min

Lab File: BF109513.D

Acq: 2 Oct 2018 20:26

Instrument :

BNA_F

ClientSampleId :

092718-TIPC-F-D-B


Tot Ion:240 Resp: 261705

Ion Ratio Lower Upper

240 100

120 11.3 9.5 14.3




236 24.6 20.7 31.1

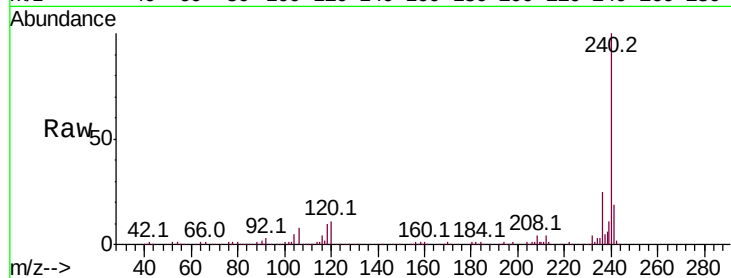

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

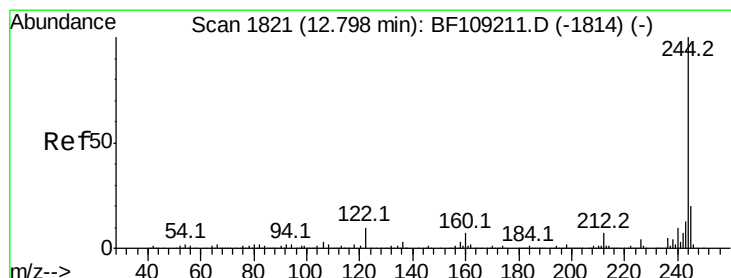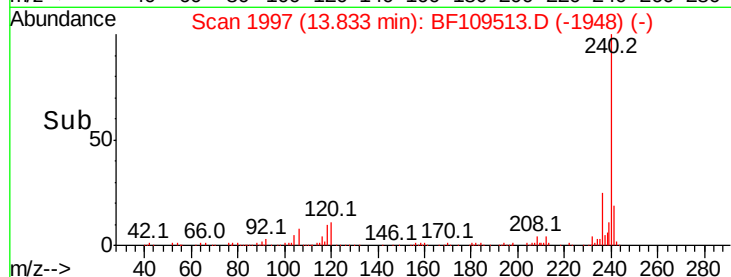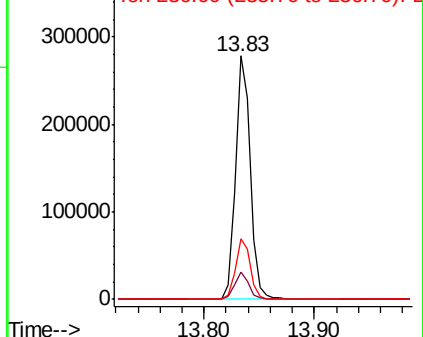

#78

Terphenyl-d14

Concen: 95.536 ng

RT: 12.79 min Scan# 1820

Delta R.T. -0.01 min

Lab File: BF109513.D

Acq: 2 Oct 2018 20:26


Tgt Ion:244 Resp: 1018769

Ion Ratio Lower Upper

244 100

212 7.2 5.4 8.0



122 11.8 11.0 16.4

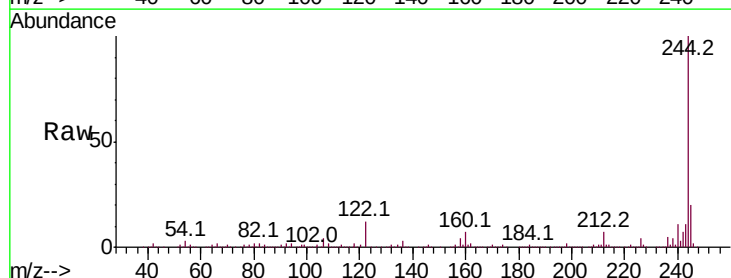


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

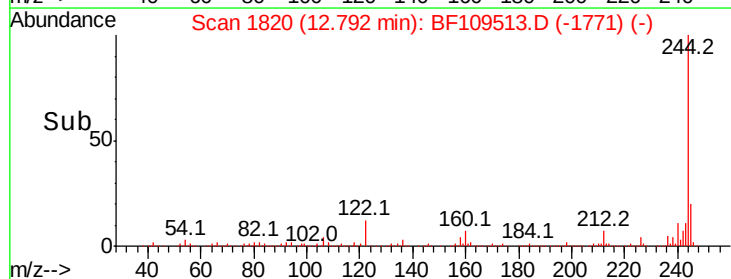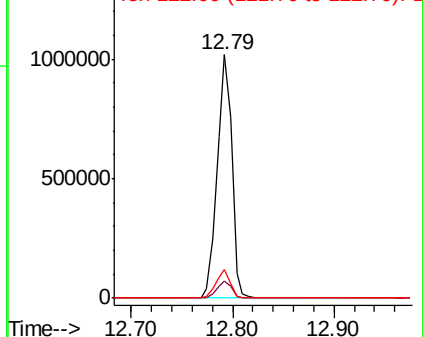

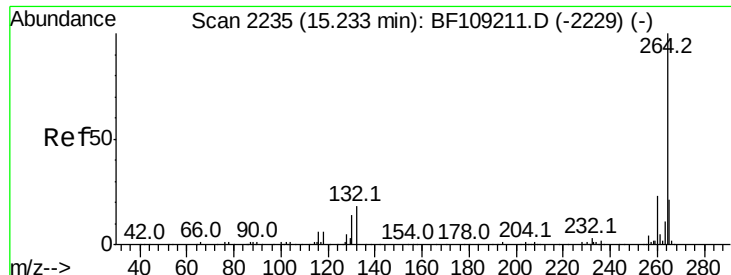

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.24 min Scan# 2236
 Delta R.T. 0.00 min
 Lab File: BF109513.D
 Acq: 2 Oct 2018 20:26

Instrument :
 BNA_F
 ClientSampleId :
 092718-TIPC-F-D-B

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.2	19.2	28.8
265	22.2	17.5	26.3

