

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF100218\
 Data File : BF109526.D
 Acq On : 3 Oct 2018 3:11
 Operator : JU/SJ
 Sample : J5187-05
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 092818-JETT-F-U-M

Quant Time: Oct 03 05:06:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 22 13:32:18 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.70	152	101809	20.00	ng	0.00
21) Naphthalene-d8	7.98	136	380426	20.00	ng	-0.01
38) Acenaphthene-d10	9.73	164	170445	20.00	ng	-0.01
63) Phenanthrene-d10	11.21	188	301201	20.00	ng	0.00
75) Chrysene-d12	13.83	240	241156	20.00	ng	-0.01
86) Perylene-d12	15.23	264	256918	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	264141	42.73	ng	0.00
7) Phenol-d6	6.34	99	208556	26.44	ng	-0.02
23) Nitrobenzene-d5	7.27	82	690443	107.14	ng	-0.01
41) 2,4,6-Tribromophenol	10.52	330	165548	98.53	ng	-0.02
44) 2-Fluorobiphenyl	9.06	172	1190300	105.32	ng	-0.01
78) Terphenyl-d14	12.79	244	1021340	103.94	ng	-0.01
Target Compounds						Qvalue
49) Dimethylphthalate	9.45	163	41848	3.376	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF100218\
Data File : BF109526.D
Acq On : 3 Oct 2018 3:11
Operator : JU/SJ
Sample : J5187-05
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
092818-JETT-F-U-M

Quant Time: Oct 03 05:06:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

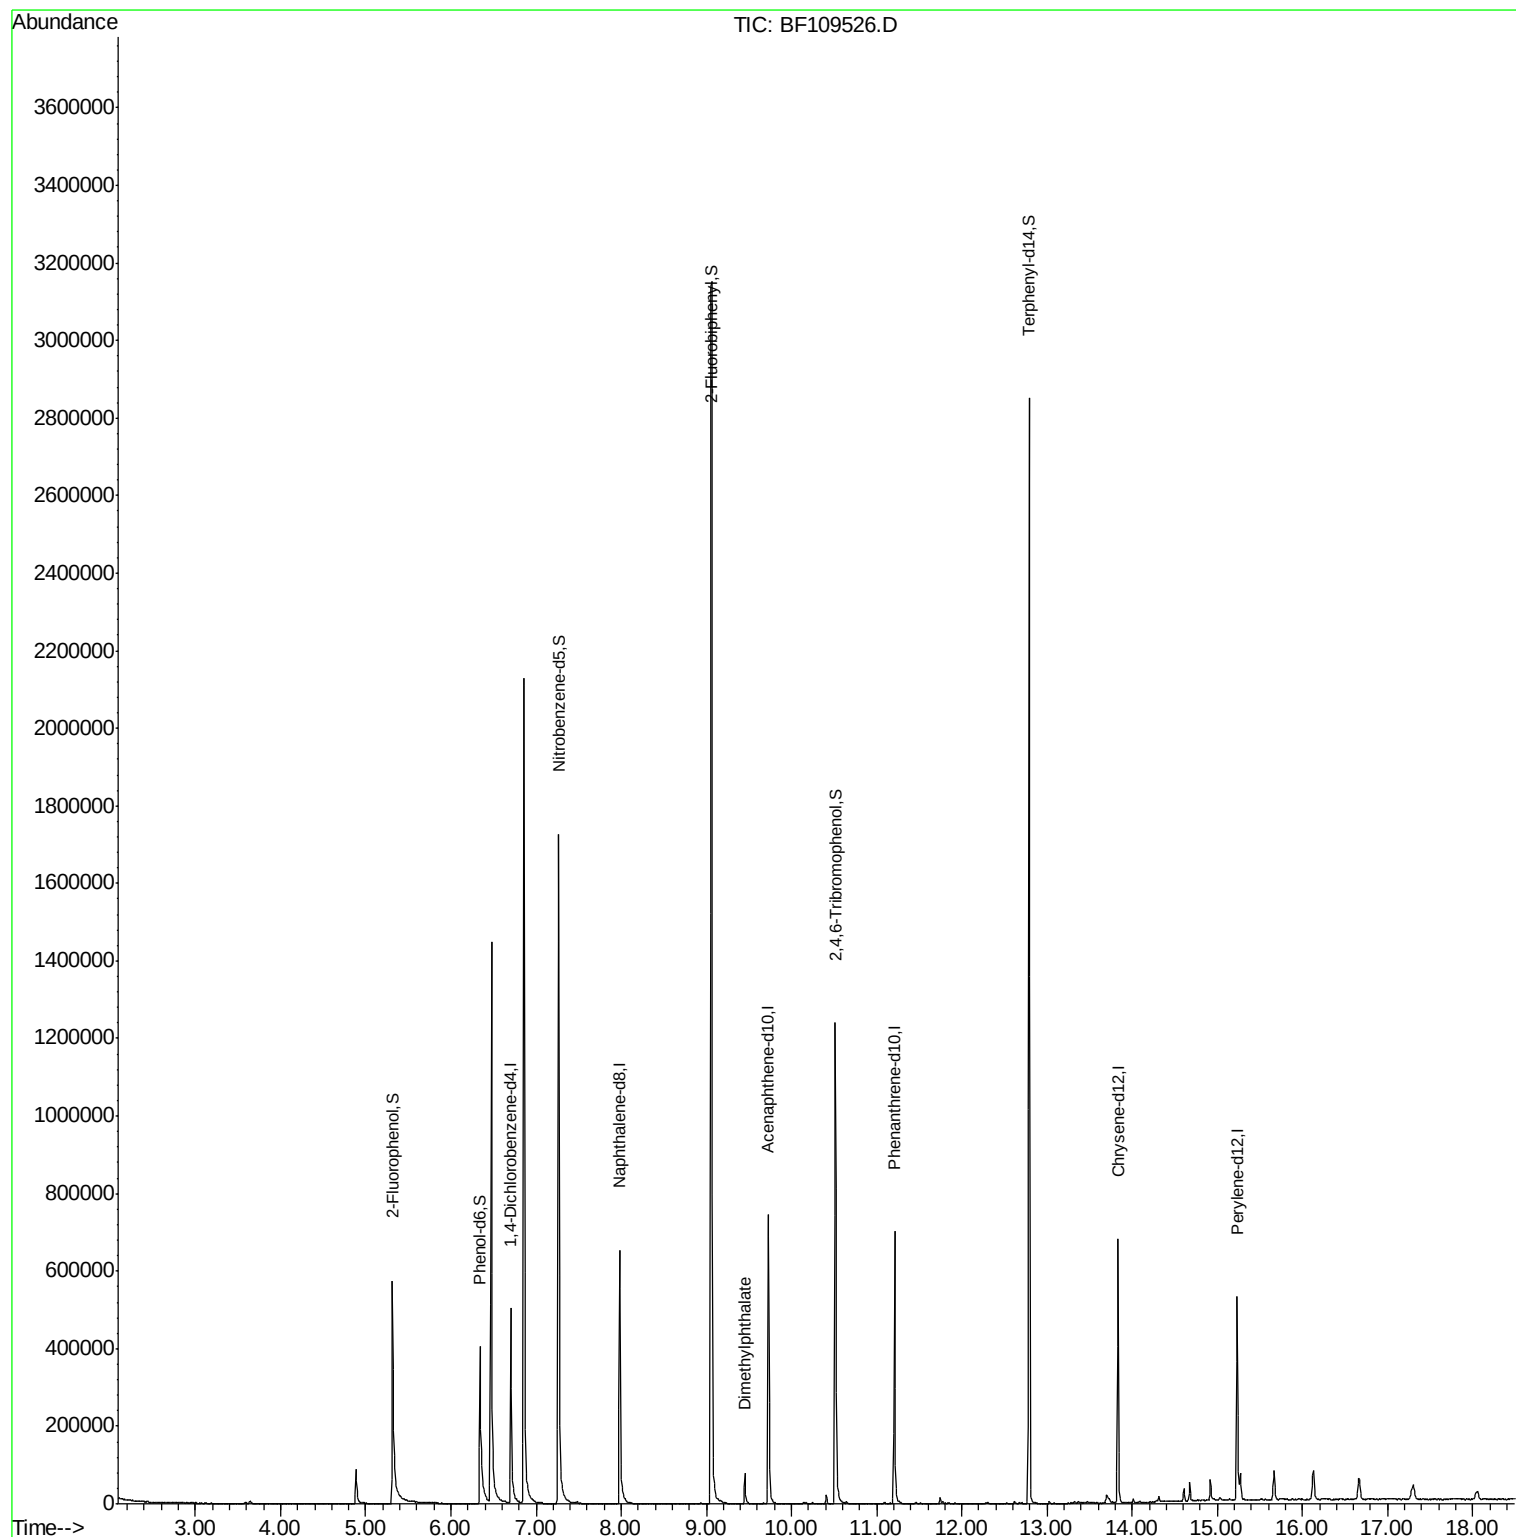

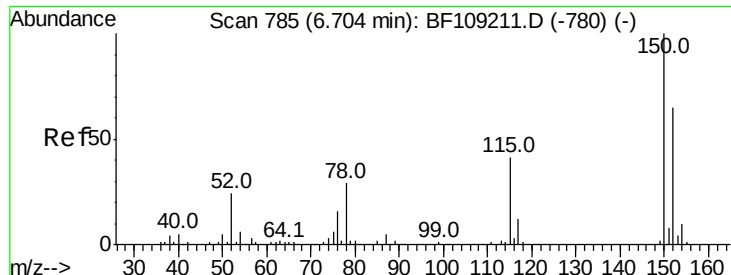


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.70 min Scan# 785
 Delta R.T. -0.01 min
 Lab File: BF109526.D
 Acq: 3 Oct 2018 3:11

Instrument :
 BNA_F
 ClientSampleId :
 092818-JETT-F-U-M

Tot Ion:152 Resp: 101809
 Ion Ratio Lower Upper
 152 100
 150 153.5 124.6 186.8
 115 58.9 50.1 75.1

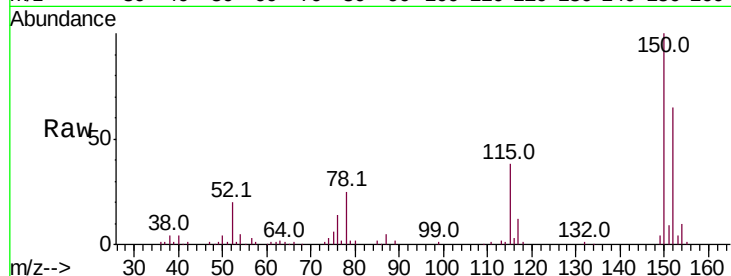


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

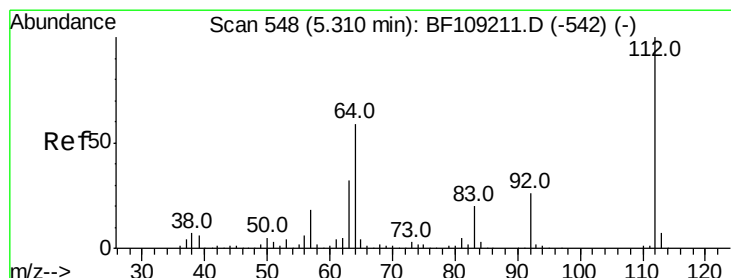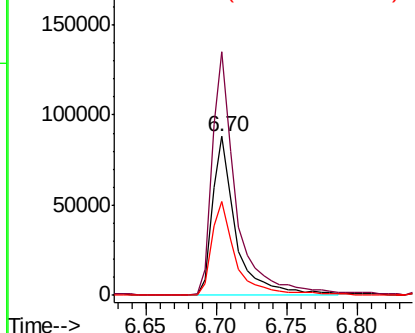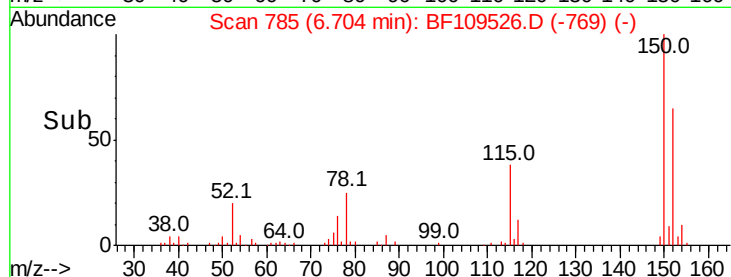



#5


2-Fluorophenol
 Concen: 42.733 ng
 RT: 5.32 min Scan# 549
 Delta R.T. -0.00 min
 Lab File: BF109526.D
 Acq: 3 Oct 2018 3:11

Tgt Ion:112 Resp: 264141
 Ion Ratio Lower Upper
 112 100
 64 56.6 47.9 71.9
 63 29.2 23.7 35.5

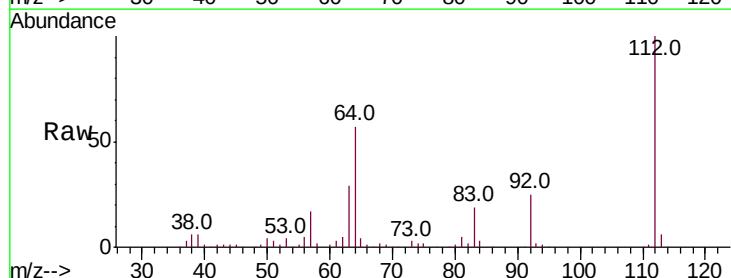

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

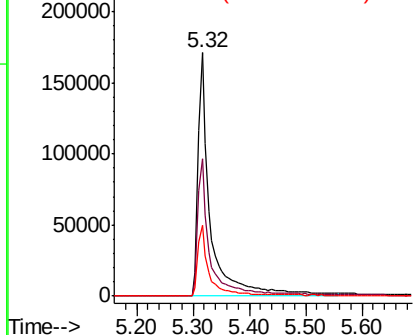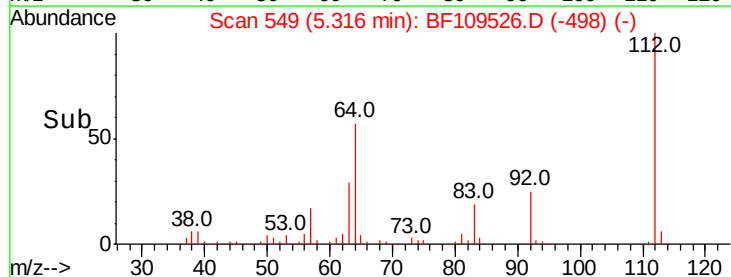

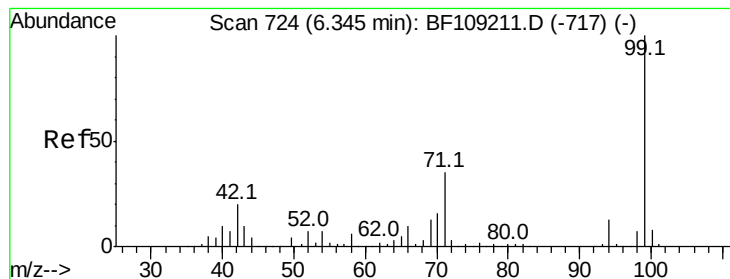

#7

Phenol-d6

Concen: 26.442 ng

RT: 6.34 min Scan# 723

Delta R.T. -0.02 min

Lab File: BF109526.D

Acq: 3 Oct 2018 3:11

Instrument :

BNA_F

ClientSampleId :

092818-JETT-F-U-M


Tot Ion: 99 Resp: 208556

Ion Ratio Lower Upper

99 100

42 18.0 14.5 21.7

71 33.3 25.4 38.0

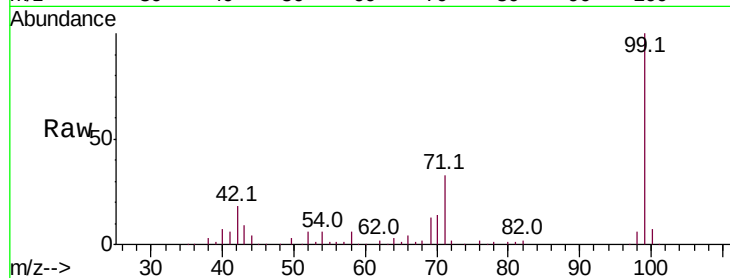

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

200000



150000

100000

50000

0

Time--> 6.30 6.40 6.50

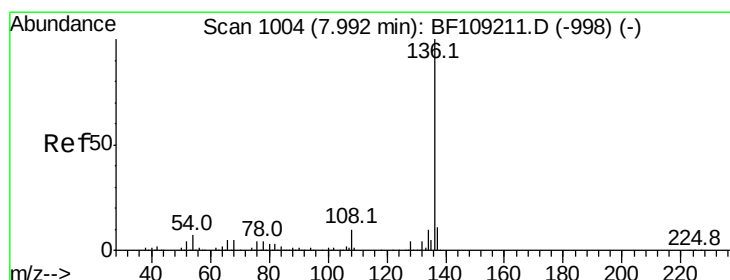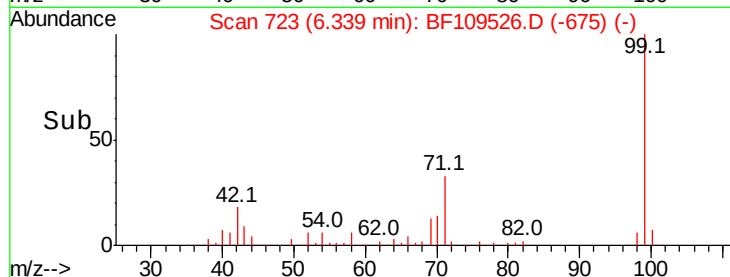

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.98 min Scan# 1002

Delta R.T. -0.01 min

Lab File: BF109526.D

Acq: 3 Oct 2018 3:11

Tgt Ion: 136 Resp: 380426


Ion Ratio Lower Upper

136 100

137 11.1 8.9 13.3

54 7.1 6.6 9.8

68 5.8 5.0 7.4

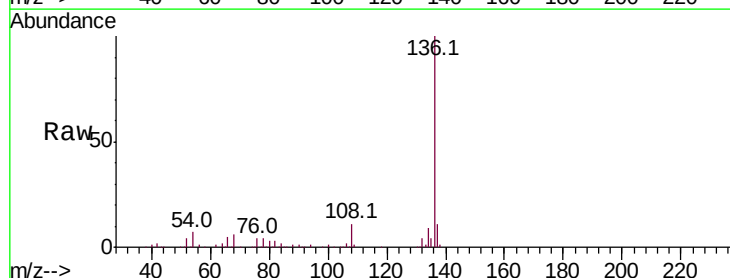

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

500000

400000


300000


200000

100000

0

Time--> 7.90 8.00 8.10 8.20




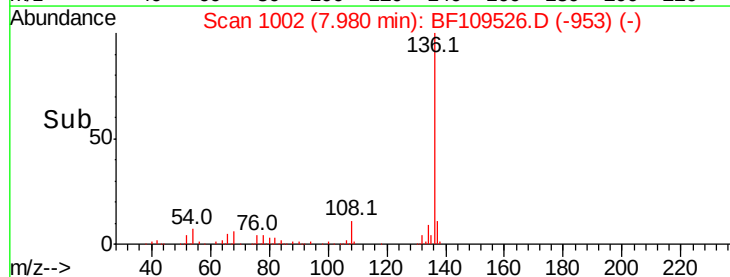


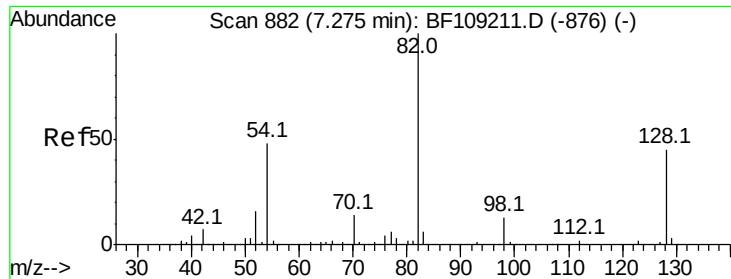

#23
 Nitrobenzene-d5
 Concen: 107.138 ng
 RT: 7.27 min Scan# 881
 Delta R.T. -0.01 min
 Lab File: BF109526.D
 Acq: 3 Oct 2018 3:11




Instrument :
 BNA_F
 ClientSampleId :
 092818-JETT-F-U-M


Tot Ion: 82 Resp: 690443
 Ion Ratio Lower Upper
 82 100
 128 44.4 36.1 54.1
 54 47.0 41.4 62.2

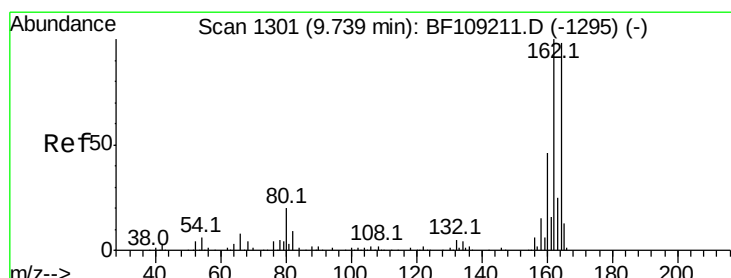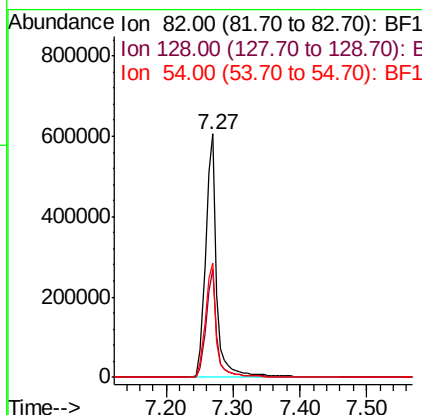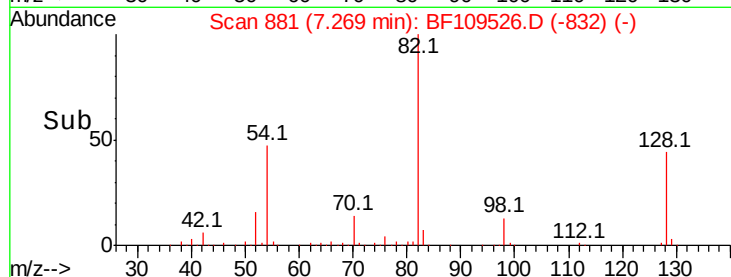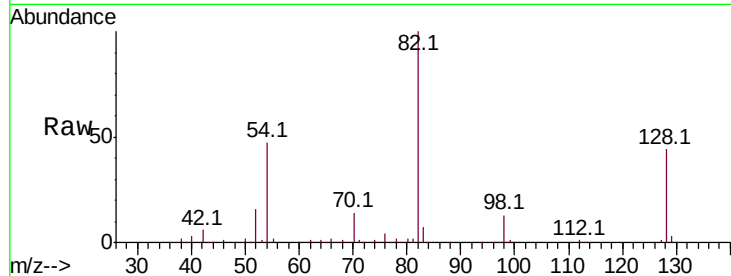

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.73 min Scan# 1299
 Delta R.T. -0.01 min
 Lab File: BF109526.D
 Acq: 3 Oct 2018 3:11

Tgt Ion:164 Resp: 170445
 Ion Ratio Lower Upper
 164 100
 162 102.5 86.1 129.1
 160 46.8 38.3 57.5

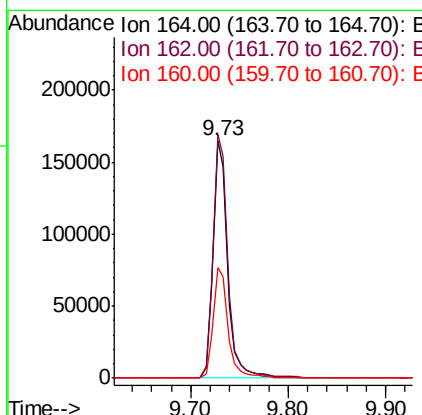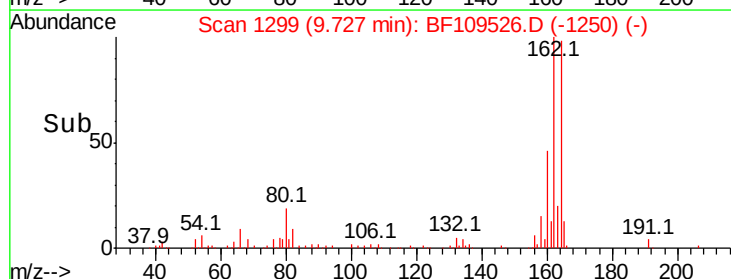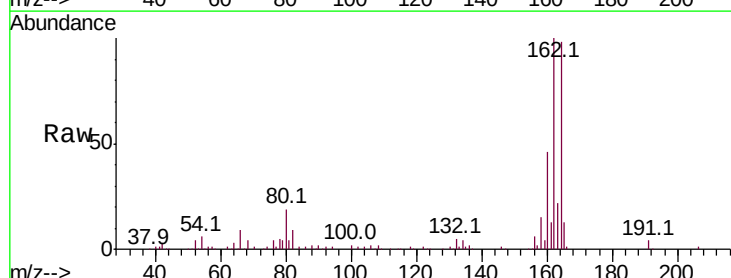


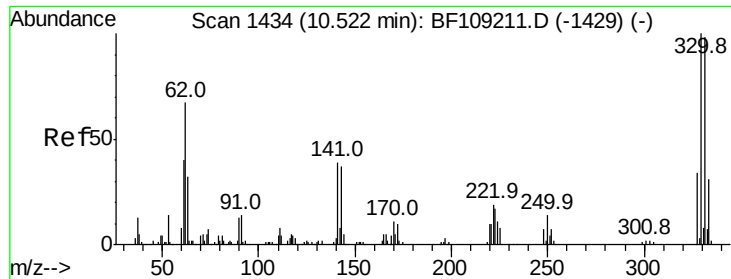




#41
 2,4,6-Tribromophenol
 Concen: 98.527 ng
 RT: 10.52 min Scan# 1433
 Delta R.T. -0.02 min
 Lab File: BF109526.D
 Acq: 3 Oct 2018 3:11

Instrument :
 BNA_F
 ClientSampleId :
 092818-JETT-F-U-M

Tot Ion:330 Resp: 165548
 Ion Ratio Lower Upper
 330 100
 332 95.5 77.0 115.6
 141 33.4 29.9 44.9

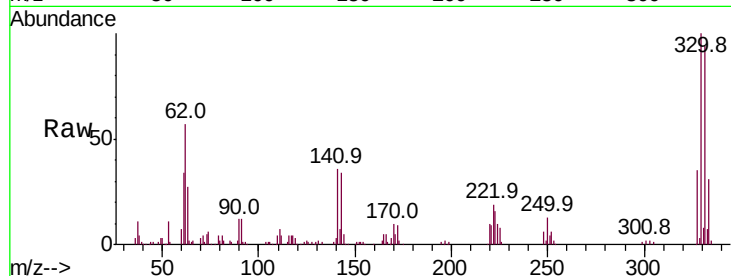


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

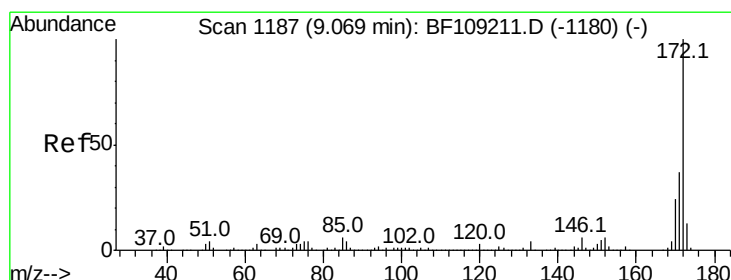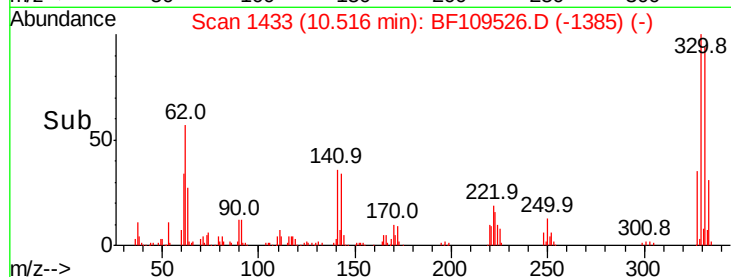
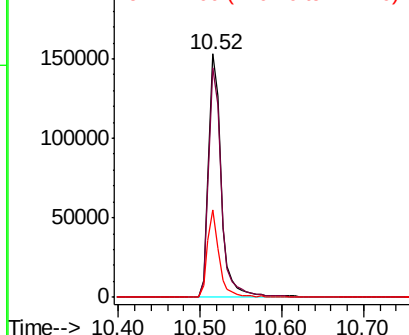



#44
 2-Fluorobiphenyl
 Concen: 105.324 ng
 RT: 9.06 min Scan# 1186
 Delta R.T. -0.01 min
 Lab File: BF109526.D
 Acq: 3 Oct 2018 3:11

Tgt Ion:172 Resp: 1190300
 Ion Ratio Lower Upper
 172 100
 171 36.2 29.7 44.5
 170 24.2 19.6 29.4

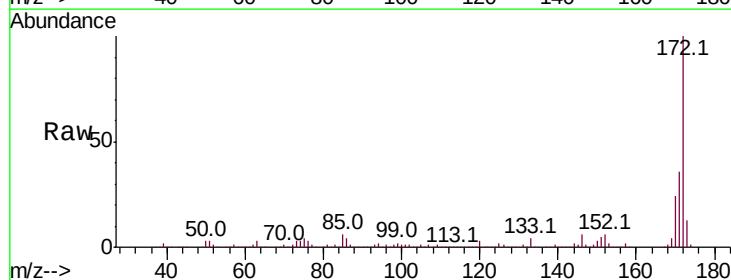

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

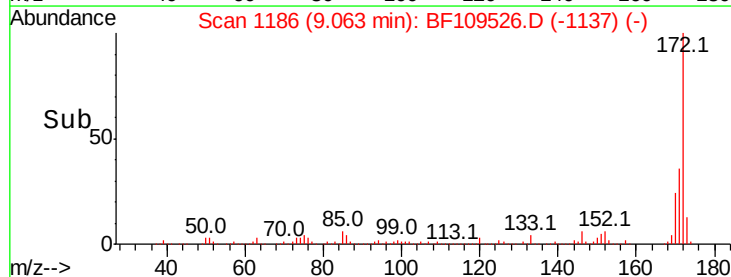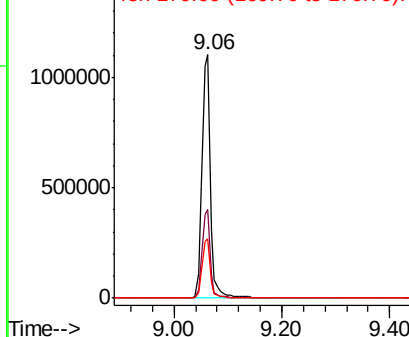


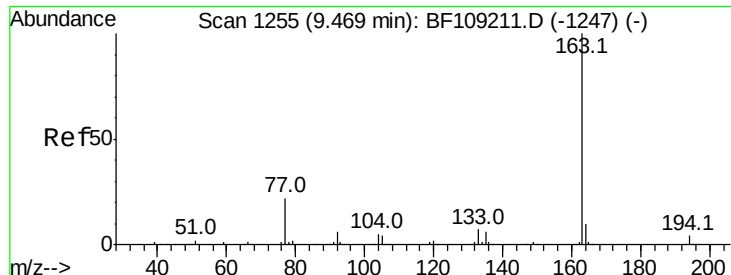




#49
Dimethylphthalate
Concen: 3.376 ng
RT: 9.45 min Scan# 1252
Delta R.T. -0.03 min
Lab File: BF109526.D
Acq: 3 Oct 2018 3:11

Instrument :
BNA_F
ClientSampleId :
092818-JETT-F-U-M

Tot Ion:163 Resp: 41848
Ion Ratio Lower Upper
163 100
194 4.0 2.7 4.1
164 9.9 8.2 12.2

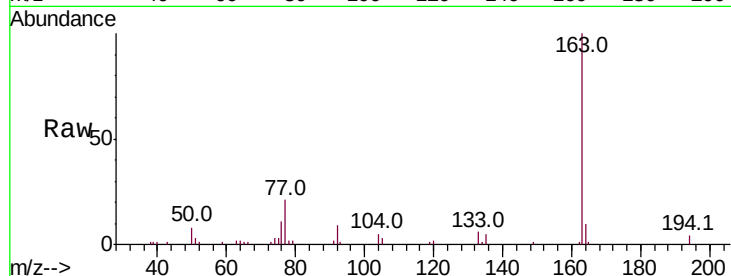


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

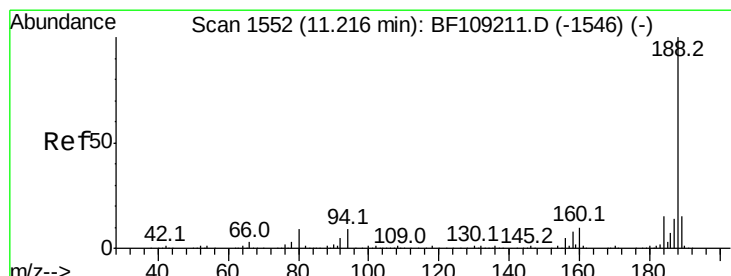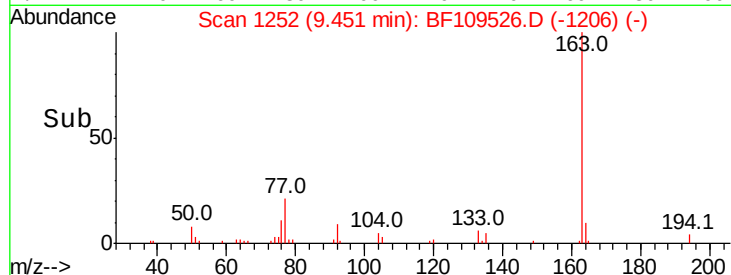
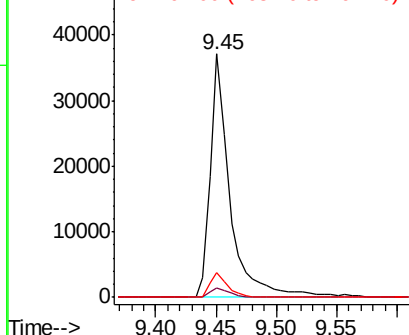



#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.21 min Scan# 1551
Delta R.T. -0.01 min
Lab File: BF109526.D
Acq: 3 Oct 2018 3:11

Tgt Ion:188 Resp: 301201
Ion Ratio Lower Upper
188 100
94 8.5 8.5 12.7
80 9.1 9.2 13.8#

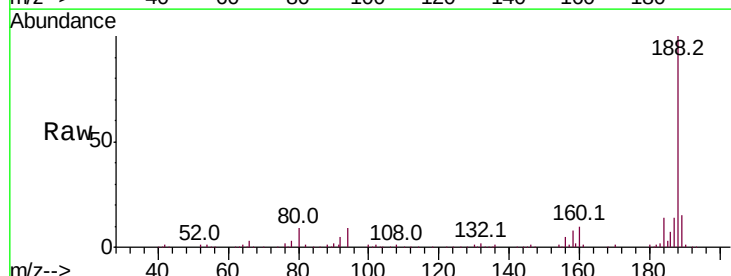

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

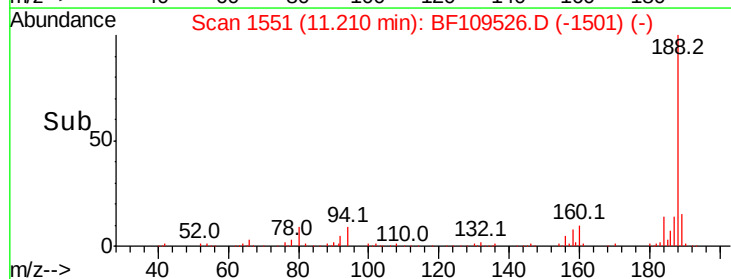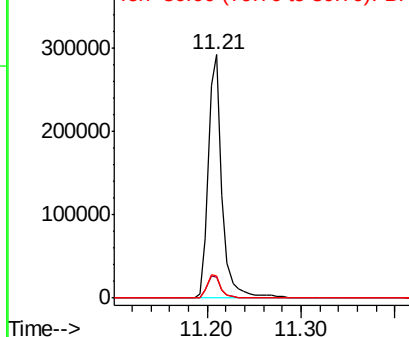

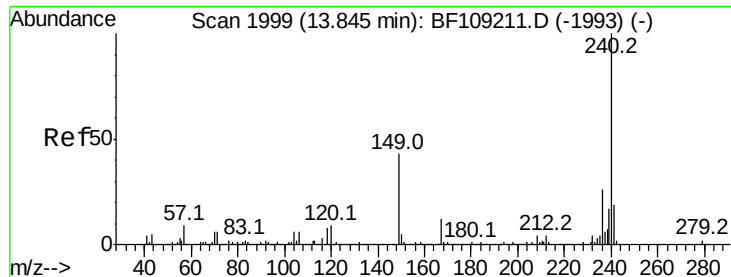

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.83 min Scan# 1997

Delta R.T. -0.01 min

Lab File: BF109526.D

Acq: 3 Oct 2018 3:11

Instrument :

BNA_F

ClientSampleId :

092818-JETT-F-U-M


Tot Ion:240 Resp: 241156

Ion Ratio Lower Upper

240 100

120 11.1 9.5 14.3




236 25.8 20.7 31.1

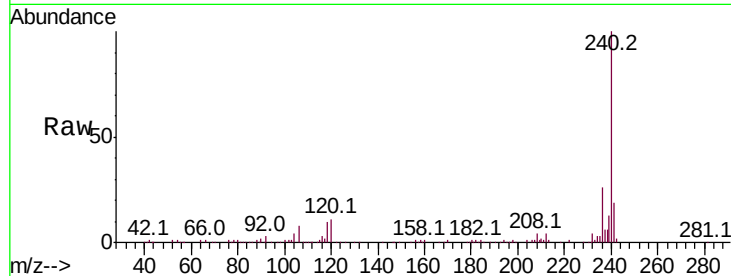

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

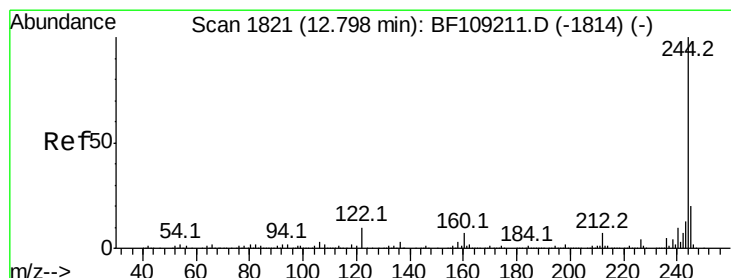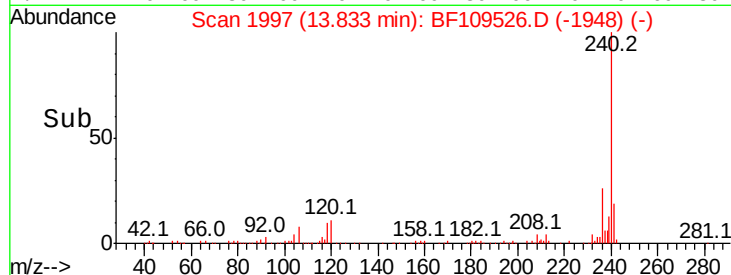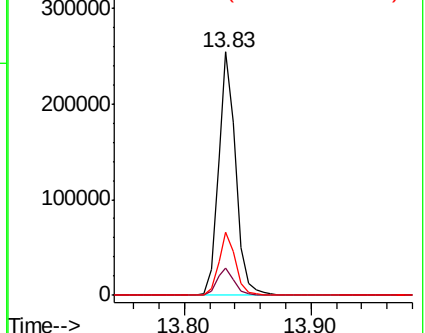

#78

Terphenyl-d14

Concen: 103.938 ng

RT: 12.79 min Scan# 1820

Delta R.T. -0.01 min

Lab File: BF109526.D

Acq: 3 Oct 2018 3:11


Tgt Ion:244 Resp: 1021340

Ion Ratio Lower Upper

244 100

212 7.3 5.4 8.0



122 11.5 11.0 16.4

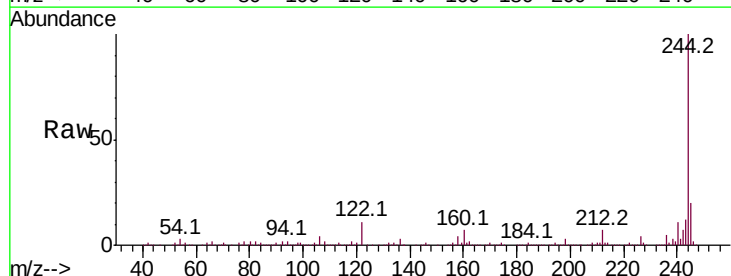


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

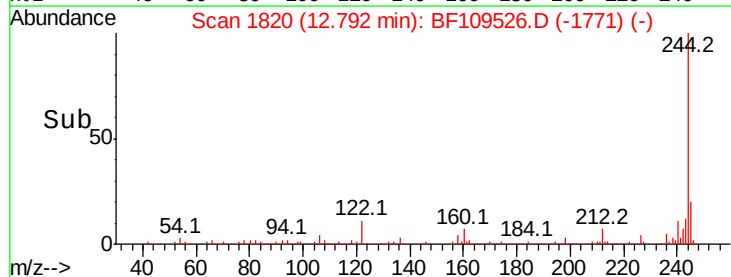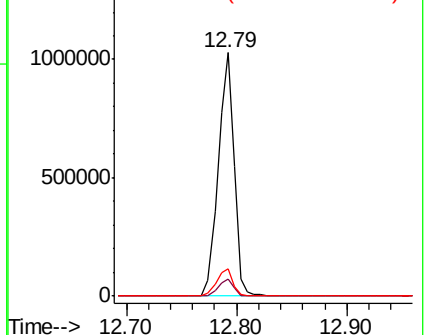

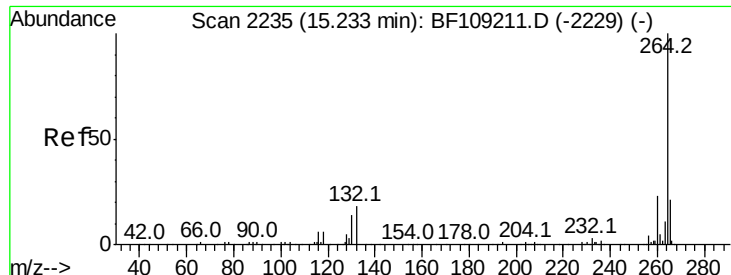

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.23 min Scan# 2235
Delta R.T. -0.01 min
Lab File: BF109526.D
Acq: 3 Oct 2018 3:11

Instrument :
BNA_F
ClientSampleId :
092818-JETT-F-U-M

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.8	19.2	28.8
265	21.9	17.5	26.3

