

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF100218\
 Data File : BF109527.D
 Acq On : 3 Oct 2018 3:37
 Operator : JU/SJ
 Sample : J5187-06
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 092818-JETT-F-U-S

Quant Time: Oct 03 05:07:31 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 22 13:32:18 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.70	152	99982	20.00	ng	0.00
21) Naphthalene-d8	7.98	136	383933	20.00	ng	-0.01
38) Acenaphthene-d10	9.73	164	178258	20.00	ng	-0.01
63) Phenanthrene-d10	11.21	188	325675	20.00	ng	0.00
75) Chrysene-d12	13.83	240	249543	20.00	ng	-0.01
86) Perylene-d12	15.23	264	251451	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	239627	39.48	ng	0.00
7) Phenol-d6	6.34	99	194991	25.17	ng	-0.02
23) Nitrobenzene-d5	7.27	82	674515	103.71	ng	-0.01
41) 2,4,6-Tribromophenol	10.52	330	179425	102.11	ng	-0.02
44) 2-Fluorobiphenyl	9.06	172	1218516	103.10	ng	-0.01
78) Terphenyl-d14	12.79	244	1079660	106.18	ng	-0.01
Target Compounds						
49) Dimethylphthalate	9.45	163	41802	3.224	ng	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF100218\
Data File : BF109527.D
Acq On : 3 Oct 2018 3:37
Operator : JU/SJ
Sample : J5187-06
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
092818-JETT-F-U-S

Quant Time: Oct 03 05:07:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

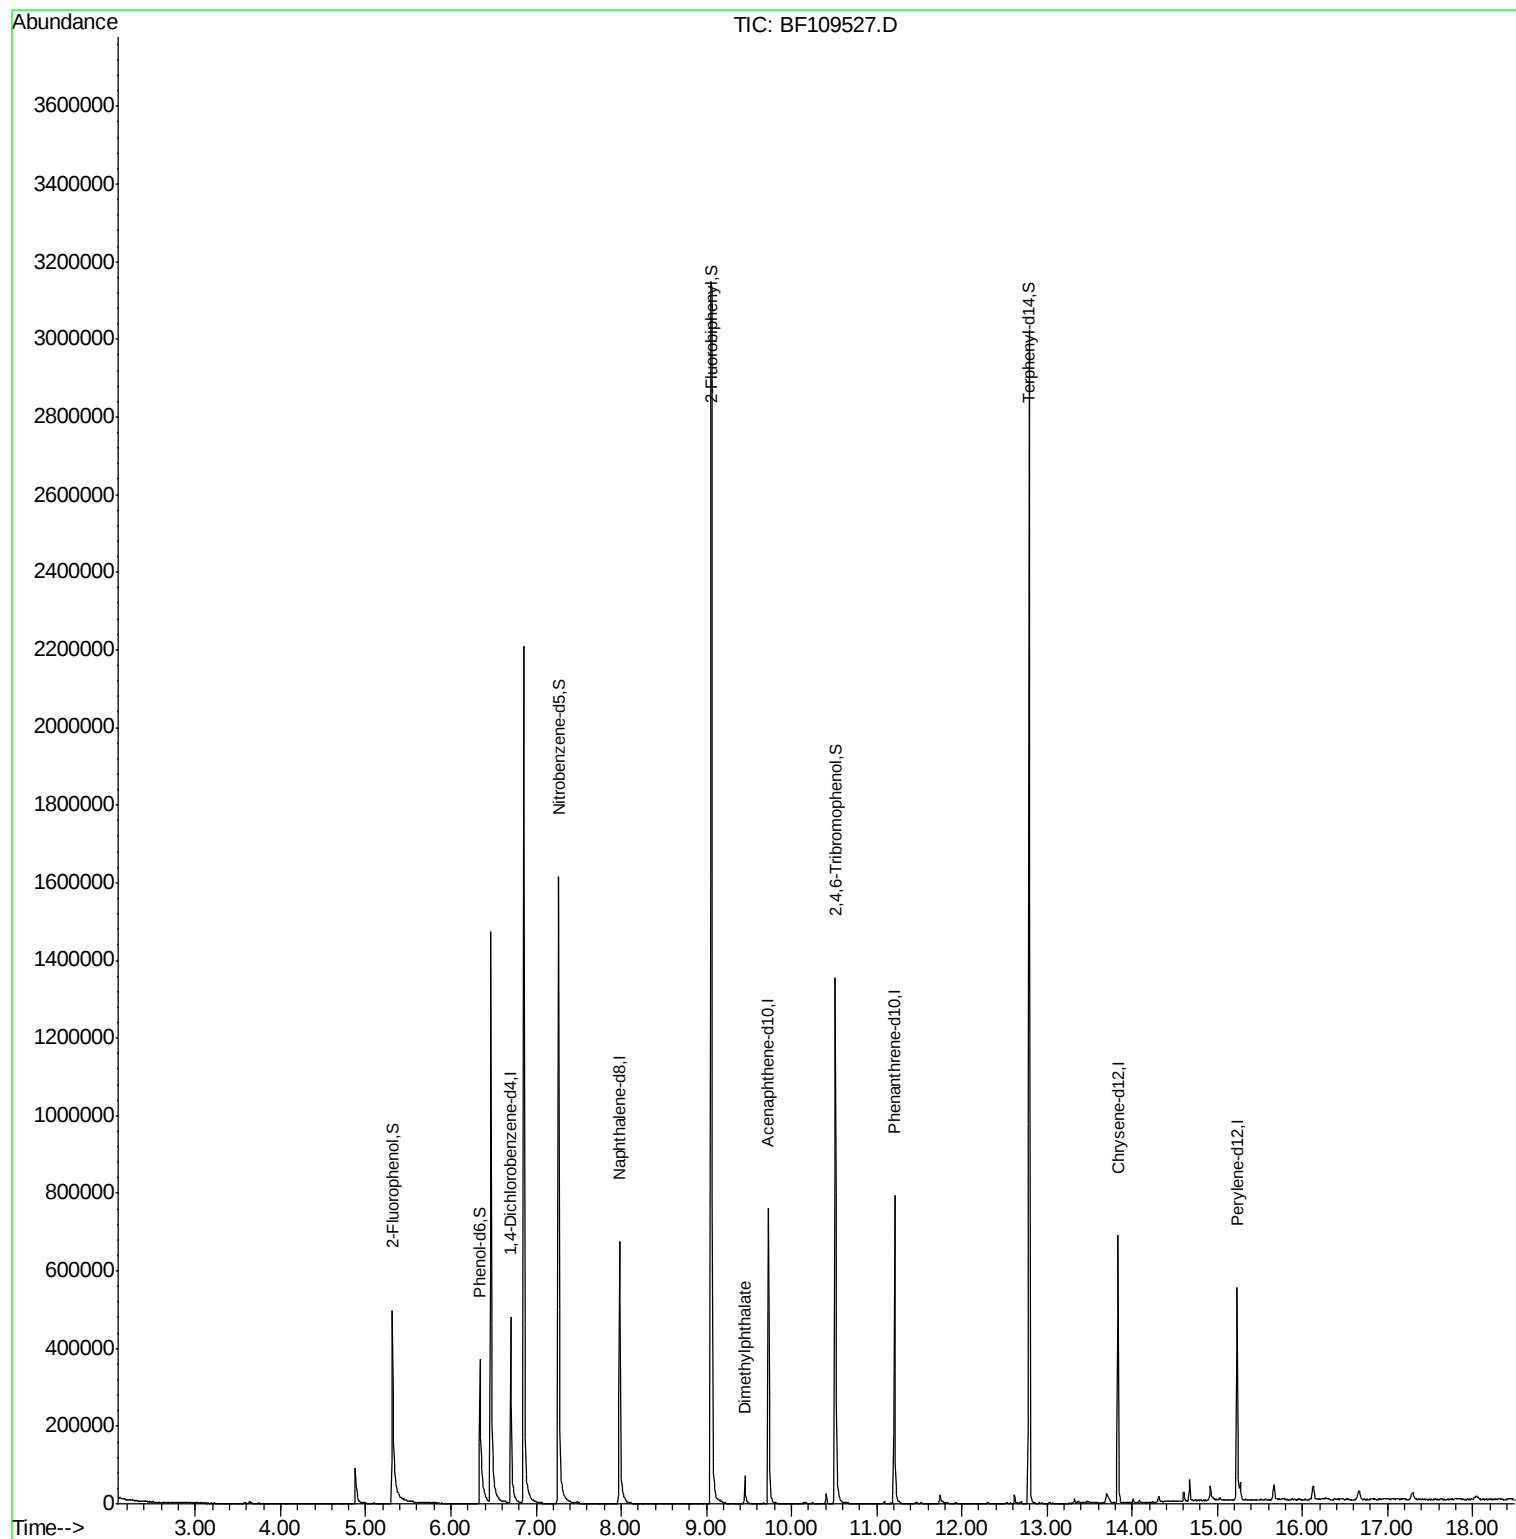




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.70 min Scan# 785
Delta R.T. -0.01 min
Lab File: BF109527.D
Acq: 3 Oct 2018 3:37

Instrument :
BNA_F
ClientSampleId :
092818-JETT-F-U-S

Tot Ion:152 Resp: 99982
Ion Ratio Lower Upper
152 100
150 154.1 124.6 186.8
115 58.2 50.1 75.1

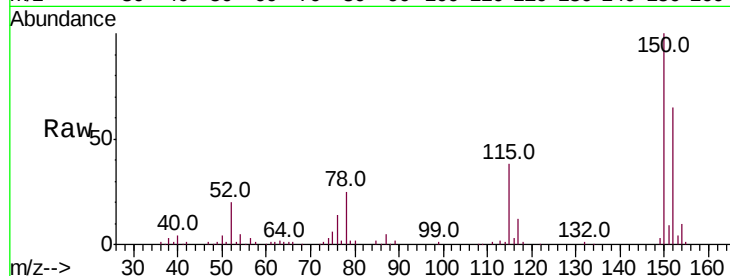


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

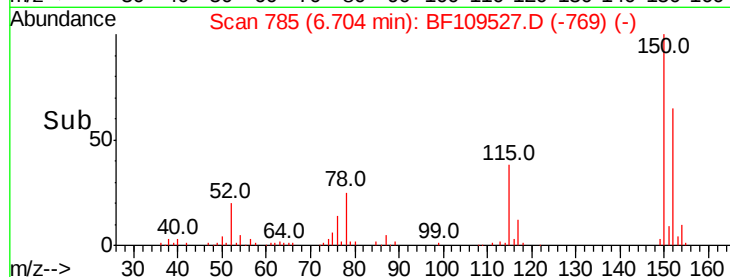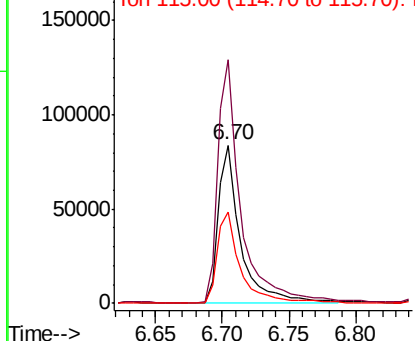



#5

2-Fluorophenol
Concen: 39.476 ng
RT: 5.32 min Scan# 549
Delta R.T. 0.00 min
Lab File: BF109527.D
Acq: 3 Oct 2018 3:37

Tgt Ion:112 Resp: 239627
Ion Ratio Lower Upper
112 100
64 55.0 47.9 71.9
63 28.9 23.7 35.5

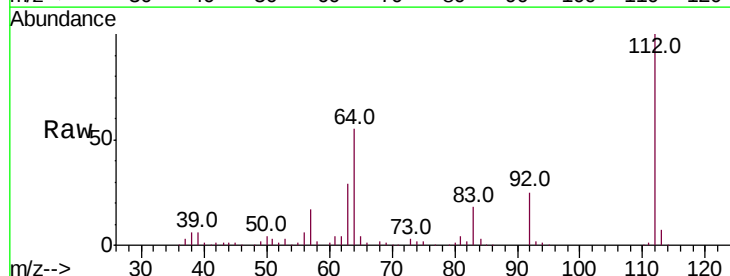

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

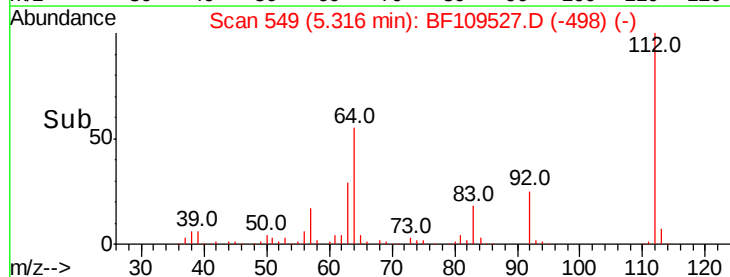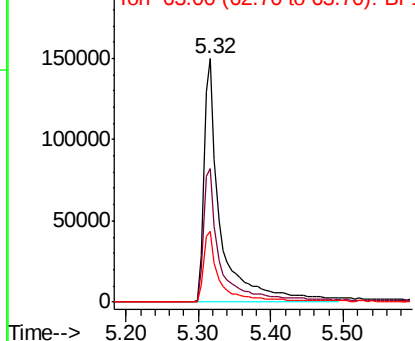



#7

Phenol-d6

Concen: 25.173 ng

RT: 6.34 min Scan# 723

Delta R.T. -0.02 min

Lab File: BF109527.D

Acq: 3 Oct 2018 3:37

Instrument :

BNA_F

ClientSampleId :

092818-JETT-F-U-S


Tot Ion: 99 Resp: 194991

Ion Ratio Lower Upper




99 100

42 17.7 14.5 21.7

71 33.1 25.4 38.0

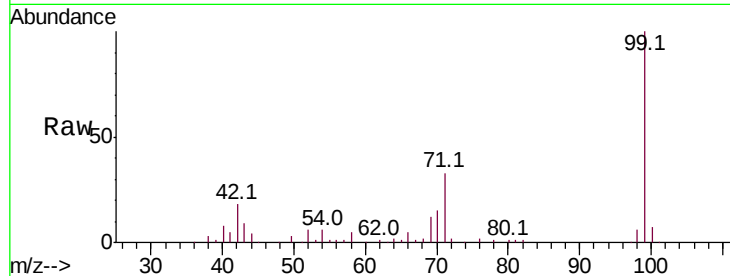

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

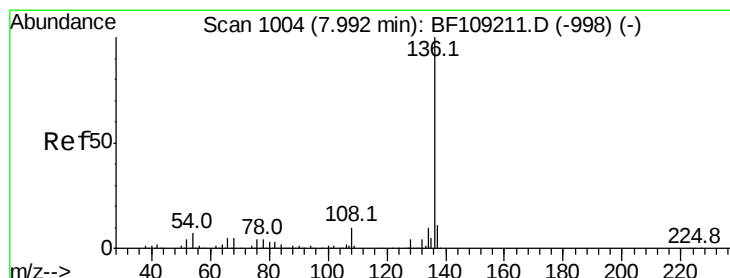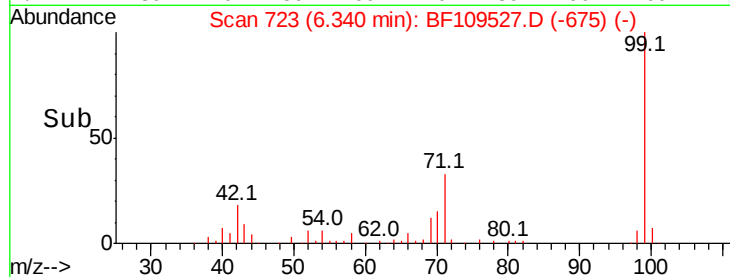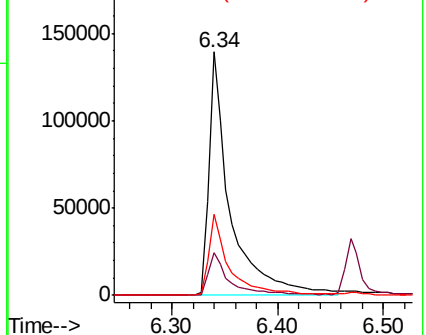

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.98 min Scan# 1002

Delta R.T. -0.01 min

Lab File: BF109527.D

Acq: 3 Oct 2018 3:37

Tgt Ion: 136 Resp: 383933


Ion Ratio Lower Upper

136 100



137 10.9 8.9 13.3

54 7.4 6.6 9.8

68 5.7 5.0 7.4

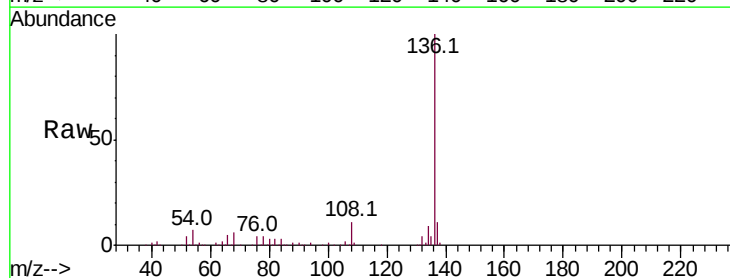

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

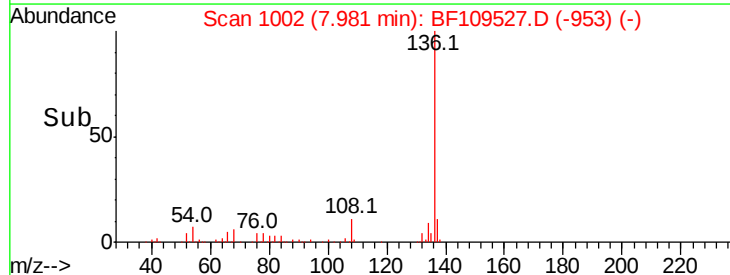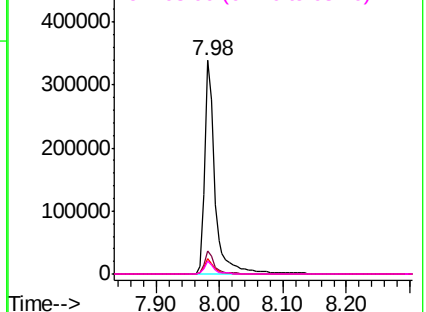







#23
 Nitrobenzene-d5
 Concen: 103.710 ng
 RT: 7.27 min Scan# 881
 Delta R.T. -0.01 min
 Lab File: BF109527.D
 Acq: 3 Oct 2018 3:37

Instrument :
 BNA_F
 ClientSampleId :
 092818-JETT-F-U-S

Tot Ion: 82 Resp: 674515
 Ion Ratio Lower Upper
 82 100
 128 45.0 36.1 54.1
 54 46.4 41.4 62.2

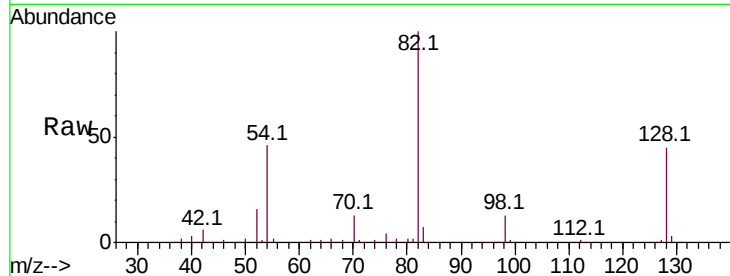


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

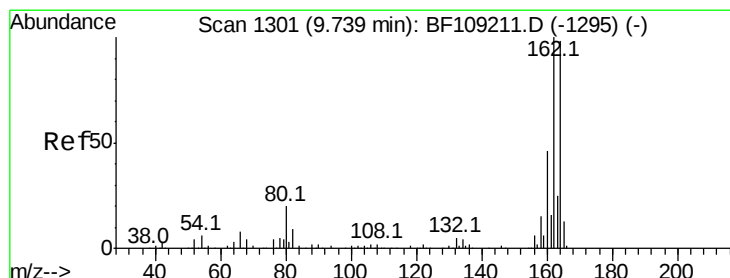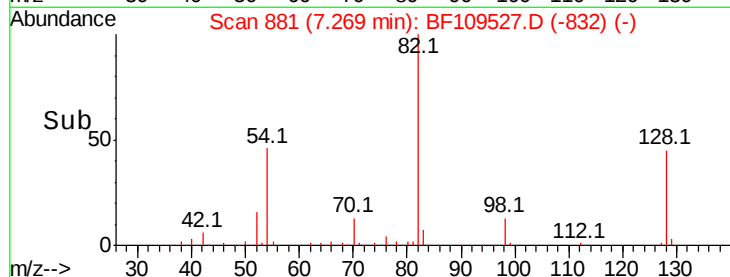
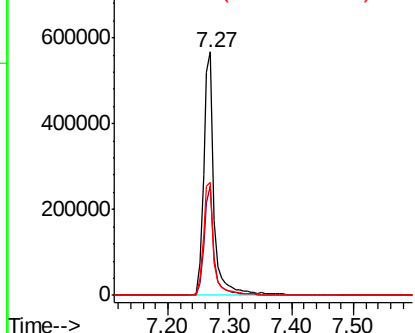


#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.73 min Scan# 1299
 Delta R.T. -0.01 min
 Lab File: BF109527.D
 Acq: 3 Oct 2018 3:37

Tgt Ion: 164 Resp: 178258
 Ion Ratio Lower Upper
 164 100
 162 100.7 86.1 129.1
 160 45.9 38.3 57.5

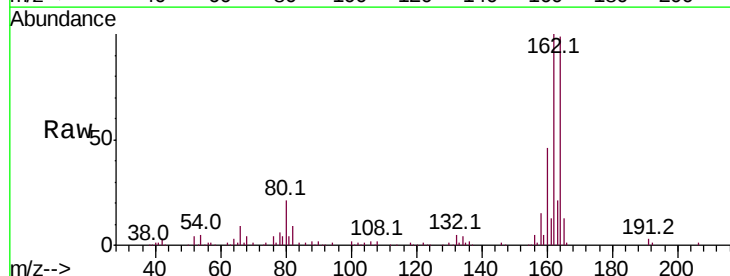

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

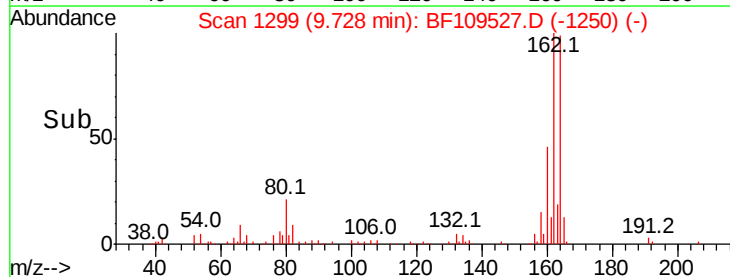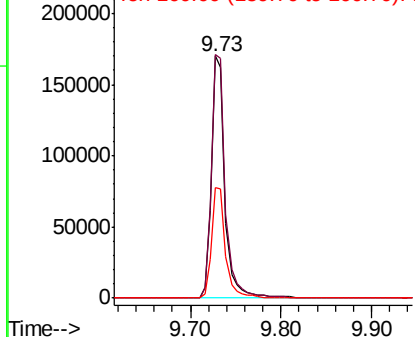







#41
 2,4,6-Tribromophenol
 Concen: 102.105 ng
 RT: 10.52 min Scan# 1433
 Delta R.T. -0.02 min
 Lab File: BF109527.D
 Acq: 3 Oct 2018 3:37

Instrument :
 BNA_F
 ClientSampleId :
 092818-JETT-F-U-S

Tot Ion:330 Resp: 179425
 Ion Ratio Lower Upper
 330 100
 332 94.3 77.0 115.6
 141 33.2 29.9 44.9

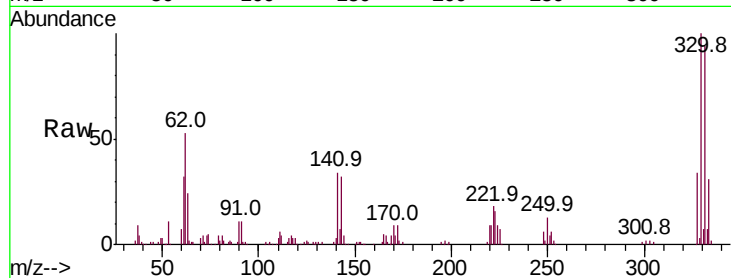


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

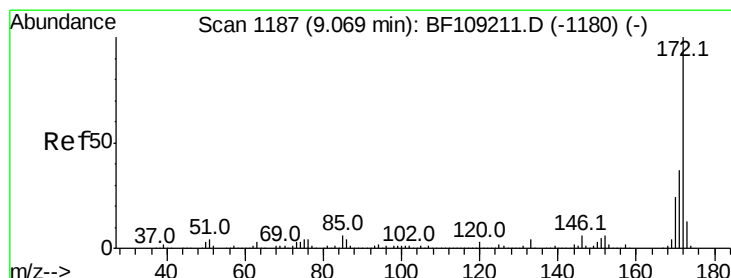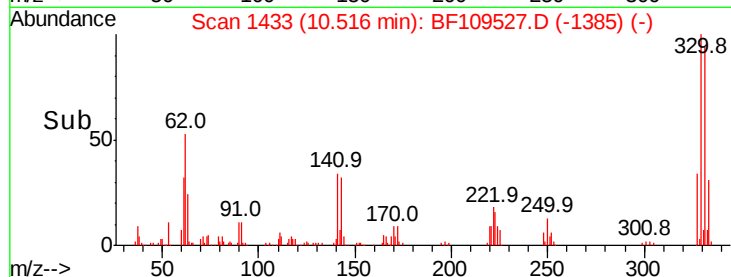
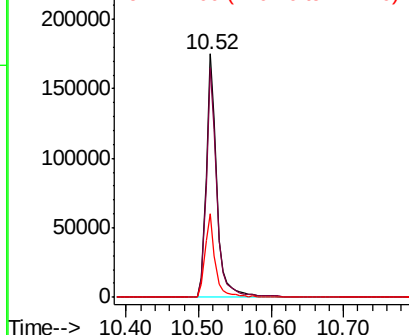



#44
 2-Fluorobiphenyl
 Concen: 103.095 ng
 RT: 9.06 min Scan# 1186
 Delta R.T. -0.01 min
 Lab File: BF109527.D
 Acq: 3 Oct 2018 3:37

Tgt Ion:172 Resp: 1218516
 Ion Ratio Lower Upper
 172 100
 171 35.6 29.7 44.5
 170 23.6 19.6 29.4

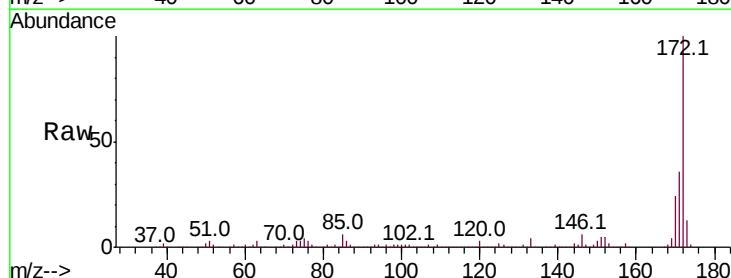

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

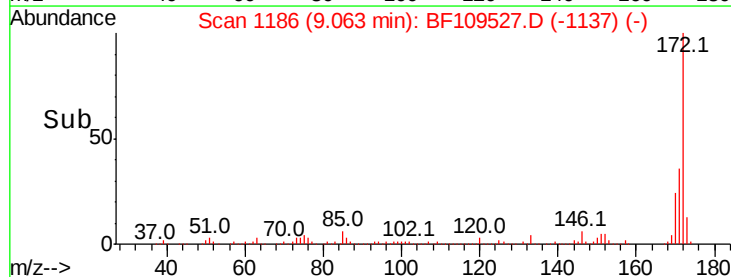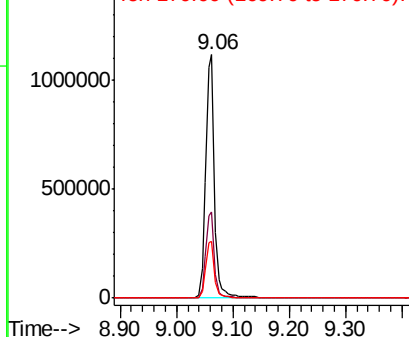

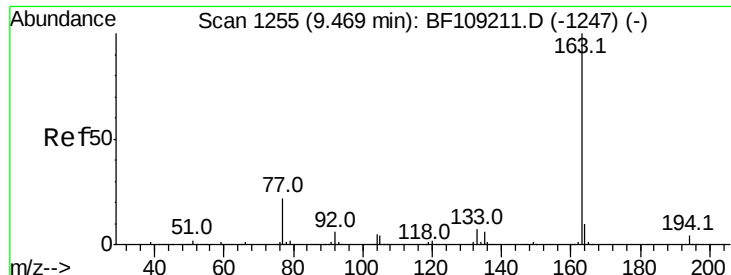

#49

Dimethylphthalate

Concen: 3.224 ng

RT: 9.45 min Scan# 1252

Delta R.T. -0.03 min

Lab File: BF109527.D

Acq: 3 Oct 2018 3:37

Instrument :

BNA_F

ClientSampleId :

092818-JETT-F-U-S


Tot Ion:163 Resp: 41802

Ion Ratio Lower Upper

163 100

194 4.0 2.7 4.1




164 9.8 8.2 12.2

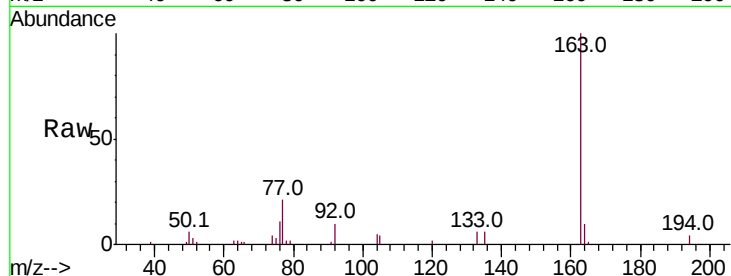

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

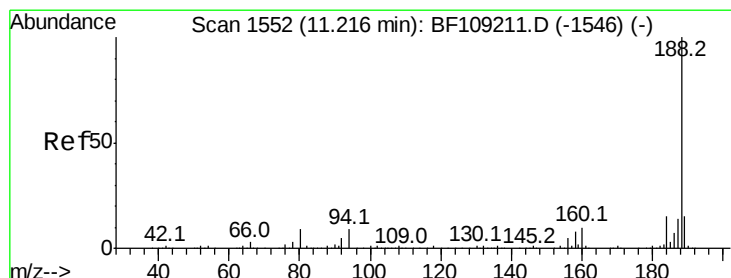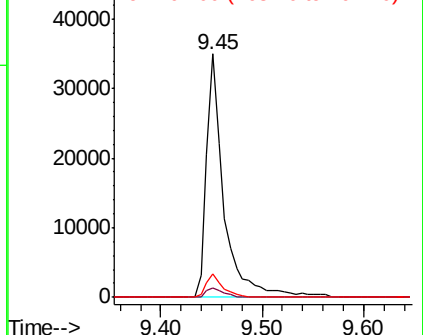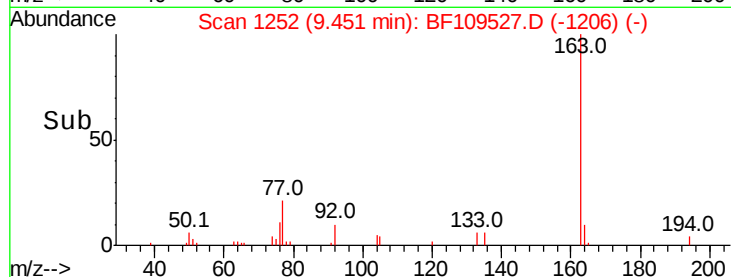

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.21 min Scan# 1551

Delta R.T. -0.01 min

Lab File: BF109527.D

Acq: 3 Oct 2018 3:37


Tgt Ion:188 Resp: 325675

Ion Ratio Lower Upper

188 100

94 8.5 8.5 12.7



80 9.5 9.2 13.8

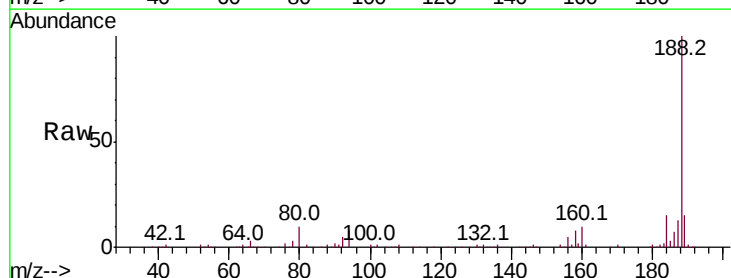

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

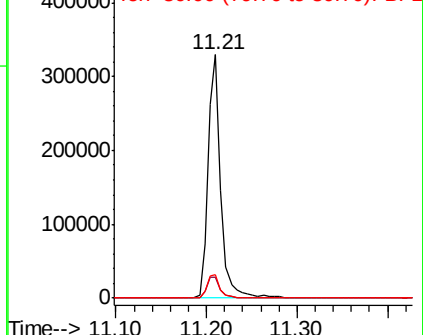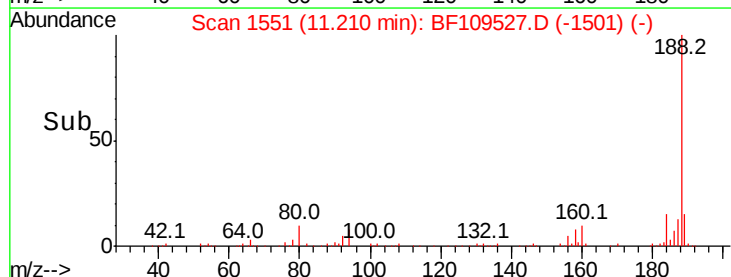



#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.83 min Scan# 1997

Delta R.T. -0.01 min

Lab File: BF109527.D

Acq: 3 Oct 2018 3:37

Instrument :

BNA_F

ClientSampleId :

092818-JETT-F-U-S


Tot Ion:240 Resp: 249543

Ion Ratio Lower Upper

240 100

120 10.7 9.5 14.3



236 24.7 20.7 31.1

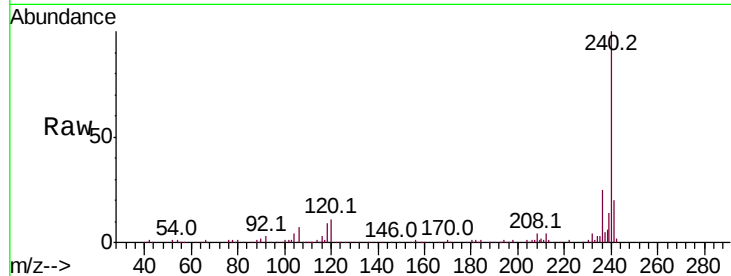

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

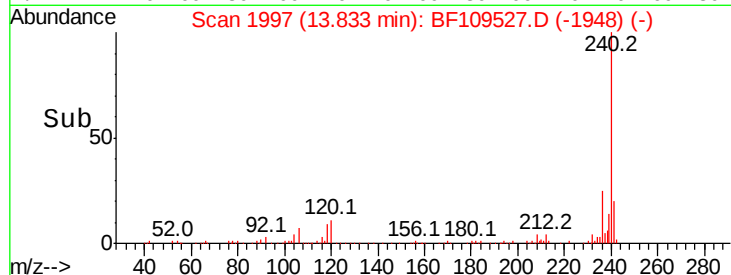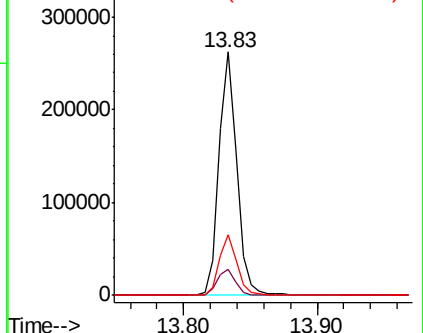

#78

Terphenyl-d14

Concen: 106.181 ng

RT: 12.79 min Scan# 1820

Delta R.T. -0.01 min

Lab File: BF109527.D

Acq: 3 Oct 2018 3:37


Tgt Ion:244 Resp: 1079660

Ion Ratio Lower Upper

244 100

212 7.2 5.4 8.0



122 11.7 11.0 16.4

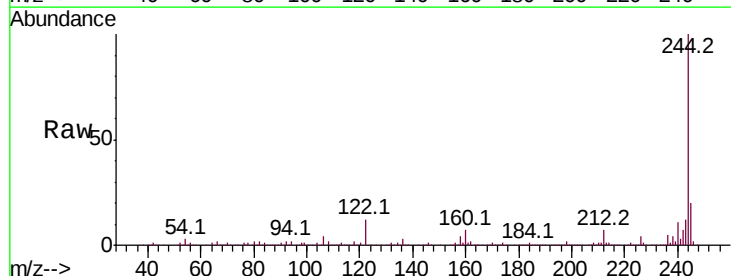


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

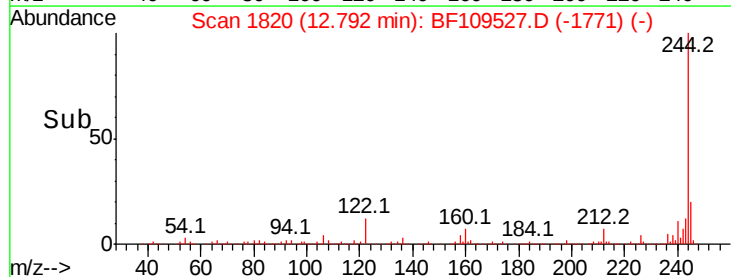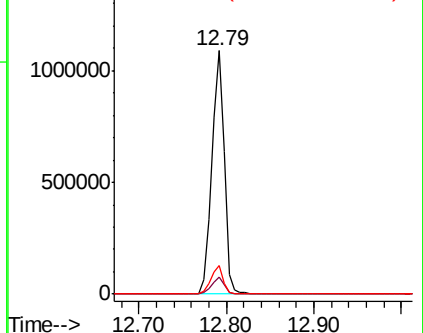

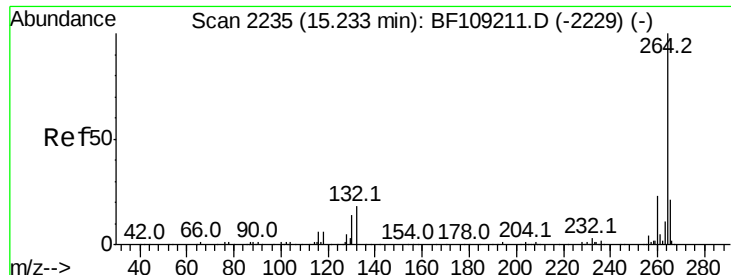

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.23 min Scan# 2235
 Delta R.T. -0.01 min
 Lab File: BF109527.D
 Acq: 3 Oct 2018 3:37

Instrument :
 BNA_F
 ClientSampleId :
 092818-JETT-F-U-S

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.9	19.2	28.8
265	21.5	17.5	26.3

