


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100218\
 Data File : BF109492.D
 Acq On : 2 Oct 2018 11:14
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 22 13:32:18 2018

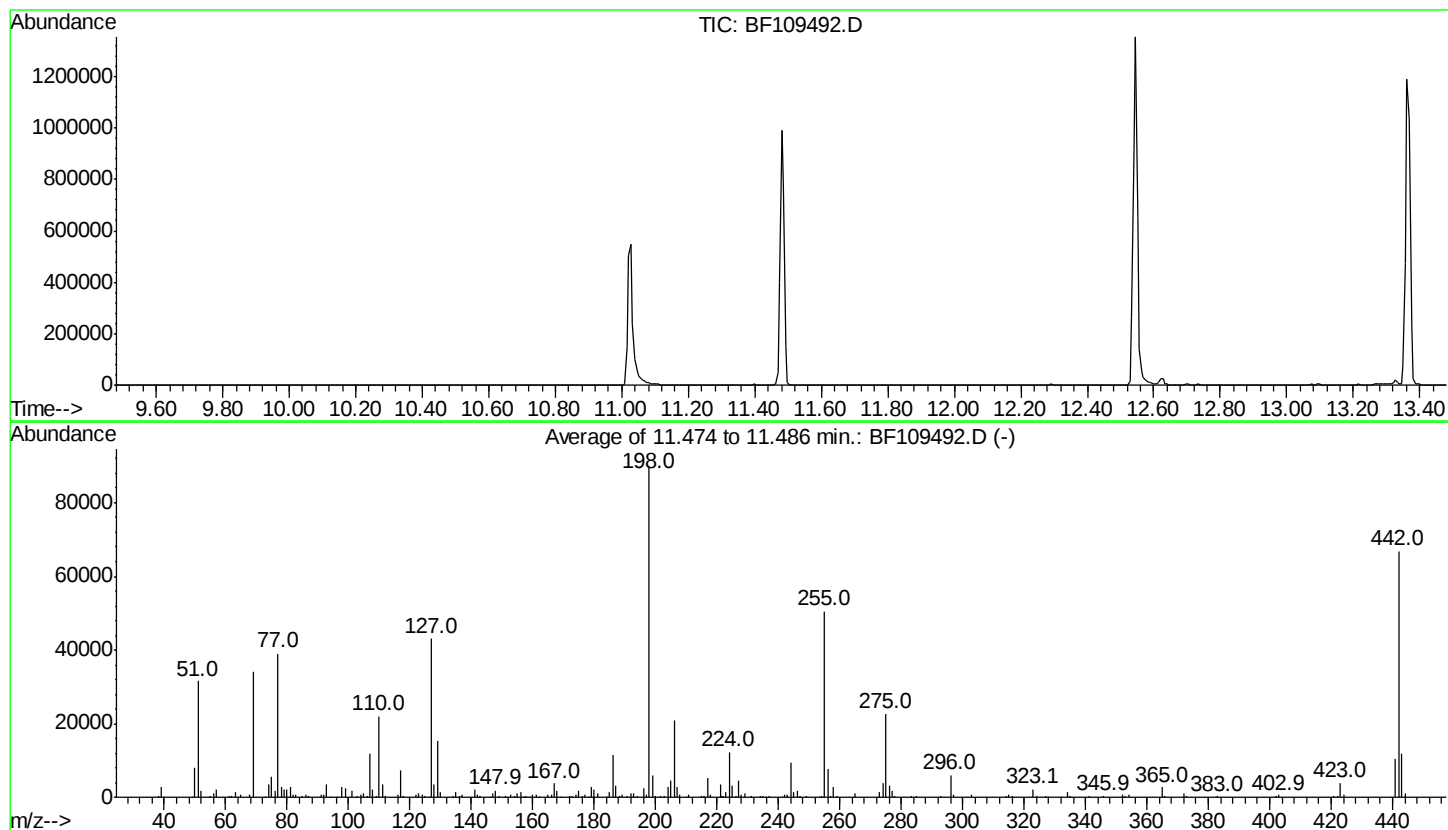

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	31570	PASS
68	69	0.00	2	1.6	537	PASS
69	198	0.00	100	37.8	34034	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.7	42986	PASS
197	198	0.00	2	0.8	715	PASS
198	198	100	100	100.0	90088	PASS
199	198	5	9	6.5	5875	PASS
275	198	10	60	25.3	22764	PASS
365	198	1	100	3.0	2733	PASS
441	198	0.01	100	11.7	10533	PASS
442	198	50	100	74.2	66874	PASS
443	442	15	24	17.8	11897	PASS