


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100220\
 Data File : BF121786.D
 Acq On : 2 Oct 2020 10:56
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 01 14:29:14 2020

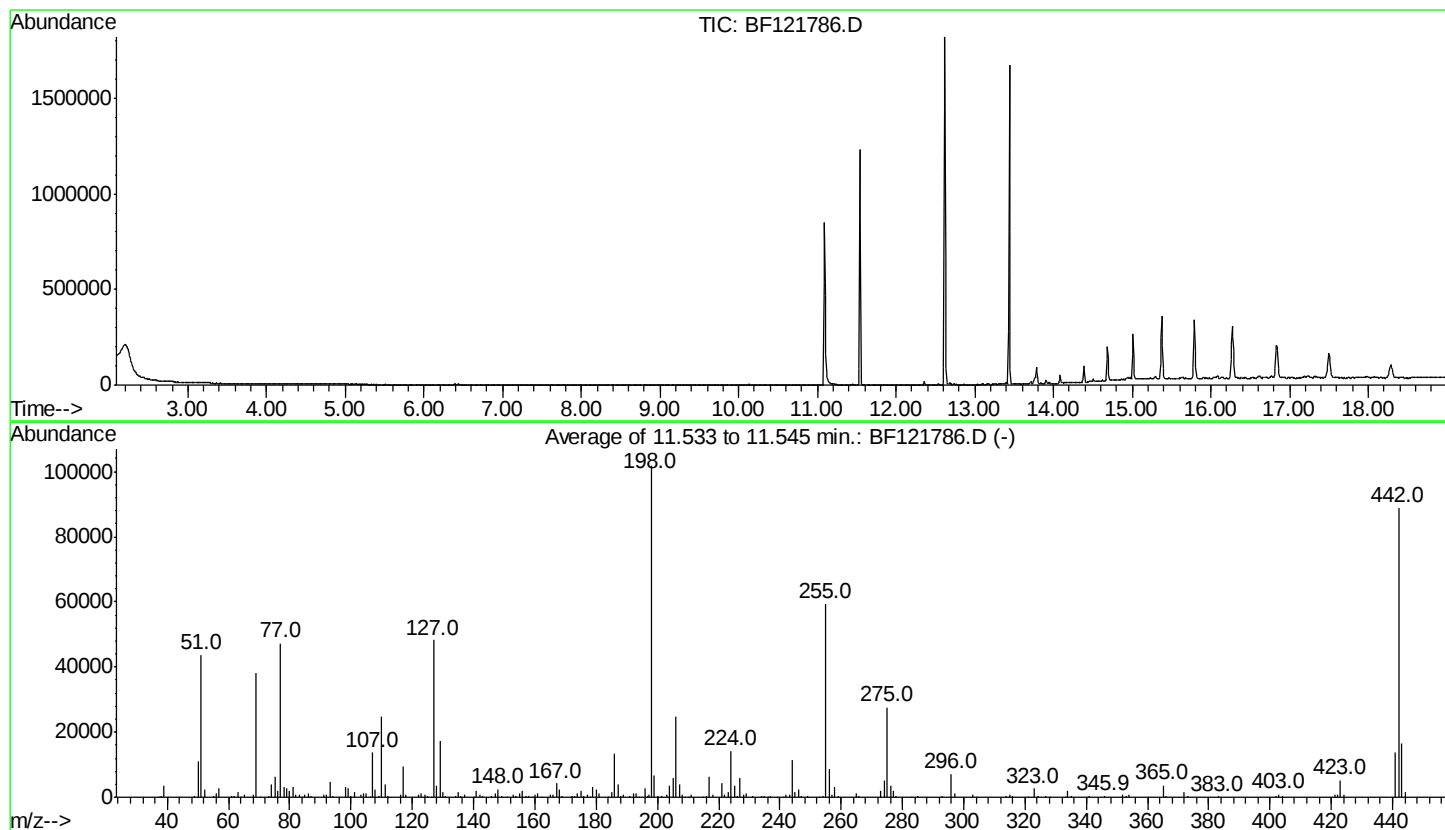

Spectrum Information: Average of 11.533 to 11.545 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.9	43664	PASS
68	69	0.00	2	1.6	624	PASS
69	198	0.00	100	37.3	38016	PASS
70	69	0.00	2	0.3	101	PASS
127	198	10	80	47.4	48229	PASS
197	198	0.00	2	0.6	641	PASS
198	198	100	100	100.0	101832	PASS
199	198	5	9	6.6	6761	PASS
275	198	10	60	27.1	27588	PASS
365	198	1	100	3.5	3549	PASS
441	198	0.01	100	13.4	13668	PASS
442	198	50	100	87.4	89029	PASS
443	442	15	24	18.8	16708	PASS