

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100224\
 Data File : BF139609.D
 Acq On : 02 Oct 2024 16:25
 Operator : RC/JU
 Sample : P4222-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-5

Quant Time: Oct 02 16:56:43 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 02 04:58:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.863	152	101112	20.000	ng	0.00
21) Naphthalene-d8	8.145	136	394179	20.000	ng	0.00
39) Acenaphthene-d10	9.898	164	218030	20.000	ng	-0.01
64) Phenanthrene-d10	11.386	188	410414	20.000	ng	0.00
76) Chrysene-d12	14.027	240	231616	20.000	ng	0.00
86) Perylene-d12	15.498	264	202388	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.498	112	787712	135.028	ng	0.01
7) Phenol-d6	6.498	99	976782	124.509	ng	0.00
23) Nitrobenzene-d5	7.428	82	766018	98.391	ng	0.00
42) 2,4,6-Tribromophenol	10.692	330	293816	139.598	ng	0.00
45) 2-Fluorobiphenyl	9.222	172	1332886	93.851	ng	0.00
79) Terphenyl-d14	12.974	244	1472818	104.338	ng	0.00
Target Compounds						
						Qvalue
19) n-Nitroso-di-n-propyla...	7.428	70	104385	20.696	ng	# 76
25) Isophorone	7.428	82	762358	55.132	ng	# 66
51) 2,6-Dinitrotoluene	9.898	165	28524	8.847	ng	# 18
57) 2,4-Dinitrotoluene	9.898	165	28524	6.768	ng	# 17
67) 4-Bromophenyl-phenylether	10.692	248	19482	4.630	ng	# 1
77) Benzidine	12.727	184	602050	147.365	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100224\
Data File : BF139609.D
Acq On : 02 Oct 2024 16:25
Operator : RC/JU
Sample : P4222-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-5

Quant Time: Oct 02 16:56:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration




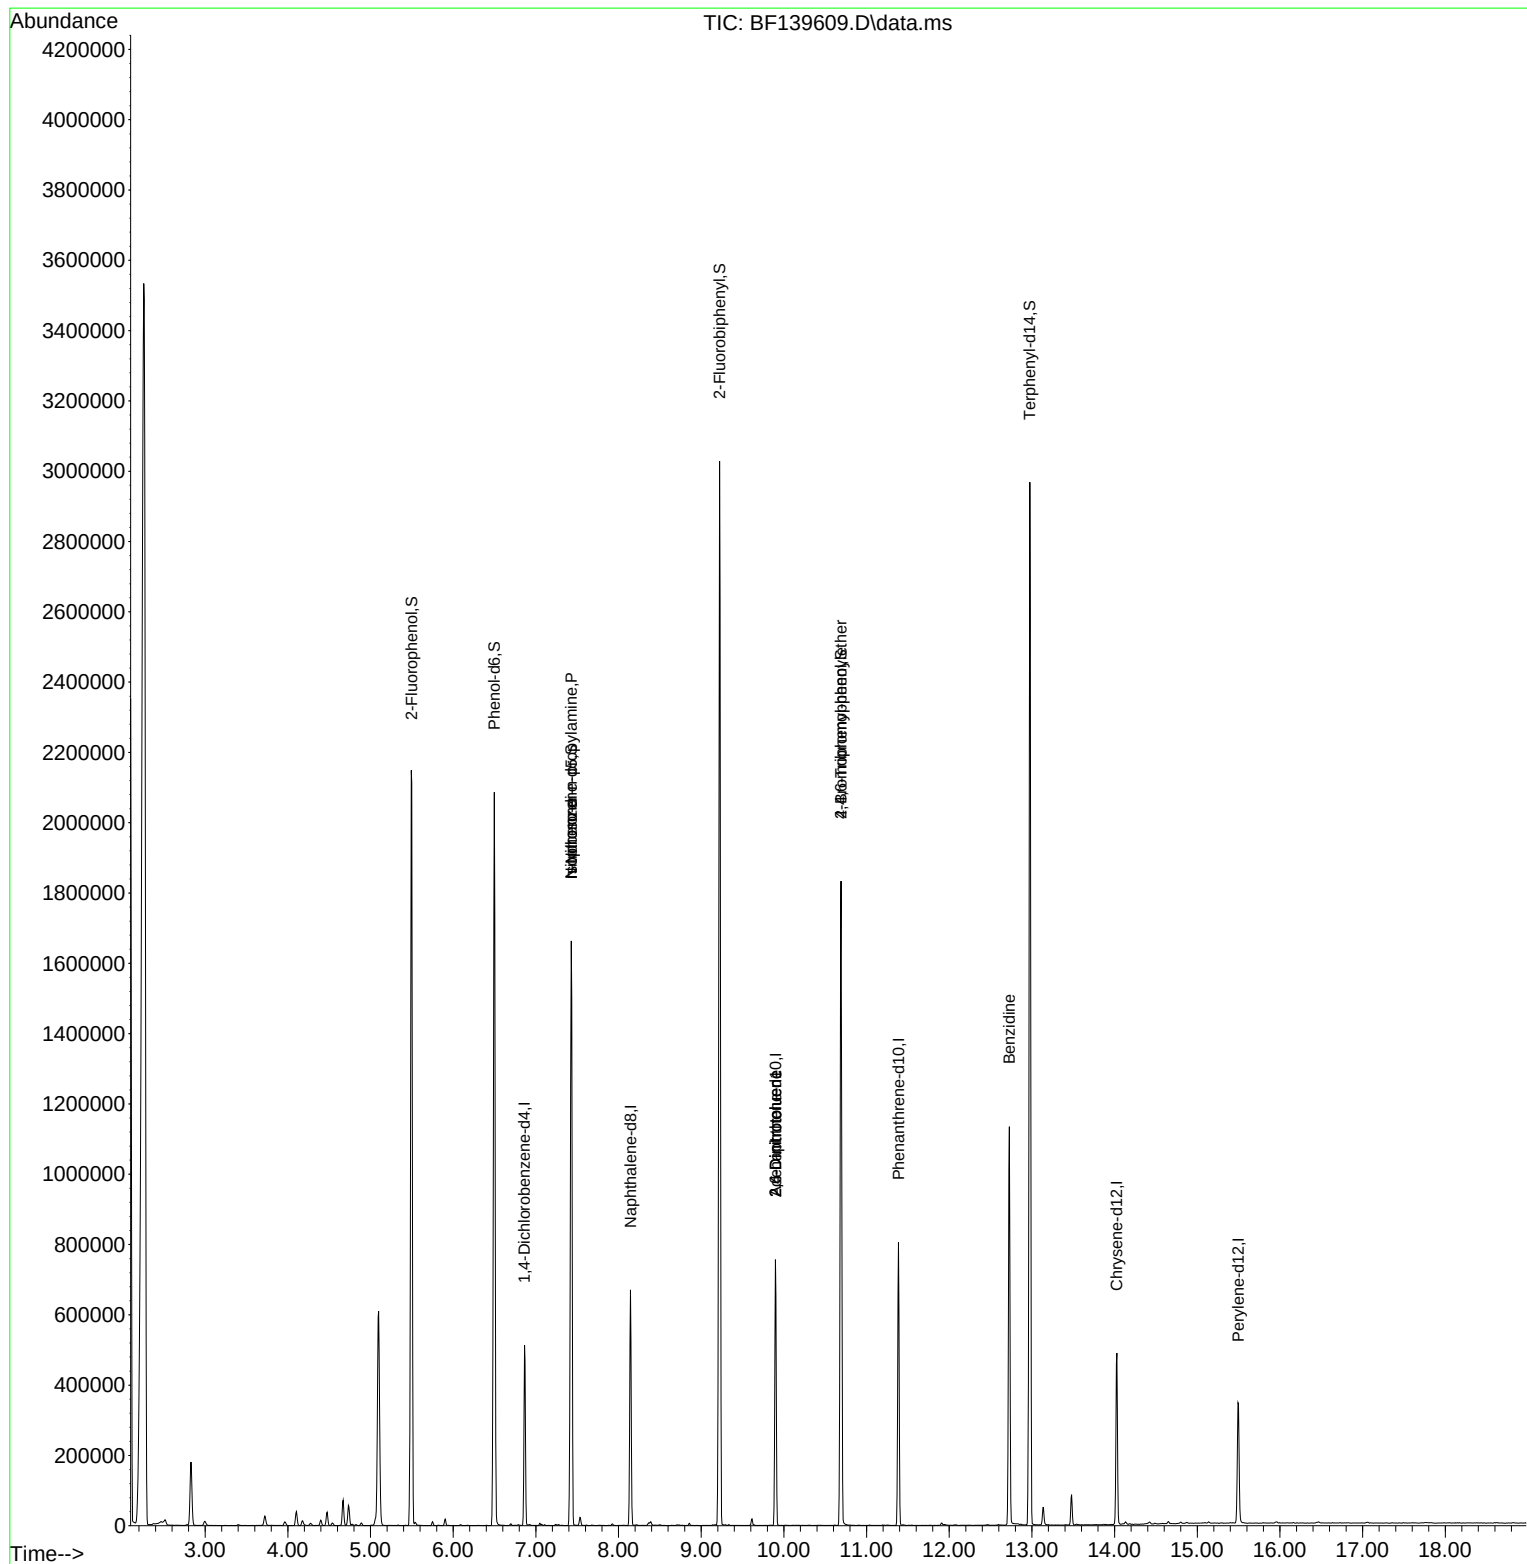




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.863 min Scan# 812
Delta R.T. -0.006 min
Lab File: BF139609.D
Acq: 02 Oct 2024 16:25




Instrument :
BNA_F
ClientSampleId :
TP-5


Tgt Ion:152 Resp: 101112
Ion Ratio Lower Upper
152 100
150 159.9 127.2 190.8
115 62.7 49.0 73.4

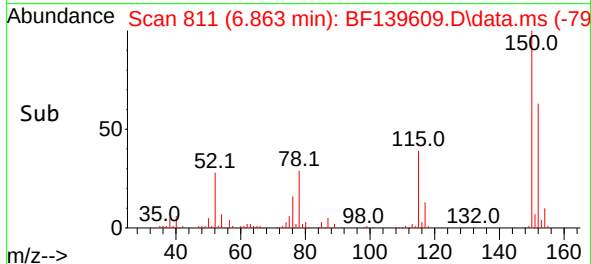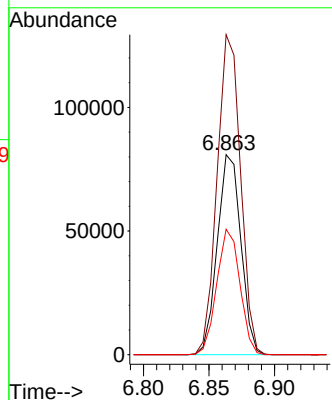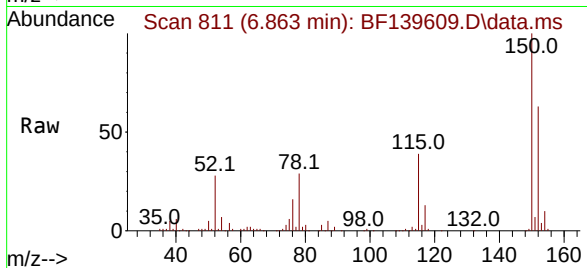

#5
2-Fluorophenol
Concen: 135.028 ng
RT: 5.498 min Scan# 579
Delta R.T. 0.011 min
Lab File: BF139609.D
Acq: 02 Oct 2024 16:25

Tgt Ion:112 Resp: 787712
Ion Ratio Lower Upper
112 100
64 67.1 54.2 81.4
63 37.3 29.4 44.2

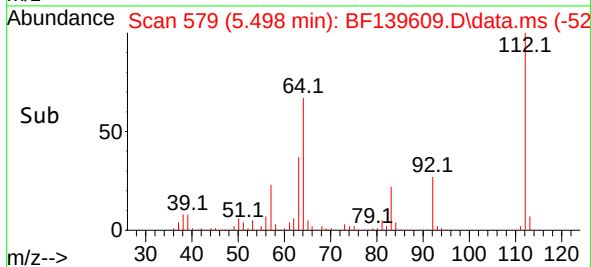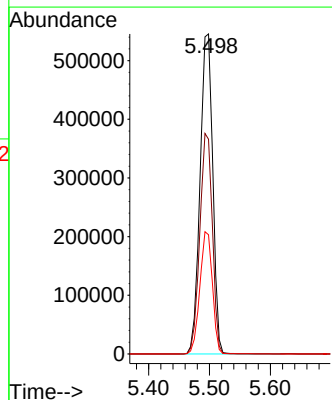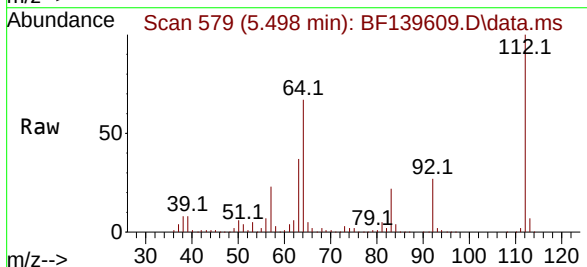







#7
Phenol-d6
Concen: 124.509 ng
RT: 6.498 min Scan# 74
Delta R.T. -0.006 min
Lab File: BF139609.D
Acq: 02 Oct 2024 16:25

Instrument :
BNA_F
ClientSampleId :
TP-5

Tgt Ion: 99 Resp: 976782




Ion	Ratio	Lower	Upper
99	100		
42	23.5	19.1	28.7
71	37.4	29.7	44.5

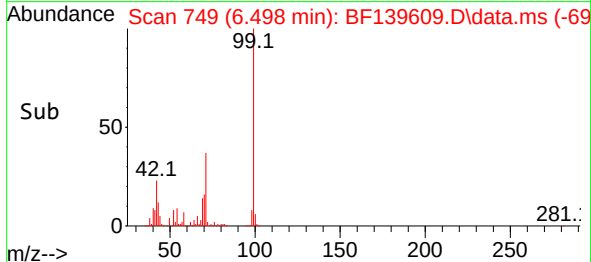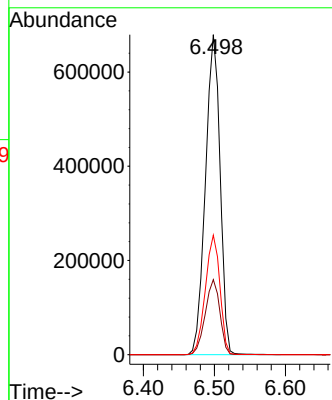


#19
n-Nitroso-di-n-propylamine
Concen: 20.696 ng
RT: 7.428 min Scan# 907
Delta R.T. 0.141 min
Lab File: BF139609.D
Acq: 02 Oct 2024 16:25

Tgt Ion: 70 Resp: 104385

Ion	Ratio	Lower	Upper
70	100		
42	56.4	58.0	87.0#
101	0.0	7.8	11.8#
130	2.0	15.9	23.9#


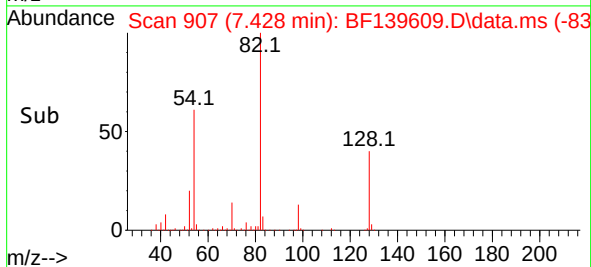
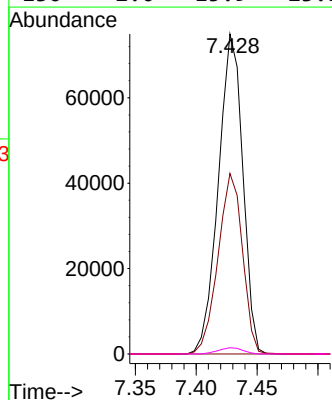
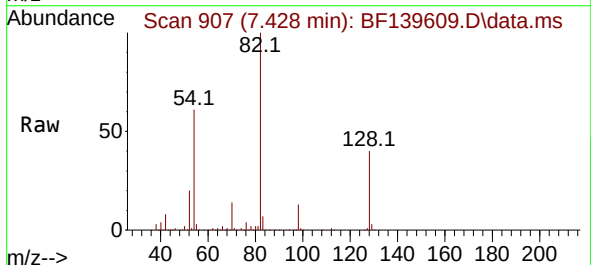




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.145 min Scan# 1030
Delta R.T. -0.006 min
Lab File: BF139609.D
Acq: 02 Oct 2024 16:25




Instrument :
BNA_F
ClientSampleId :
TP-5


Tgt Ion:	136	Resp:	394179
Ion	Ratio	Lower	Upper
136	100		
137	10.7	8.6	13.0
54	9.9	8.3	12.5
68	5.9	4.6	7.0

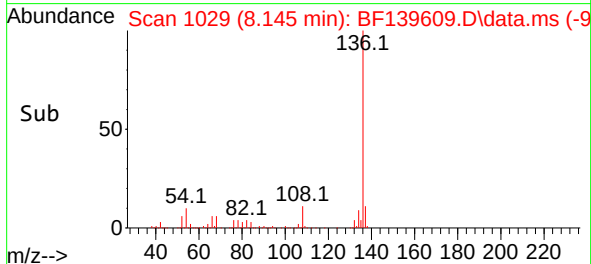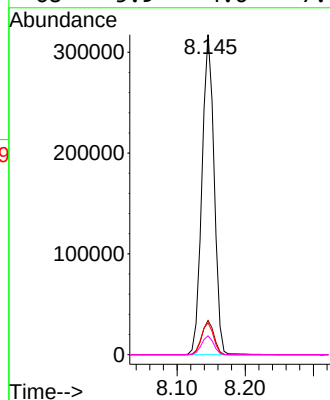

#23
Nitrobenzene-d5
Concen: 98.391 ng
RT: 7.428 min Scan# 907
Delta R.T. -0.006 min
Lab File: BF139609.D
Acq: 02 Oct 2024 16:25

Tgt Ion:	82	Resp:	766018
Ion	Ratio	Lower	Upper
82	100		
128	40.5	32.4	48.6
54	60.6	49.1	73.7


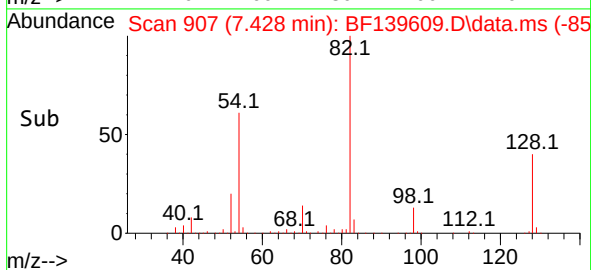
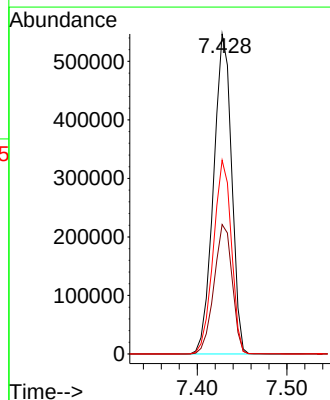
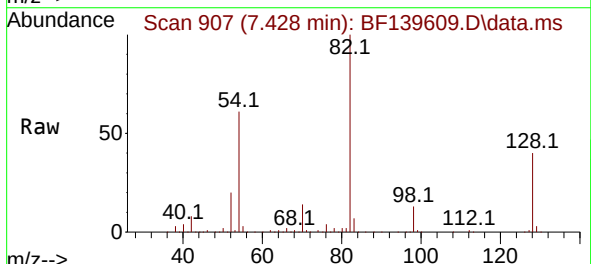




#25
Isophorone
Concen: 55.132 ng
RT: 7.428 min Scan# 90
Delta R.T. -0.265 min
Lab File: BF139609.D
Acq: 02 Oct 2024 16:25




Instrument :
BNA_F
ClientSampleId :
TP-5


Tgt Ion: 82 Resp: 762358
Ion Ratio Lower Upper
82 100
95 0.0 6.1 9.1#
138 0.0 13.4 20.2#

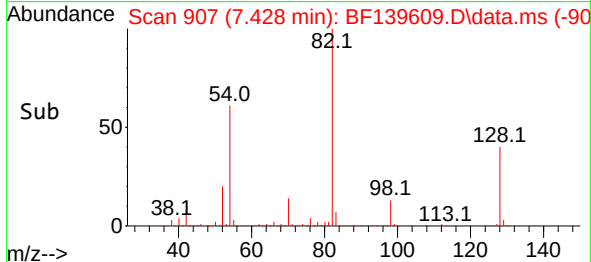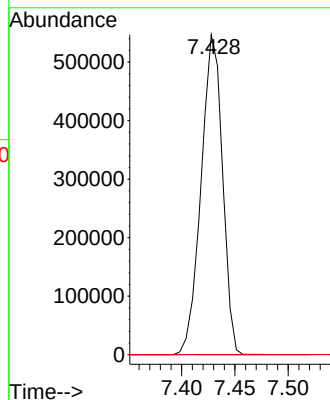

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.898 min Scan# 1327
Delta R.T. -0.012 min
Lab File: BF139609.D
Acq: 02 Oct 2024 16:25


Tgt Ion:164 Resp: 218030
Ion Ratio Lower Upper
164 100
162 99.9 79.4 119.0
160 43.6 35.1 52.7

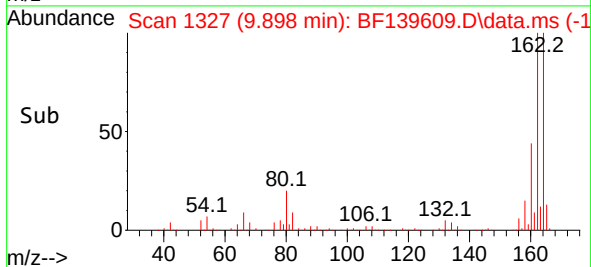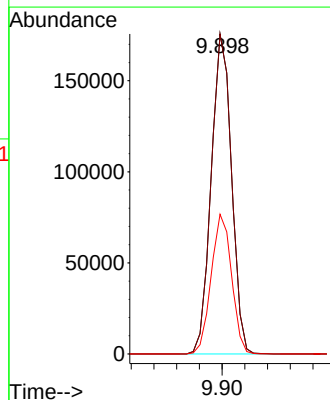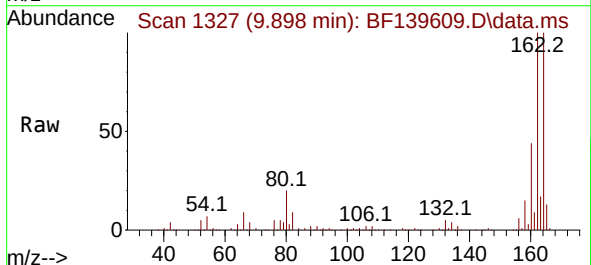






#42
2,4,6-Tribromophenol
Concen: 139.598 ng
RT: 10.692 min Scan# 1462
Delta R.T. -0.006 min
Lab File: BF139609.D
Acq: 02 Oct 2024 16:25


Instrument :
BNA_F
ClientSampleId :
TP-5

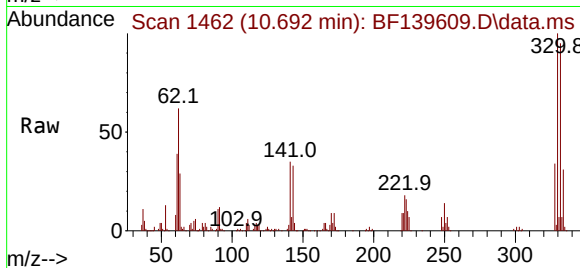



Tgt Ion:330 Resp: 293816
Ion Ratio Lower Upper
330 100
332 95.4 76.5 114.7
141 35.5 29.3 43.9

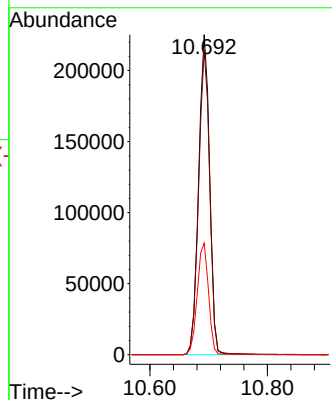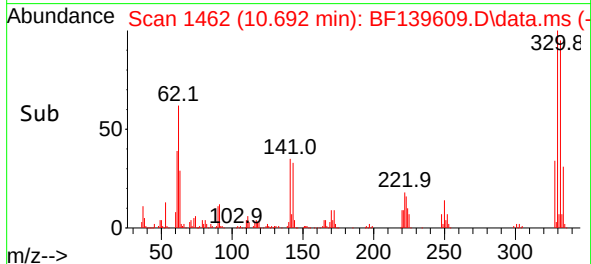


#45
2-Fluorobiphenyl
Concen: 93.851 ng
RT: 9.222 min Scan# 1212
Delta R.T. -0.006 min
Lab File: BF139609.D
Acq: 02 Oct 2024 16:25

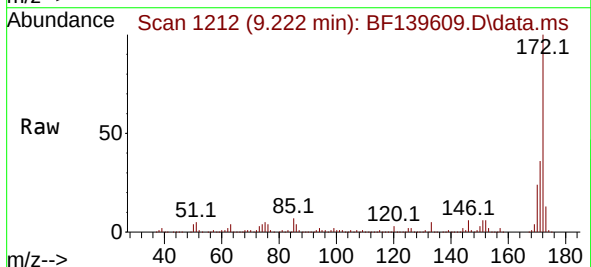

Tgt Ion:172 Resp: 1332886
Ion Ratio Lower Upper
172 100
171 35.8 28.2 42.4
170 23.7 18.8 28.2



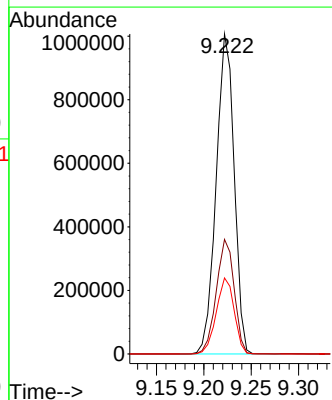
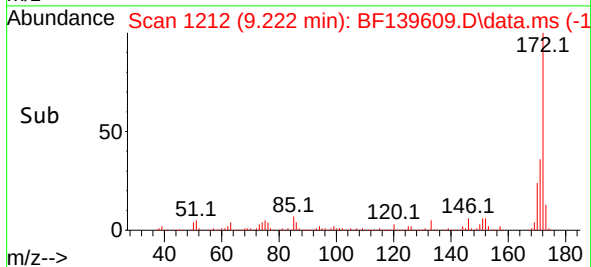




#51
2,6-Dinitrotoluene
Concen: 8.847 ng
RT: 9.898 min Scan# 11
Delta R.T. 0.206 min
Lab File: BF139609.D
Acq: 02 Oct 2024 16:25




Instrument :
BNA_F
ClientSampleId :
TP-5


Tgt Ion:165 Resp: 28524
Ion Ratio Lower Upper
165 100
63 1.4 56.7 85.1#
89 1.3 51.6 77.4#

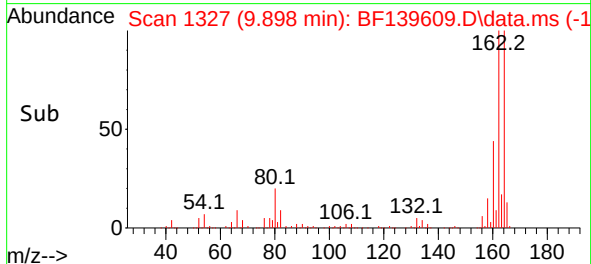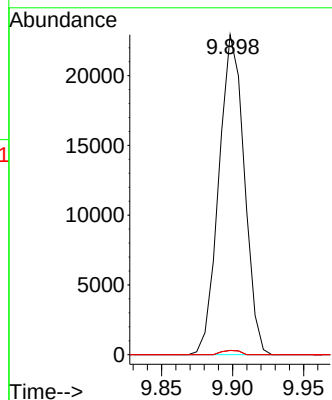

#57
2,4-Dinitrotoluene
Concen: 6.768 ng
RT: 9.898 min Scan# 1327
Delta R.T. -0.200 min
Lab File: BF139609.D
Acq: 02 Oct 2024 16:25

Tgt Ion:165 Resp: 28524
Ion Ratio Lower Upper
165 100
63 1.4 46.9 70.3#
89 1.3 64.4 96.6#
182 0.0 2.2 3.2#

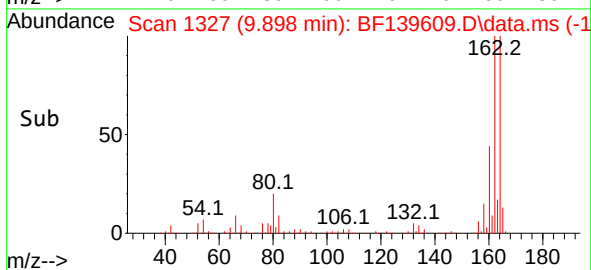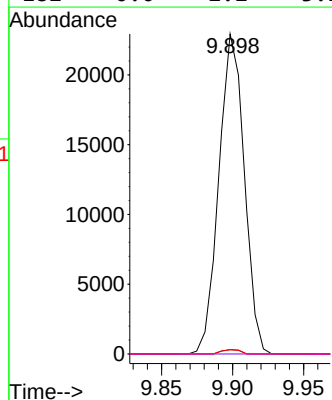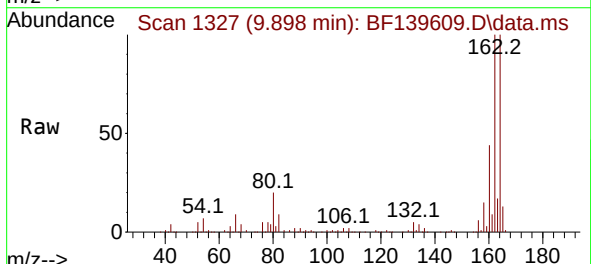



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.386 min Scan# 1

Delta R.T. -0.006 min

Lab File: BF139609.D

Acq: 02 Oct 2024 16:25

Instrument :

BNA_F

ClientSampleId :

TP-5





Tgt Ion:188 Resp: 410414

Ion Ratio Lower Upper

188 100

94 9.2 7.4 11.2

80 9.9 8.2 12.2

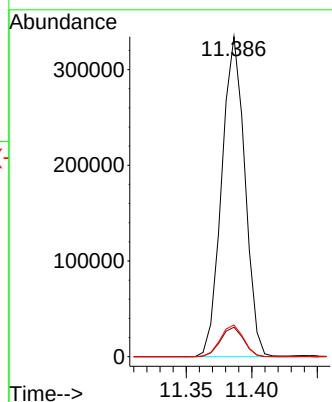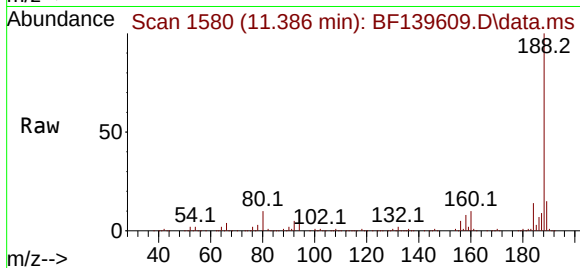

#67

4-Bromophenyl-phenylether

Concen: 4.630 ng

RT: 10.692 min Scan# 1462

Delta R.T. -0.247 min

Lab File: BF139609.D

Acq: 02 Oct 2024 16:25




Tgt Ion:248 Resp: 19482


Ion Ratio Lower Upper

248 100

250 201.7 77.1 115.7#

141 520.2 60.4 90.6#

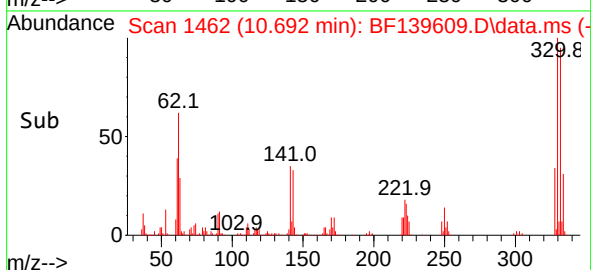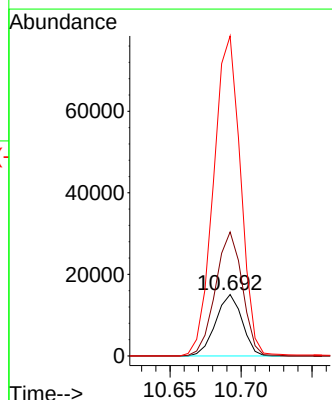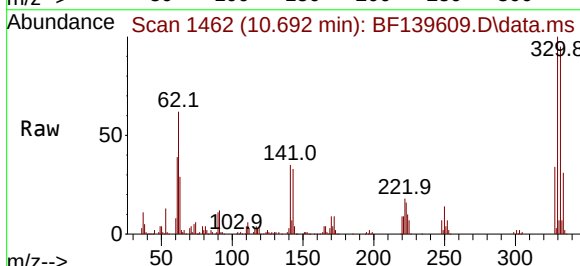



#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.027 min Scan# 2030

Delta R.T. -0.006 min

Lab File: BF139609.D

Acq: 02 Oct 2024 16:25

Instrument :

BNA_F

ClientSampleId :

TP-5





Tgt Ion:240 Resp: 231616

Ion Ratio Lower Upper

240 100

120 9.6 8.4 12.6

236 25.8 20.3 30.5

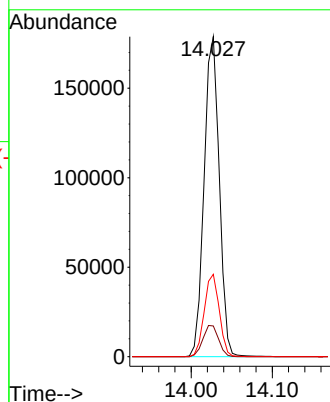

#77

Benzidine

Concen: 147.365 ng

RT: 12.727 min Scan# 1808

Delta R.T. -0.000 min

Lab File: BF139609.D

Acq: 02 Oct 2024 16:25




Tgt Ion:184 Resp: 602050


Ion Ratio Lower Upper

184 100

185 14.1 11.4 17.0

183 11.0 8.8 13.2


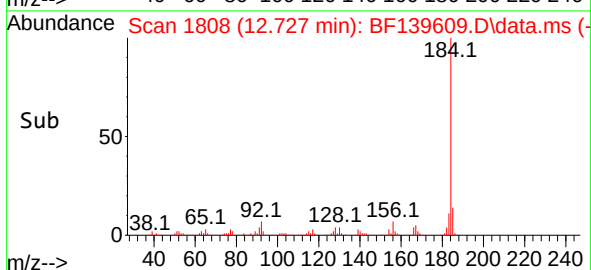
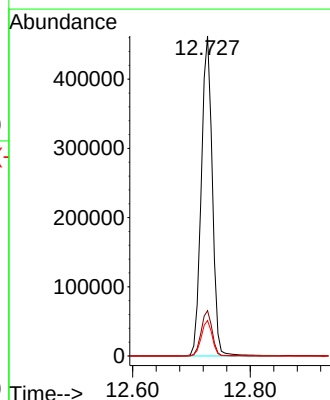





#79
 Terphenyl-d14
 Concen: 104.338 ng
 RT: 12.974 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BF139609.D
 Acq: 02 Oct 2024 16:25

Instrument :
 BNA_F
 ClientSampleId :
 TP-5

Tgt Ion:244 Resp: 1472818
 Ion Ratio Lower Upper
 244 100
 212 7.1 5.8 8.6
 122 11.0 8.6 12.8

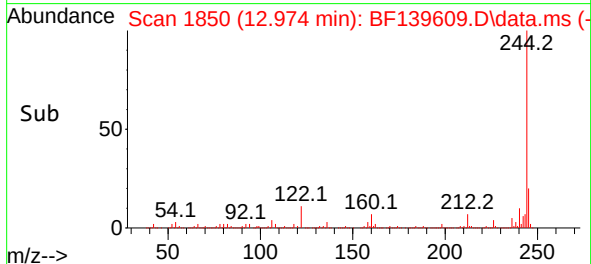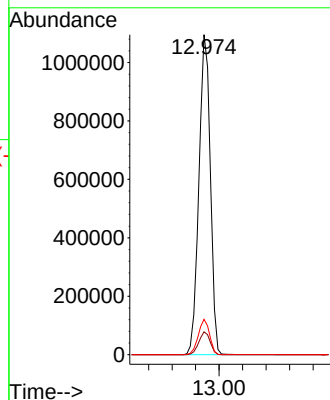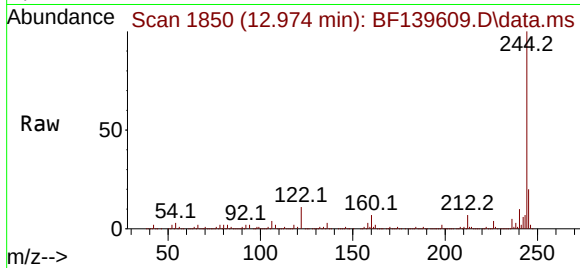

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.498 min Scan# 2279
 Delta R.T. -0.006 min
 Lab File: BF139609.D
 Acq: 02 Oct 2024 16:25

Tgt Ion:264 Resp: 202388
 Ion Ratio Lower Upper
 264 100
 260 23.3 18.7 28.1
 265 21.3 16.9 25.3

