
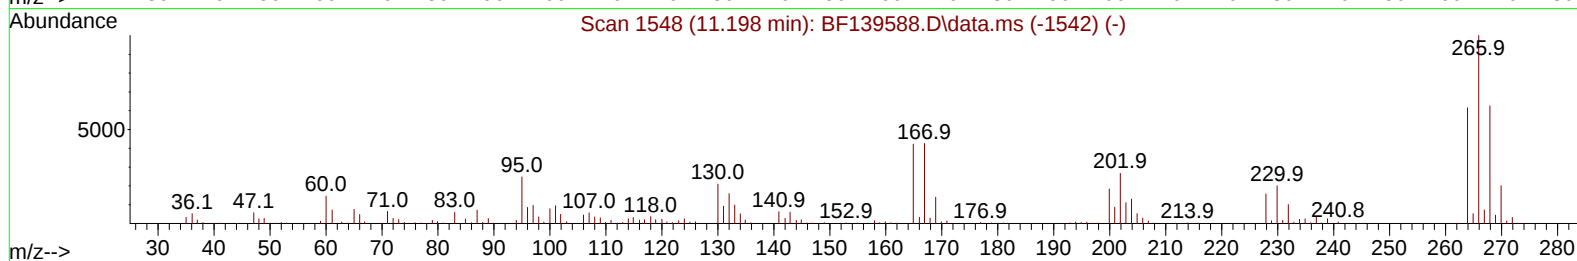
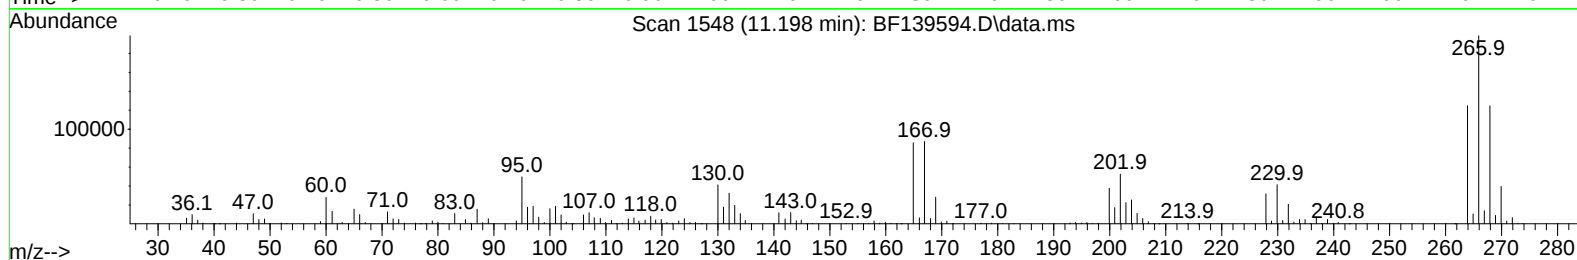


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100224\
Data File : BF139594.D
Acq On : 02 Oct 2024 09:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 02 11:21:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

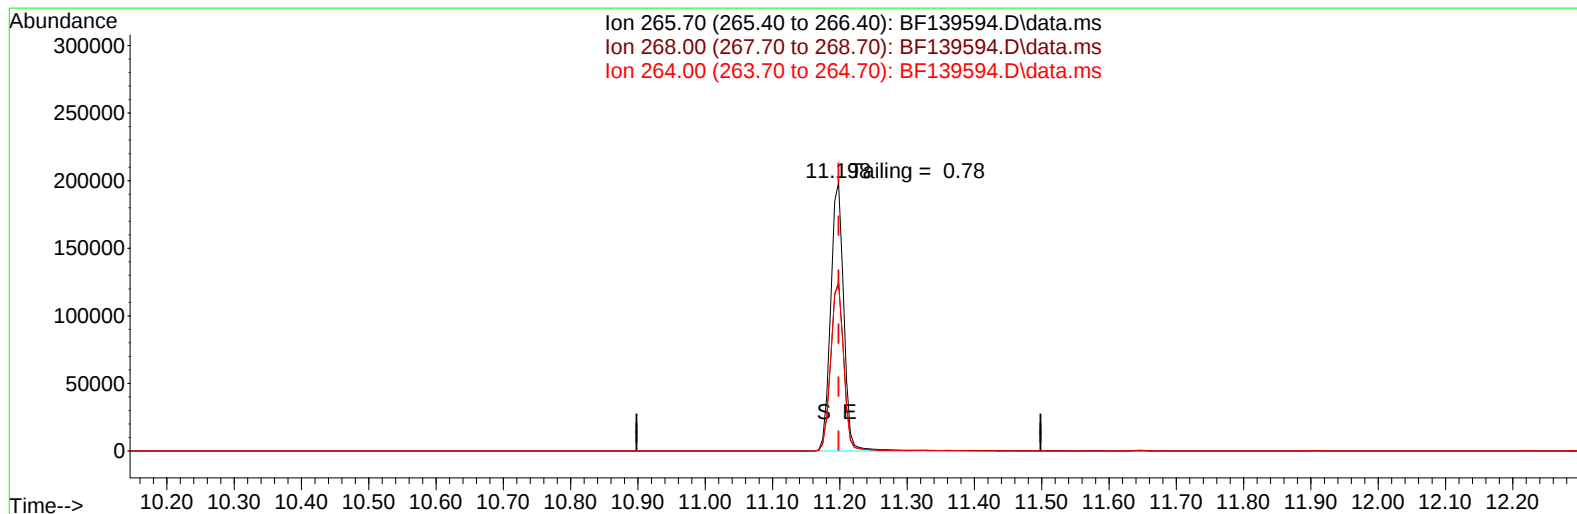

TIC: BF139594.D\data.ms

(70) Pentachlorophenol (C)




11.198min (-0.000) 748144.01 ng

response 268623

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	62.80
264.00	61.60	62.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100224\
Data File : BF139594.D
Acq On : 02 Oct 2024 09:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 02 11:21:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

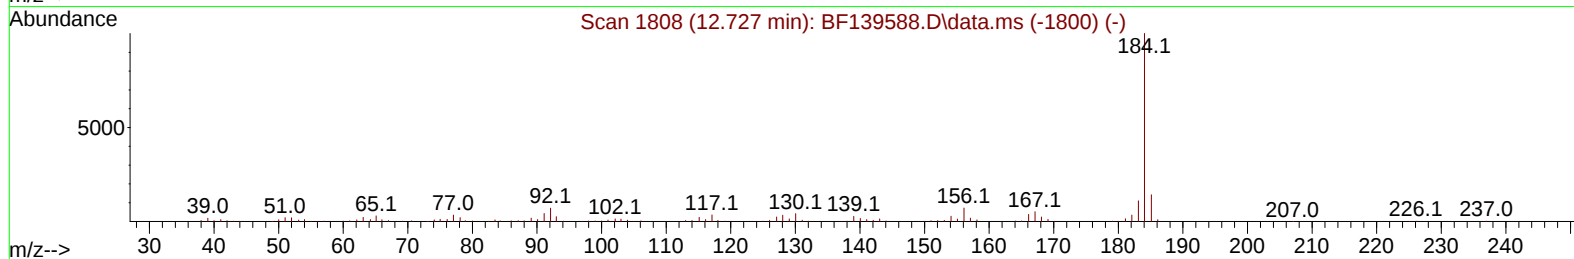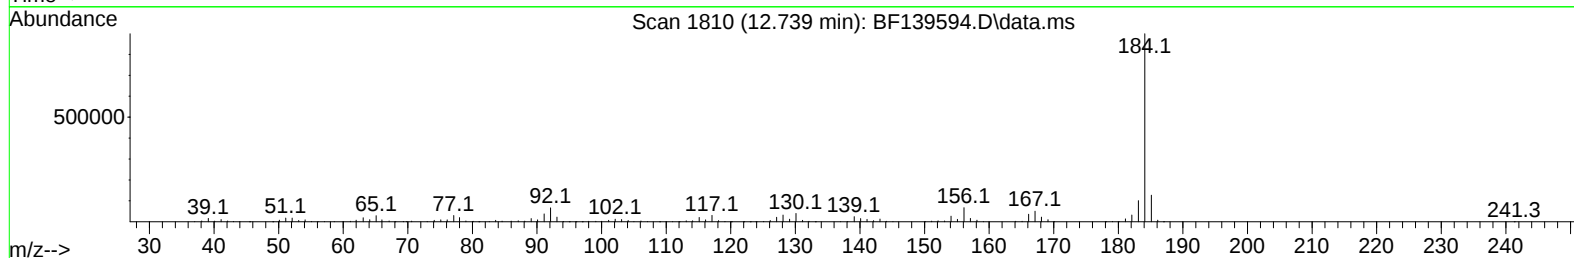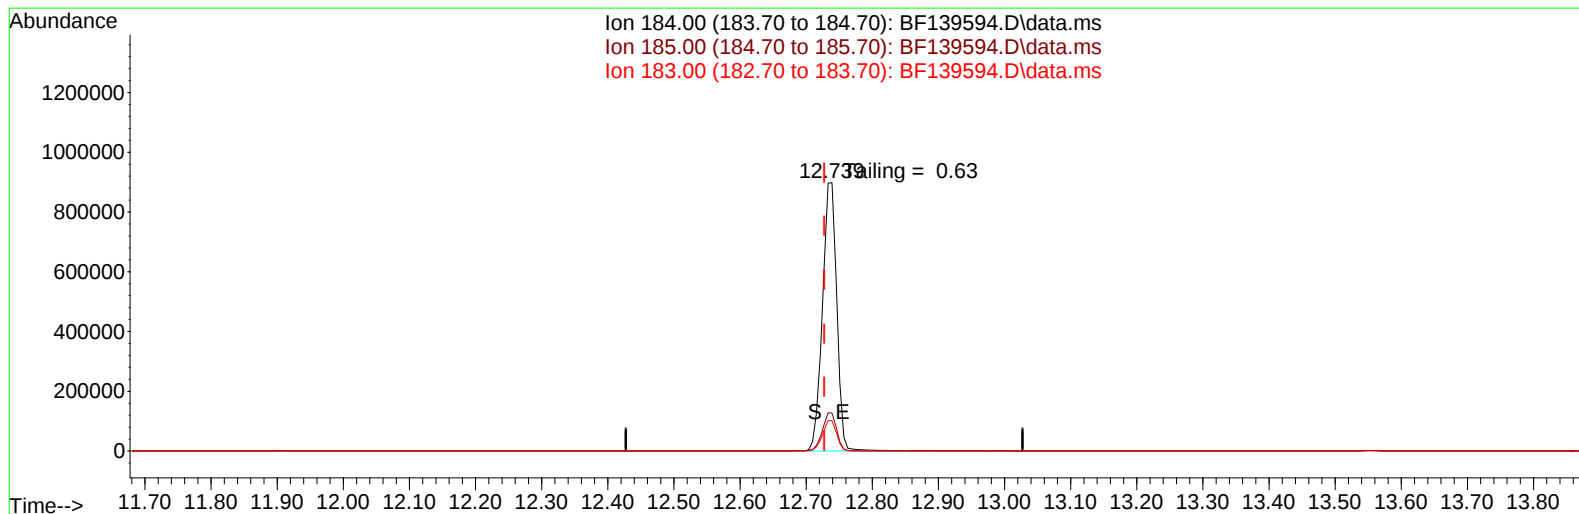

TIC: BF139594.D\data.ms

(77) Benzidine

12.739min (+ 0.012) 1239918.61 ng

response 1355983

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.16
183.00	11.00	11.29
0.00	0.00	0.00