


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100224\
Data File : BF139594.D
Acq On : 02 Oct 2024 09:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 02 04:58:47 2024

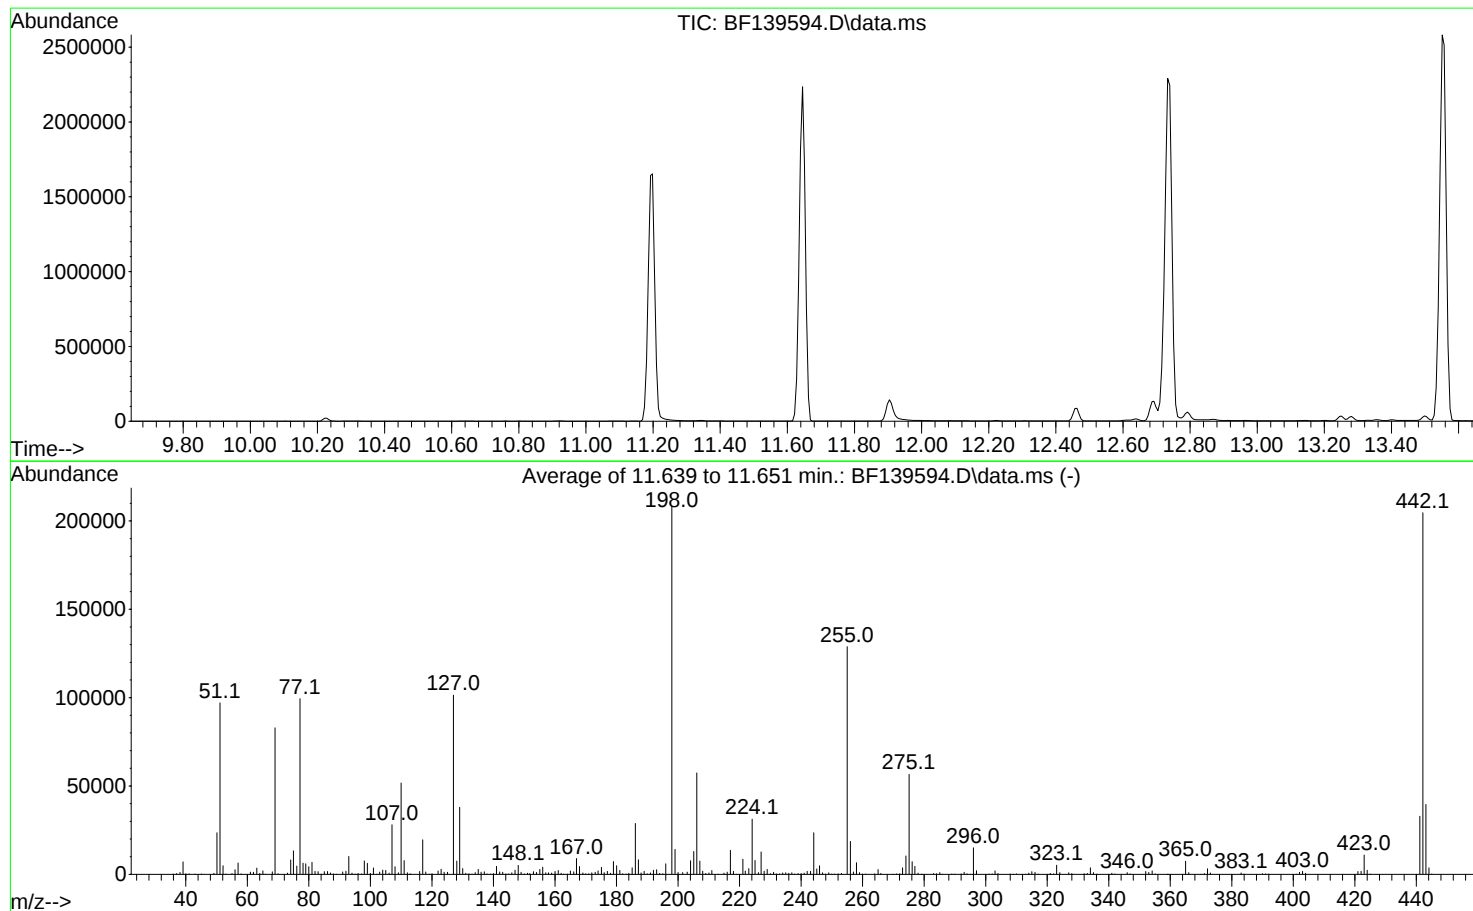




AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.6	97072	PASS
68	69	0.00	2	1.8	1493	PASS
69	198	0.00	100	39.8	82952	PASS
70	69	0.00	2	0.5	392	PASS
127	198	10	80	48.7	101400	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	208171	PASS
199	198	5	9	6.8	14141	PASS
275	198	10	60	27.2	56629	PASS
365	198	1	100	3.6	7421	PASS
441	198	0.01	100	15.8	32867	PASS
442	442	50	100	100.0	204672	PASS
443	442	15	24	19.3	39581	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100224\
Data File : BF139594.D
Acq On : 02 Oct 2024 09:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 02 11:21:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

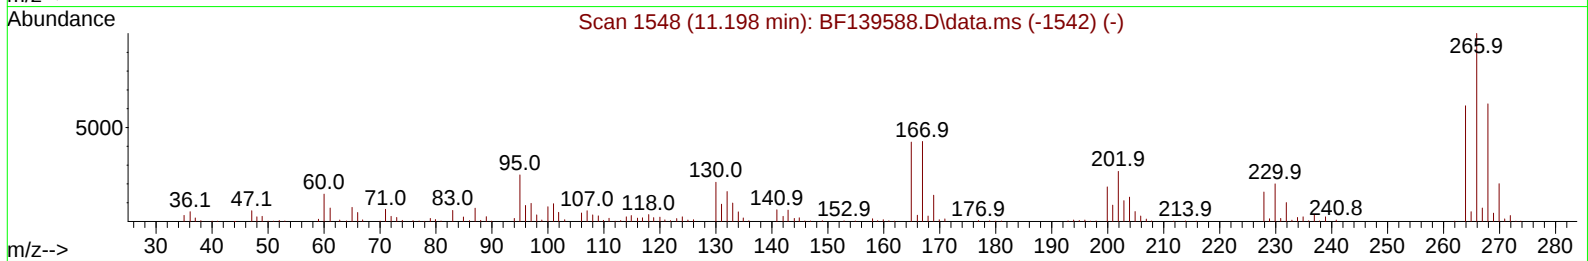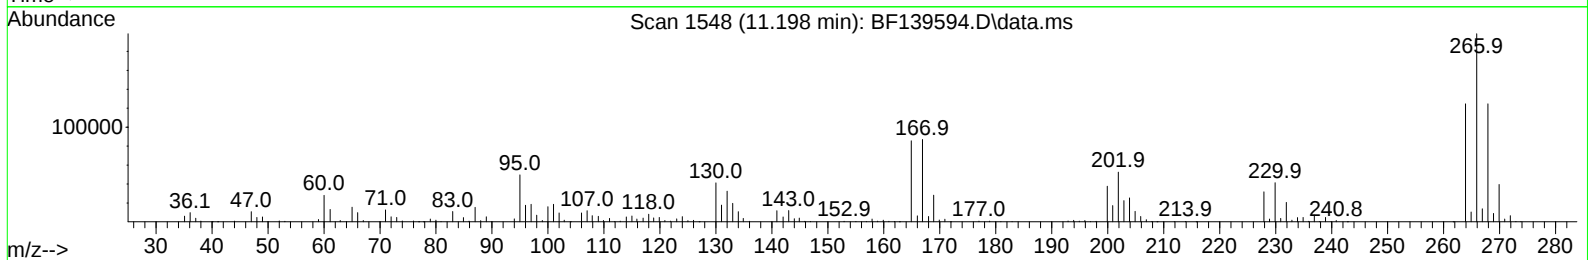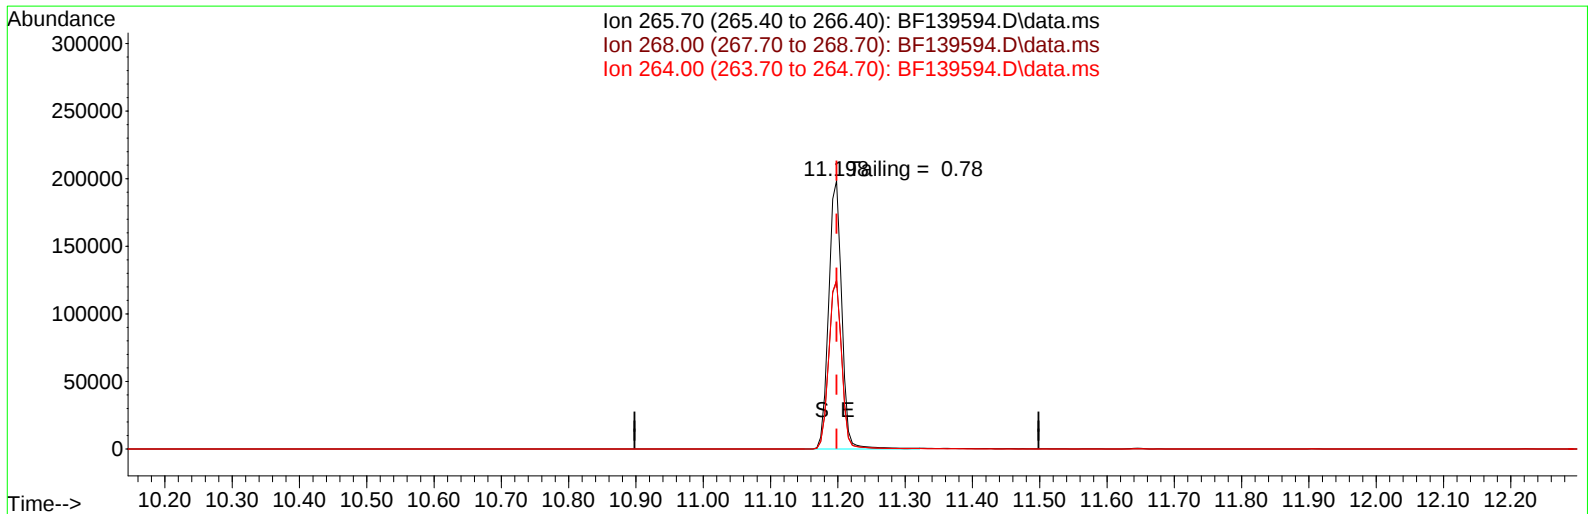

TIC: BF139594.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.000) 748144.01 ng




response 268623

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	62.80
264.00	61.60	62.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100224\
Data File : BF139594.D
Acq On : 02 Oct 2024 09:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 02 11:21:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

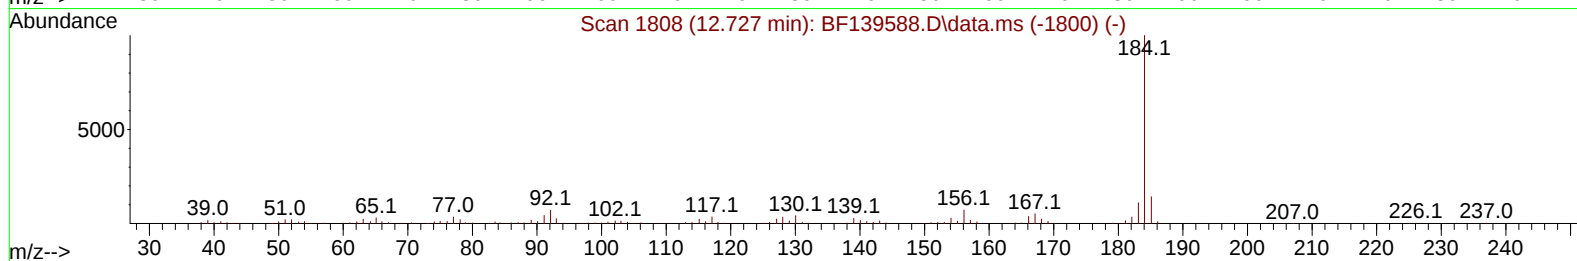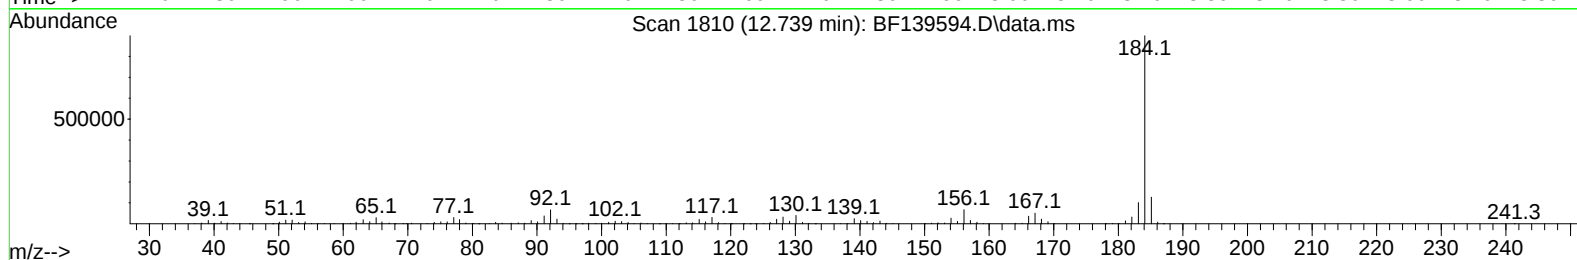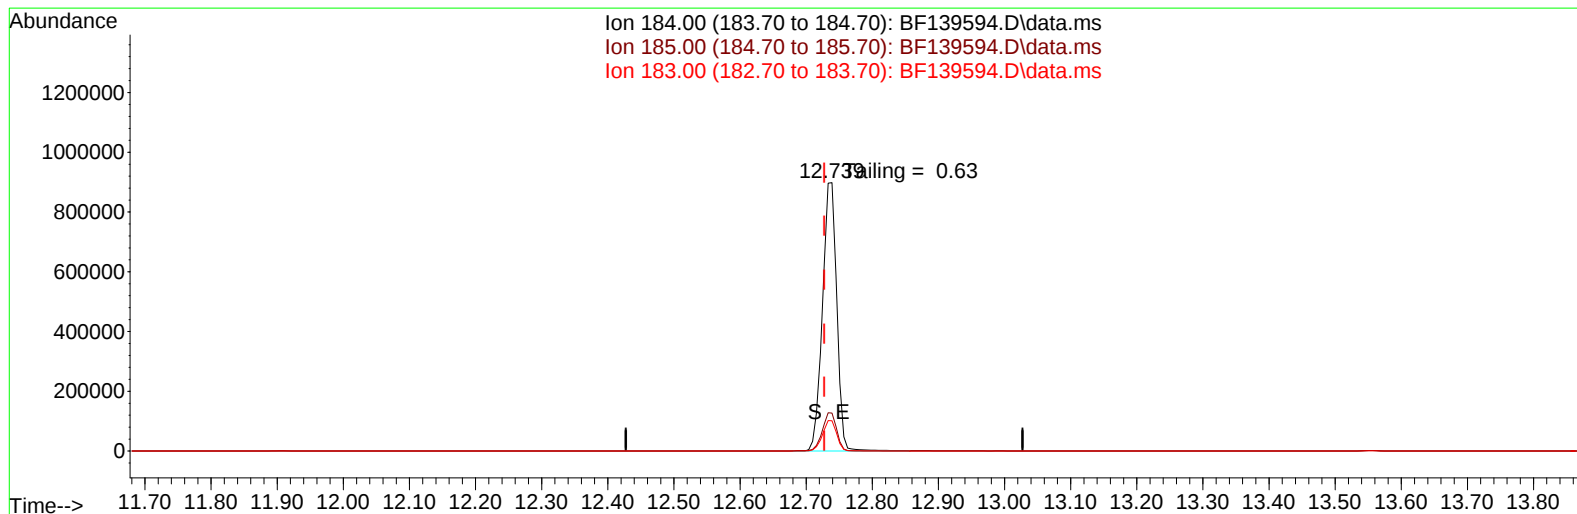

TIC: BF139594.D\data.ms

(77) Benzidine

12.739min (+ 0.012) 1239918.61 ng

response 1355983

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.16
183.00	11.00	11.29
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/2/2024	BNA_F	<u>BF139594.D</u>
Compound Name	Response	Retention Time
DDT	679427	13.557
DDD	16026	13.251
DDE	308	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16334	695761	2.35

Instrument :
BNA_F
ClientSampleId :
DFTPP