

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100317\
 Data File : BF099052.D
 Acq On : 4 Oct 2017 1:25
 Operator : SJ/JU
 Sample : I5610-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Oct 04 03:43:49 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 23 13:50:58 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.87	152	119285	20.00	ng	-0.05
21) Naphthalene-d8	8.16	136	433294	20.00	ng	-0.05
38) Acenaphthene-d10	9.91	164	154198	20.00	ng	-0.05
63) Phenanthrene-d10	11.40	188	225788	20.00	ng	-0.05
75) Chrysene-d12	14.03	240	238906	20.00	ng	-0.05
86) Perylene-d12	15.51	264	234350	20.00	ng	-0.06

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.50	112	994255	132.69	ng	-0.04
7) Phenol-d6	6.50	99	1170541	126.63	ng	-0.04
23) Nitrobenzene-d5	7.44	82	678694	100.45	ng	-0.05
41) 2,4,6-Tribromophenol	10.70	330	147254	116.71	ng	-0.05
44) 2-Fluorobiphenyl	9.23	172	923296	99.96	ng	-0.05
78) Terphenyl-d14	12.98	244	653321	62.19	ng	-0.05


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
9) Benzaldehyde	6.65	77	19883	3.71	ng	87
10) Phenol	6.52	94	28538	2.76	ng	97
15) Benzyl Alcohol	7.03	79	14404	2.12	ng	# 57
19) n-Nitroso-di-n-propylamine	7.44	70	88389	14.98	ng	# 77
25) Isophorone	7.44	82	671009	48.04	ng	# 64
49) Dimethylphthalate	9.62	163	208554	17.92	ng	99
56) 2,4-Dinitrotoluene	9.91	165	19905	6.05	ng	# 23
66) 4-Bromophenyl-phenylether	10.70	248	10032	4.54	ng	# 1
70) Phenanthrene	11.42	178	98964	8.19	ng	97
71) Anthracene	11.47	178	30417	2.46	ng	98
74) Fluoranthene	12.62	202	184097	15.04	ng	99
77) Pyrene	12.84	202	160742	8.82	ng	98
80) Benzo(a)anthracene	14.02	228	88795	6.14	ng	98
82) Chrysene	14.06	228	77701	5.64	ng	95
85) Indeno(1,2,3-cd)pyrene	16.99	276	33644	3.05	ng	96
87) Benzo(b)fluoranthene	15.07	252	134609	9.34	ng	# 95
88) Benzo(k)fluoranthene	15.07	252	134609	9.46	ng	# 95
89) Benzo(a)pyrene	15.44	252	72385	5.47	ng	# 94
91) Benzo(a,h,i)perylene	17.44	276	32646	3.12	ng	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100317\
Data File : BF099052.D
Acq On : 4 Oct 2017 1:25
Operator : SJ/JU
Sample : I5610-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Oct 04 03:43:49 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration




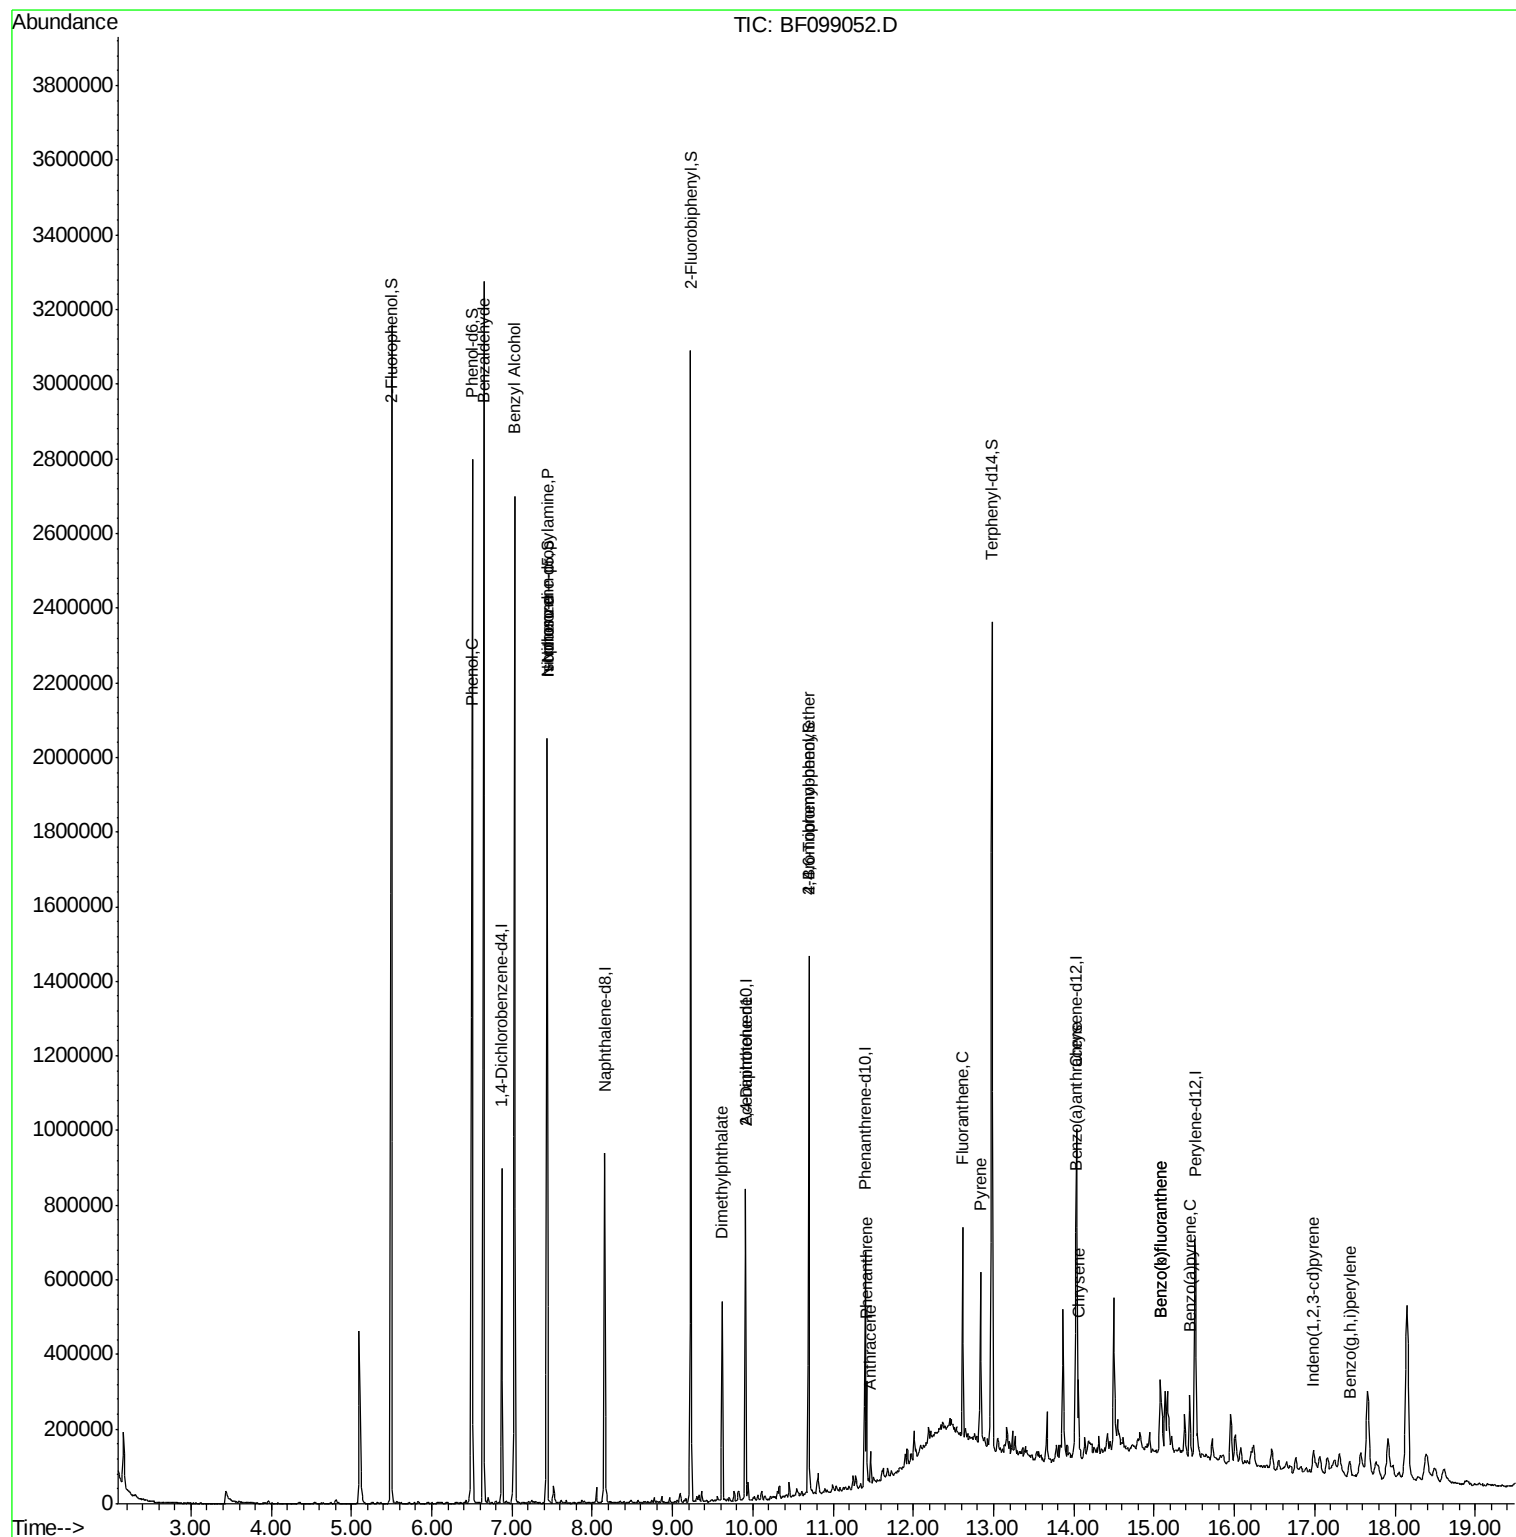




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.87 min Scan# 814
 Delta R.T. -0.05 min
 Lab File: BF099052.D
 Acq: 4 Oct 2017 1:25




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:152 Resp: 119285
 Ion Ratio Lower Upper
 152 100
 150 158.4 124.6 186.8
 115 59.4 50.1 75.1

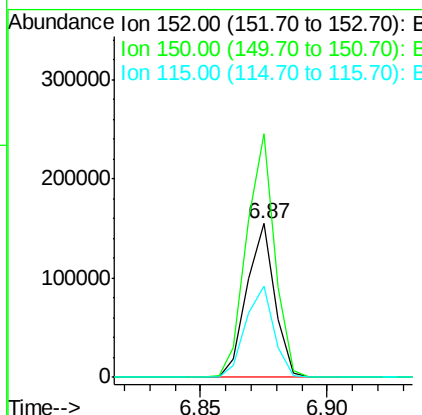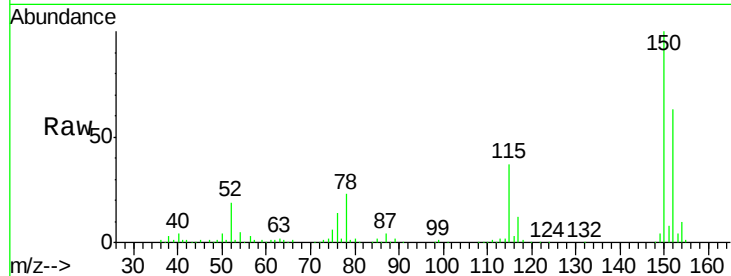

#5
 2-Fluorophenol
 Concen: 132.69 ng
 RT: 5.50 min Scan# 580
 Delta R.T. -0.04 min
 Lab File: BF099052.D
 Acq: 4 Oct 2017 1:25

Tgt Ion:112 Resp: 994255
 Ion Ratio Lower Upper
 112 100
 64 55.4 47.9 71.9
 63 27.8 23.7 35.5

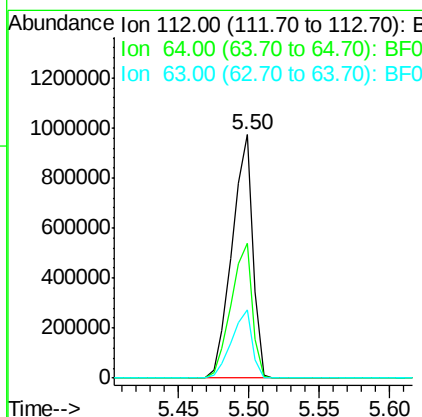



#7

Phenol-d6

Concen: 126.63 ng

RT: 6.50 min Scan# 751

Delta R.T. -0.04 min

Lab File: BF099052.D

Acq: 4 Oct 2017 1:25

Instrument :

BNA_F

ClientSampled :


Tot Ion: 99 Resp: 1170541

Ion Ratio Lower Upper

99 100

42 16.6 14.5 21.7




71 31.4 25.4 38.0



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

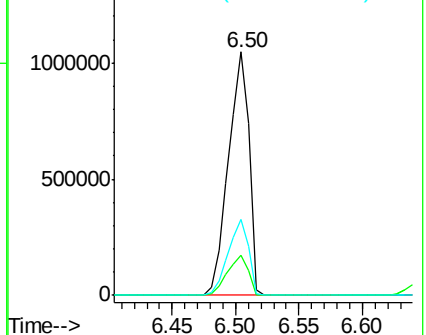

#9

Benzaldehyde

Concen: 3.71 ng

RT: 6.65 min Scan# 775

Delta R.T. 0.17 min

Lab File: BF099052.D

Acq: 4 Oct 2017 1:25


Tgt Ion: 77 Resp: 19883

Ion Ratio Lower Upper

77 100

105 88.4 81.1 121.1



106 82.0 74.5 114.5




Abundance Ion 77.00 (76.70 to 77.70): BF0

Ion 105.00 (104.70 to 105.70): B

Ion 106.00 (105.70 to 106.70): B




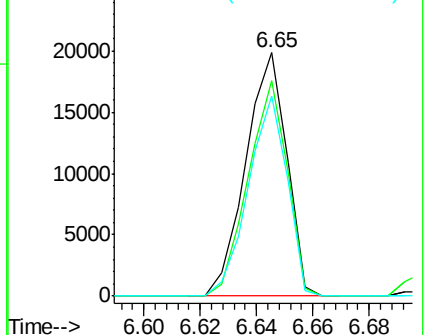




#10
Phenol
Concen: 2.76 ng
RT: 6.52 min Scan# 753
Delta R.T. -0.04 min
Lab File: BF099052.D
Acq: 4 Oct 2017 1:25




Instrument :
BNA_F
ClientSampleId :


Tot Ion: 94 Resp: 28538
Ion Ratio Lower Upper
94 100
65 26.9 7.9 47.9
66 34.1 16.2 56.2

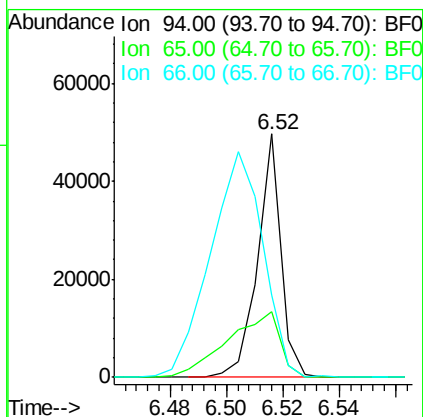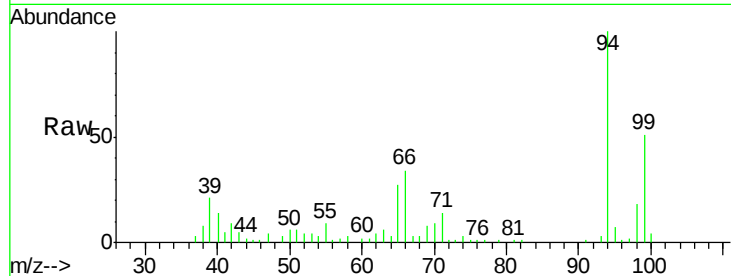

#15
Benzyl Alcohol
Concen: 2.12 ng
RT: 7.03 min Scan# 840
Delta R.T. -0.04 min
Lab File: BF099052.D
Acq: 4 Oct 2017 1:25

Tgt Ion: 79 Resp: 14404
Ion Ratio Lower Upper
79 100
108 48.0 65.1 97.7#
77 102.0 50.6 75.8#

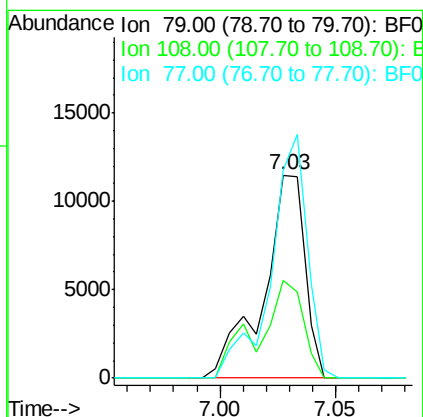







#19
n-Nitroso-di-n-propylamine
Concen: 14.98 ng
RT: 7.44 min Scan# 910
Delta R.T. 0.11 min
Lab File: BF099052.D
Acq: 4 Oct 2017 1:25

Instrument :
BNA_F
ClientSampleId :

Tot Ion: 70 Resp: 88389
Ion Ratio Lower Upper
70 100
42 46.4 47.5 71.3#
101 0.0 7.4 11.2#
130 2.6 16.6 25.0#

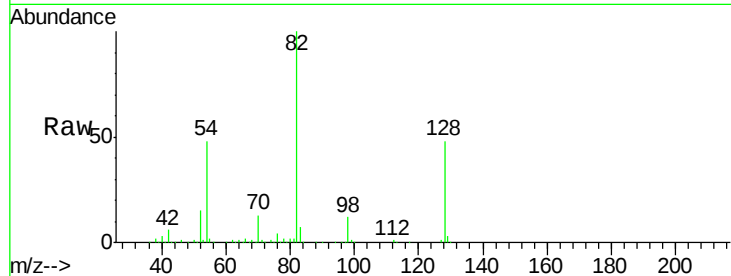


Abundance Ion 70.00 (69.70 to 70.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 101.00 (100.70 to 101.70): E
Ion 130.00 (129.70 to 130.70): E


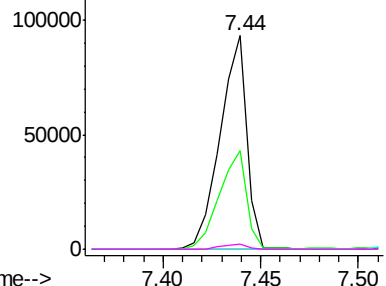



#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.16 min Scan# 1032
Delta R.T. -0.05 min
Lab File: BF099052.D
Acq: 4 Oct 2017 1:25

Tgt Ion: 136 Resp: 433294
Ion Ratio Lower Upper
136 100
137 10.9 8.9 13.3
54 6.7 6.6 9.8
68 5.4 5.0 7.4

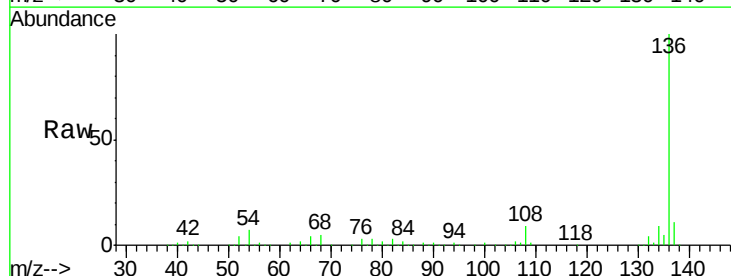

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

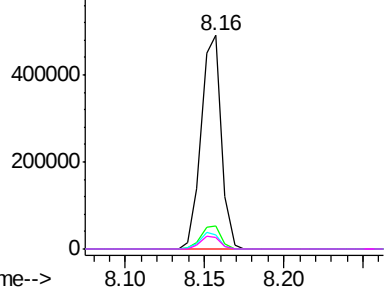







#23
 Nitrobenzene-d5
 Concen: 100.45 ng
 RT: 7.44 min Scan# 910
 Delta R.T. -0.05 min
 Lab File: BF099052.D
 Acq: 4 Oct 2017 1:25

Instrument :
 BNA_F
 ClientSampleID :

Tot Ion	82	Resp	678694
Ion Ratio	100	Lower	Upper
128	48.0	36.1	54.1
54	47.5	41.4	62.2




Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): BF0
 Ion 54.00 (53.70 to 54.70): BF0

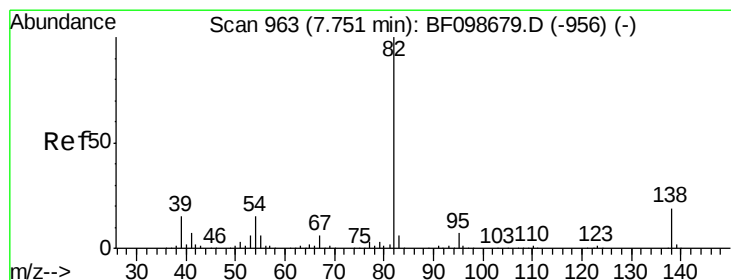
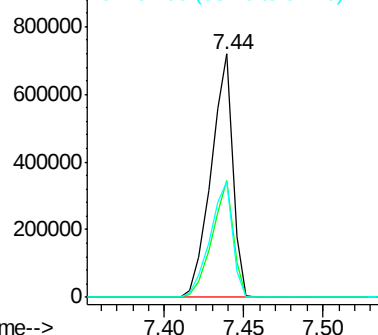



#25
 Isophorone
 Concen: 48.04 ng
 RT: 7.44 min Scan# 910
 Delta R.T. -0.31 min
 Lab File: BF099052.D
 Acq: 4 Oct 2017 1:25

Tgt Ion	82	Resp	671009
Ion Ratio	100	Lower	Upper
95	0.0	5.2	7.8#
138	0.0	14.9	22.3#

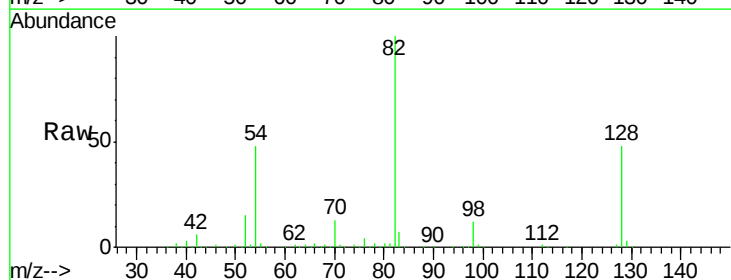

Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 95.00 (94.70 to 95.70): BF0
 Ion 138.00 (137.70 to 138.70): BF0

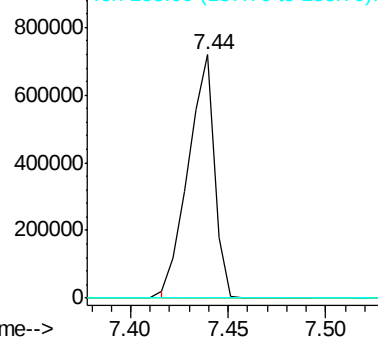



#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.91 min Scan# 1330

Delta R.T. -0.05 min

Lab File: BF099052.D

Acq: 4 Oct 2017 1:25

Instrument :

BNA_F

ClientSampled :


Tot Ion:164 Resp: 154198

Ion Ratio Lower Upper

164 100

162 102.6 86.1 129.1




160 44.9 38.3 57.5

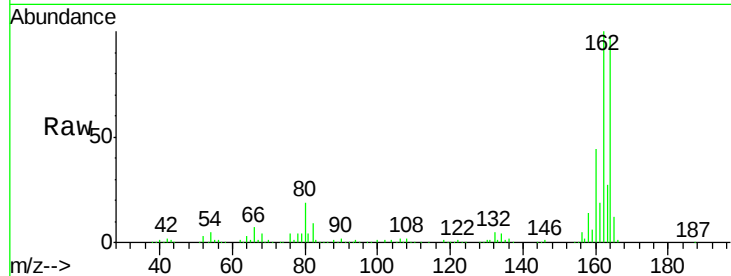

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

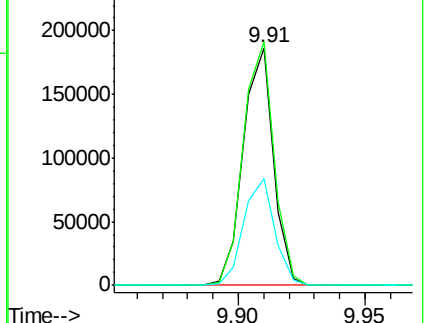

#41

2,4,6-Tribromophenol

Concen: 116.71 ng

RT: 10.70 min Scan# 1464

Delta R.T. -0.05 min

Lab File: BF099052.D

Acq: 4 Oct 2017 1:25


Tgt Ion:330 Resp: 147254

Ion Ratio Lower Upper

330 100

332 97.9 77.0 115.6



141 42.0 29.9 44.9




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

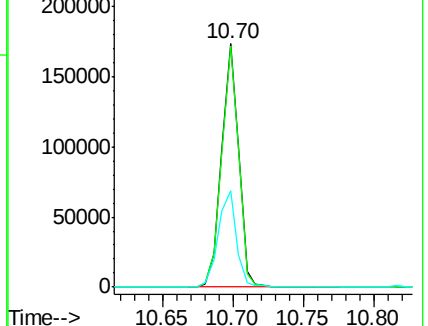







#44
 2-Fluorobiphenyl
 Concen: 99.96 ng
 RT: 9.23 min Scan# 1214
 Delta R.T. -0.05 min
 Lab File: BF099052.D
 Acq: 4 Oct 2017 1:25

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:172 Resp: 923296
 Ion Ratio Lower Upper
 172 100
 171 35.9 29.7 44.5
 170 24.3 19.6 29.4

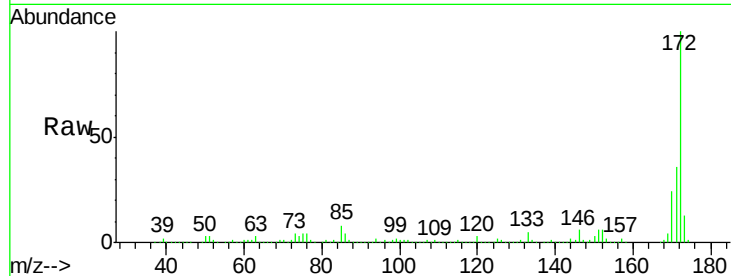


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

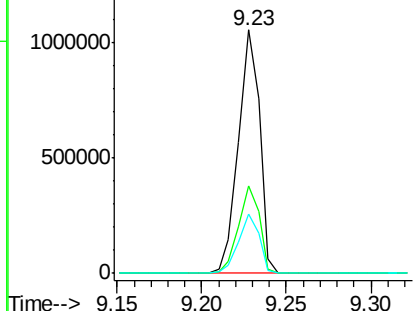
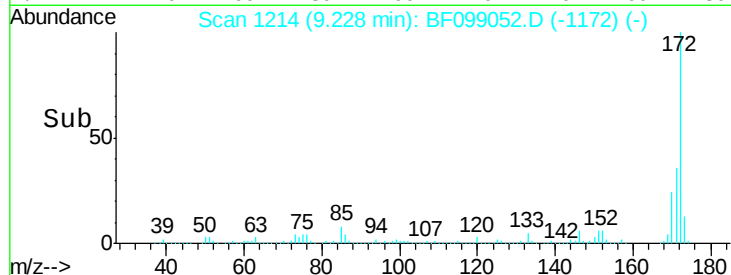



#49
 Dimethylphthalate
 Concen: 17.92 ng
 RT: 9.62 min Scan# 1281
 Delta R.T. -0.06 min
 Lab File: BF099052.D
 Acq: 4 Oct 2017 1:25

Tgt Ion:163 Resp: 208554
 Ion Ratio Lower Upper
 163 100
 194 3.6 2.7 4.1
 164 9.6 8.2 12.2



Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

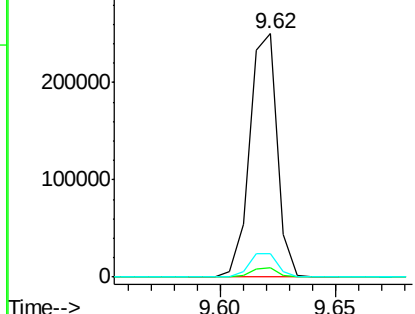



#56

2,4-Dinitrotoluene

Concen: 6.05 ng

RT: 9.91 min Scan# 1330

Delta R.T. -0.24 min

Lab File: BF099052.D

Acq: 4 Oct 2017 1:25

Instrument :

BNA_F

ClientSampleId :

Tot Ion:165 Resp: 19905


Ion Ratio Lower Upper

165 100

63 1.3 36.4 54.6#

89 1.7 57.8 86.6#

182 0.0 1.6 2.4#






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E

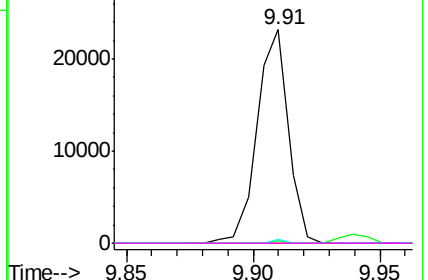

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.40 min Scan# 1583

Delta R.T. -0.05 min

Lab File: BF099052.D

Acq: 4 Oct 2017 1:25


Tgt Ion:188 Resp: 225788

Ion Ratio Lower Upper

188 100

94 9.9 8.5 12.7



80 9.9 9.2 13.8




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

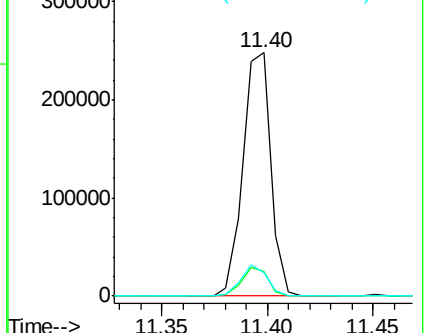


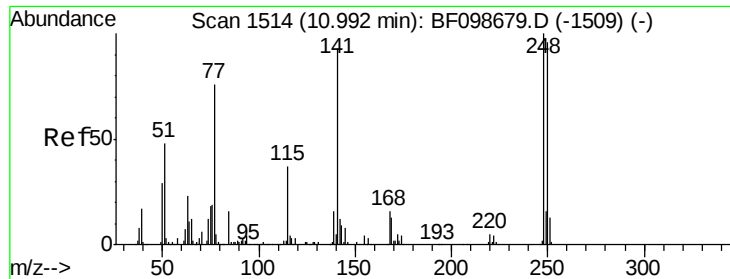




#66
 4-Bromophenyl-phenylether
 Concen: 4.54 ng
 RT: 10.70 min Scan# 1464
 Delta R.T. -0.29 min
 Lab File: BF099052.D
 Acq: 4 Oct 2017 1:25

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:248 Resp: 10032
 Ion Ratio Lower Upper
 248 100
 250 206.0 76.9 115.3#
 141 574.9 74.4 111.6#

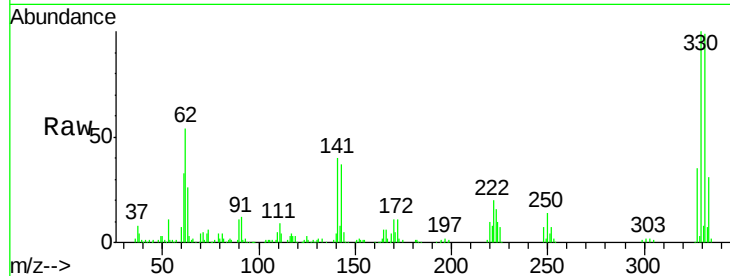


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

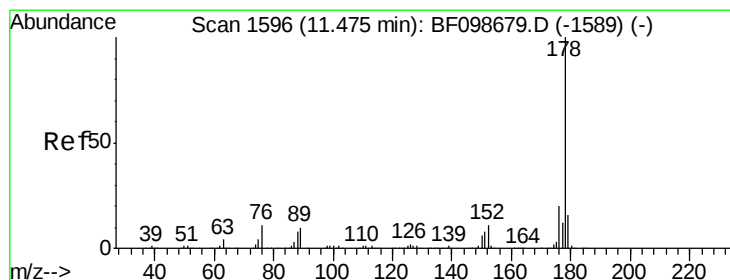
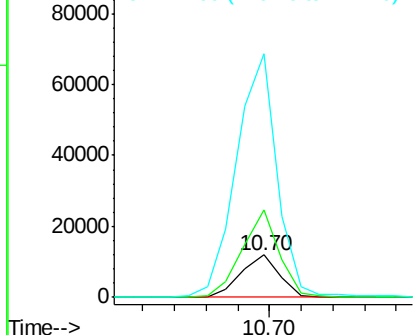



#70
 Phenanthrene
 Concen: 8.19 ng
 RT: 11.42 min Scan# 1587
 Delta R.T. -0.05 min
 Lab File: BF099052.D
 Acq: 4 Oct 2017 1:25

Tgt Ion:178 Resp: 98964
 Ion Ratio Lower Upper
 178 100
 176 19.1 15.8 23.8
 179 14.6 13.0 19.6



Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 176.00 (175.70 to 176.70): E
 Ion 179.00 (178.70 to 179.70): E

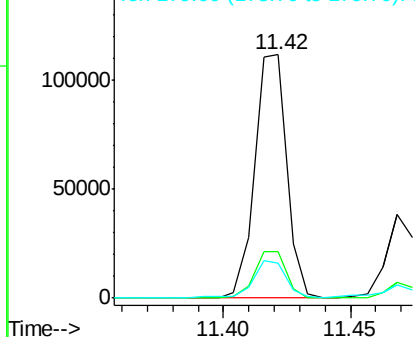







#71
 Anthracene
 Concen: 2.46 ng
 RT: 11.47 min Scan# 1595
 Delta R.T. -0.06 min
 Lab File: BF099052.D
 Acq: 4 Oct 2017 1:25

Instrument :
 BNA_F
 ClientSampled :

Tot Ion:178 Resp: 30417
 Ion Ratio Lower Upper
 178 100
 176 18.6 15.4 23.2
 179 16.5 12.6 19.0

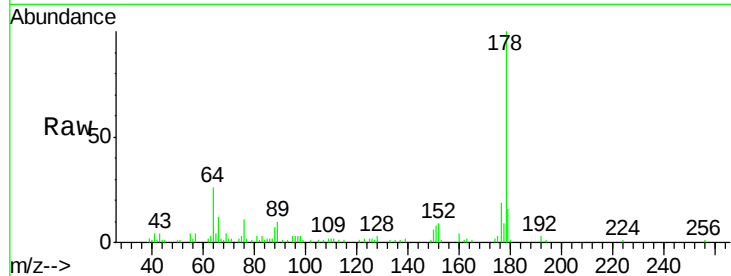


Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 176.00 (175.70 to 176.70): E
 Ion 179.00 (178.70 to 179.70): E

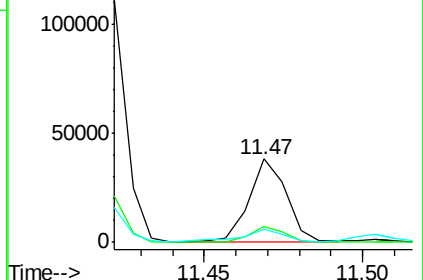
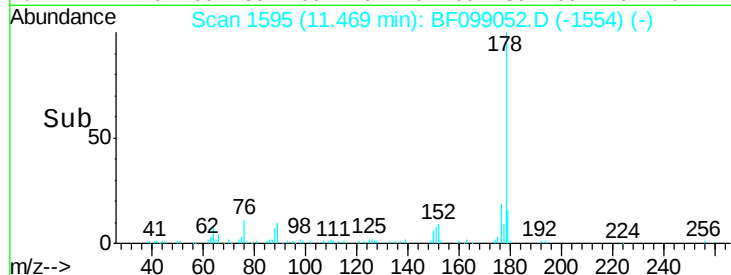



#74
 Fluoranthene
 Concen: 15.04 ng
 RT: 12.62 min Scan# 1790
 Delta R.T. -0.05 min
 Lab File: BF099052.D
 Acq: 4 Oct 2017 1:25

Tgt Ion:202 Resp: 184097
 Ion Ratio Lower Upper
 202 100
 101 13.6 0.0 34.1
 203 17.4 0.0 38.1



Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 203.00 (202.70 to 203.70): E

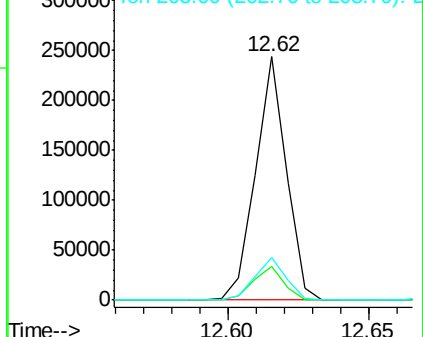



#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.03 min Scan# 2031

Delta R.T. -0.05 min

Lab File: BF099052.D

Acq: 4 Oct 2017 1:25

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 238906

Ion Ratio Lower Upper

240 100

120 15.3 9.5 14.3#




236 25.6 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

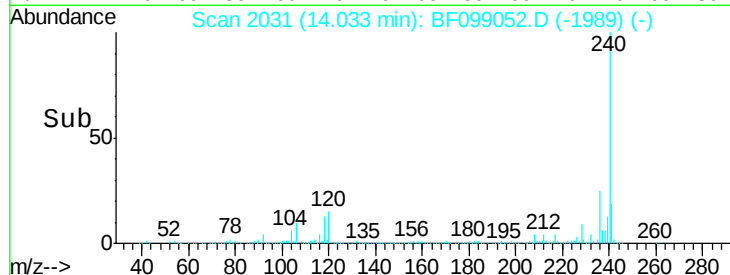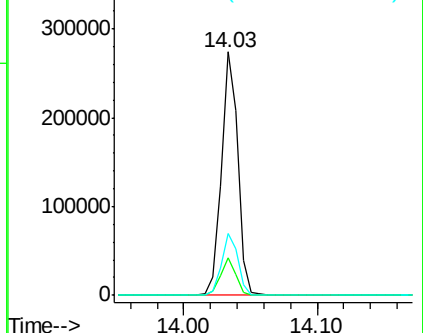

#77

Pyrene

Concen: 8.82 ng

RT: 12.84 min Scan# 1828

Delta R.T. -0.05 min

Lab File: BF099052.D

Acq: 4 Oct 2017 1:25


Tgt Ion:202 Resp: 160742

Ion Ratio Lower Upper

202 100

200 20.8 17.4 26.2



203 17.4 14.3 21.5




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

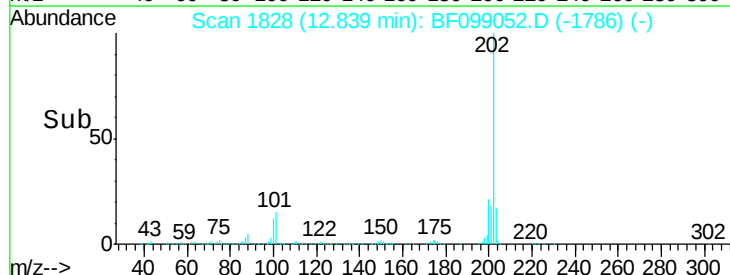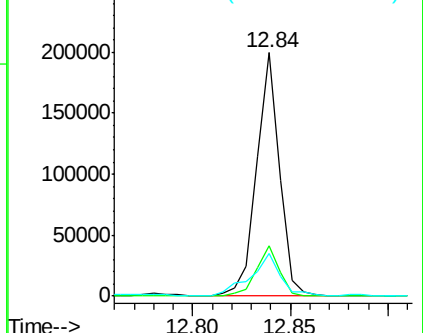



#78

Terphenyl-d14

Concen: 62.19 ng

RT: 12.98 min Scan# 1852

Delta R.T. -0.05 min

Lab File: BF099052.D

Acq: 4 Oct 2017 1:25

Instrument :

BNA_F

ClientSampleId :


Tot Ion:244 Resp: 653321

Ion Ratio Lower Upper

244 100

212 7.1 5.4 8.0

122 13.8 11.0 16.4





Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

12.98

Time-->

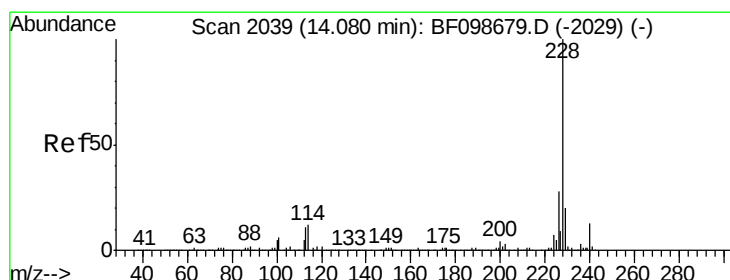

#80

Benzo(a)anthracene

Concen: 6.14 ng

RT: 14.02 min Scan# 2029

Delta R.T. -0.05 min

Lab File: BF099052.D

Acq: 4 Oct 2017 1:25


Tgt Ion:228 Resp: 88795

Ion Ratio Lower Upper

228 100

226 28.3 22.6 33.8

229 21.4 15.8 23.6




Abundance Ion 228.00 (227.70 to 228.70): E


Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

14.02

Time-->





#82

Chrysene

Concen: 5.64 ng

RT: 14.06 min Scan# 2035

Delta R.T. -0.06 min

Lab File: BF099052.D

Acq: 4 Oct 2017 1:25

Instrument :

BNA_F

ClientSampleId :


Tot Ion:228 Resp: 77701

Ion Ratio Lower Upper

228 100

226 29.1 25.0 37.6




229 23.6 16.2 24.4



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

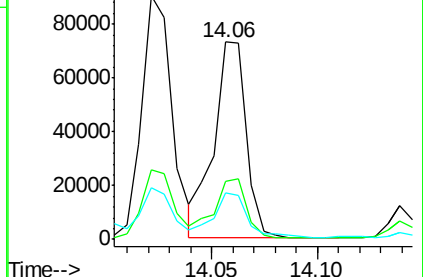

#85

Indeno(1,2,3-cd)pyrene

Concen: 3.05 ng

RT: 16.99 min Scan# 2533

Delta R.T. -0.10 min

Lab File: BF099052.D

Acq: 4 Oct 2017 1:25


Tgt Ion:276 Resp: 33644

Ion Ratio Lower Upper

276 100

138 31.6 25.0 37.6



277 28.7 20.1 30.1




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

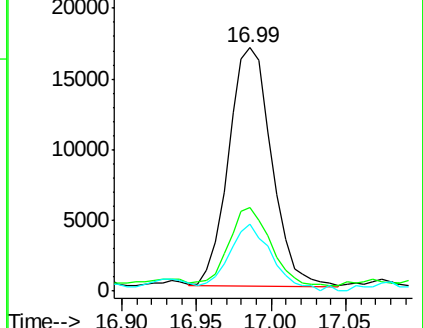







#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.51 min Scan# 2282
Delta R.T. -0.06 min
Lab File: BF099052.D
Acq: 4 Oct 2017 1:25

Instrument :
BNA_F
ClientSampled :

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.2	19.2	28.8
265	22.3	17.5	26.3




Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

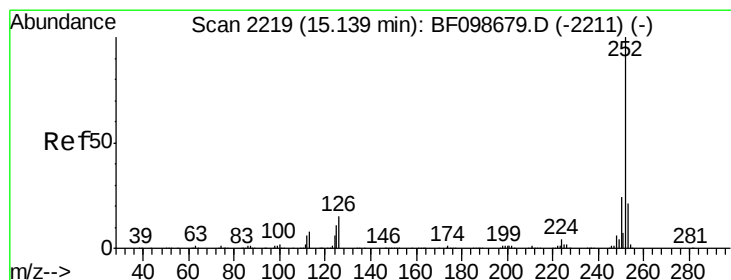
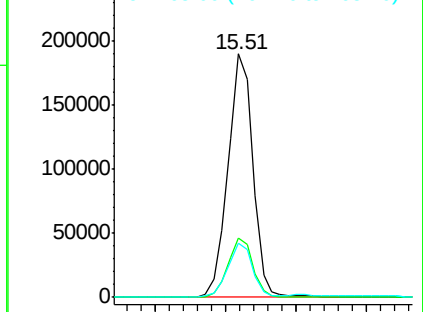



#87
Benzo(b)fluoranthene
Concen: 9.34 ng
RT: 15.07 min Scan# 2208
Delta R.T. -0.06 min
Lab File: BF099052.D
Acq: 4 Oct 2017 1:25

Tgt Ion	Ratio	Lower	Upper
252	100		
253	21.0	17.0	25.6
125	16.0	9.0	13.6



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

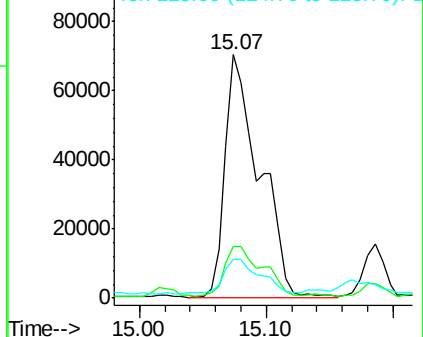


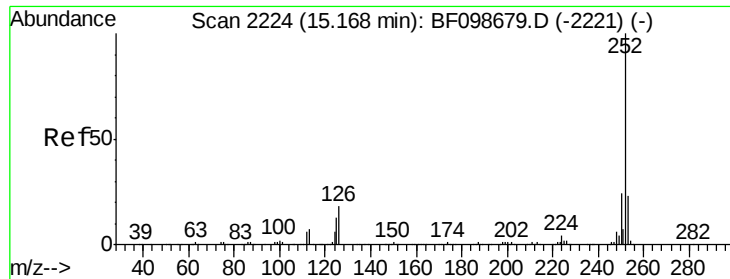




#88
Benzo(k)fluoranthene
Concen: 9.46 ng
RT: 15.07 min Scan# 2208
Delta R.T. -0.09 min
Lab File: BF099052.D
Acq: 4 Oct 2017 1:25

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
252	100		
253	21.0	17.9	26.9
125	16.0	10.2	15.2#




Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

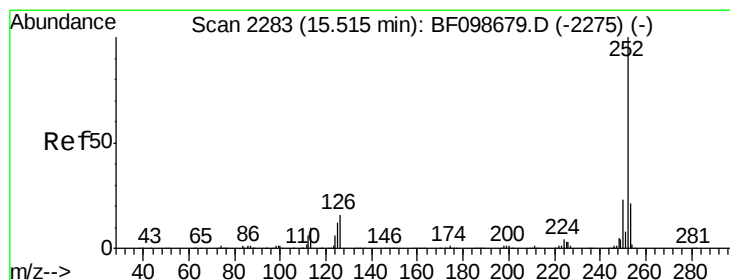
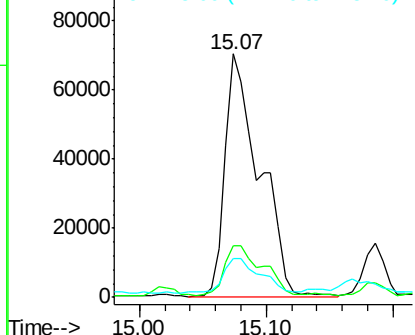



#89
Benzo(a)pyrene
Concen: 5.47 ng
RT: 15.44 min Scan# 2271
Delta R.T. -0.07 min
Lab File: BF099052.D
Acq: 4 Oct 2017 1:25

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.7	17.1	25.7
125	14.8	9.8	14.6#

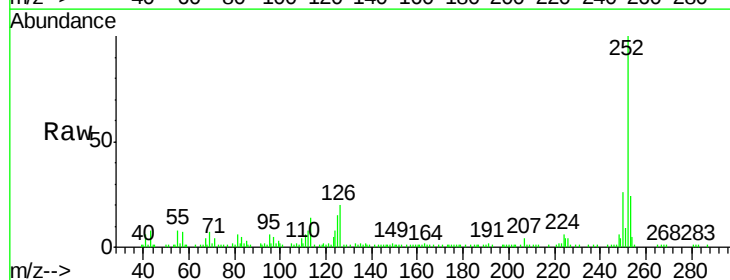

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

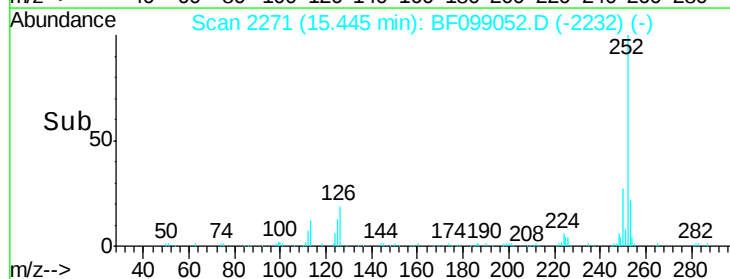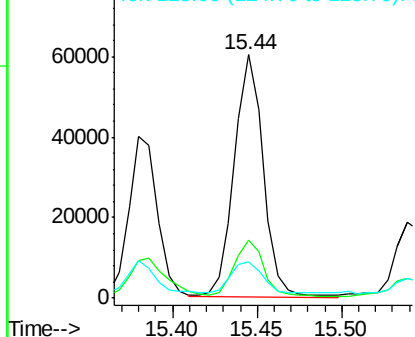

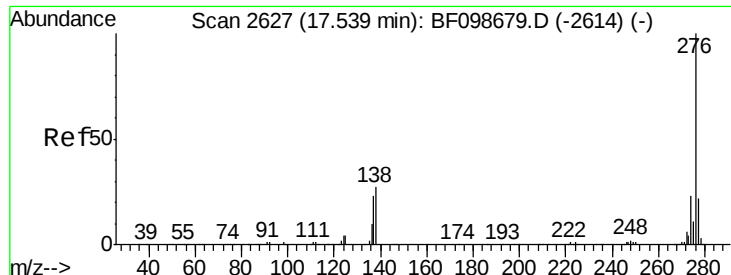

#91
 Benzo(a,h,i)perylene
 Concen: 3.12 ng
 RT: 17.44 min Scan# 2610
 Delta R.T. -0.11 min
 Lab File: BF099052.D
 Acq: 4 Oct 2017 1:25

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
276	100		
277	23.6	17.9	26.9
138	30.9	21.8	32.8

