

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100317\
 Data File : BF099043.D
 Acq On : 3 Oct 2017 21:16
 Operator : SJ/JU
 Sample : I5531-11RE 2X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-62A-2.5-5RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.151	7	11	29	rVB	123230	236058	9.47%	1.280%
2	4.475	402	406	411	rBV	86431	98369	3.94%	0.533%
3	4.604	425	428	433	rBV	32885	34011	1.36%	0.184%
4	4.781	456	458	470	rBV	23033	36006	1.44%	0.195%
5	5.104	506	513	516	rBV	1839791	2493769	100.00%	13.522%
6	5.487	572	578	582	rVB2	75557	79504	3.19%	0.431%
7	6.486	743	748	755	rVB	840011	752849	30.19%	4.082%
8	6.633	770	773	777	rVB	265328	211639	8.49%	1.148%
9	6.698	781	784	788	rVB2	28461	28800	1.15%	0.156%
10	6.869	810	813	817	rBV	898154	783558	31.42%	4.249%
11	6.928	819	823	826	rBV	146798	119506	4.79%	0.648%
12	7.028	836	840	843	rBV	1918948	1567098	62.84%	8.497%
13	7.433	905	909	912	rVB	1396337	1178939	47.28%	6.393%
14	8.128	1023	1027	1028	rBV2	34081	28424	1.14%	0.154%
15	8.151	1028	1031	1034	rVV	1100092	965318	38.71%	5.234%
16	8.439	1073	1080	1085	rBV6	18927	31139	1.25%	0.169%
17	8.569	1098	1102	1104	rBV	31552	27242	1.09%	0.148%
18	8.739	1128	1131	1134	rBV	49422	38638	1.55%	0.210%
19	8.863	1150	1152	1155	rVB	39469	30301	1.22%	0.164%
20	8.963	1166	1169	1173	rBV2	33263	38004	1.52%	0.206%
21	9.169	1201	1204	1206	rBV	37818	29852	1.20%	0.162%
22	9.227	1209	1214	1217	rBV	2490417	2049264	82.18%	11.112%
23	9.304	1224	1227	1229	rBV	89973	82037	3.29%	0.445%
24	9.492	1255	1259	1262	rBV4	26410	37457	1.50%	0.203%
25	9.563	1268	1271	1273	rBV	37272	33014	1.32%	0.179%
26	9.616	1277	1280	1283	rBV	378469	315720	12.66%	1.712%
27	9.769	1303	1306	1309	rBV2	31738	30736	1.23%	0.167%
28	9.833	1312	1317	1319	rVB2	75595	86310	3.46%	0.468%
29	9.910	1324	1330	1333	rVV	1094179	949133	38.06%	5.146%
30	9.939	1333	1335	1339	rVB	51614	36348	1.46%	0.197%
31	10.110	1361	1364	1367	rVV2	38865	41663	1.67%	0.226%
32	10.151	1368	1371	1375	rVB3	35130	37450	1.50%	0.203%
33	10.222	1380	1383	1385	rBV3	29646	27338	1.10%	0.148%
34	10.327	1395	1401	1404	rBV	112890	119806	4.80%	0.650%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100317\
 Data File : BF099043.D
 Acq On : 3 Oct 2017 21:16
 Operator : SJ/JU
 Sample : I5531-11RE 2X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-62A-2.5-5RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	10.410	1409	1415	1417	rVB5	18017	28525	1.14%	0.155%
36	10.451	1419	1422	1425	rBV2	34563	34721	1.39%	0.188%
37	10.551	1435	1439	1444	rVB	50513	69952	2.81%	0.379%
38	10.804	1479	1482	1483	rBV	114798	109883	4.41%	0.596%
39	11.251	1554	1558	1560	rBV	128987	111767	4.48%	0.606%
40	11.280	1560	1563	1570	rVB3	61289	81896	3.28%	0.444%
41	11.392	1578	1582	1585	rBV	879605	759621	30.46%	4.119%
42	11.416	1585	1586	1589	rVV	209722	134893	5.41%	0.731%
43	11.468	1593	1595	1597	rVB	36828	28149	1.13%	0.153%
44	11.604	1614	1618	1620	rBV	52873	59756	2.40%	0.324%
45	11.674	1627	1630	1634	rVB2	58293	46819	1.88%	0.254%
46	11.721	1634	1638	1644	rBV2	17015	26136	1.05%	0.142%
47	11.892	1664	1667	1669	rBV	32454	30492	1.22%	0.165%
48	11.921	1669	1672	1674	rVB	36963	29572	1.19%	0.160%
49	12.004	1682	1686	1689	rBV3	38027	45764	1.84%	0.248%
50	12.080	1697	1699	1704	rBV	47375	49440	1.98%	0.268%
51	12.439	1757	1760	1762	rBV2	31555	32312	1.30%	0.175%
52	12.468	1762	1765	1769	rVB3	52867	59256	2.38%	0.321%
53	12.604	1785	1788	1792	rBV	187293	153433	6.15%	0.832%
54	12.792	1816	1820	1822	rVB3	39801	37162	1.49%	0.202%
55	12.851	1822	1830	1835	rBV2	455585	627456	25.16%	3.402%
56	12.974	1847	1851	1854	rBV	1450098	1190689	47.75%	6.456%
57	13.051	1860	1864	1867	rBV5	22752	43150	1.73%	0.234%
58	13.198	1887	1889	1892	rVB3	31151	25437	1.02%	0.138%
59	13.451	1929	1932	1936	rBV	145200	115172	4.62%	0.624%
60	13.539	1945	1947	1950	rBV2	33038	30560	1.23%	0.166%
61	13.862	2000	2002	2006	rVB2	82009	83840	3.36%	0.455%
62	14.033	2027	2031	2034	rBV	707193	681584	27.33%	3.696%
63	14.057	2034	2035	2039	rVB	61758	34557	1.39%	0.187%
64	14.486	2106	2108	2114	rBV	60314	73136	2.93%	0.397%
65	15.139	2216	2219	2224	rVB	85939	101606	4.07%	0.551%
66	15.509	2278	2282	2291	rVB	617123	850322	34.10%	4.611%


Sum of corrected areas: 18442358

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100317\
Data File : BF099043.D
Acq On : 3 Oct 2017 21:16
Operator : SJ/JU
Sample : I5531-11RE 2X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
G-62A-2.5-5RE

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

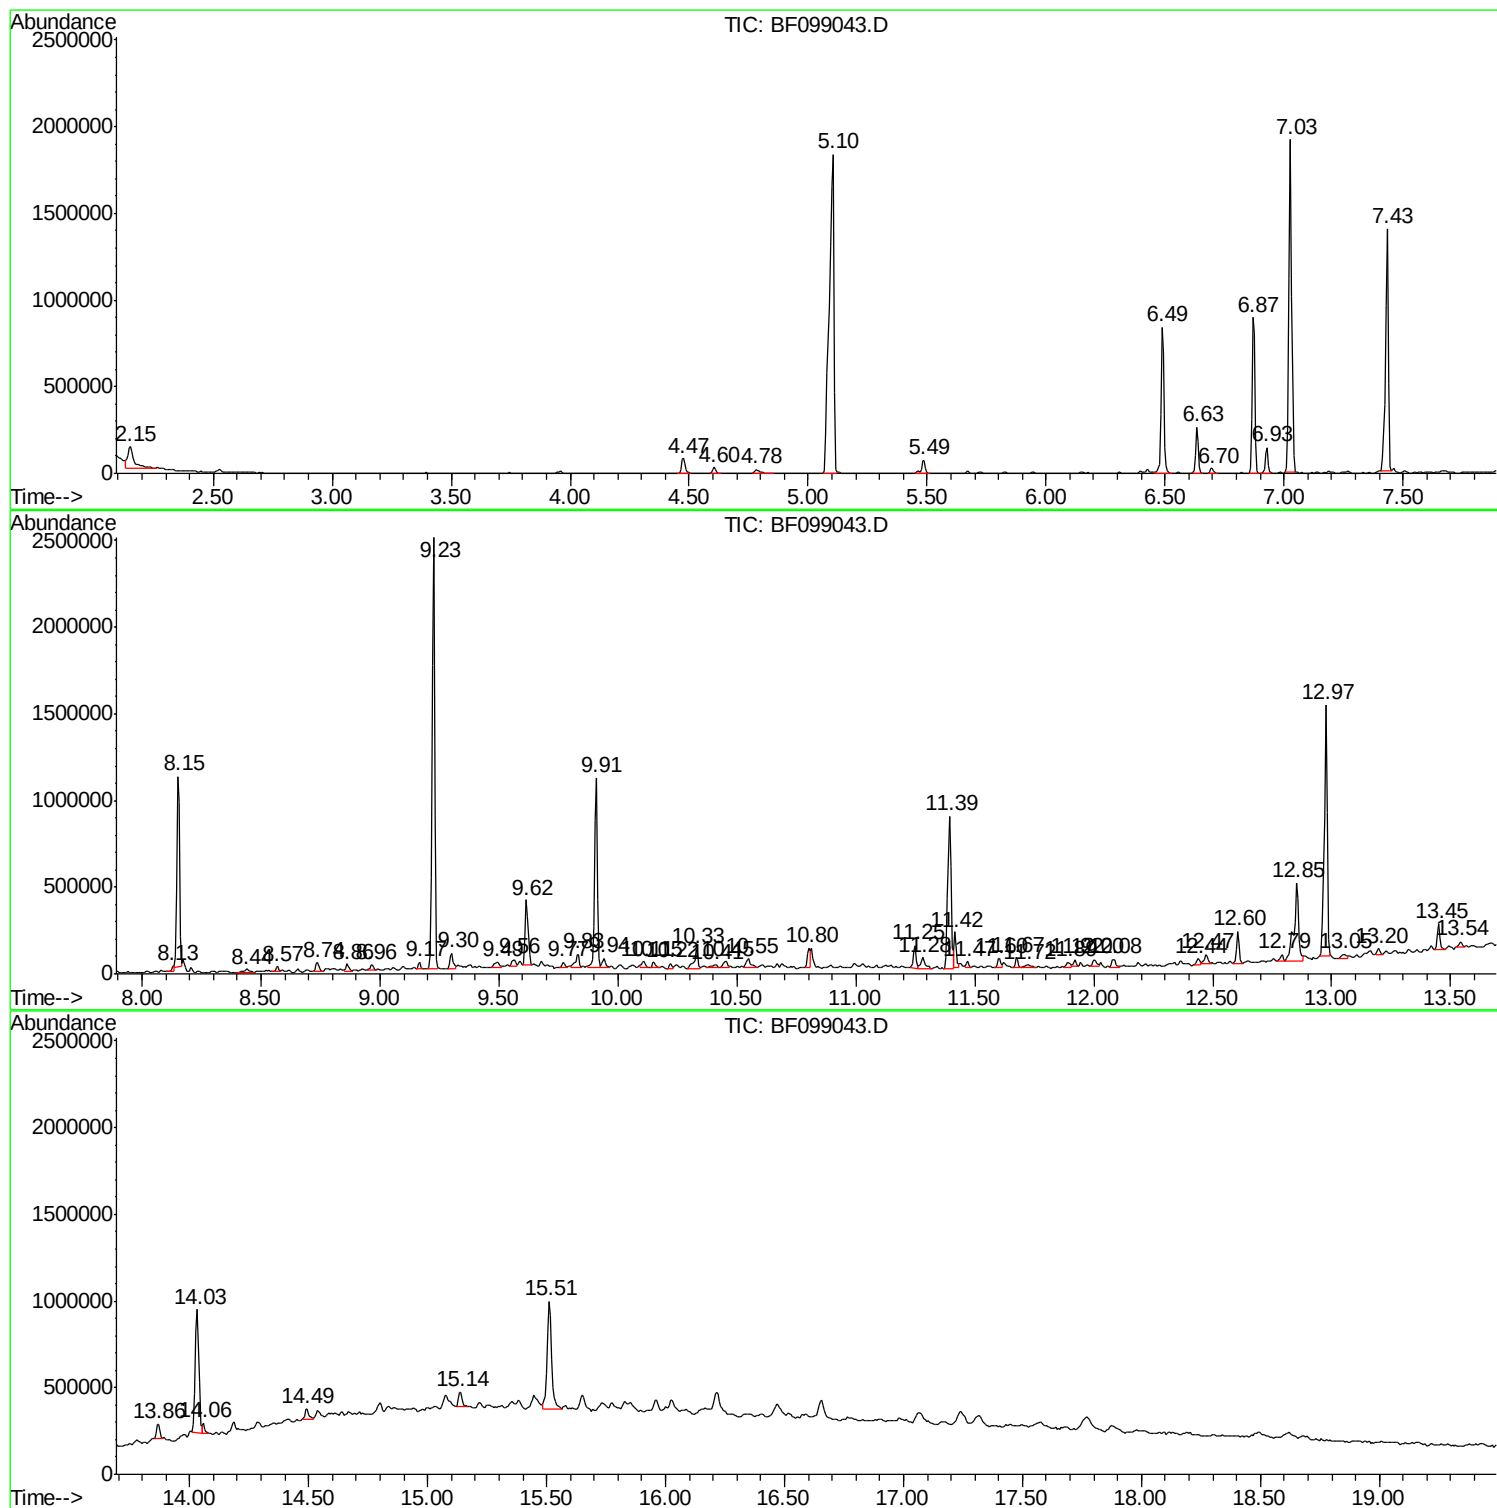

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF100317\
Data_File : BF099043.D
Acq_On : 3_Oct_2017. 21:166
Operator : SJ/JUU
Sample : I5531-11RE_2XX
Misc :
ALS_Vial : 9 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
G-62A-2.5-5RE

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
