

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100317\
 Data File : BF099045.D
 Acq On : 3 Oct 2017 22:12
 Operator : SJ/JU
 Sample : I5531-09RE 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-62A-0-2.5RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.463	400	404	413	rBV	151823	164236	18.15%	1.734%
2	5.081	505	509	522	rBV	824695	904723	100.00%	9.555%
3	5.481	575	577	582	rVB	25687	20825	2.30%	0.220%
4	6.487	745	748	758	rVB	371553	292338	32.31%	3.087%
5	6.634	770	773	777	rVB	81183	68169	7.53%	0.720%
6	6.875	810	814	817	rVB	804575	695714	76.90%	7.347%
7	6.928	819	823	826	rBV	29487	23996	2.65%	0.253%
8	7.028	836	840	843	rBV	586472	456922	50.50%	4.825%
9	7.428	905	908	912	rBV	390683	311860	34.47%	3.293%
10	7.769	960	966	968	rBV2	7803	10474	1.16%	0.111%
11	8.157	1028	1032	1035	rVV	911596	822199	90.88%	8.683%
12	8.210	1037	1041	1043	rVB2	32684	29936	3.31%	0.316%
13	8.439	1073	1080	1082	rBV5	17992	23974	2.65%	0.253%
14	8.533	1092	1096	1099	rBV3	8922	11297	1.25%	0.119%
15	8.569	1099	1102	1104	rBV	38048	30178	3.34%	0.319%
16	8.657	1113	1117	1119	rBV2	15010	13324	1.47%	0.141%
17	8.739	1128	1131	1135	rBV2	25826	25171	2.78%	0.266%
18	8.775	1135	1137	1140	rVV3	11249	15364	1.70%	0.162%
19	8.839	1144	1148	1150	rVV4	13306	17599	1.95%	0.186%
20	8.863	1150	1152	1156	rVB	25610	21391	2.36%	0.226%
21	8.963	1165	1169	1173	rVB2	27338	31633	3.50%	0.334%
22	9.033	1176	1181	1182	rBV5	7555	9845	1.09%	0.104%
23	9.057	1182	1185	1189	rVB4	16228	18982	2.10%	0.200%
24	9.098	1189	1192	1195	rBV4	14521	17729	1.96%	0.187%
25	9.169	1201	1204	1210	rVB	47621	36010	3.98%	0.380%
26	9.227	1210	1214	1217	rBV	633326	542886	60.01%	5.733%
27	9.304	1223	1227	1232	rBV4	33469	43190	4.77%	0.456%
28	9.375	1237	1239	1241	rVV2	15466	14205	1.57%	0.150%
29	9.422	1245	1247	1251	rVB2	14867	14334	1.58%	0.151%
30	9.492	1255	1259	1264	rVB2	41335	56802	6.28%	0.600%
31	9.563	1268	1271	1274	rVV	55229	52427	5.79%	0.554%
32	9.592	1274	1276	1278	rVV	36279	26890	2.97%	0.284%
33	9.616	1278	1280	1284	rVV2	120996	118529	13.10%	1.252%
34	9.680	1288	1291	1293	rBV2	23953	21824	2.41%	0.230%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100317\
 Data File : BF099045.D
 Acq On : 3 Oct 2017 22:12
 Operator : SJ/JU
 Sample : I5531-09RE 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-62A-0-2.5RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	9.769	1303	1306	1309	rBV2	22940	22887	2.53%	0.242%
36	9.816	1311	1314	1316	rBV3	15028	17804	1.97%	0.188%
37	9.910	1326	1330	1333	rBV	824383	691846	76.47%	7.306%
38	9.939	1334	1335	1338	rVB2	16232	12009	1.33%	0.127%
39	10.010	1344	1347	1351	rBV2	26848	31642	3.50%	0.334%
40	10.051	1351	1354	1358	rBV4	9709	14864	1.64%	0.157%
41	10.110	1358	1364	1367	rVV3	31839	43410	4.80%	0.458%
42	10.151	1367	1371	1380	rVB3	40641	62376	6.89%	0.659%
43	10.222	1380	1383	1385	rBV	32313	30017	3.32%	0.317%
44	10.251	1385	1388	1390	rVB	20913	14813	1.64%	0.156%
45	10.316	1395	1399	1400	rBV2	24095	29468	3.26%	0.311%
46	10.327	1400	1401	1404	rVB	30050	19393	2.14%	0.205%
47	10.451	1417	1422	1424	rBV4	18065	23770	2.63%	0.251%
48	10.551	1435	1439	1445	rVB2	51377	61633	6.81%	0.651%
49	10.727	1467	1469	1474	rVB5	9641	12153	1.34%	0.128%
50	10.816	1479	1484	1487	rBV	112491	110651	12.23%	1.169%
51	10.892	1495	1497	1502	rBV4	12417	12319	1.36%	0.130%
52	11.027	1517	1520	1525	rBV5	17001	18827	2.08%	0.199%
53	11.192	1546	1548	1552	rBV4	8282	9775	1.08%	0.103%
54	11.251	1552	1558	1560	rVV3	25995	28460	3.15%	0.301%
55	11.280	1560	1563	1569	rVB3	46669	56235	6.22%	0.594%
56	11.345	1569	1574	1576	rBV3	8979	11960	1.32%	0.126%
57	11.392	1579	1582	1585	rBV	688942	599175	66.23%	6.328%
58	11.416	1585	1586	1589	rVB	43020	27494	3.04%	0.290%
59	11.504	1597	1601	1603	rBV4	9663	12077	1.33%	0.128%
60	11.627	1619	1622	1626	rVV4	12738	12431	1.37%	0.131%
61	11.674	1628	1630	1634	rVB3	13498	11038	1.22%	0.117%
62	11.892	1665	1667	1670	rBV2	13806	17433	1.93%	0.184%
63	11.921	1670	1672	1675	rVB	18171	16195	1.79%	0.171%
64	12.004	1684	1686	1689	rBV2	14213	11710	1.29%	0.124%
65	12.192	1715	1718	1721	rBV3	10720	10674	1.18%	0.113%
66	12.368	1745	1748	1751	rBV5	15220	17541	1.94%	0.185%
67	12.445	1758	1761	1763	rBV3	22193	15967	1.76%	0.169%
68	12.474	1763	1766	1769	rVB4	22106	22466	2.48%	0.237%
69	12.568	1779	1782	1786	rBV5	10432	12334	1.36%	0.130%
70	12.604	1786	1788	1793	rBV	54348	51817	5.73%	0.547%
71	12.757	1812	1814	1817	rBV3	10621	10996	1.22%	0.116%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100317\
Data File : BF099045.D
Acq On : 3 Oct 2017 22:12
Operator : SJ/JU
Sample : I5531-09RE 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-62A-0-2.5RE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	12.792	1817	1820	1822	rBV4	18608	17599	1.95%	0.186%
73	12.839	1824	1828	1829	rBV	57535	61787	6.83%	0.653%
74	12.851	1829	1830	1835	rVB	66907	59001	6.52%	0.623%
75	12.974	1845	1851	1854	rBV	523653	453493	50.13%	4.789%
76	13.451	1929	1932	1937	rBV	67154	59229	6.55%	0.626%
77	13.539	1945	1947	1950	rBV3	23595	18559	2.05%	0.196%
78	14.033	2027	2031	2034	rBV	805715	711708	78.67%	7.516%
79	15.139	2216	2219	2227	rVB2	88974	132821	14.68%	1.403%
80	15.509	2278	2282	2291	rVB	591634	804164	88.89%	8.493%


Sum of corrected areas: 9468997

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100317\
Data File : BF099045.D
Acq On : 3 Oct 2017 22:12
Operator : SJ/JU
Sample : I5531-09RE 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
G-62A-0-2.5RE

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

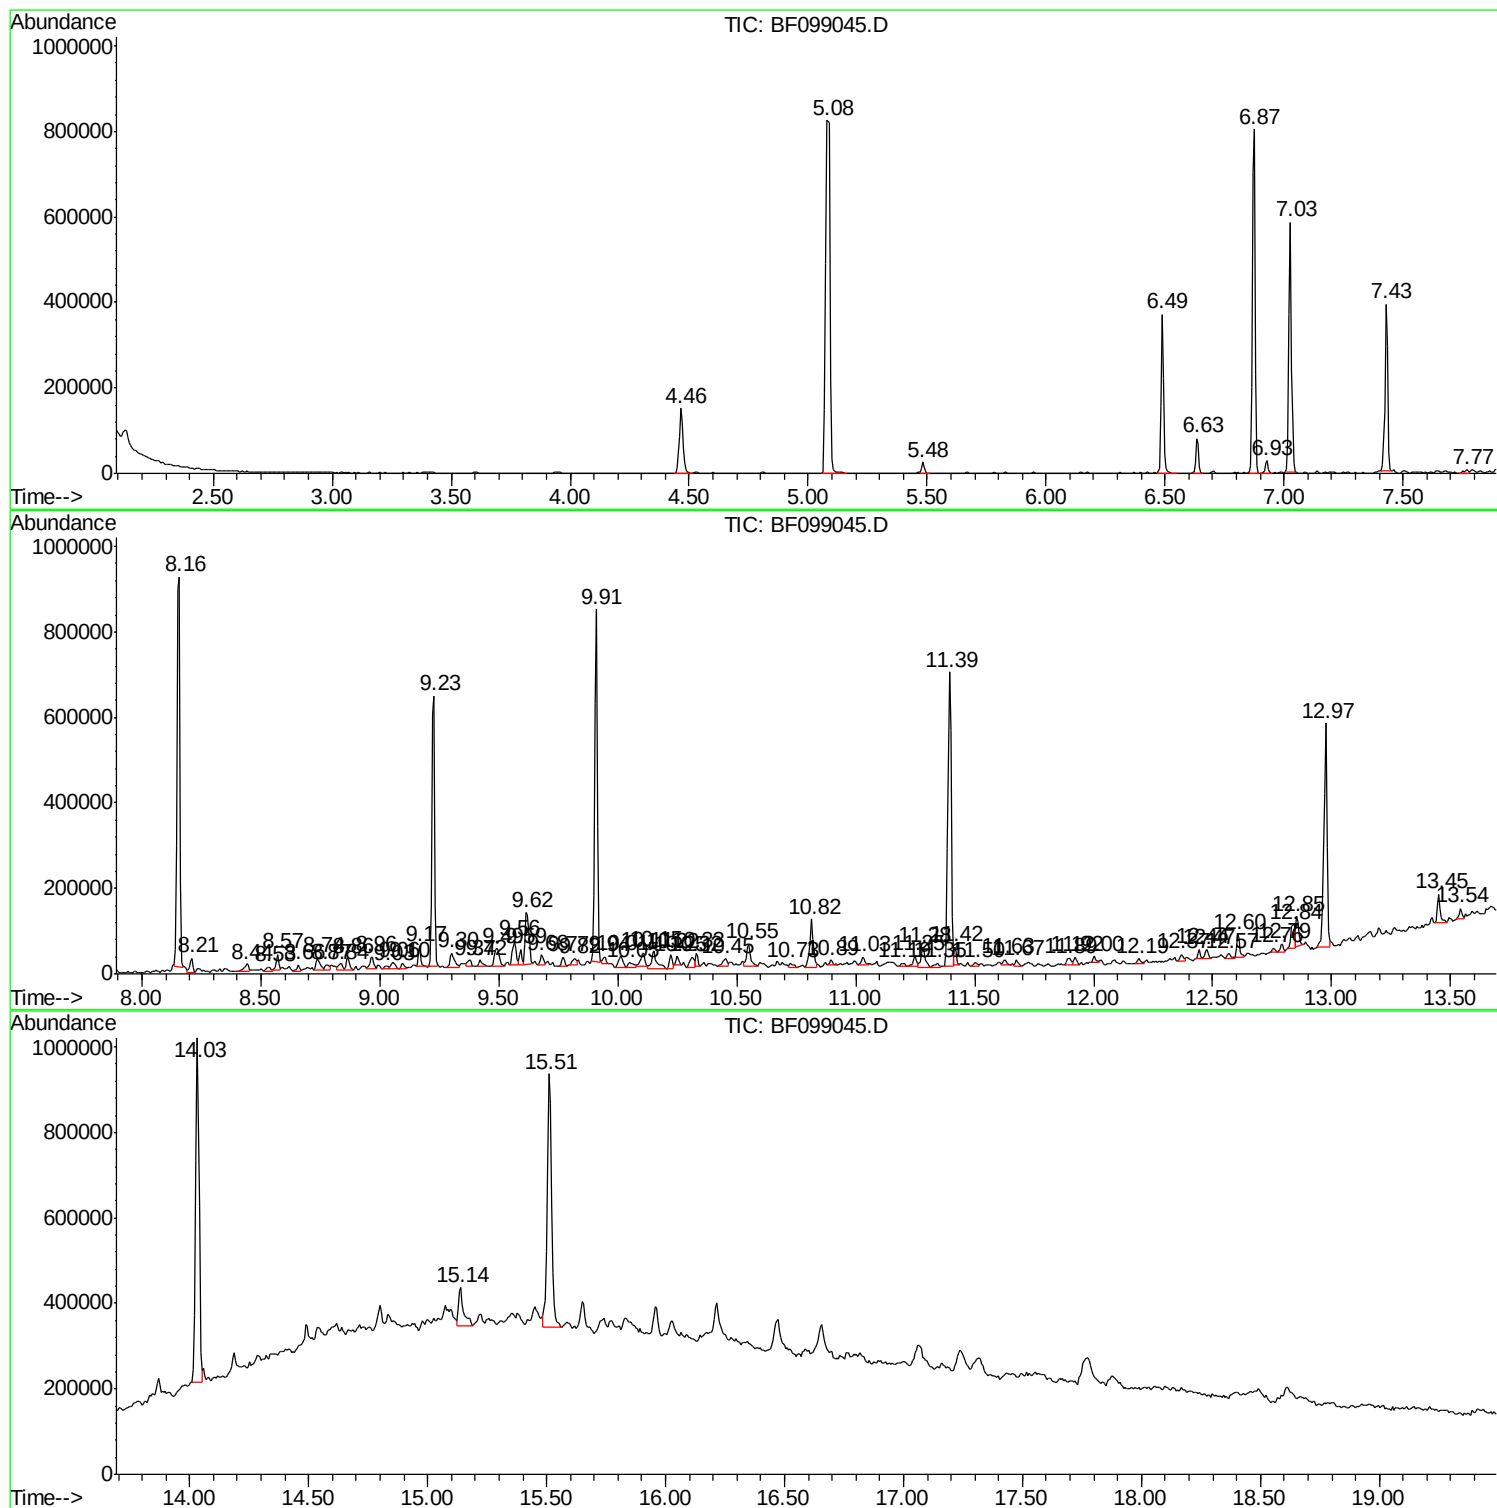

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF100317\
Data_File : BF099045.D
Acq_On : 3_Oct_2017. 22:122
Operator : SJ/JUU
Sample : I5531-09RE_5XX
Misc :
ALS_Vial : 11 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
G-62A-0-2.5RE

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
