

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100317\
 Data File : BF099062.D
 Acq On : 4 Oct 2017 6:28
 Operator : SJ/JU
 Sample : I5531-07DL 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-63-2.5-5DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.481	571	577	581	rVB2	306178	360544	12.77%	0.448%
2	6.034	666	671	674	rVB4	154880	215196	7.62%	0.267%
3	6.116	680	685	692	rBV3	314597	550137	19.49%	0.683%
4	6.310	713	718	720	rBV2	214963	274936	9.74%	0.342%
5	6.369	726	728	731	rVB	267880	200024	7.09%	0.248%
6	6.404	731	734	740	rBV5	268953	462264	16.38%	0.574%
7	6.487	745	748	752	rBV	340543	280263	9.93%	0.348%
8	6.616	765	770	771	rBV3	230016	310055	10.98%	0.385%
9	6.634	771	773	781	rVB2	391224	637575	22.59%	0.792%
10	6.875	811	814	818	rVB2	1123243	1291736	45.76%	1.605%
11	6.928	818	823	826	rBV4	176445	231663	8.21%	0.288%
12	7.016	835	838	842	rBV2	565810	699567	24.78%	0.869%
13	7.051	842	844	846	rVB	309123	219704	7.78%	0.273%
14	7.145	857	860	863	rVB	587209	539418	19.11%	0.670%
15	7.269	874	881	883	rBV2	486849	598945	21.22%	0.744%
16	7.298	883	886	890	rVB5	218536	286200	10.14%	0.356%
17	7.404	898	904	907	rBV3	898086	1198919	42.47%	1.489%
18	7.445	907	911	915	rVB4	358794	463773	16.43%	0.576%
19	7.516	918	923	926	rBV5	691766	1008073	35.71%	1.252%
20	7.575	926	933	936	rBV4	523014	1079828	38.25%	1.341%
21	7.645	943	945	948	rBV3	506163	544445	19.29%	0.676%
22	7.681	948	951	953	rVB3	567608	531647	18.83%	0.660%
23	7.751	959	963	965	rBV3	485586	553618	19.61%	0.688%
24	7.775	965	967	968	rBV	370413	232484	8.24%	0.289%
25	7.798	968	971	974	rVB3	805341	708713	25.11%	0.880%
26	7.828	974	976	980	rVB4	570685	562703	19.93%	0.699%
27	7.869	980	983	985	rBV3	254731	249290	8.83%	0.310%
28	7.892	985	987	989	rBV	592120	495407	17.55%	0.615%
29	7.922	989	992	997	rVB5	396960	508911	18.03%	0.632%
30	7.975	997	1001	1006	rBV5	431751	653669	23.16%	0.812%
31	8.022	1006	1009	1013	rBV2	539731	690408	24.46%	0.858%
32	8.057	1013	1015	1019	rBV2	298789	354633	12.56%	0.441%
33	8.104	1019	1023	1026	rBV4	465193	811259	28.74%	1.008%
34	8.157	1026	1032	1035	rVV4	1088196	1954328	69.23%	2.428%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100317\
 Data File : BF099062.D
 Acq On : 4 Oct 2017 6:28
 Operator : SJ/JU
 Sample : I5531-07DL 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-63-2.5-5DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	8.216	1038	1042	1044	rVB2	2045536	2156957	76.41%	2.679%
36	8.245	1044	1047	1049	rBV3	792876	829806	29.40%	1.031%
37	8.310	1054	1058	1059	rBV2	382953	420158	14.88%	0.522%
38	8.334	1059	1062	1064	rVV3	347238	362007	12.82%	0.450%
39	8.363	1064	1067	1069	rVB2	599592	551939	19.55%	0.686%
40	8.445	1077	1081	1085	rVB6	1050958	1335061	47.29%	1.658%
41	8.504	1089	1091	1094	rVB4	460223	374004	13.25%	0.465%
42	8.539	1094	1097	1100	rBV4	741866	772410	27.36%	0.959%
43	8.575	1100	1103	1105	rBV	1793262	1640653	58.12%	2.038%
44	8.598	1105	1107	1109	rVV3	593718	430487	15.25%	0.535%
45	8.622	1109	1111	1115	rVB4	797275	704869	24.97%	0.876%
46	8.663	1115	1118	1120	rBV2	842481	656606	23.26%	0.816%
47	8.698	1120	1124	1126	rBV4	614866	717426	25.41%	0.891%
48	8.745	1130	1132	1136	rBV4	531991	701084	24.84%	0.871%
49	8.787	1136	1139	1141	rBV4	411581	543494	19.25%	0.675%
50	8.845	1146	1149	1151	rVV3	954568	1104919	39.14%	1.372%
51	8.875	1151	1154	1157	rVB	933733	737530	26.13%	0.916%
52	8.904	1157	1159	1162	rBV3	661576	483841	17.14%	0.601%
53	8.934	1162	1164	1166	rBV3	575873	607588	21.52%	0.755%
54	8.975	1168	1171	1174	rVV	1418121	1526673	54.08%	1.896%
55	9.004	1174	1176	1178	rVB2	499885	367651	13.02%	0.457%
56	9.039	1178	1182	1184	rBV4	484378	762713	27.02%	0.947%
57	9.063	1184	1186	1189	rVV3	814826	764084	27.07%	0.949%
58	9.104	1190	1193	1195	rVV4	365794	435919	15.44%	0.541%
59	9.151	1199	1201	1203	rVV3	584084	551431	19.53%	0.685%
60	9.181	1203	1206	1211	rVV	2066892	2189851	77.57%	2.720%
61	9.228	1212	1214	1216	rVB3	515769	379991	13.46%	0.472%
62	9.316	1225	1229	1233	rBV3	1082872	1576258	55.84%	1.958%
63	9.357	1233	1236	1238	rBV2	399466	464652	16.46%	0.577%
64	9.428	1246	1248	1253	rVB3	586013	624890	22.14%	0.776%
65	9.504	1257	1261	1264	rBV	1298535	1724124	61.08%	2.142%
66	9.575	1270	1273	1276	rBV	1352022	1690770	59.89%	2.100%
67	9.604	1276	1278	1280	rVV	1121863	915385	32.43%	1.137%
68	9.634	1280	1283	1286	rVB3	2548172	2822948	100.00%	3.507%
69	9.692	1290	1293	1295	rBV2	901621	852230	30.19%	1.059%
70	9.781	1305	1308	1311	rBV2	1238556	1312657	46.50%	1.631%
71	9.828	1311	1316	1319	rVB3	1298351	1464796	51.89%	1.819%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100317\
 Data File : BF099062.D
 Acq On : 4 Oct 2017 6:28
 Operator : SJ/JU
 Sample : I5531-07DL 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-63-2.5-5DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	9.951	1335	1337	1340	rBV3	528928	495463	17.55%	0.615%
73	10.022	1346	1349	1353	rVB2	1066924	1424129	50.45%	1.769%
74	10.063	1353	1356	1359	rBV3	517405	654402	23.18%	0.813%
75	10.116	1361	1365	1368	rVV3	1235599	1664299	58.96%	2.067%
76	10.163	1370	1373	1382	rVB3	1508862	2140401	75.82%	2.659%
77	10.233	1382	1385	1387	rBV	1181811	1186008	42.01%	1.473%
78	10.263	1387	1390	1392	rVV	904965	801413	28.39%	0.995%
79	10.328	1396	1401	1402	rBV3	1072769	1288696	45.65%	1.601%
80	10.369	1406	1408	1411	rBV3	379971	430635	15.25%	0.535%
81	10.457	1421	1423	1426	rBV2	464671	499798	17.70%	0.621%
82	10.533	1434	1436	1437	rBV	345033	226850	8.04%	0.282%
83	10.563	1437	1441	1446	rVB2	1653000	2212910	78.39%	2.749%
84	10.681	1459	1461	1463	rVB2	466471	346593	12.28%	0.431%
85	10.704	1463	1465	1466	rBV	374975	296788	10.51%	0.369%
86	10.828	1482	1486	1489	rBV	2779364	2812159	99.62%	3.493%
87	10.904	1497	1499	1501	rVB	498229	372007	13.18%	0.462%
88	11.039	1520	1522	1525	rVB4	651743	640447	22.69%	0.796%
89	11.292	1561	1565	1571	rVB2	1810630	2253731	79.84%	2.799%
90	11.404	1581	1584	1586	rBV2	711419	716810	25.39%	0.890%
91	11.428	1586	1588	1591	rVB	635053	501782	17.78%	0.623%
92	11.639	1621	1624	1626	rBV2	594059	608309	21.55%	0.756%
93	11.904	1667	1669	1671	rBV	385880	362661	12.85%	0.450%
94	11.933	1672	1674	1678	rVB	578737	494283	17.51%	0.614%
95	12.010	1685	1687	1690	rVB3	386024	316804	11.22%	0.394%
96	12.451	1759	1762	1765	rBV	395127	329393	11.67%	0.409%
97	12.616	1787	1790	1794	rVB	303625	272348	9.65%	0.338%
98	12.845	1826	1829	1831	rBV	237493	246257	8.72%	0.306%
99	14.033	2027	2031	2034	rBV	751811	809831	28.69%	1.006%
100	15.515	2278	2283	2291	rVB	584877	782054	27.70%	0.971%


Sum of corrected areas: 80505458

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100317\
Data File : BF099062.D
Acq On : 4 Oct 2017 6:28
Operator : SJ/JU
Sample : I5531-07DL 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-63-2.5-5DL

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

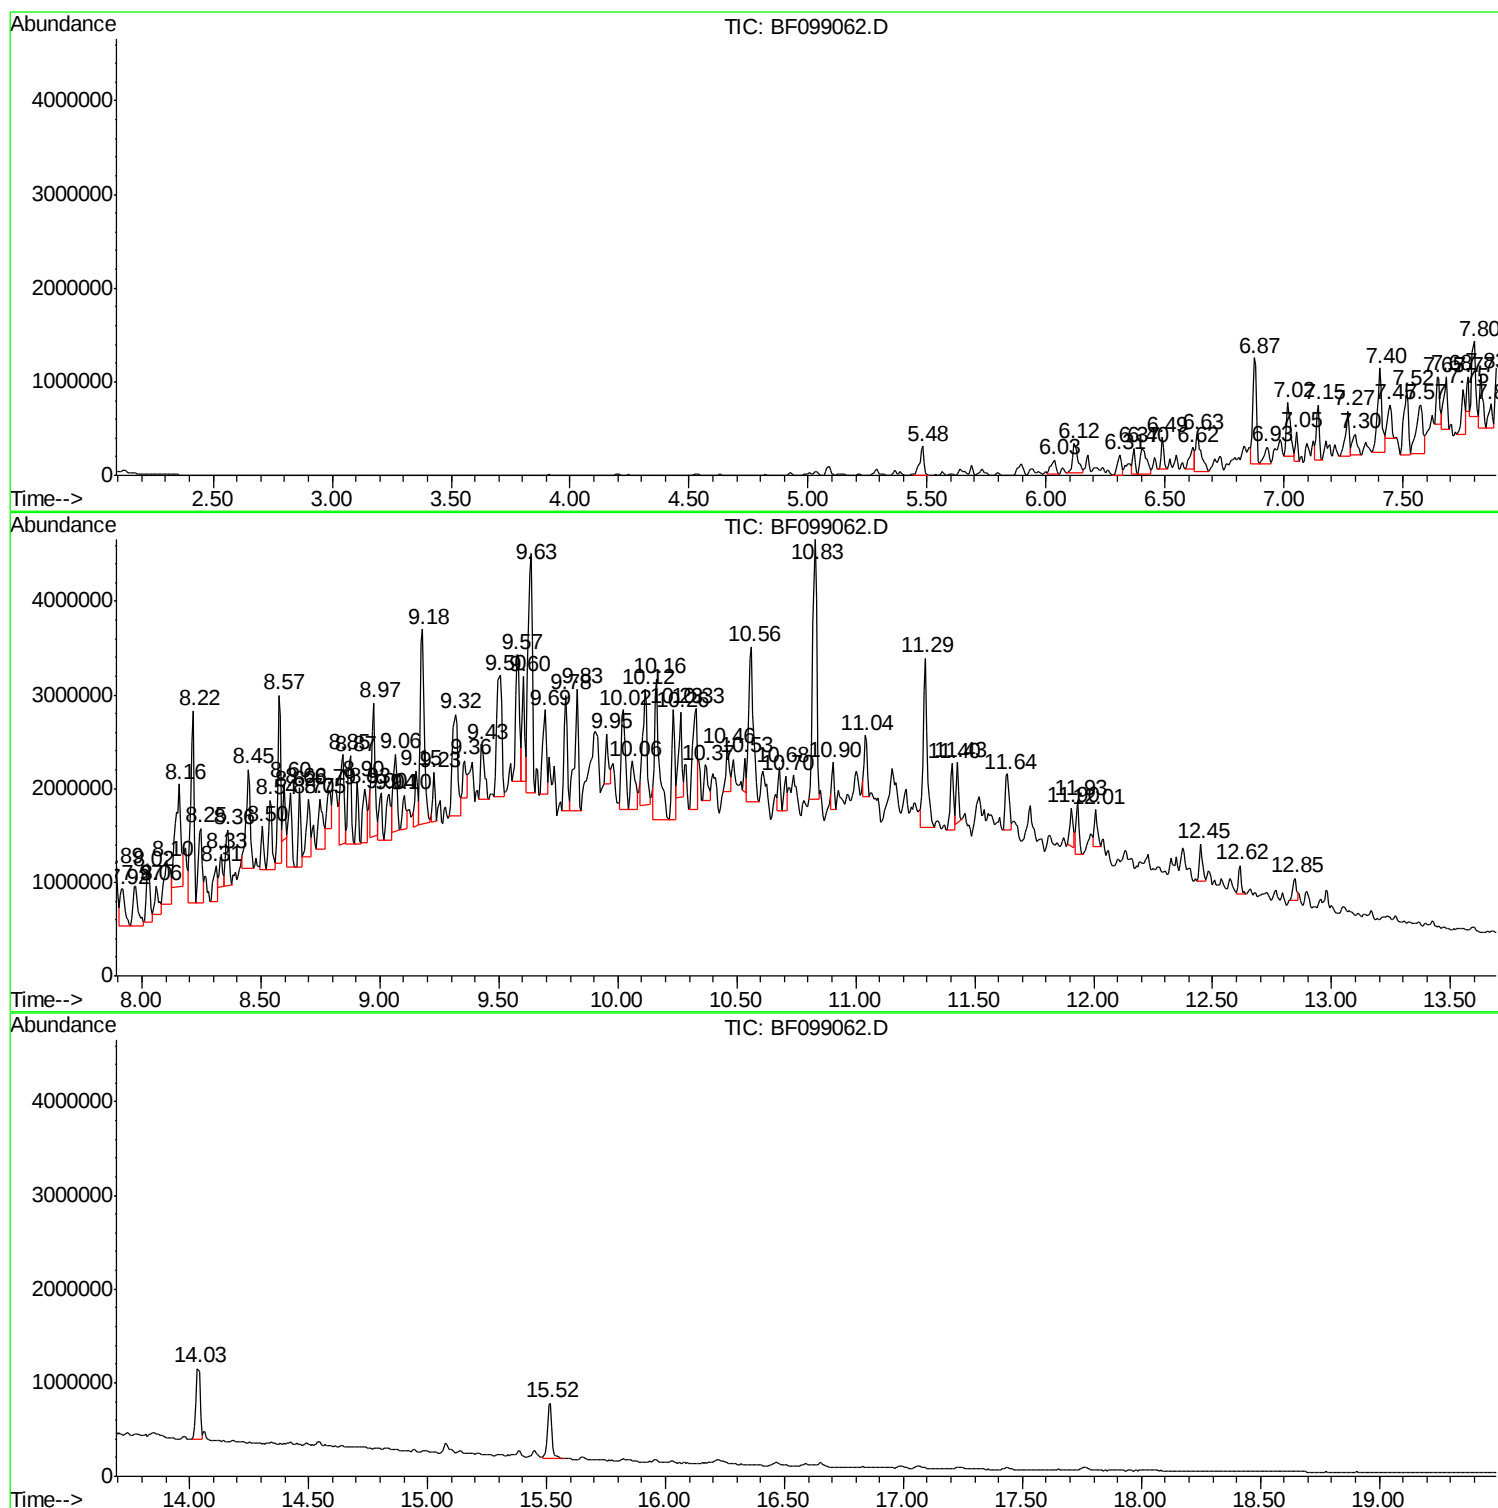

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF100317\
Data_File : BF099062.D
Acq_On : 4 Oct 2017 6:288
Operator : SJ/JUU
Sample : I5531-07DL_10XX
Misc :
ALS_Vial : 26 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
G-63-2.5-5DL

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
