


Data Path : Z:\HPCHEM1\BNA_F\Data\BF100317\
Data File : BF099023.D
Acq On : 3 Oct 2017 10:56
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Sep 23 13:50:58 2017

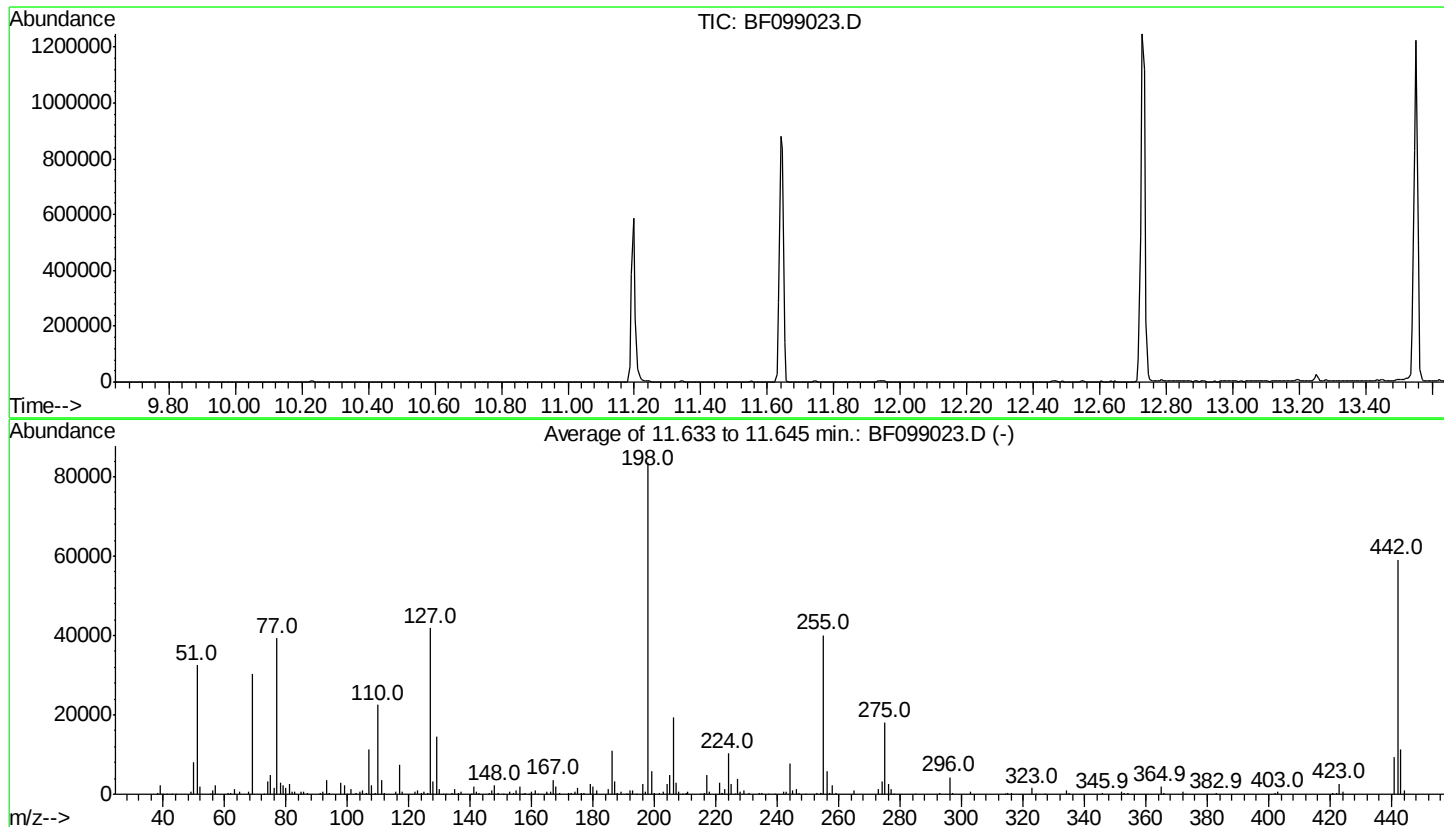

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	32544	PASS
68	69	0.00	2	1.9	581	PASS
69	198	0.00	100	36.4	30376	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.2	41904	PASS
197	198	0.00	2	1.0	798	PASS
198	198	100	100	100.0	83525	PASS
199	198	5	9	7.0	5860	PASS
275	198	10	60	21.5	17985	PASS
365	198	1	100	2.3	1919	PASS
441	442	0.01	24	15.8	9309	PASS
442	198	50	100	70.7	59050	PASS
443	442	15	24	19.4	11438	PASS