


Data Path : Z:\HPCHEM1\BNA F\Data\BF100317\
 Data File : BF099060.D
 Acq On : 4 Oct 2017 5:33
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 23 13:50:58 2017

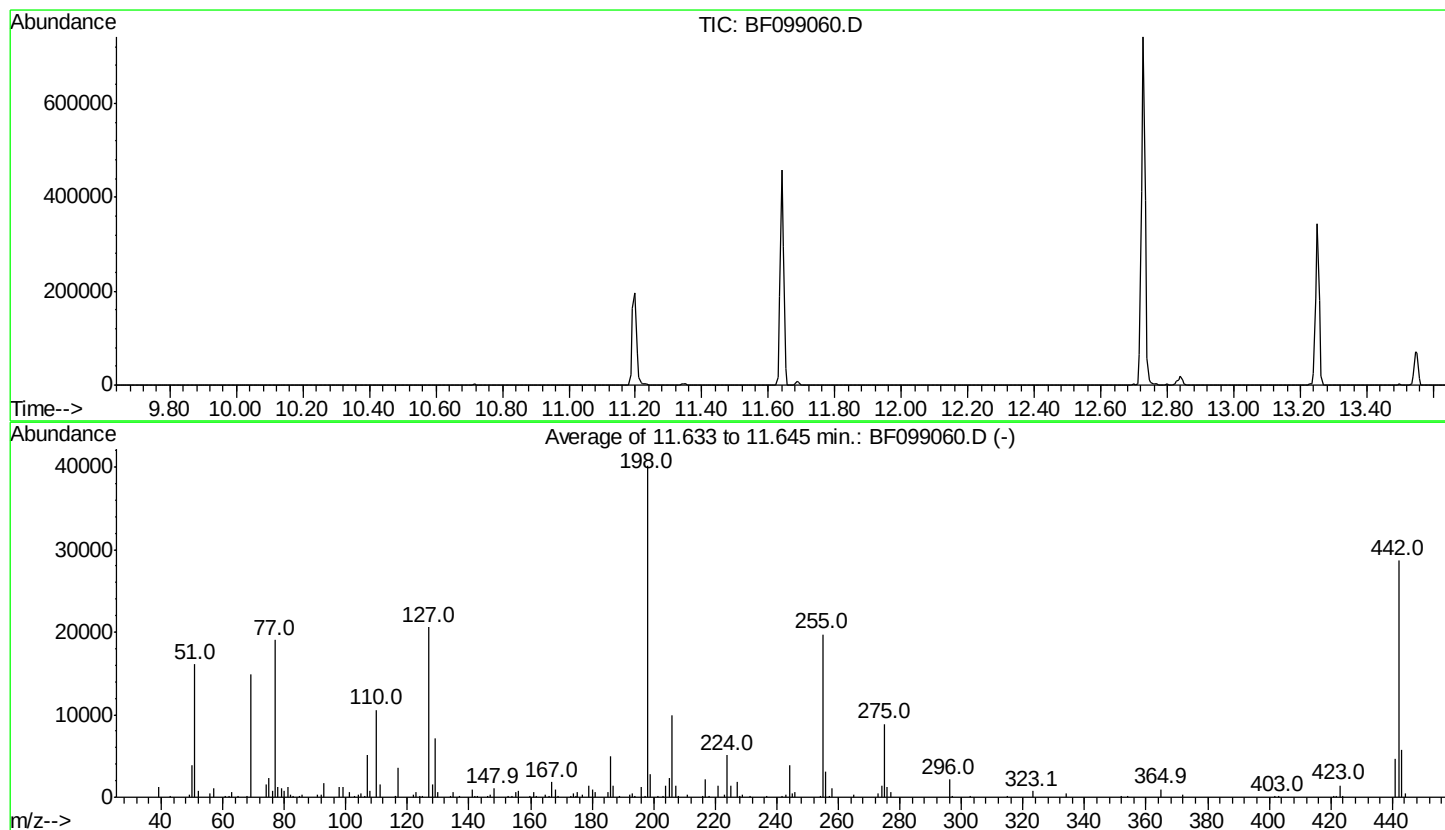

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	16106	PASS
68	69	0.00	2	1.5	222	PASS
69	198	0.00	100	37.0	14858	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.2	20562	PASS
197	198	0.00	2	0.5	192	PASS
198	198	100	100	100.0	40170	PASS
199	198	5	9	7.0	2804	PASS
275	198	10	60	22.1	8858	PASS
365	198	1	100	2.4	967	PASS
441	442	0.01	24	16.3	4665	PASS
442	198	50	100	71.3	28645	PASS
443	442	15	24	19.9	5696	PASS