


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF100319\
 Data File : BF117315.D
 Acq On : 3 Oct 2019 13:27
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 13 16:23:17 2019

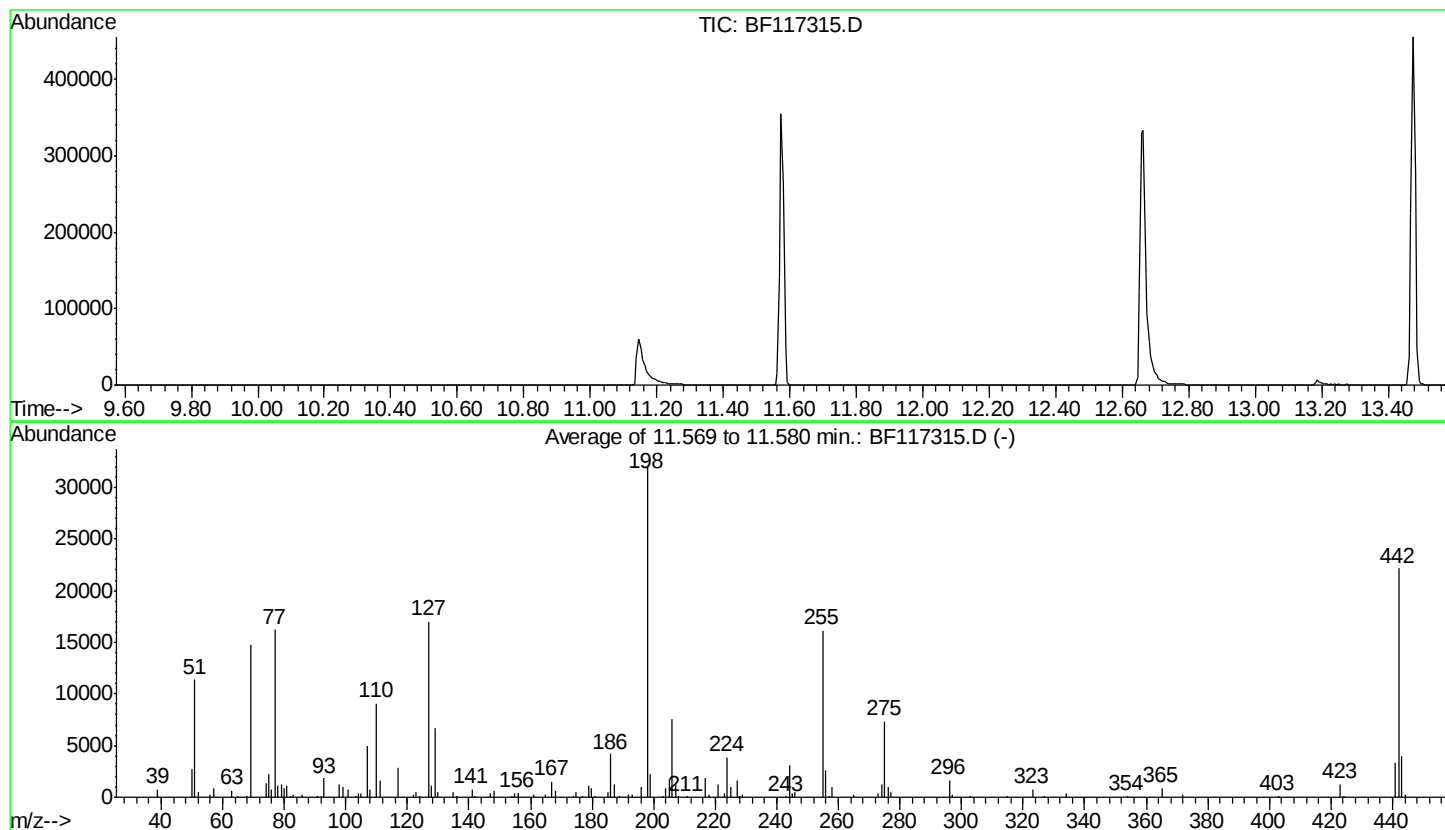

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	11378	PASS
68	69	0.00	2	0.7	108	PASS
69	198	0.00	100	45.9	14740	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.0	17025	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	32101	PASS
199	198	5	9	7.0	2242	PASS
275	198	10	60	22.9	7344	PASS
365	198	1	100	2.7	878	PASS
441	198	0.01	100	10.6	3389	PASS
442	198	50	100	69.0	22157	PASS
443	442	15	24	17.8	3937	PASS