


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100324\
Data File : BF139619.D
Acq On : 03 Oct 2024 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 02 04:58:47 2024

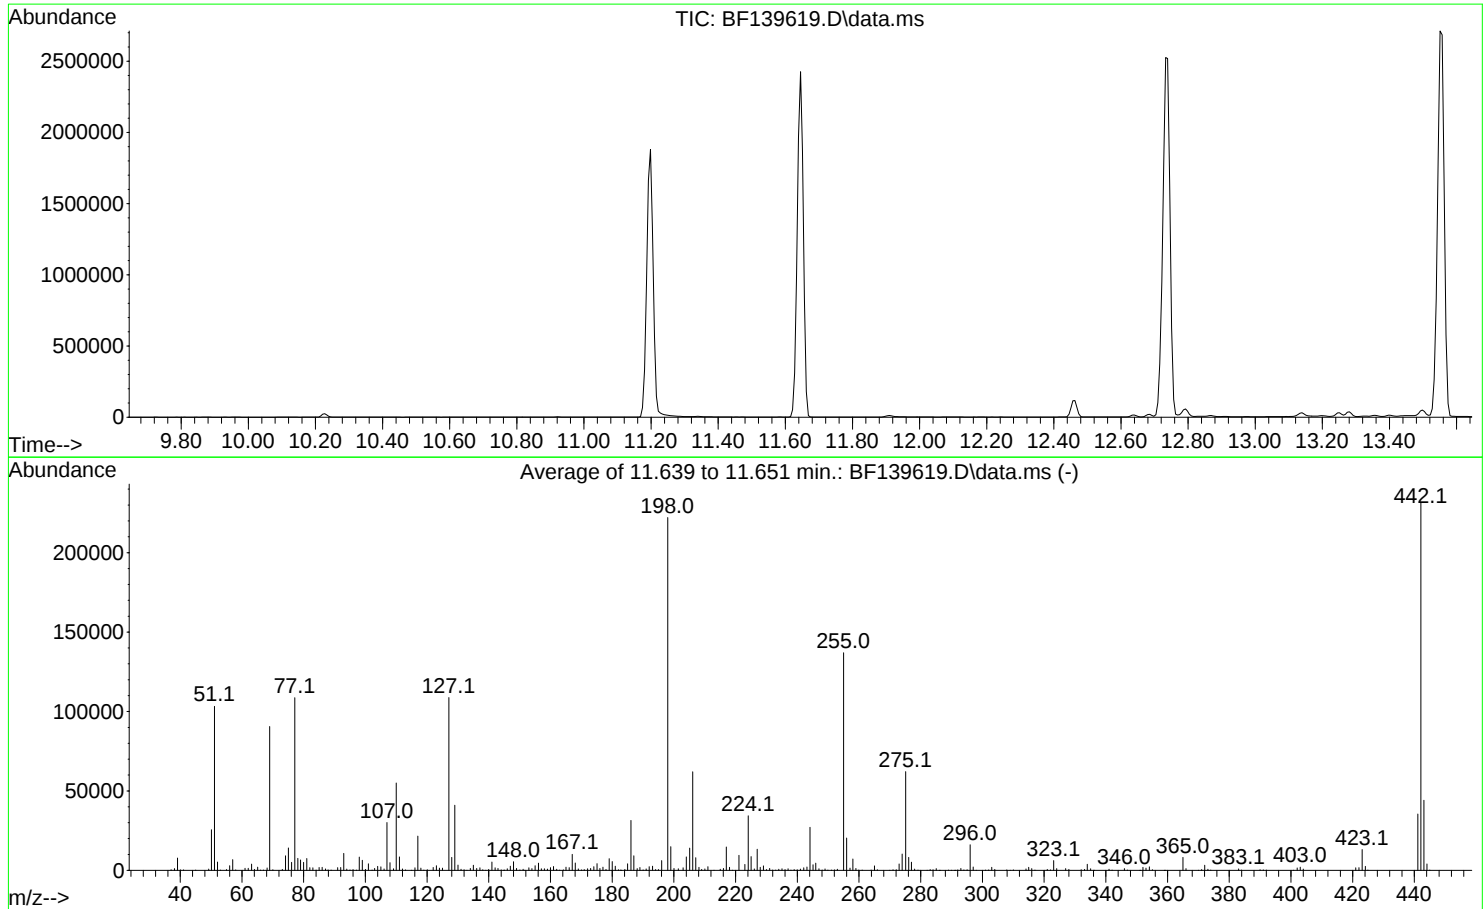




AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.5	103285	PASS
68	69	0.00	2	1.6	1490	PASS
69	198	0.00	100	40.8	90592	PASS
70	69	0.00	2	0.5	443	PASS
127	198	10	80	49.0	108792	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	222123	PASS
199	198	5	9	6.7	14962	PASS
275	198	10	60	28.0	62120	PASS
365	198	1	100	3.7	8152	PASS
441	198	0.01	100	16.0	35477	PASS
442	442	50	100	100.0	231595	PASS
443	442	15	24	19.0	44099	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100324\
Data File : BF139619.D
Acq On : 03 Oct 2024 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 03 11:20:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

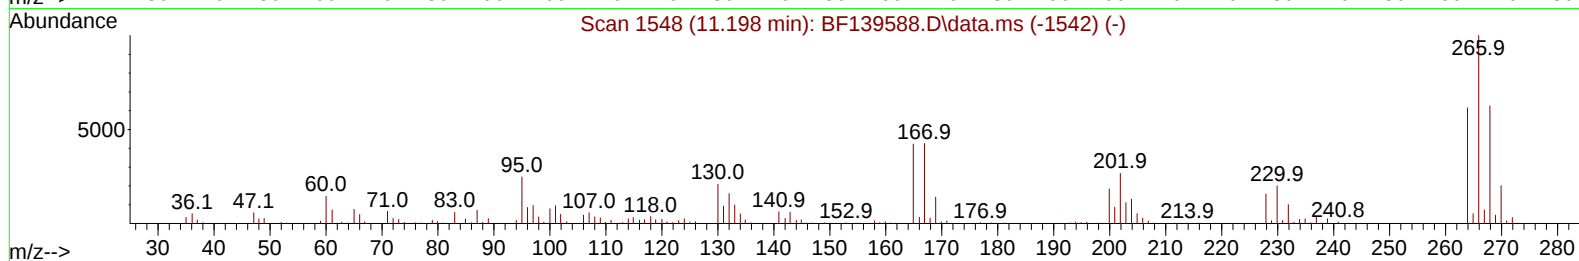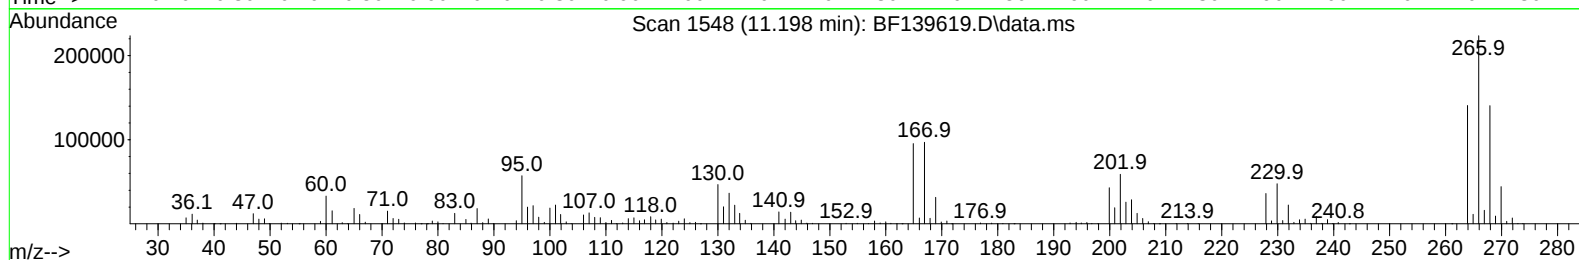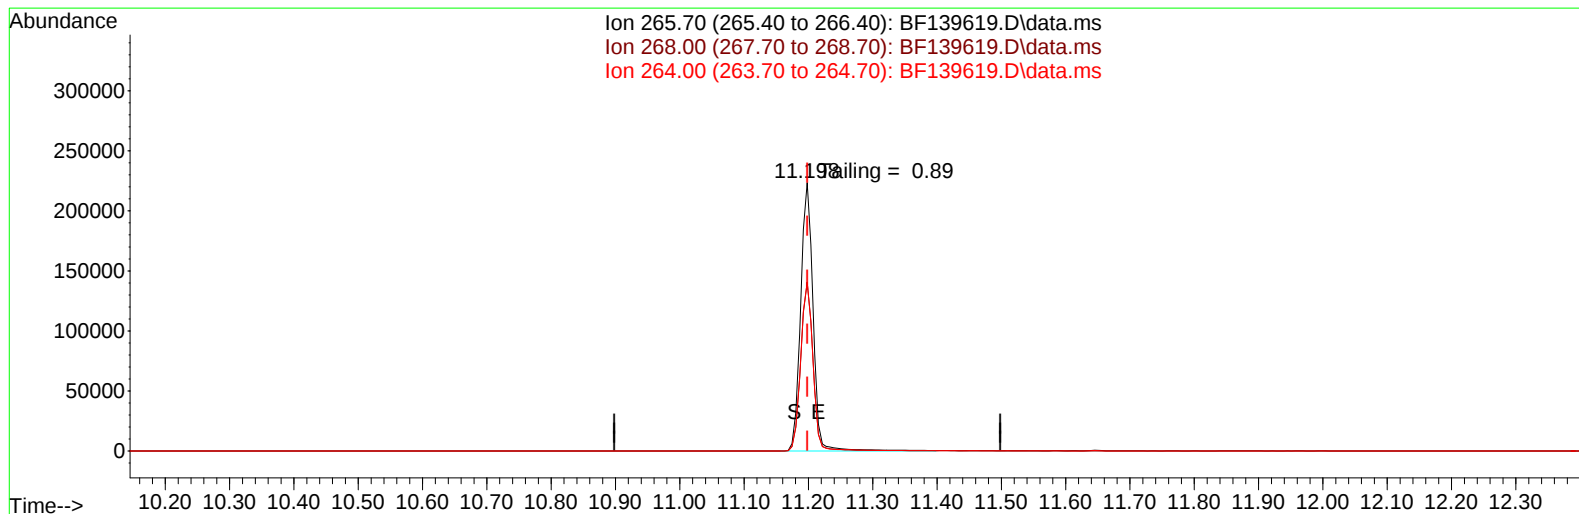

TIC: BF139619.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.000) 29177.65 ng




response 303220

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	62.84
264.00	61.60	62.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100324\
Data File : BF139619.D
Acq On : 03 Oct 2024 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 03 11:20:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

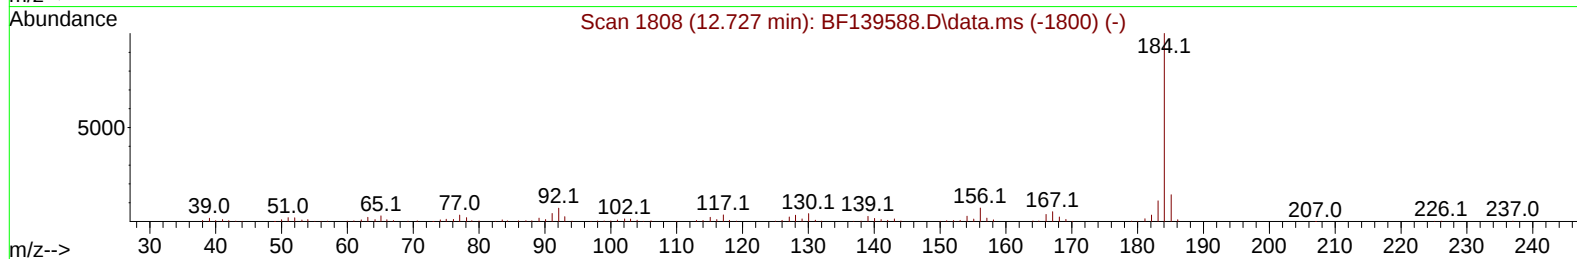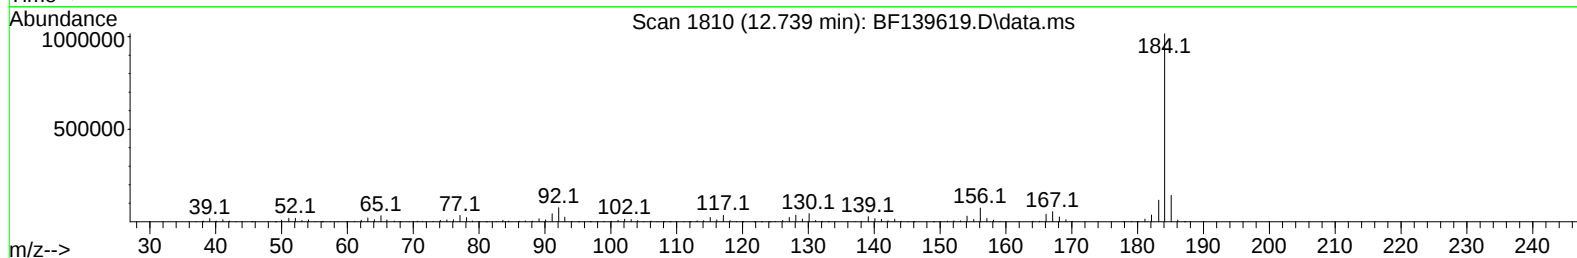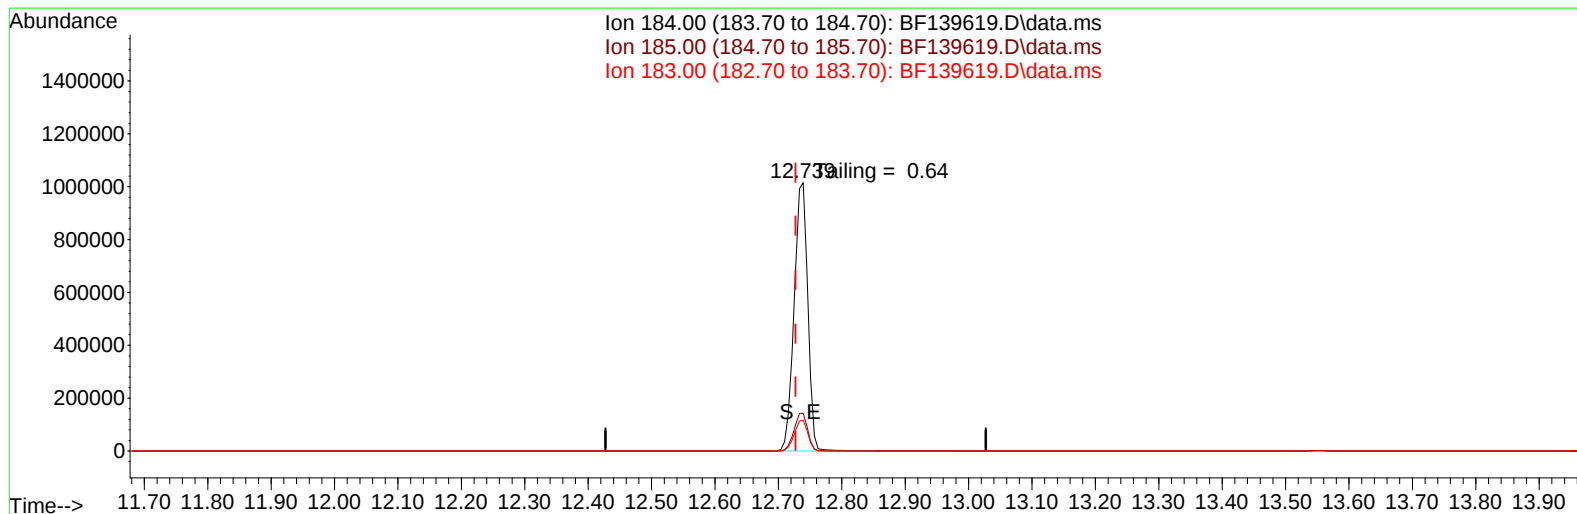

TIC: BF139619.D\data.ms

(77) Benzidine

12.739min (+ 0.012) 0.00 ng

response 1528256

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.05
183.00	11.00	11.53
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/3/2024	BNA_F	<u>BF139619.D</u>
Compound Name	Response	Retention Time
DDT	729915	13.557
DDD	16661	13.28
DDE	656	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17317	747232	2.32

Instrument :
BNA_F
ClientSampleId :
DFTPP