



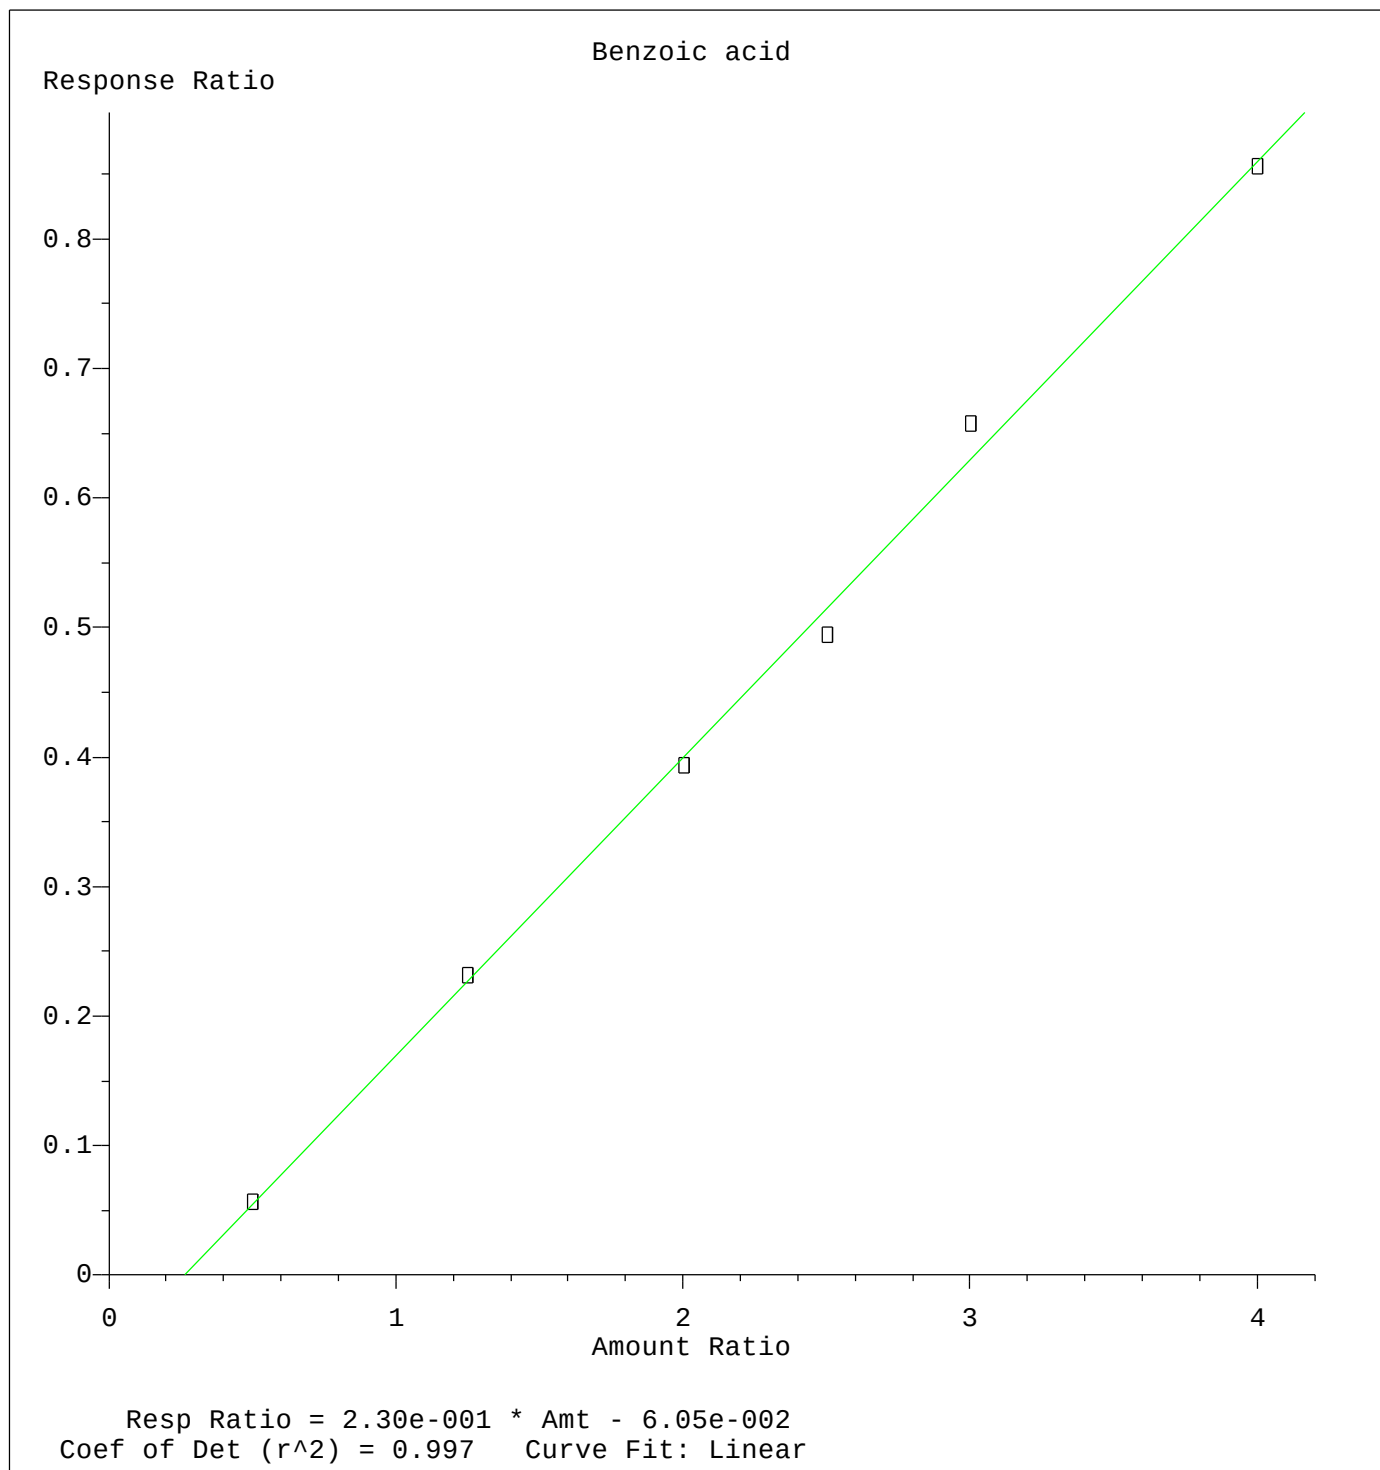

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF100416.M
Calibration Table Last Updated: Tue Oct 04 14:16:07 2016


Hexachlorocyclopentadiene

Response Ratio

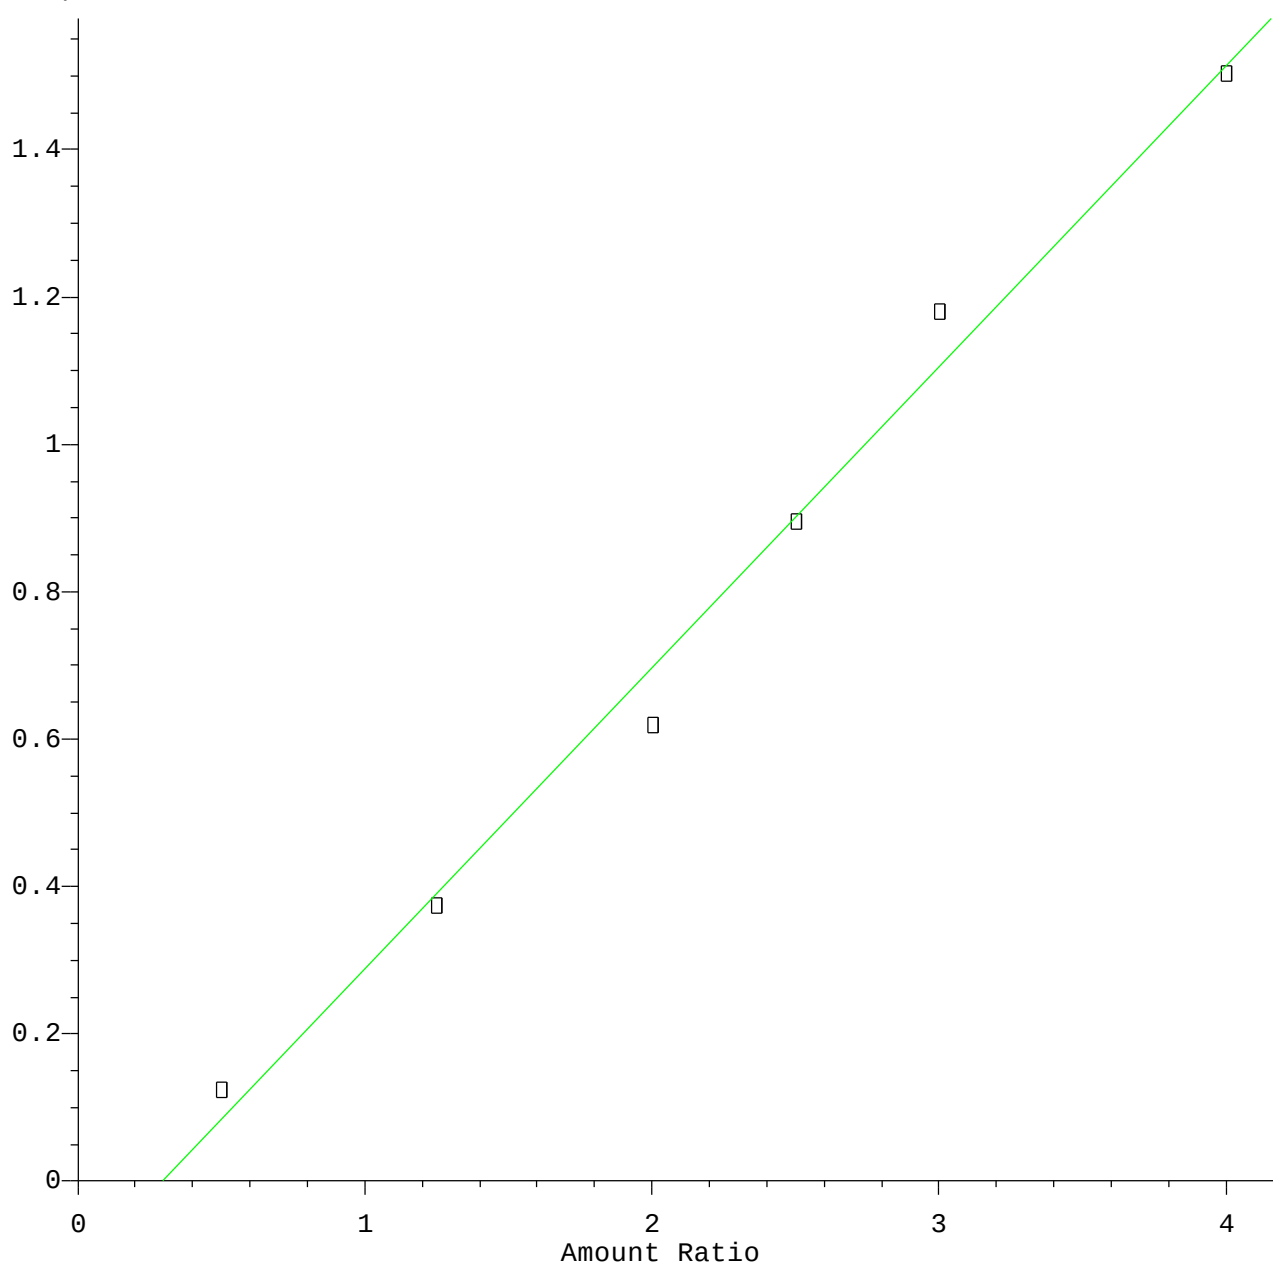


Resp Ratio = $4.09 \times 10^{-1} \times \text{Amt} - 1.21 \times 10^{-1}$
Coef of Det (r^2) = 0.990 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF100416.M
Calibration Table Last Updated: Tue Oct 04 14:16:07 2016

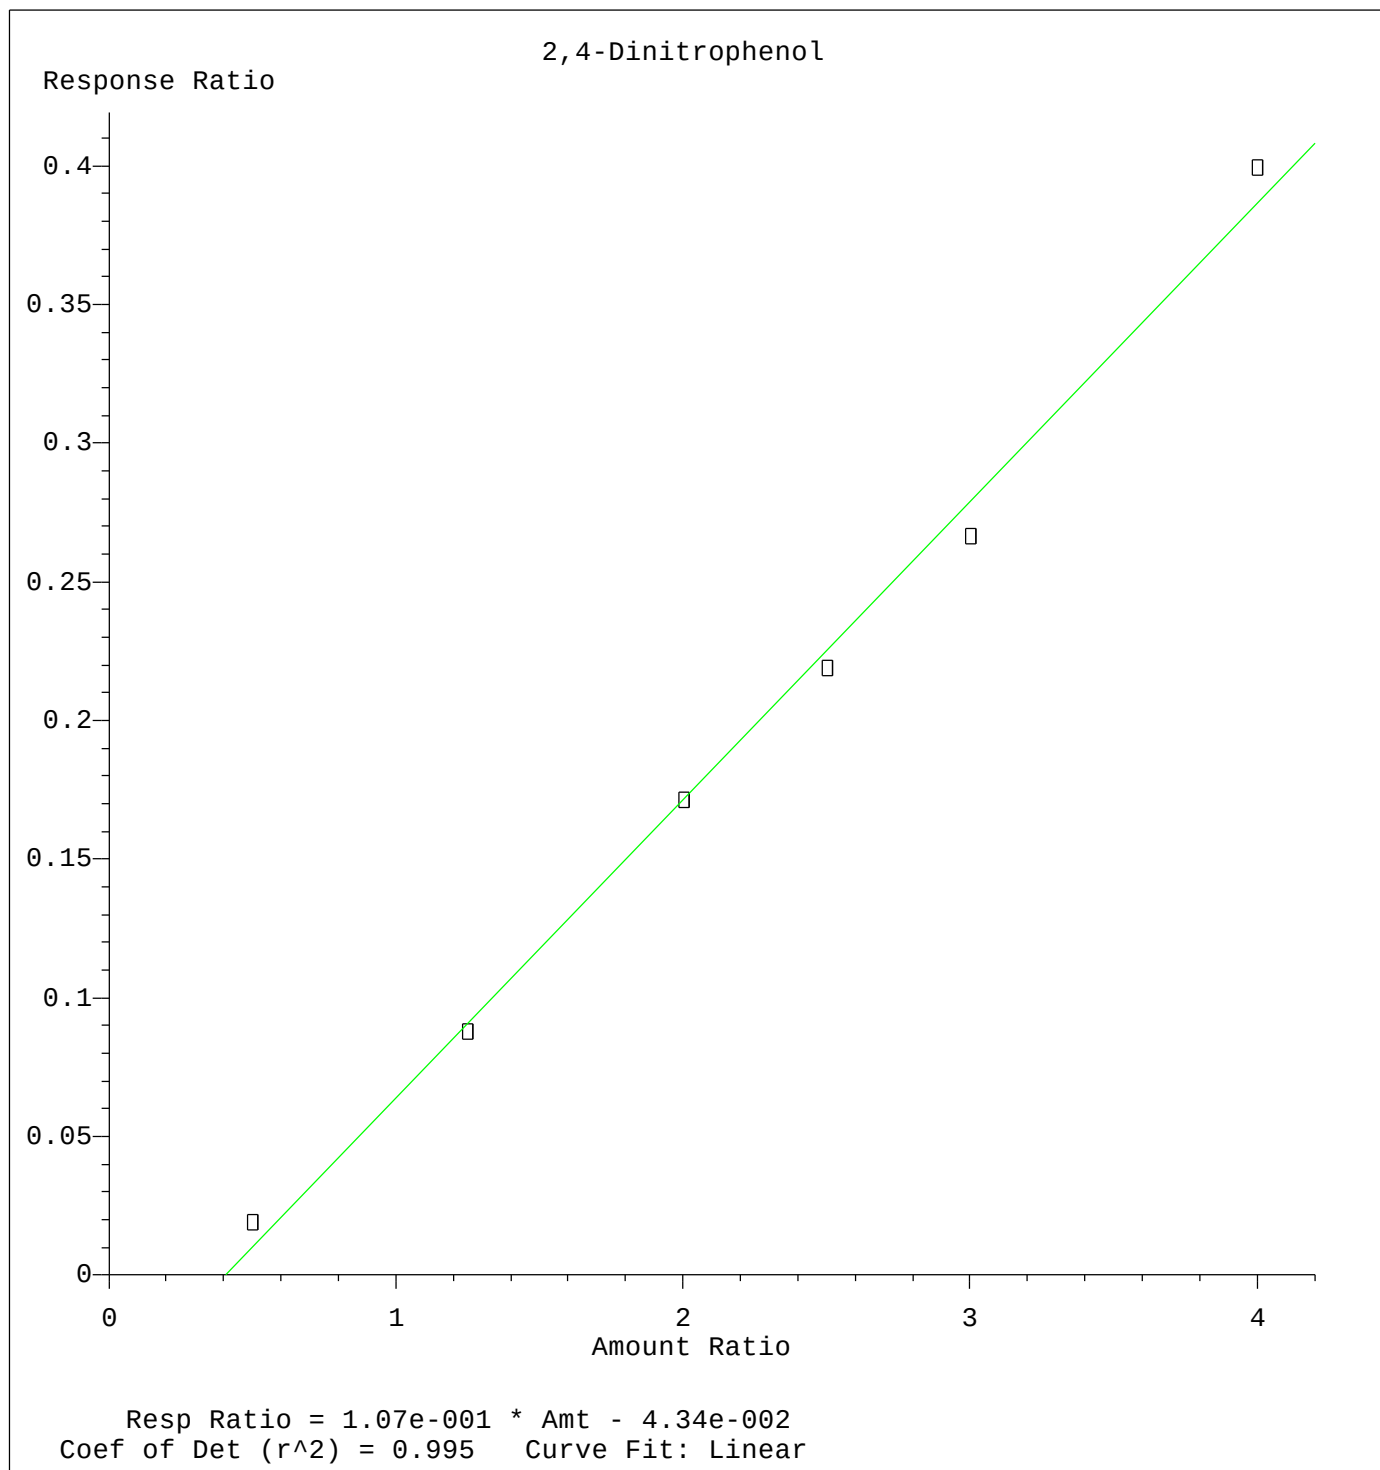

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF100416.M
Calibration Table Last Updated: Tue Oct 04 14:16:07 2016

4,6-Dinitro-2-methylphenol

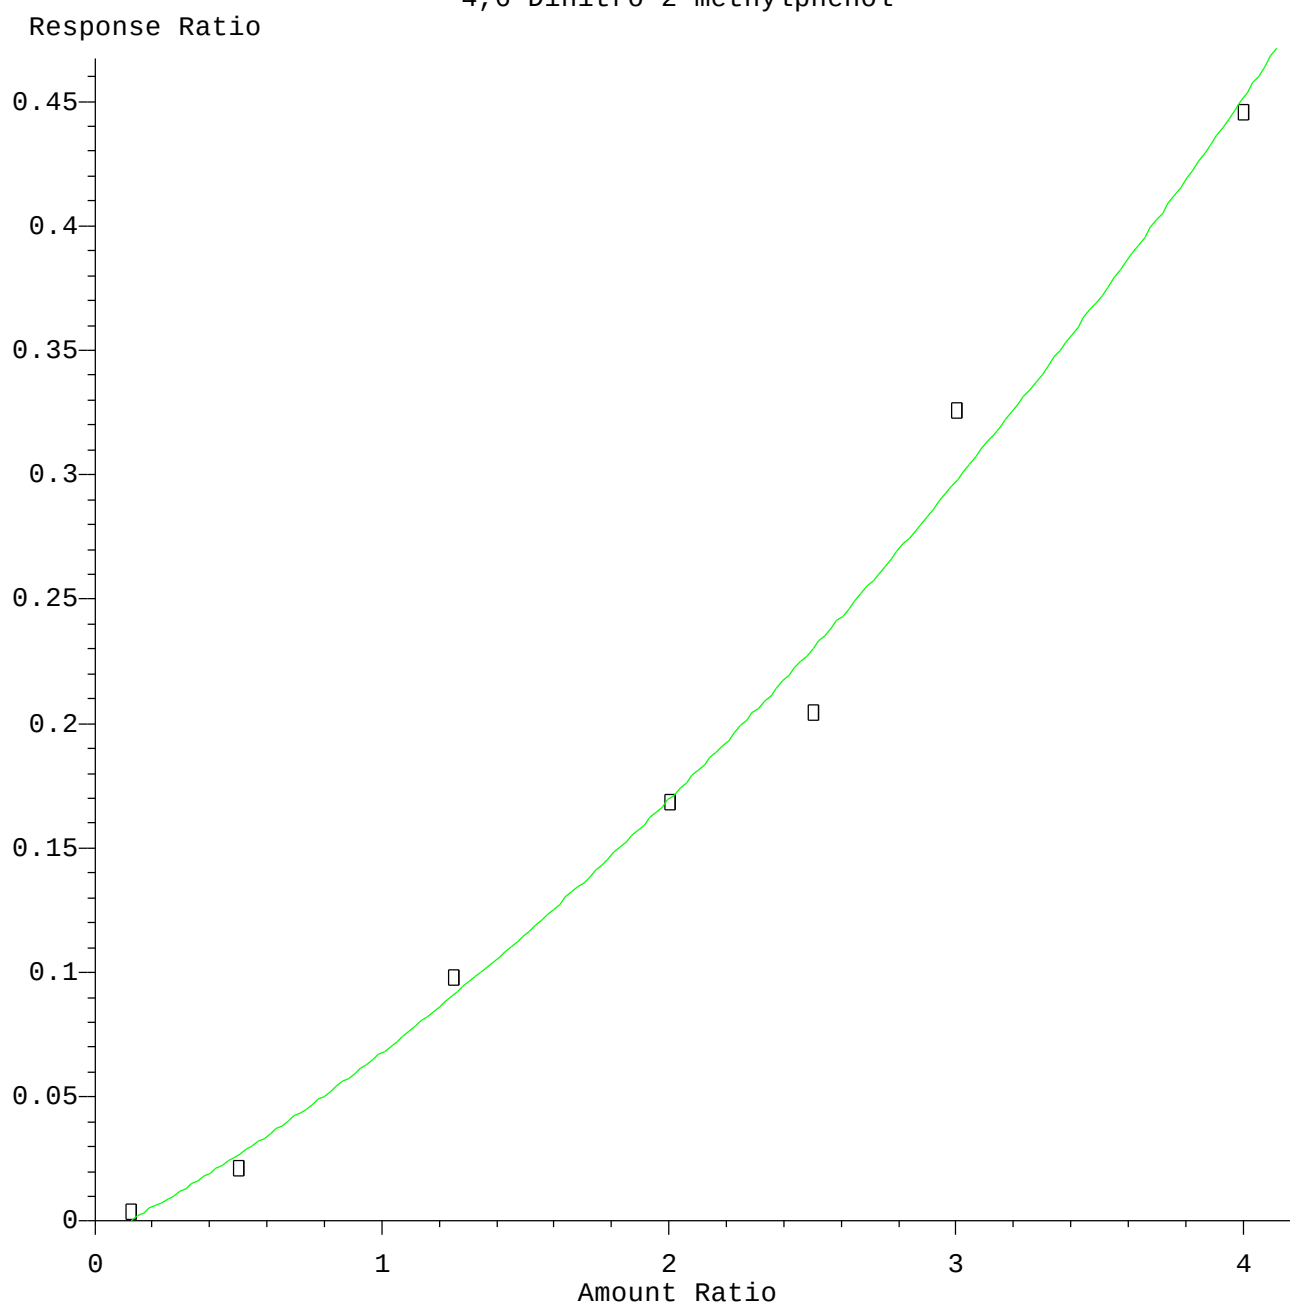

$R = 1.31e-002 A^2 + 6.22e-002 A - 7.64e-003$
Coef of Det (r^2) = 0.990 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF100416.M
Calibration Table Last Updated: Tue Oct 04 14:16:07 2016