


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100416\
 Data File : BF090333.D
 Acq On : 4 Oct 2016 9:25
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF100416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 04 14:16:07 2016

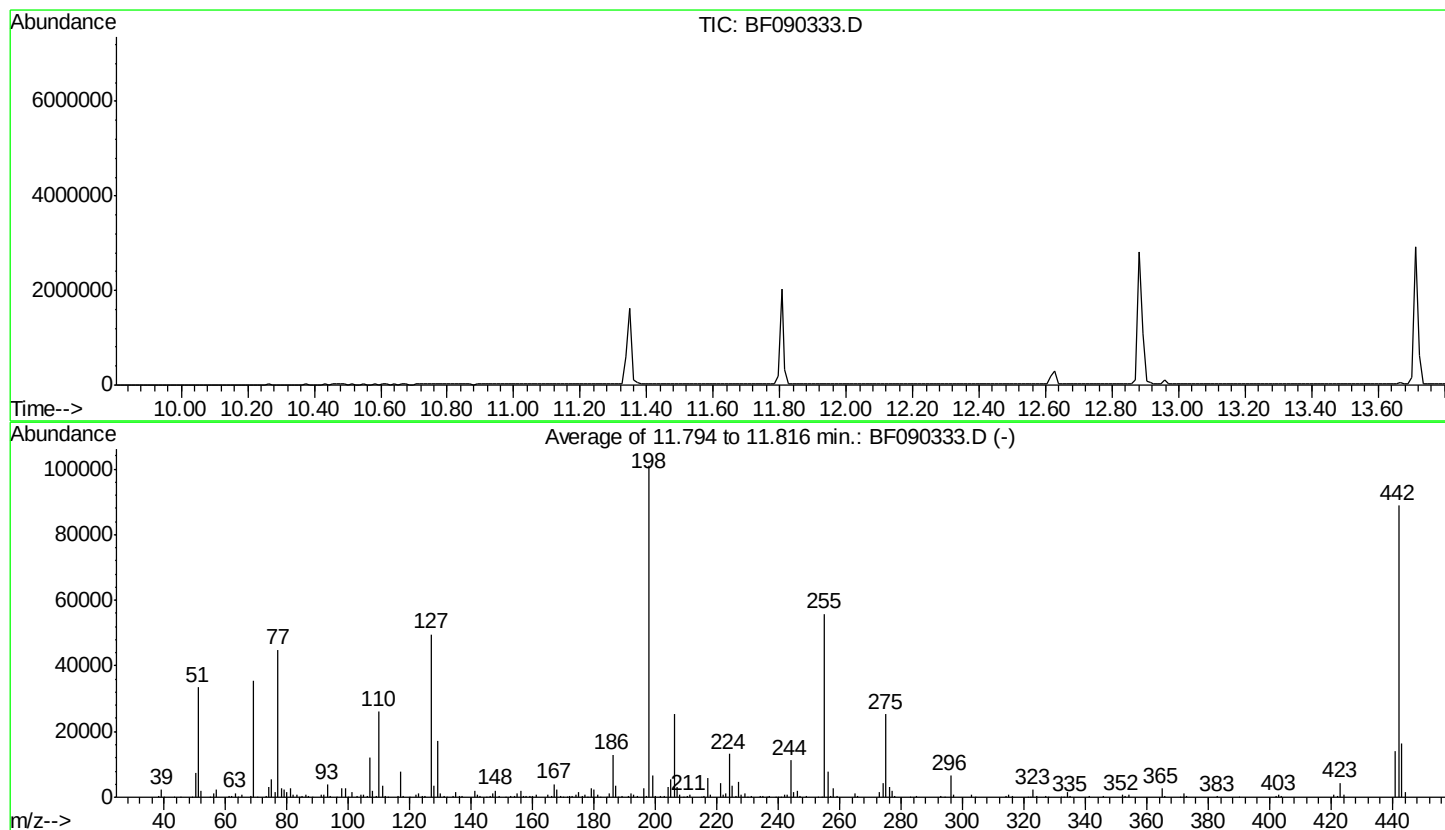

AutoFind: Scans 893, 894, 895; Background Corrected with Scan 890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.1	33456	PASS
68	69	0.00	2	1.5	536	PASS
69	198	0.00	100	35.2	35583	PASS
70	69	0.00	2	0.5	167	PASS
127	198	10	80	49.1	49600	PASS
197	198	0.00	2	0.3	289	PASS
198	198	100	100	100.0	101017	PASS
199	198	5	9	6.7	6803	PASS
275	198	10	60	24.9	25189	PASS
365	198	1	100	2.7	2718	PASS
441	442	0.01	24	15.9	14133	PASS
442	198	50	100	88.0	88898	PASS
443	442	15	24	18.3	16264	PASS