


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100416\
Data File : BF090345.D
Acq On : 4 Oct 2016 16:50
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF100416.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 04 14:16:07 2016

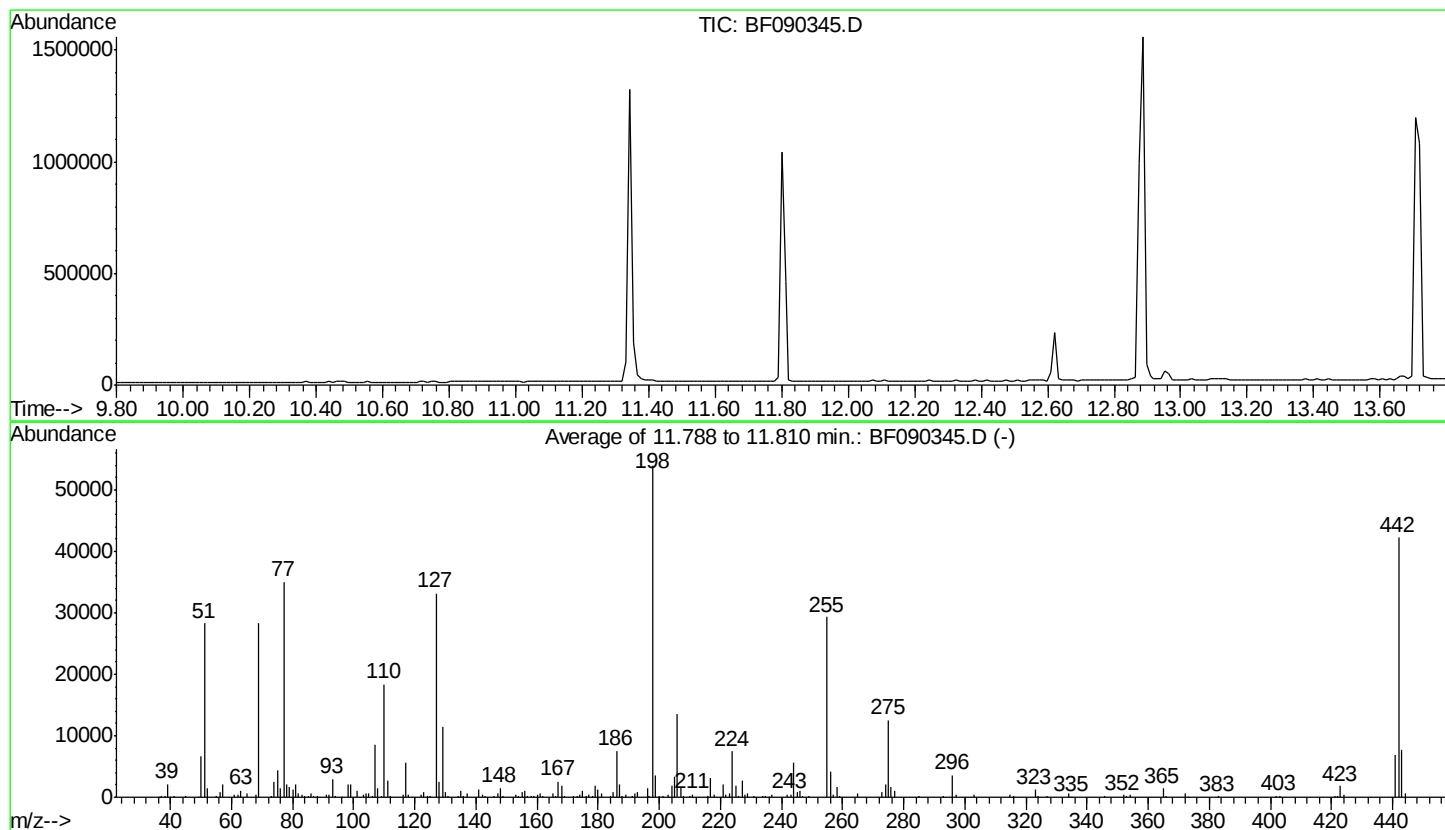

AutoFind: Scans 805, 806, 807; Background Corrected with Scan 802

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.5	28288	PASS
68	69	0.00	2	1.3	367	PASS
69	198	0.00	100	52.7	28399	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	61.5	33174	PASS
197	198	0.00	2	0.3	163	PASS
198	198	100	100	100.0	53903	PASS
199	198	5	9	6.5	3527	PASS
275	198	10	60	23.2	12488	PASS
365	198	1	100	2.5	1370	PASS
441	442	0.01	24	16.4	6933	PASS
442	198	50	100	78.2	42160	PASS
443	442	15	24	18.5	7787	PASS