


Data Path : Z:\HPCHEM1\BNA F\DATA\BF100417\
 Data File : BF099065.D
 Acq On : 4 Oct 2017 14:24
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 05 09:04:50 2017

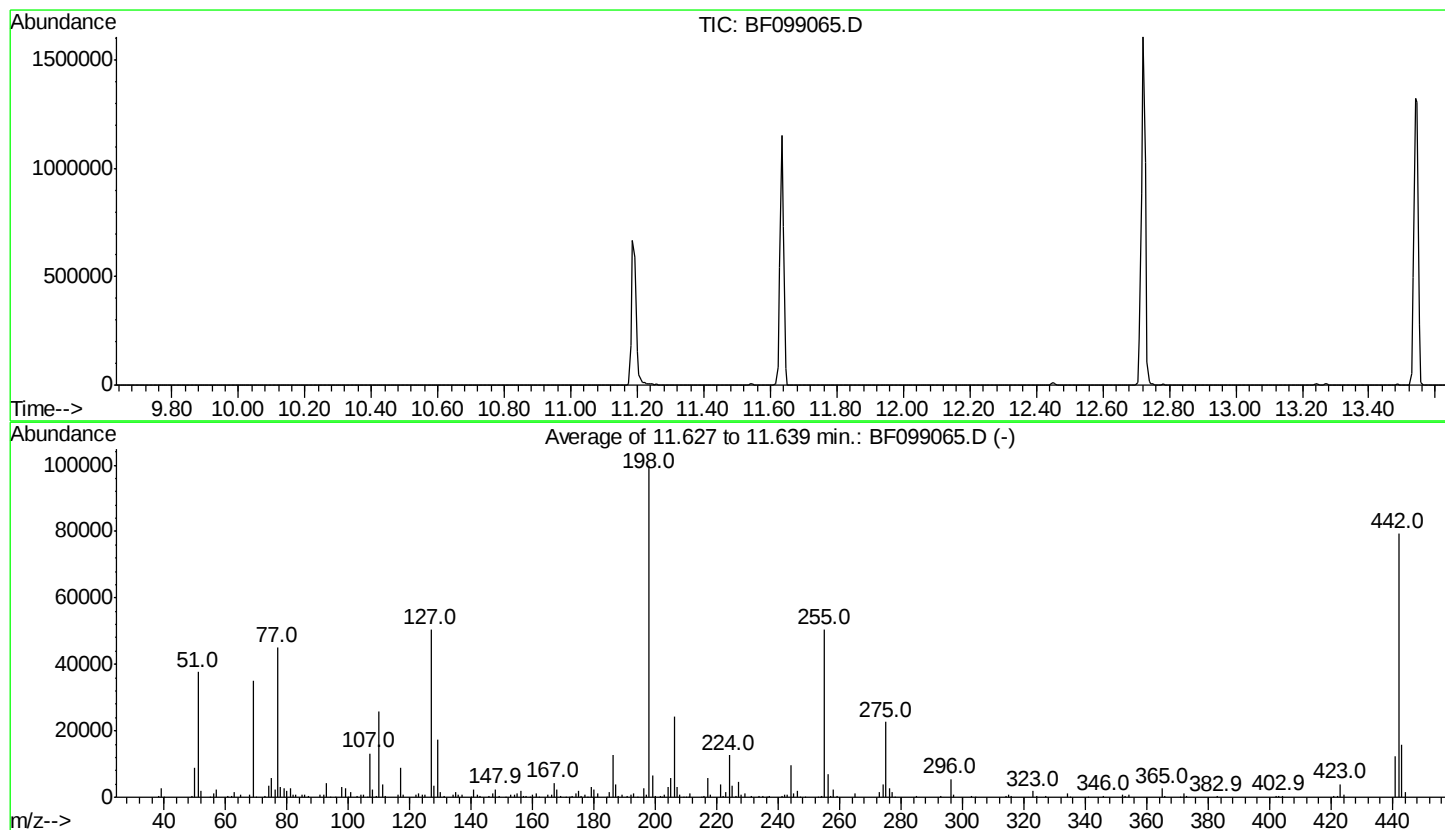

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	37626	PASS
68	69	0.00	2	1.8	640	PASS
69	198	0.00	100	35.0	34989	PASS
70	69	0.00	2	0.3	102	PASS
127	198	10	80	50.5	50402	PASS
197	198	0.00	2	0.8	809	PASS
198	198	100	100	100.0	99834	PASS
199	198	5	9	6.6	6626	PASS
275	198	10	60	22.7	22660	PASS
365	198	1	100	2.7	2665	PASS
441	442	0.01	24	15.8	12515	PASS
442	198	50	100	79.4	79258	PASS
443	442	15	24	19.8	15688	PASS