
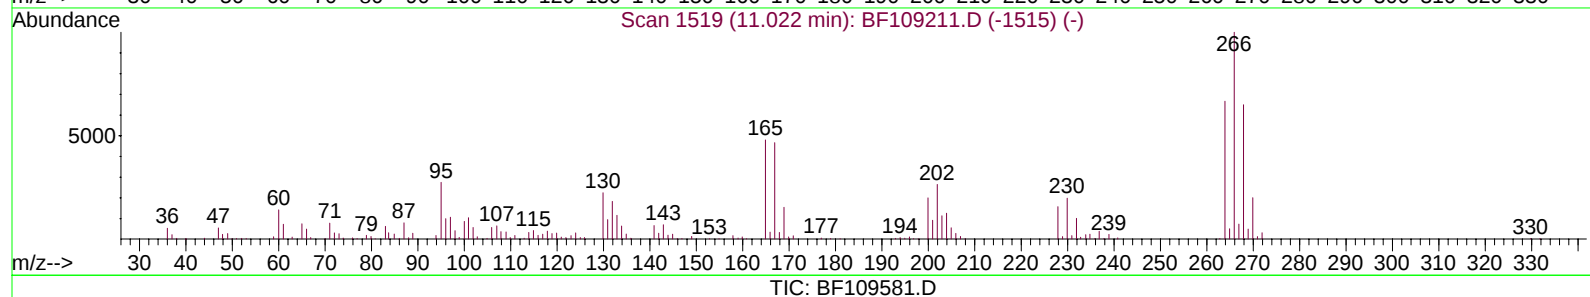
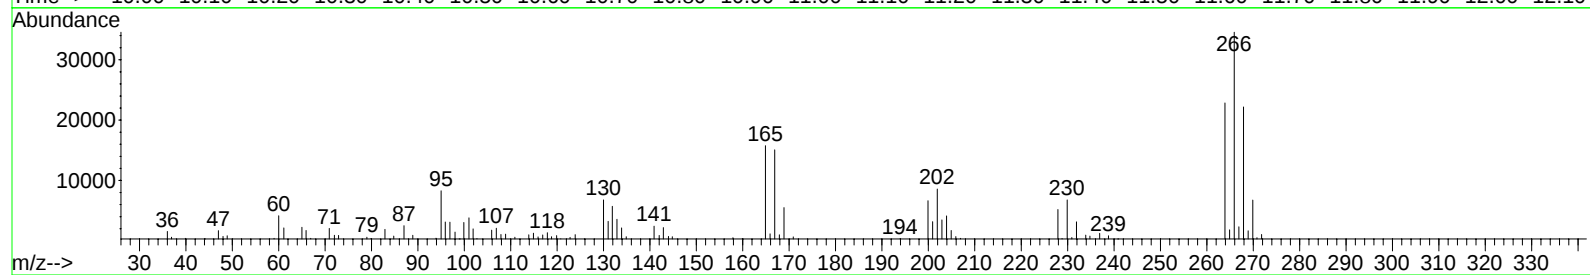


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF100418\
Data File : BF109581.D
Acq On : 4 Oct 2018 12:49
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 11:48:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

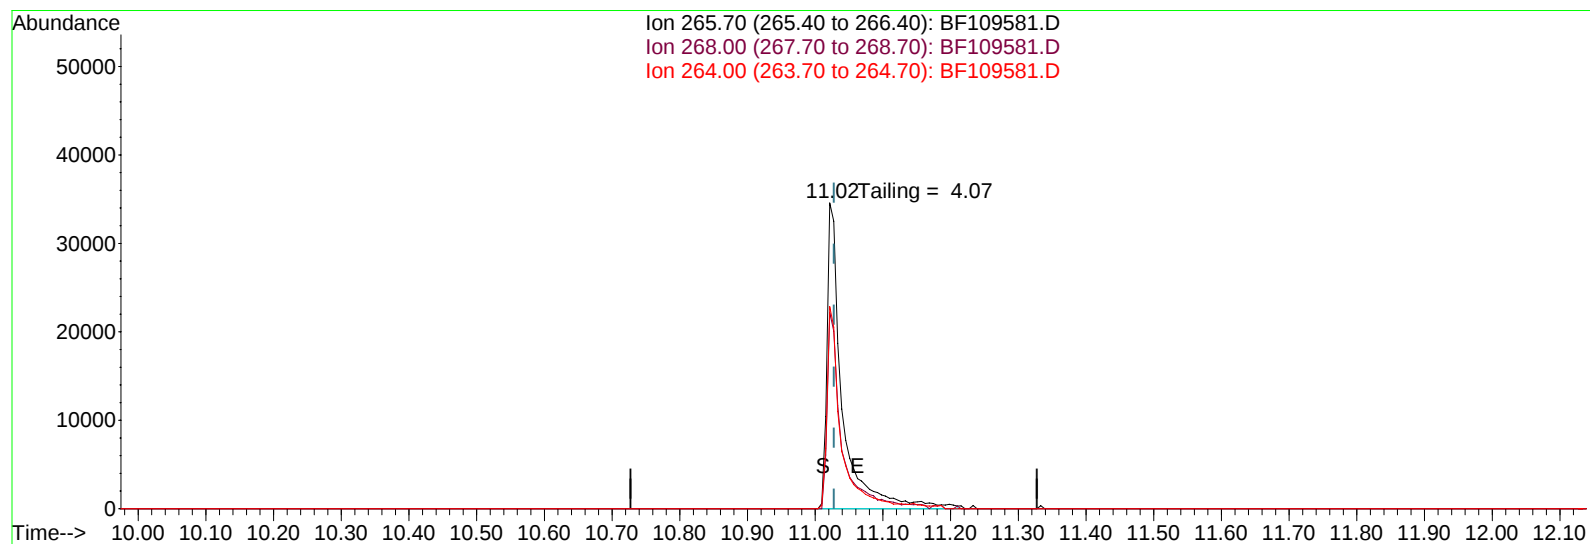

TIC: BF109581.D

(69) Pentachlorophenol (C)




11.021min (-0.006) 59443.64ng

response 52869

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.17
264.00	61.90	66.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF100418\
Data File : BF109581.D
Acq On : 4 Oct 2018 12:49
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 11:48:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

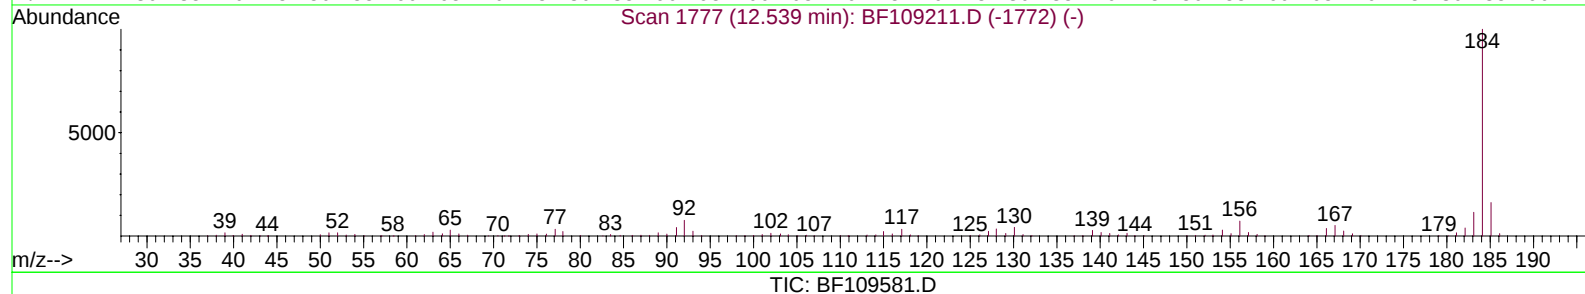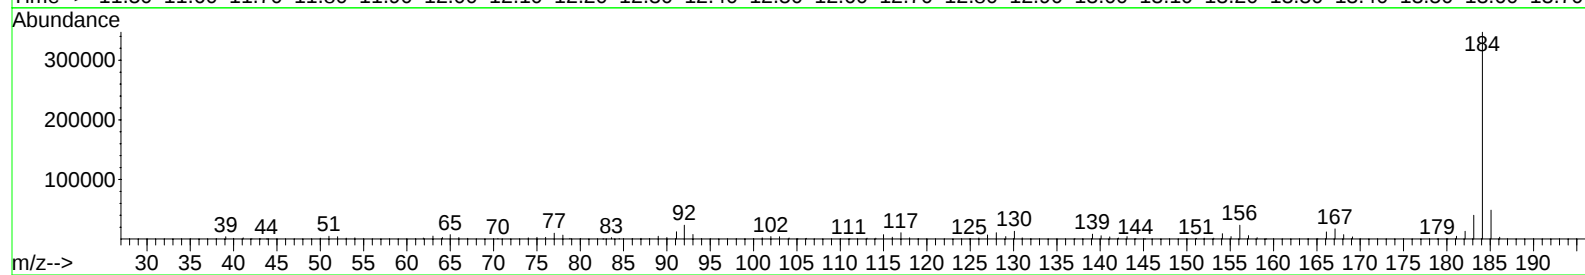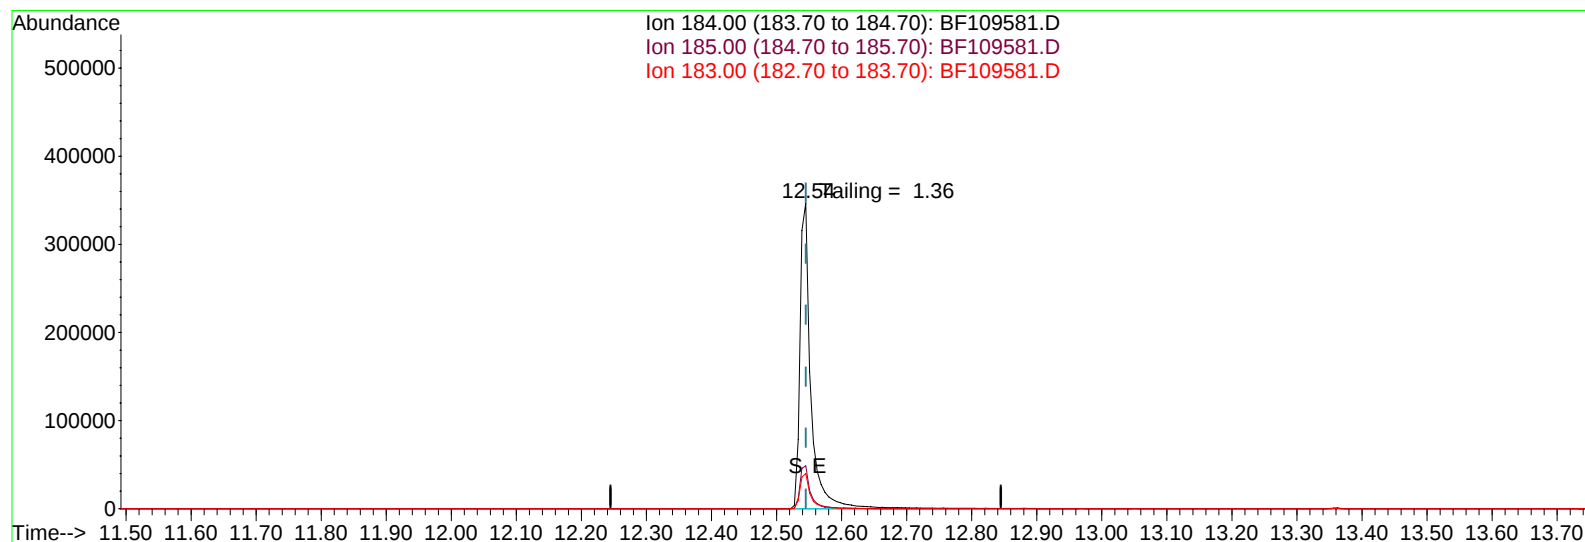

(76) Benzidine

12.545min (-0.000) 0.00ng

response 405383

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.01
183.00	11.60	11.53
0.00	0.00	0.00