
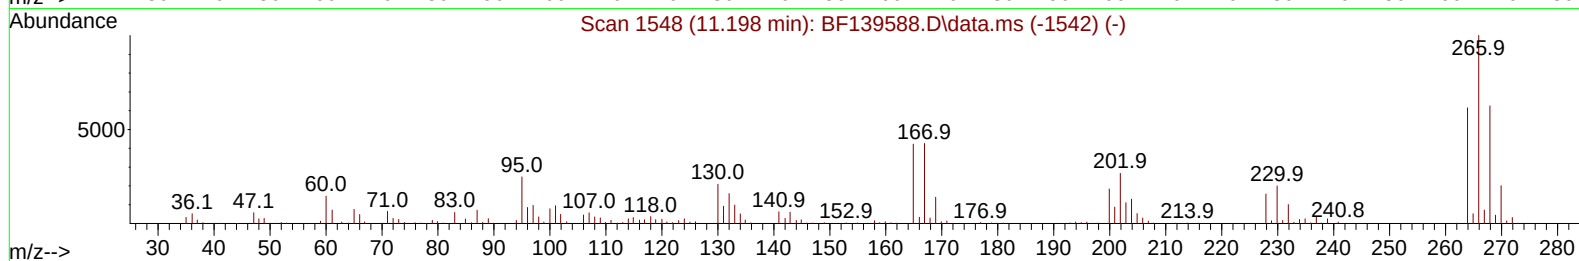
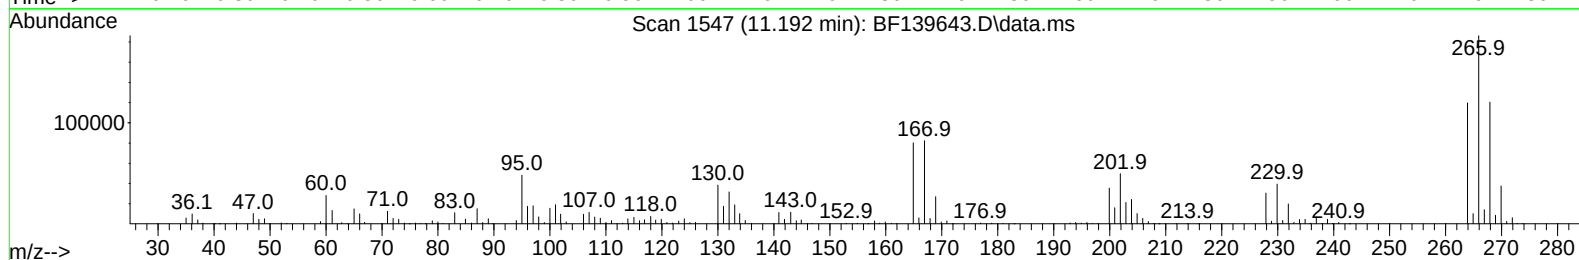


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100424\
Data File : BF139643.D
Acq On : 04 Oct 2024 08:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 04 11:21:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

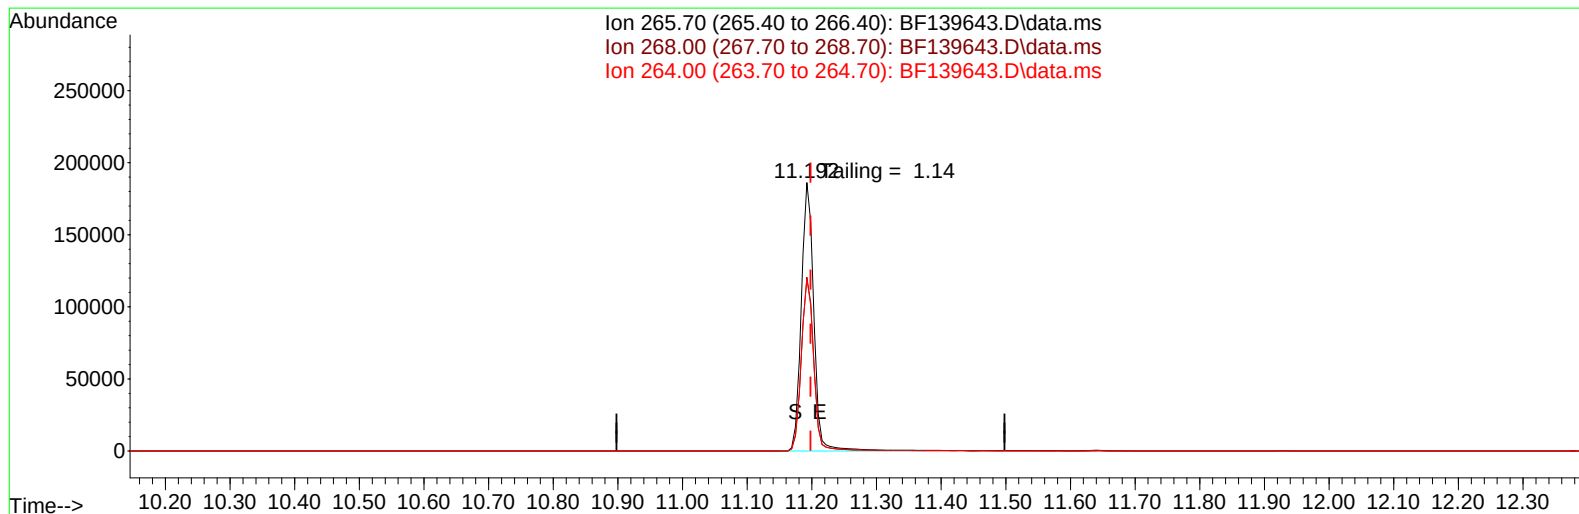

TIC: BF139643.D\data.ms

(70) Pentachlorophenol (C)




11.192min (-0.006) 33586.23 ng

response 252106

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	64.69
264.00	61.60	64.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100424\
Data File : BF139643.D
Acq On : 04 Oct 2024 08:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 04 11:21:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

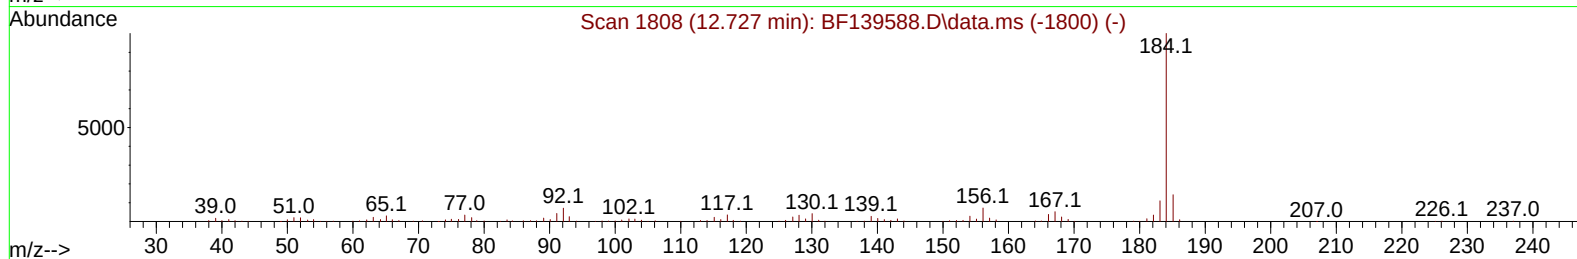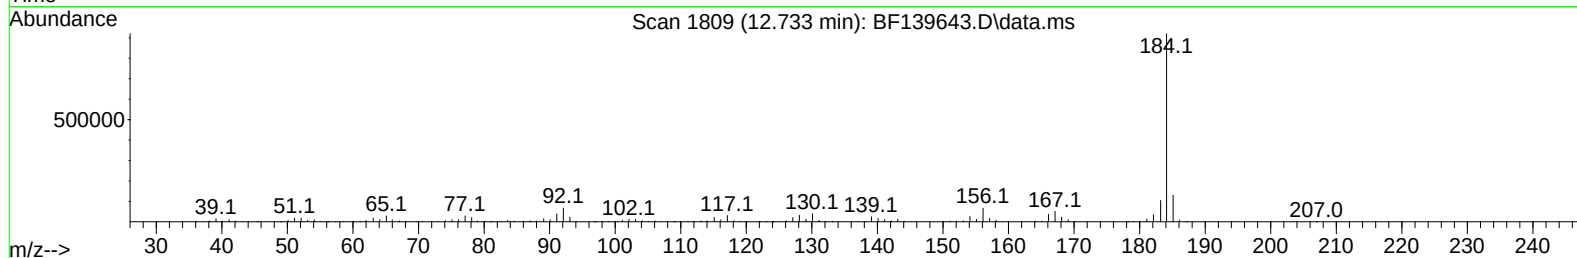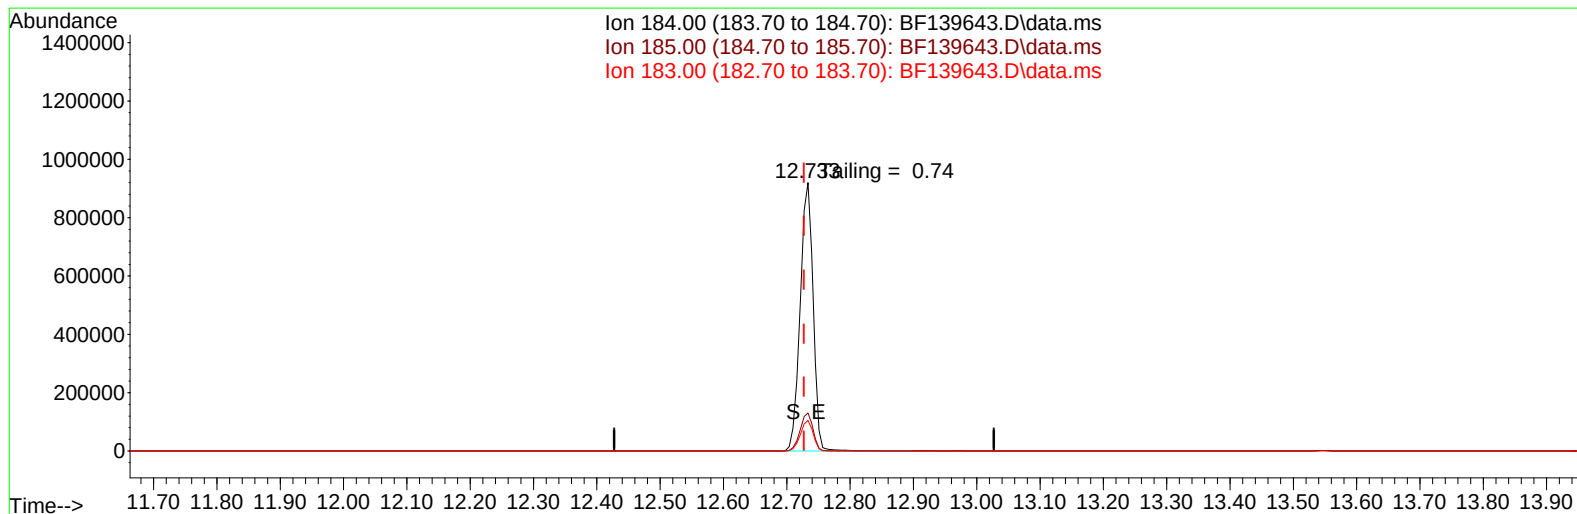

TIC: BF139643.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 0.00 ng

response 1313048

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.18
183.00	11.00	11.38
0.00	0.00	0.00