


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100424\
Data File : BF139643.D
Acq On : 04 Oct 2024 08:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 02 04:58:47 2024

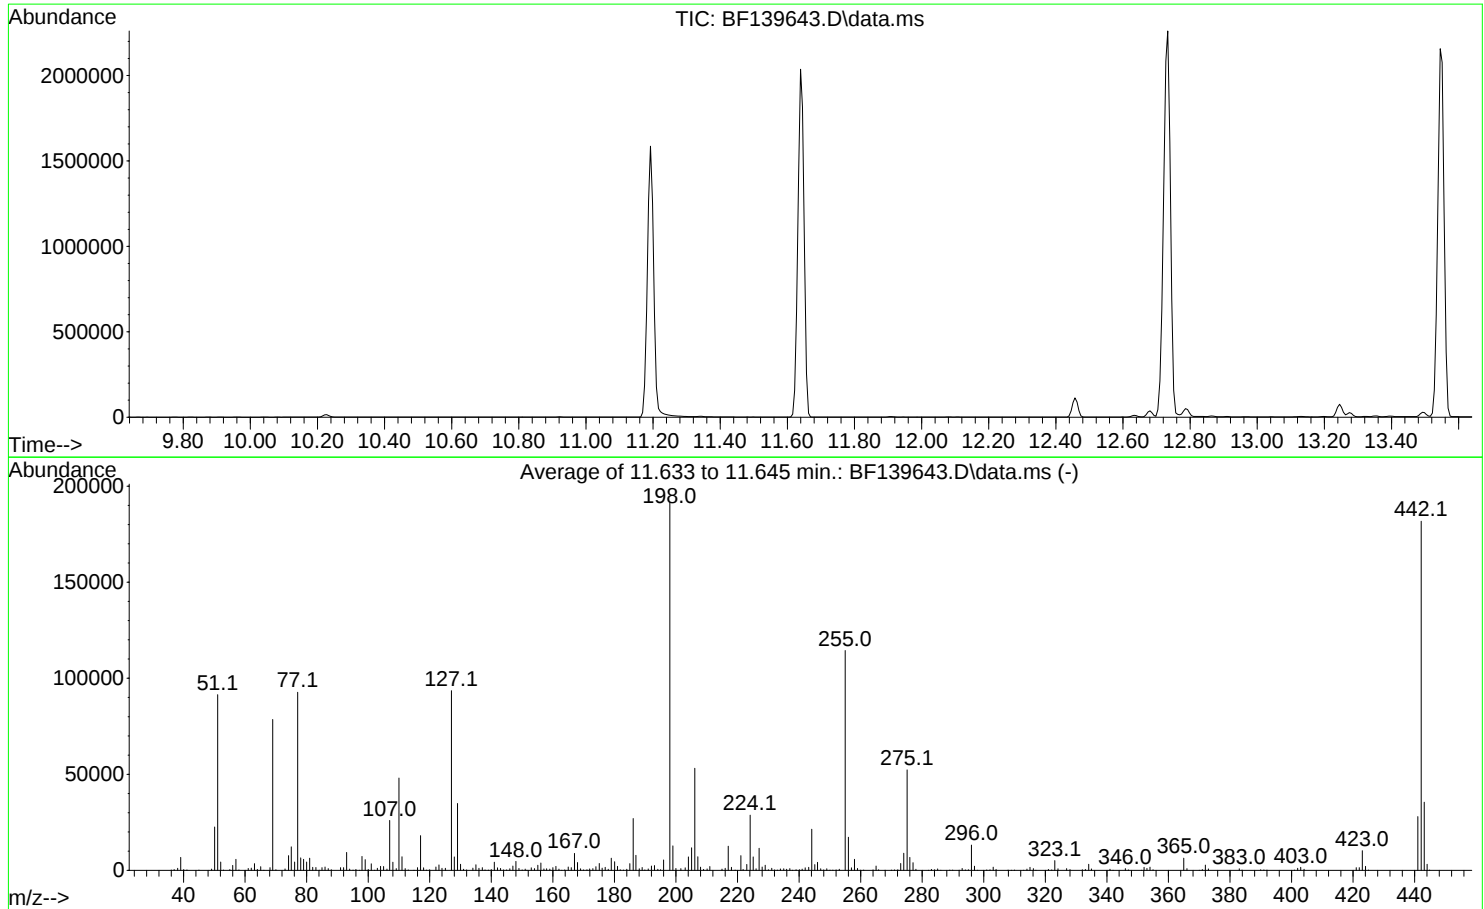

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.8	91467	PASS
68	69	0.00	2	1.8	1449	PASS
69	198	0.00	100	41.0	78565	PASS
70	69	0.00	2	0.4	308	PASS
127	198	10	80	48.8	93523	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	191488	PASS
199	198	5	9	6.7	12770	PASS
275	198	10	60	27.3	52349	PASS
365	198	1	100	3.3	6338	PASS
441	198	0.01	100	14.6	27992	PASS
442	442	50	100	100.0	181771	PASS
443	442	15	24	19.5	35459	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/4/2024	BNA_F	<u>BF139643.D</u>
Compound Name	Response	Retention Time
DDT	555091	13.545
DDD	25562	13.245
DDE	794	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26356	581447	4.53

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100424\
Data File : BF139643.D
Acq On : 04 Oct 2024 08:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 04 11:21:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

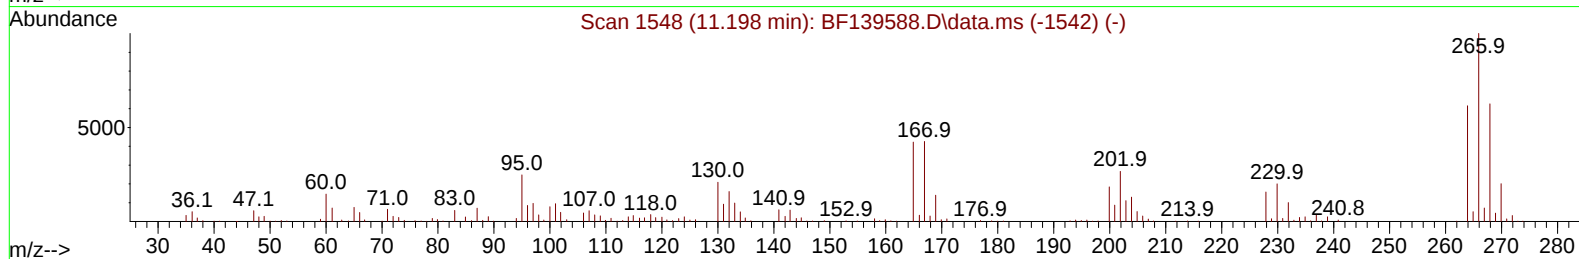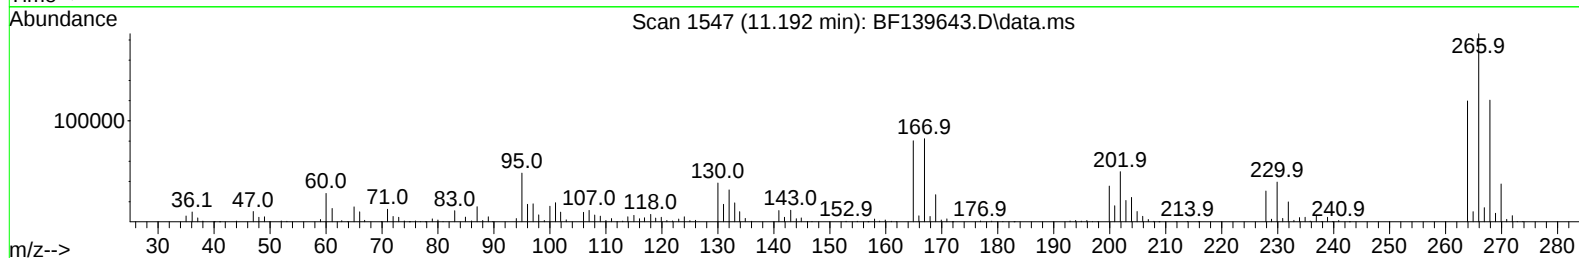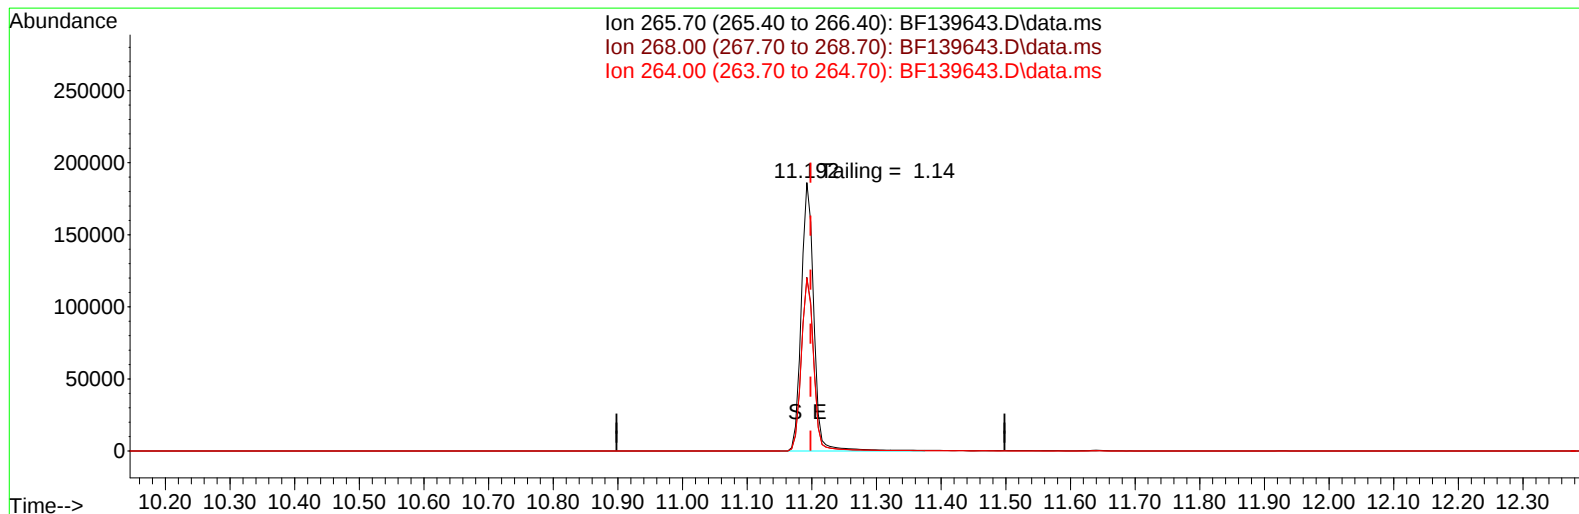

TIC: BF139643.D\data.ms

(70) Pentachlorophenol (C)

11.192min (-0.006) 33586.23 ng




response 252106

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	64.69
264.00	61.60	64.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100424\
Data File : BF139643.D
Acq On : 04 Oct 2024 08:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 04 11:21:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

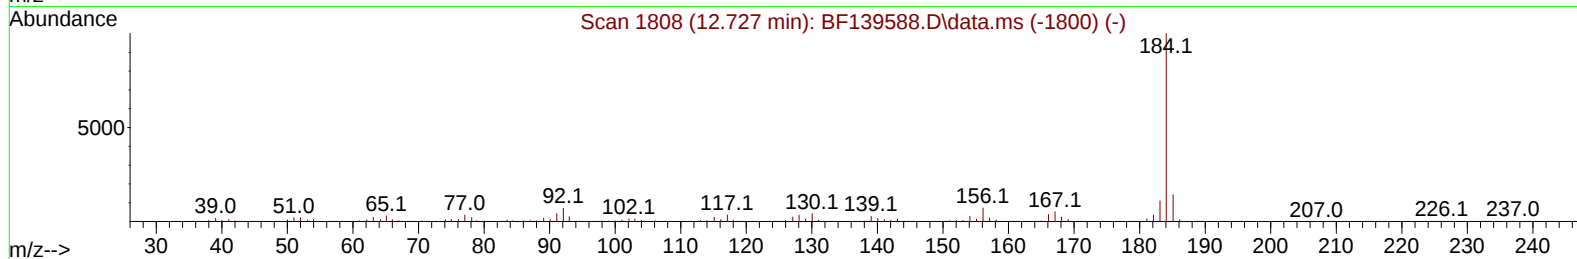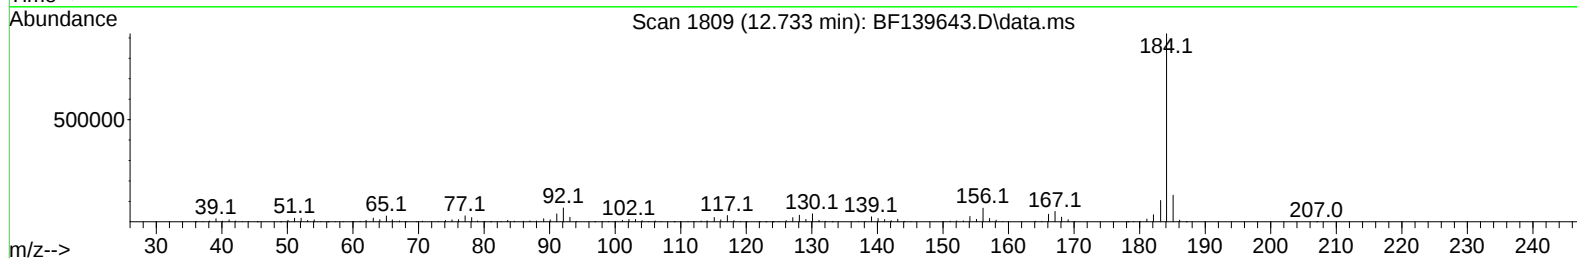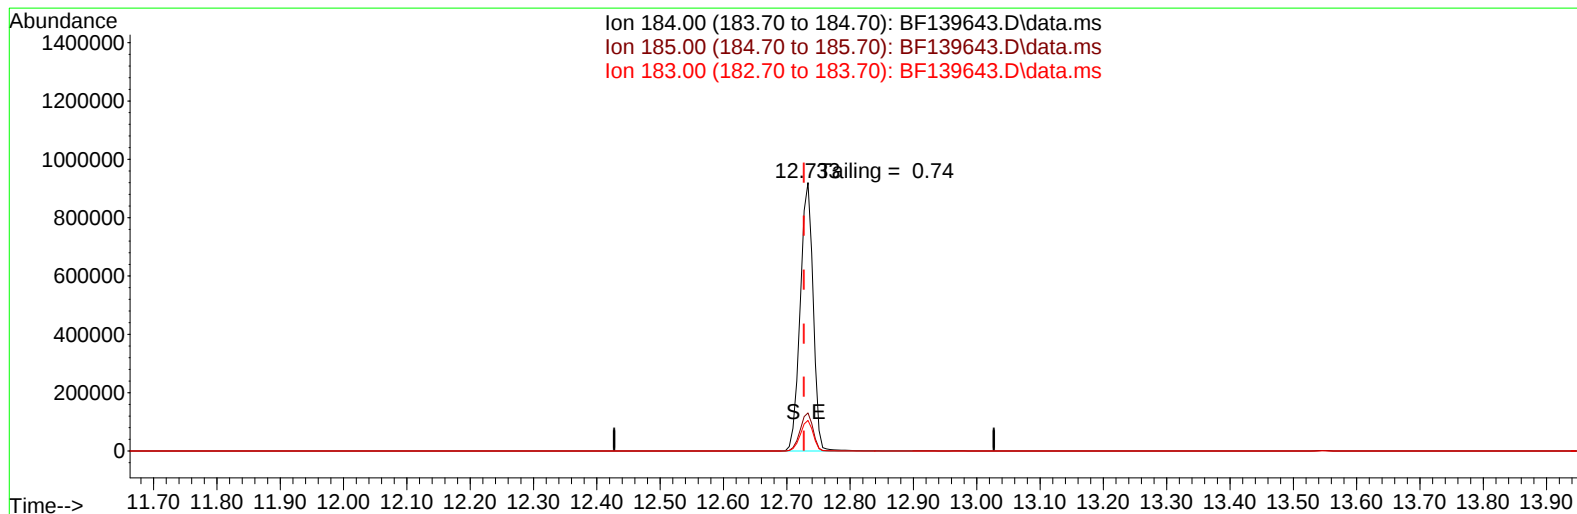

TIC: BF139643.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 0.00 ng

response 1313048

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.18
183.00	11.00	11.38
0.00	0.00	0.00