


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100424\
Data File : BF139651.D
Acq On : 04 Oct 2024 12:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 02 04:58:47 2024

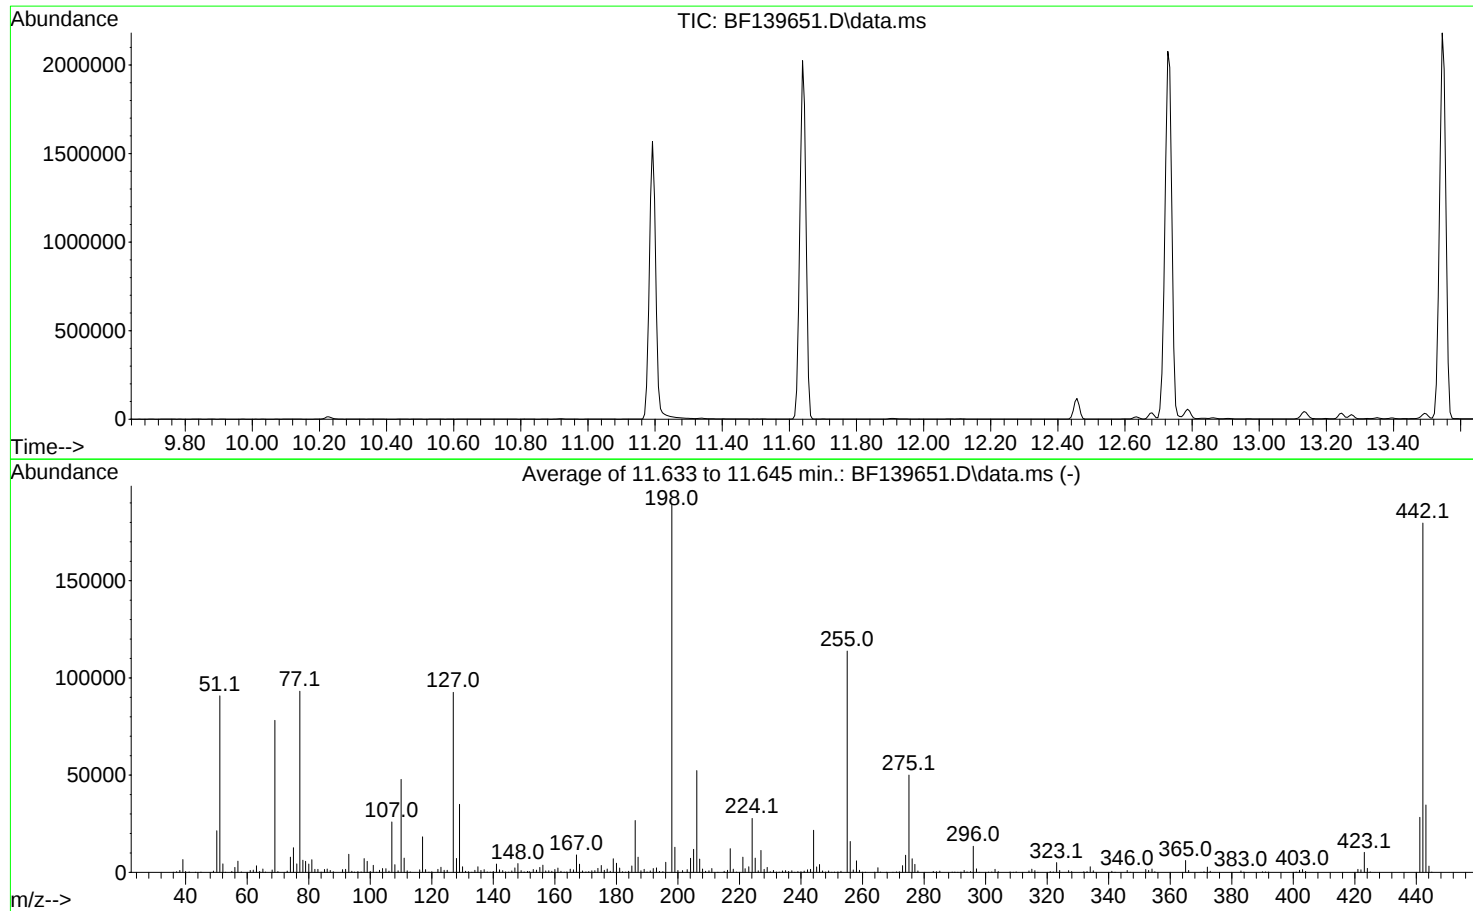

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.0	90763	PASS
68	69	0.00	2	1.6	1235	PASS
69	198	0.00	100	41.3	78184	PASS
70	69	0.00	2	0.6	431	PASS
127	198	10	80	48.9	92595	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	189184	PASS
199	198	5	9	6.9	12960	PASS
275	198	10	60	26.5	50072	PASS
365	198	1	100	3.2	6088	PASS
441	198	0.01	100	14.9	28272	PASS
442	442	50	100	100.0	179648	PASS
443	442	15	24	19.3	34672	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/4/2024	BNA_F	<u>BF139651.D</u>
Compound Name	Response	Retention Time
DDT	556295	13.545
DDD	15210	13.245
DDE	917	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16127	572422	2.82

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100424\
Data File : BF139651.D
Acq On : 04 Oct 2024 12:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 04 12:43:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

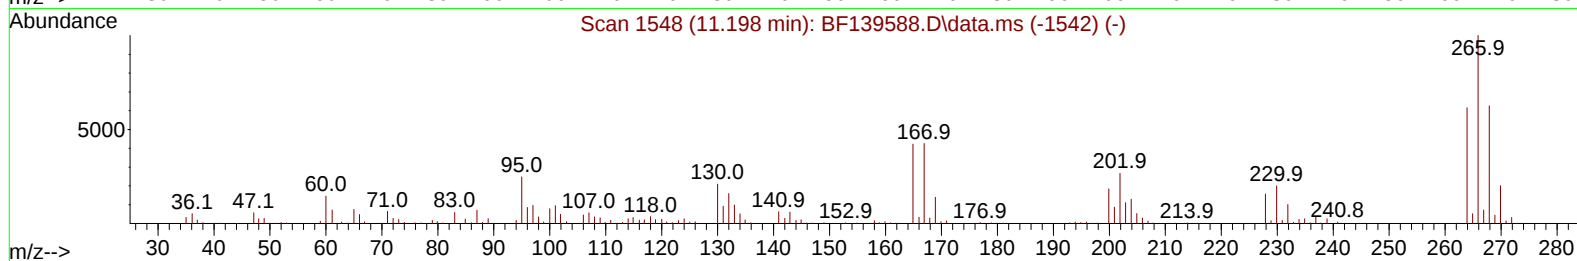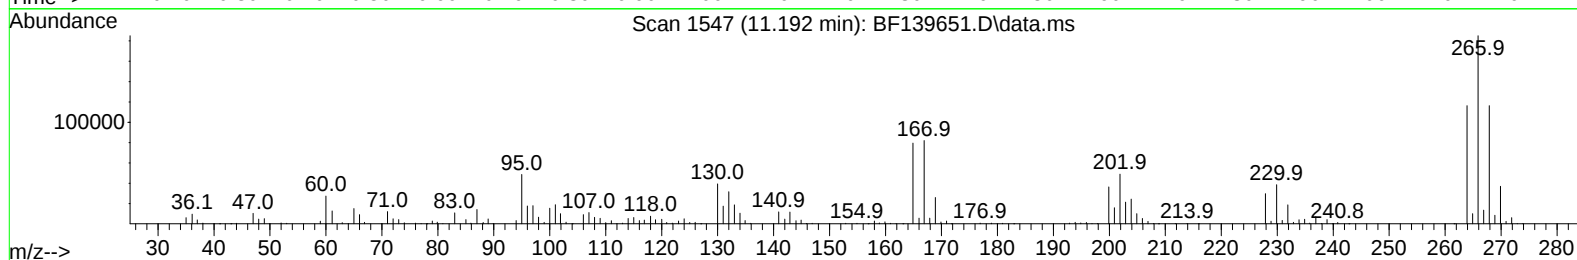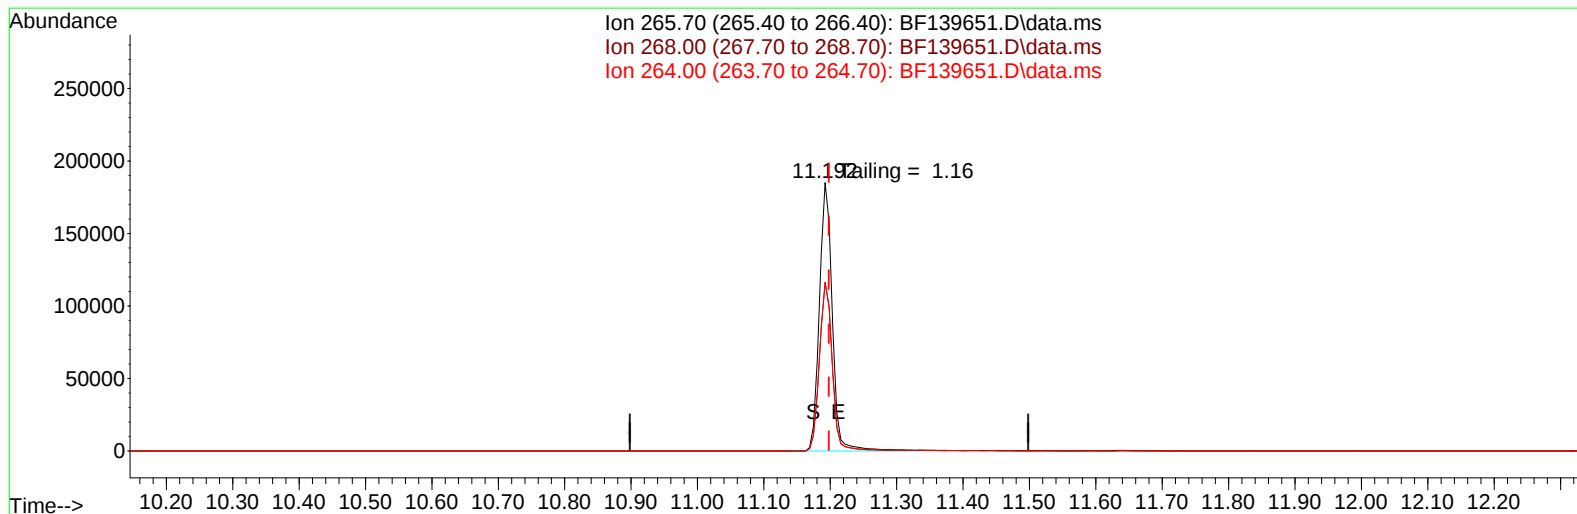

TIC: BF139651.D\data.ms

(70) Pentachlorophenol (C)

11.192min (-0.006) 616269.81 ng




response 250498

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	62.85
264.00	61.60	62.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100424\
Data File : BF139651.D
Acq On : 04 Oct 2024 12:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 04 12:43:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

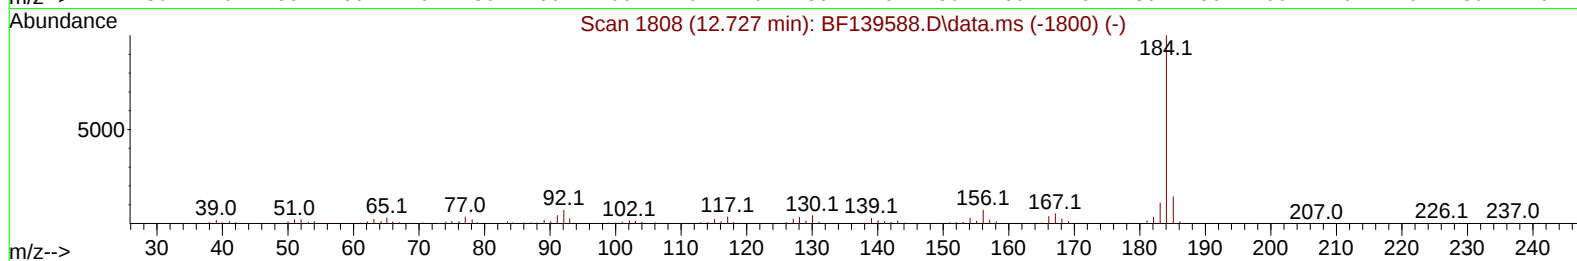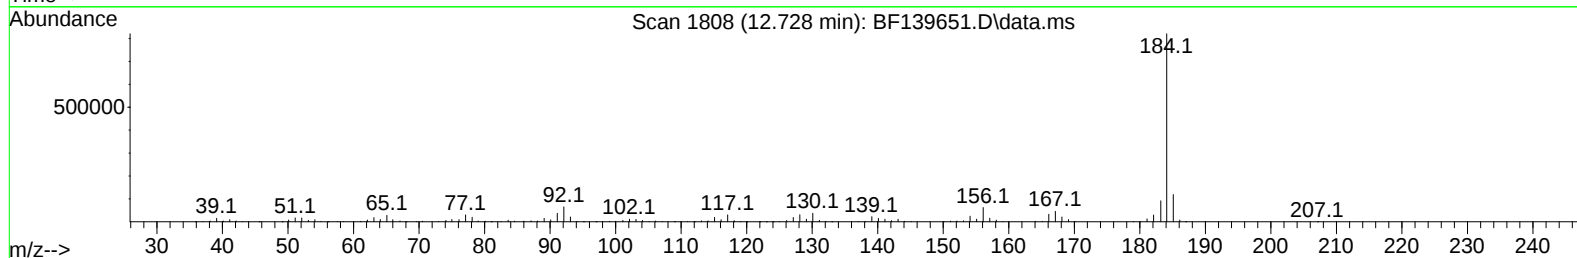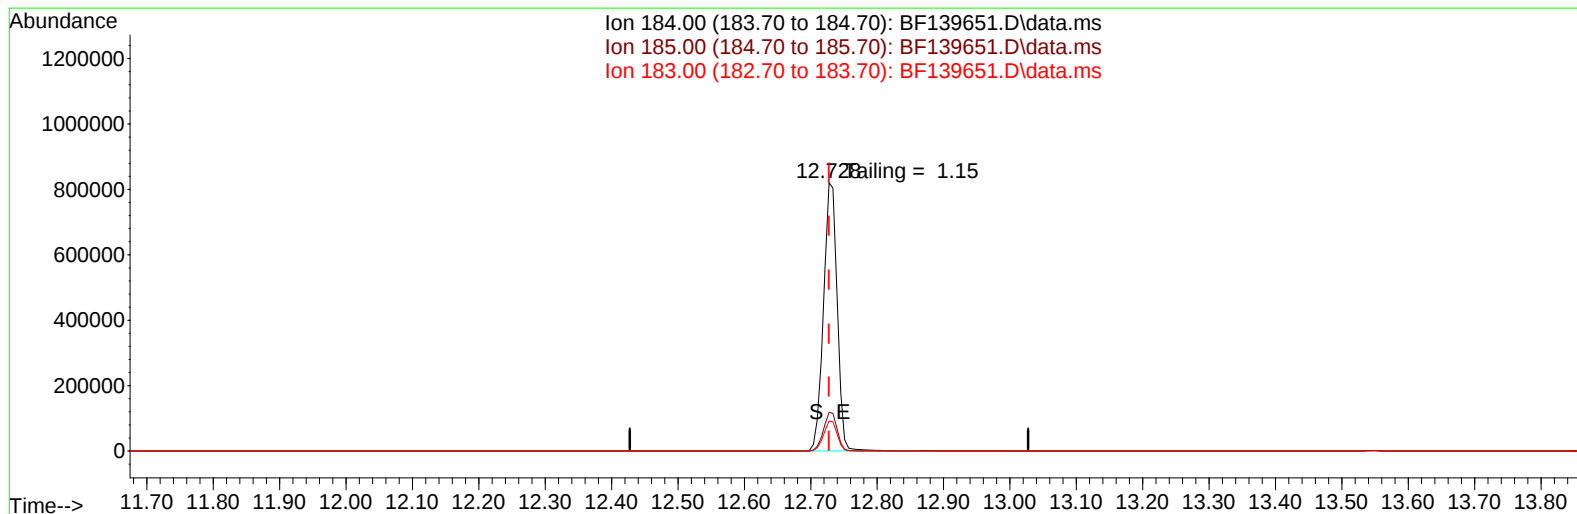

TIC: BF139651.D\data.ms

(77) Benzidine

12.728min (+ 0.000) 165307.58 ng

response 1180911

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.47
183.00	11.00	11.15
0.00	0.00	0.00