
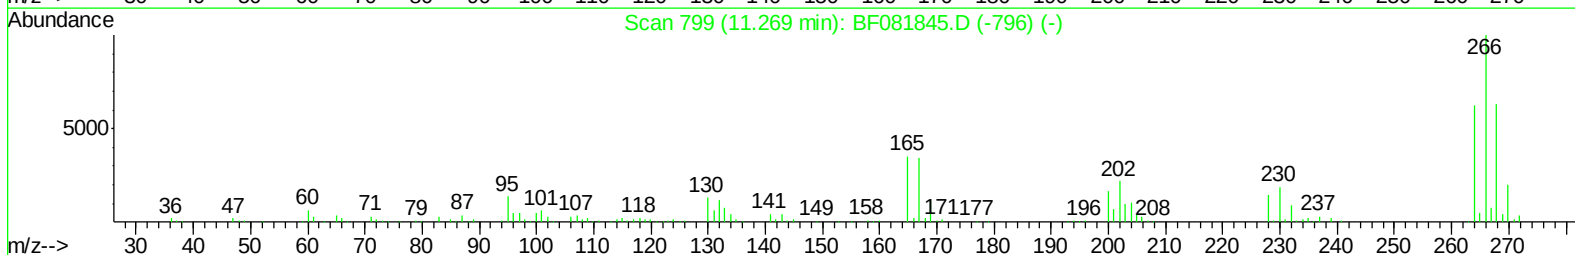
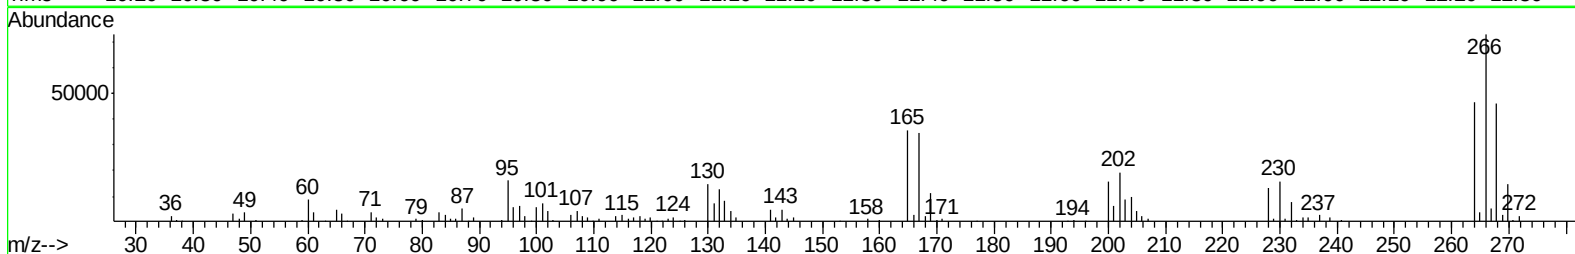


Data Path : Z:\HPCHEM1\BNA_F\Data\BF100515\
Data File : BF082041.D
Acq On : 5 Oct 2015 11:52
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 18:42:10 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 05 18:00:00 2015
Response via : Initial Calibration

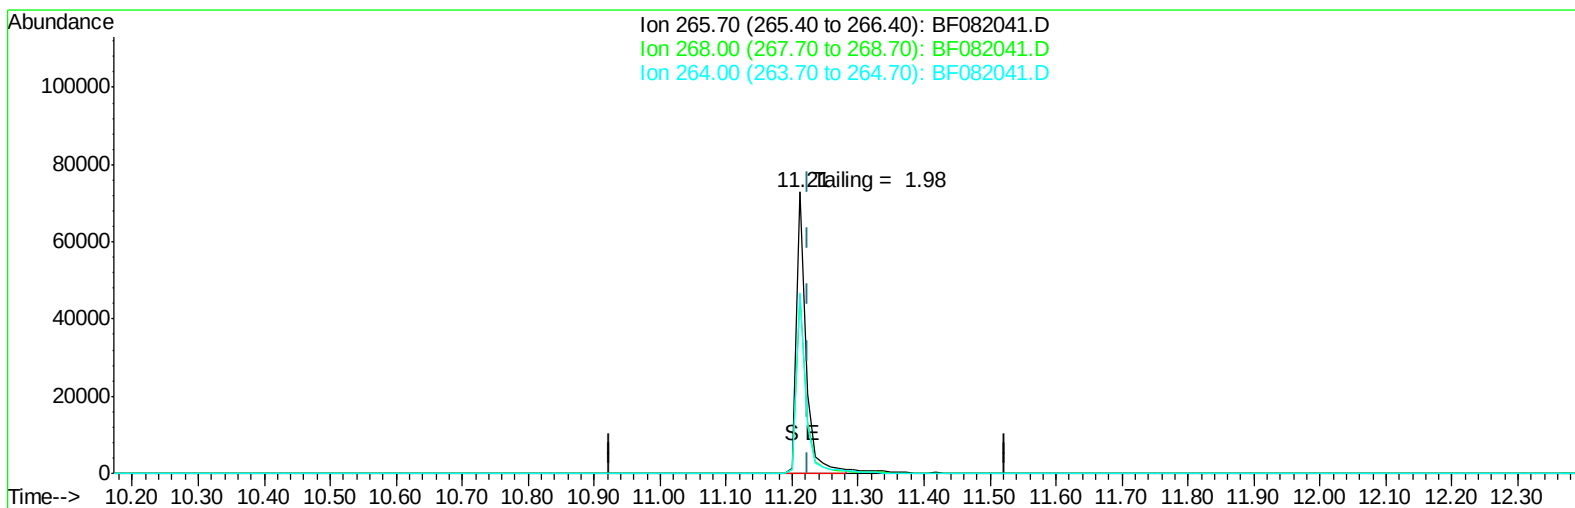

TIC: BF082041.D

(69) Pentachlorophenol (C)




11.212min (-0.011) 0.00ng

response 75827

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	63.38
264.00	62.70	63.99
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF100515\
Data File : BF082041.D
Acq On : 5 Oct 2015 11:52
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 18:42:10 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 05 18:00:00 2015
Response via : Initial Calibration

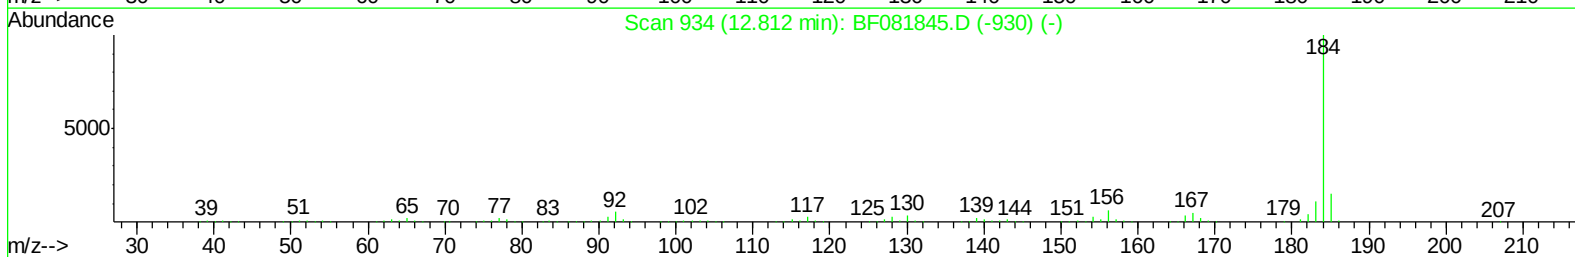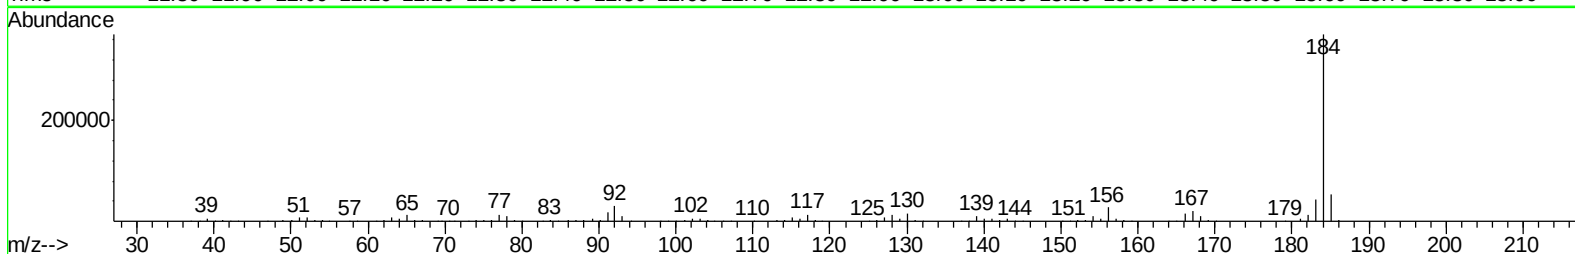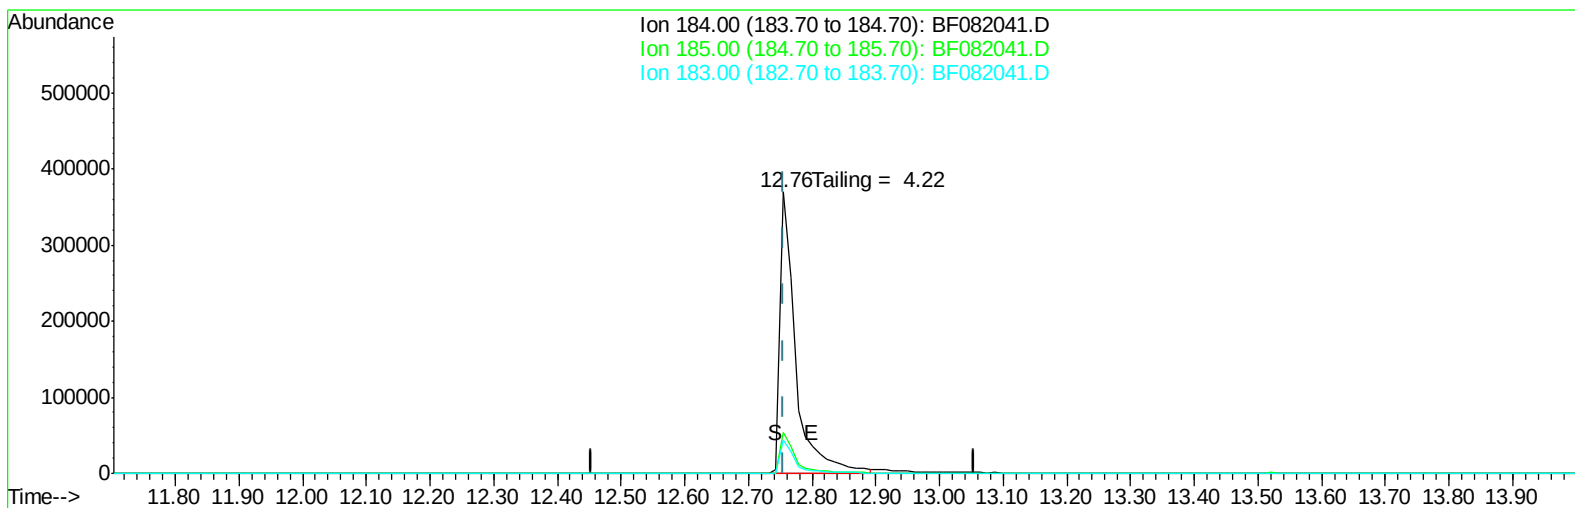

TIC: BF082041.D

(76) Benzidine

12.755min (0.000) 0.00ng

response 634016

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.41
183.00	9.50	11.68#
0.00	0.00	0.00